

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026053.D
 Acq On : 27 Dec 2021 11:54
 Operator : JC/MD
 Sample : VIBLK621
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK621

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M

Title : VOC Analysis

Signal : TIC: VX026053.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	56	rVB	150955	150603	15.38%	2.092%
2	1.666	91	95	105	rVB	103488	136063	13.89%	1.890%
3	2.312	194	201	217	rVB	219379	361151	36.87%	5.016%
4	2.520	230	235	242	rVB	2282	3701	0.38%	0.051%
5	2.794	275	280	287	rVB3	1888	3136	0.32%	0.044%
6	2.959	303	307	309	rBV3	253	424	0.04%	0.006%
7	3.093	325	329	334	rBV4	1014	1946	0.20%	0.027%
8	3.349	367	371	372	rBV	260	307	0.03%	0.004%
9	3.452	387	388	391	rVB	316	312	0.03%	0.004%
10	3.574	405	408	410	rBV	271	267	0.03%	0.004%
11	3.593	410	411	413	rVV2	320	265	0.03%	0.004%
12	3.641	417	419	422	rVV3	241	271	0.03%	0.004%
13	3.770	436	440	442	rBV2	290	431	0.04%	0.006%
14	4.178	502	507	508	rBV2	248	320	0.03%	0.004%
15	4.196	508	510	513	rVB2	279	313	0.03%	0.004%
16	4.458	544	553	568	rBV	73258	229188	23.40%	3.183%
17	4.702	590	593	595	rVB	521	459	0.05%	0.006%
18	4.727	595	597	601	rVB	250	267	0.03%	0.004%
19	4.916	626	628	630	rVB2	317	292	0.03%	0.004%
20	5.068	640	653	671	rBV3	104294	384838	39.29%	5.345%
21	5.269	684	686	690	rVB2	223	268	0.03%	0.004%
22	5.312	690	693	696	rBV2	262	501	0.05%	0.007%
23	5.391	702	706	707	rBV4	488	650	0.07%	0.009%
24	5.470	716	719	720	rBV2	684	747	0.08%	0.010%
25	5.544	726	731	733	rBV3	669	839	0.09%	0.012%
26	5.641	741	747	748	rBV2	232	363	0.04%	0.005%
27	5.976	789	802	819	rBV2	329240	979464	100.00%	13.604%
28	6.220	838	842	845	rVV2	253	337	0.03%	0.005%
29	6.458	878	881	884	rBV3	346	559	0.06%	0.008%
30	6.763	920	931	947	rBV	184842	445554	45.49%	6.189%
31	7.129	983	991	1000	rVB3	28268	64379	6.57%	0.894%
32	7.238	1006	1009	1012	rBV2	296	451	0.05%	0.006%
33	7.312	1012	1021	1040	rVV	211434	445634	45.50%	6.190%
34	7.476	1046	1048	1052	rVB3	564	705	0.07%	0.010%
35	7.811	1099	1103	1104	rBV2	678	755	0.08%	0.010%
36	7.933	1119	1123	1129	rVV3	613	1105	0.11%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026053.D
 Acq On : 27 Dec 2021 11:54
 Operator : JC/MD
 Sample : VIBLK621
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK621

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

37	8.244	1169	1174	1180	rVV	8247	13607	1.39%	0.189%
38	8.324	1181	1187	1204	rVB	131027	223550	22.82%	3.105%
39	8.464	1209	1210	1212	rBV	276	251	0.03%	0.003%
40	8.580	1227	1229	1234	rVV	485	605	0.06%	0.008%
41	8.653	1234	1241	1248	rVV	523622	797521	81.42%	11.077%
42	8.720	1248	1252	1260	rVB2	7782	13258	1.35%	0.184%
43	8.952	1284	1290	1305	rVV	97718	139256	14.22%	1.934%
44	9.147	1320	1322	1326	rVB2	324	326	0.03%	0.005%
45	9.189	1326	1329	1332	rVB2	303	309	0.03%	0.004%
46	9.281	1339	1344	1350	rBV2	5318	10967	1.12%	0.152%
47	9.384	1356	1361	1375	rVB	354132	492380	50.27%	6.839%
48	9.701	1410	1413	1416	rBV4	795	1096	0.11%	0.015%
49	9.817	1429	1432	1433	rBV2	255	299	0.03%	0.004%
50	10.055	1465	1471	1483	rBV	405003	548608	56.01%	7.620%
51	10.195	1491	1494	1498	rVV2	1960	2009	0.21%	0.028%
52	10.299	1506	1511	1517	rVB3	2978	4264	0.44%	0.059%
53	10.524	1544	1548	1550	rBV2	233	346	0.04%	0.005%
54	10.561	1552	1554	1556	rVB2	310	256	0.03%	0.004%
55	10.646	1563	1568	1574	rVB4	1500	3074	0.31%	0.043%
56	10.719	1574	1580	1582	rBV2	239	427	0.04%	0.006%
57	10.841	1599	1600	1603	rBV	300	283	0.03%	0.004%
58	10.963	1615	1620	1625	rBV3	1228	1720	0.18%	0.024%
59	11.122	1641	1646	1650	rBV	4323	5097	0.52%	0.071%
60	11.195	1652	1658	1667	rBV	355160	455860	46.54%	6.332%
61	11.317	1674	1678	1683	rVB5	3062	5716	0.58%	0.079%
62	11.384	1685	1689	1694	rVB3	543	777	0.08%	0.011%
63	11.451	1696	1700	1703	rBV	1396	1972	0.20%	0.027%
64	11.549	1715	1716	1720	rVB2	767	577	0.06%	0.008%
65	11.634	1728	1730	1736	rVV2	461	530	0.05%	0.007%
66	11.683	1736	1738	1740	rVV2	393	426	0.04%	0.006%
67	11.713	1740	1743	1745	rVV3	526	716	0.07%	0.010%
68	11.750	1745	1749	1755	rVV3	4907	6832	0.70%	0.095%
69	11.841	1761	1764	1769	rVB2	834	852	0.09%	0.012%
70	11.933	1776	1779	1782	rVB2	1808	1976	0.20%	0.027%
71	11.969	1782	1785	1788	rVV	1847	1933	0.20%	0.027%
72	12.024	1788	1794	1806	rVV	440825	544768	55.62%	7.567%
73	12.128	1806	1811	1812	rVV2	1877	2442	0.25%	0.034%
74	12.152	1812	1815	1819	rVB3	3119	3935	0.40%	0.055%
75	12.262	1830	1833	1835	rBV2	333	398	0.04%	0.006%
76	12.323	1835	1843	1851	rVV	510418	663254	67.72%	9.212%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026053.D
 Acq On : 27 Dec 2021 11:54
 Operator : JC/MD
 Sample : VIBLK621
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK621

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	12.426	1856	1860	1864	rVB3	1031	1614	0.16%	0.022%
78	12.481	1864	1869	1874	rVB3	866	1201	0.12%	0.017%
79	12.615	1889	1891	1893	rBV2	357	297	0.03%	0.004%
80	12.658	1896	1898	1901	rVB3	588	706	0.07%	0.010%
81	12.768	1911	1916	1919	rBV2	1470	1990	0.20%	0.028%
82	12.957	1946	1947	1953	rBV3	186	267	0.03%	0.004%
83	13.048	1960	1962	1966	rBV3	743	1034	0.11%	0.014%
84	13.115	1970	1973	1977	rVB2	2200	2533	0.26%	0.035%
85	13.225	1989	1991	1992	rBV	332	251	0.03%	0.003%
86	13.359	2009	2013	2015	rVB2	271	327	0.03%	0.005%
87	13.384	2015	2017	2019	rBV2	256	257	0.03%	0.004%
88	13.439	2023	2026	2028	rBV	478	422	0.04%	0.006%
89	13.591	2047	2051	2056	rVB	3040	3543	0.36%	0.049%
90	13.664	2061	2063	2067	rVB2	227	306	0.03%	0.004%
91	13.707	2067	2070	2073	rBV2	271	408	0.04%	0.006%
92	13.780	2077	2082	2086	rVV	3143	4082	0.42%	0.057%
93	13.963	2107	2112	2116	rVV3	2952	3681	0.38%	0.051%
94	14.134	2134	2140	2144	rBV2	2530	3744	0.38%	0.052%
95	14.621	2219	2220	2224	rBV2	285	369	0.04%	0.005%
96	14.853	2257	2258	2261	rVB2	292	258	0.03%	0.004%
97	14.883	2261	2263	2265	rBV2	272	254	0.03%	0.004%
98	15.395	2342	2347	2351	rVB2	1471	1978	0.20%	0.027%
99	16.084	2459	2460	2464	rVB3	422	413	0.04%	0.006%
100	16.359	2504	2505	2507	rBV2	367	333	0.03%	0.005%




Sum of corrected areas: 7199606

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026053.D
Acq On : 27 Dec 2021 11:54
Operator : JC/MD
Sample : VIBLK621
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK621

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

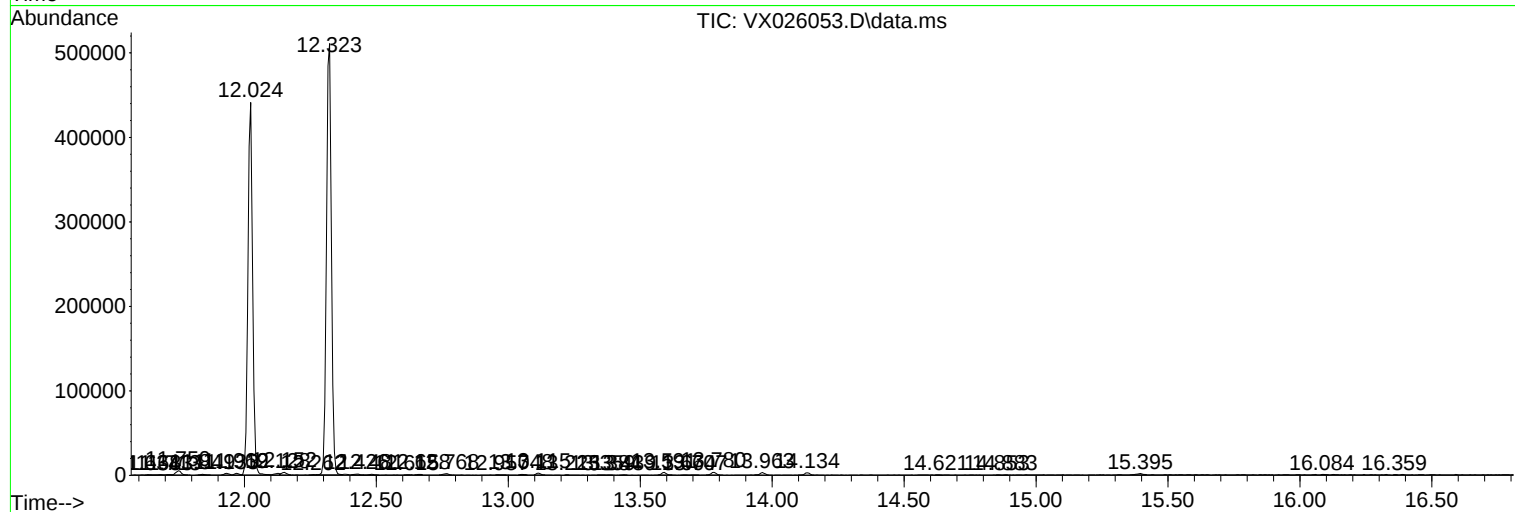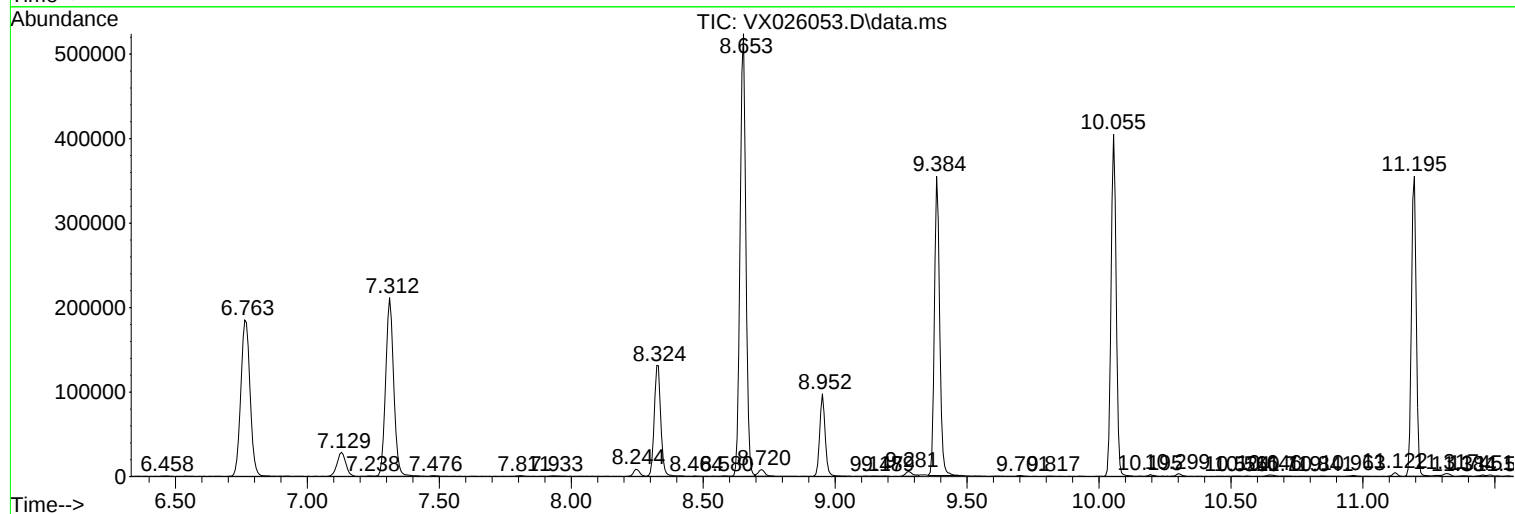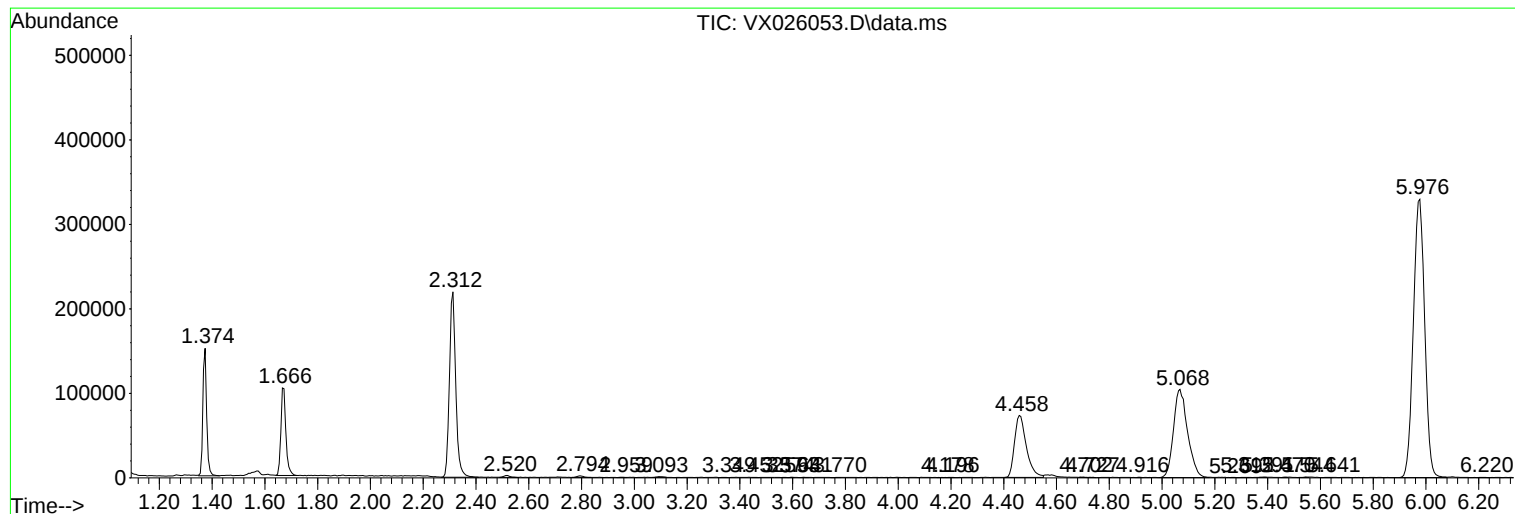

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026053.D
Acq On : 27 Dec 2021 11:54
Operator : JC/MD
Sample : VIBLK621
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK621

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026053.D
Acq On : 27 Dec 2021 11:54
Operator : JC/MD
Sample : VIBLK621
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK621

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------