

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026054.D
 Acq On : 27 Dec 2021 12:17
 Operator : JC/MD
 Sample : M5121-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026054.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.373	43	47	53	rVB	117659	114765	13.70%	1.863%
2	1.666	91	95	106	rVB	93718	111550	13.32%	1.811%
3	2.312	194	201	220	rVB	167291	282105	33.68%	4.580%
4	2.513	229	234	238	rBV3	1032	1781	0.21%	0.029%
5	2.708	259	266	269	rBV3	702	1236	0.15%	0.020%
6	2.794	276	280	288	rVB4	1982	3488	0.42%	0.057%
7	2.940	302	304	306	rVB2	303	240	0.03%	0.004%
8	2.983	306	311	312	rBV2	324	436	0.05%	0.007%
9	3.093	327	329	330	rBV	570	468	0.06%	0.008%
10	3.556	399	405	407	rBV2	181	340	0.04%	0.006%
11	3.605	409	413	417	rBV2	269	390	0.05%	0.006%
12	3.812	443	447	450	rBV2	137	228	0.03%	0.004%
13	3.897	458	461	462	rBV2	253	264	0.03%	0.004%
14	4.098	492	494	498	rBV2	155	280	0.03%	0.005%
15	4.458	540	553	567	rBV2	67225	213748	25.52%	3.470%
16	5.062	639	652	675	rVB2	92253	330367	39.44%	5.364%
17	5.379	702	704	705	rBV2	304	286	0.03%	0.005%
18	5.458	715	717	719	rBV2	480	468	0.06%	0.008%
19	5.537	728	730	731	rBV2	322	281	0.03%	0.005%
20	5.677	751	753	755	rVV2	248	249	0.03%	0.004%
21	5.879	784	786	789	rBV2	173	235	0.03%	0.004%
22	5.970	789	801	818	rBV2	279951	837724	100.00%	13.602%
23	6.330	857	860	864	rVB2	204	292	0.03%	0.005%
24	6.360	864	865	869	rVB2	247	291	0.03%	0.005%
25	6.635	909	910	913	rBV	243	218	0.03%	0.004%
26	6.763	921	931	947	rBV	163798	387560	46.26%	6.293%
27	7.128	982	991	1002	rBV5	18293	41991	5.01%	0.682%
28	7.311	1012	1021	1032	rBV	173348	382464	45.66%	6.210%
29	7.470	1045	1047	1048	rBV2	321	278	0.03%	0.005%
30	7.805	1099	1102	1108	rBV4	400	657	0.08%	0.011%
31	7.939	1118	1124	1126	rVV3	394	772	0.09%	0.013%
32	8.238	1171	1173	1175	rBV2	259	217	0.03%	0.004%
33	8.323	1181	1187	1200	rBV	115104	190759	22.77%	3.097%
34	8.415	1200	1202	1205	rVB3	426	362	0.04%	0.006%
35	8.579	1227	1229	1232	rBV2	324	336	0.04%	0.005%
36	8.652	1234	1241	1249	rVV	419213	662009	79.02%	10.749%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026054.D
 Acq On : 27 Dec 2021 12:17
 Operator : JC/MD
 Sample : M5121-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	8.726	1249	1253	1259	rVV	6128	10318	1.23%	0.168%
38	8.774	1259	1261	1264	rVB4	341	230	0.03%	0.004%
39	8.951	1284	1290	1301	rBV	80645	118792	14.18%	1.929%
40	9.238	1336	1337	1339	rBV	295	238	0.03%	0.004%
41	9.280	1339	1344	1352	rVV2	5719	12070	1.44%	0.196%
42	9.384	1356	1361	1375	rVB	328061	464780	55.48%	7.546%
43	9.579	1391	1393	1396	rVB2	233	262	0.03%	0.004%
44	9.634	1399	1402	1403	rBV	309	333	0.04%	0.005%
45	9.707	1408	1414	1416	rBV3	726	1018	0.12%	0.017%
46	10.055	1465	1471	1482	rBV	367524	482271	57.57%	7.830%
47	10.195	1491	1494	1501	rVB2	1523	2089	0.25%	0.034%
48	10.305	1507	1512	1519	rVB2	3840	4970	0.59%	0.081%
49	10.360	1519	1521	1523	rBV	475	298	0.04%	0.005%
50	10.396	1526	1527	1530	rVB	343	274	0.03%	0.004%
51	10.646	1563	1568	1575	rVB4	1636	2582	0.31%	0.042%
52	10.762	1584	1587	1588	rBV2	267	285	0.03%	0.005%
53	10.866	1601	1604	1606	rBV	281	273	0.03%	0.004%
54	10.969	1616	1621	1622	rBV2	1089	1239	0.15%	0.020%
55	11.048	1632	1634	1637	rVB	272	295	0.04%	0.005%
56	11.085	1637	1640	1641	rBV	392	392	0.05%	0.006%
57	11.122	1641	1646	1650	rVB	2941	3506	0.42%	0.057%
58	11.195	1652	1658	1666	rBV	322138	416730	49.75%	6.766%
59	11.323	1673	1679	1684	rVB5	2595	4896	0.58%	0.079%
60	11.457	1697	1701	1702	rBV2	1292	1630	0.19%	0.026%
61	11.475	1702	1704	1711	rVB3	2292	3114	0.37%	0.051%
62	11.548	1713	1716	1719	rBV2	331	384	0.05%	0.006%
63	11.670	1733	1736	1737	rBV	254	286	0.03%	0.005%
64	11.713	1741	1743	1745	rVV3	492	594	0.07%	0.010%
65	11.750	1745	1749	1753	rVB3	4574	5567	0.66%	0.090%
66	11.841	1761	1764	1769	rVB	647	861	0.10%	0.014%
67	11.896	1769	1773	1776	rBV2	226	314	0.04%	0.005%
68	11.938	1776	1780	1783	rBV3	1533	2097	0.25%	0.034%
69	11.975	1783	1786	1788	rBV2	1209	1270	0.15%	0.021%
70	12.024	1789	1794	1806	rBV	379593	457467	54.61%	7.428%
71	12.121	1807	1810	1812	rBV4	744	859	0.10%	0.014%
72	12.262	1830	1833	1836	rVB2	450	507	0.06%	0.008%
73	12.323	1836	1843	1851	rBV	438588	563283	67.24%	9.146%
74	12.377	1851	1852	1854	rVV2	823	522	0.06%	0.008%
75	12.426	1857	1860	1865	rVB2	1589	2044	0.24%	0.033%
76	12.481	1865	1869	1874	rBV3	683	1246	0.15%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026054.D
 Acq On : 27 Dec 2021 12:17
 Operator : JC/MD
 Sample : M5121-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	12.627	1890	1893	1894	rVV2	339	305	0.04%	0.005%
78	12.664	1896	1899	1901	rVB2	518	566	0.07%	0.009%
79	12.762	1911	1915	1922	rBV	1764	2820	0.34%	0.046%
80	12.829	1922	1926	1927	rBV2	212	315	0.04%	0.005%
81	12.926	1940	1942	1948	rBV	198	234	0.03%	0.004%
82	13.054	1959	1963	1966	rBV	731	944	0.11%	0.015%
83	13.115	1970	1973	1976	rBV2	1536	1766	0.21%	0.029%
84	13.158	1979	1980	1983	rBV	257	224	0.03%	0.004%
85	13.292	2000	2002	2005	rVV2	232	253	0.03%	0.004%
86	13.591	2047	2051	2057	rVB2	1475	1967	0.23%	0.032%
87	13.646	2057	2060	2064	rBV2	211	377	0.05%	0.006%
88	13.780	2079	2082	2088	rVV2	1666	1843	0.22%	0.030%
89	13.963	2109	2112	2116	rVV3	875	1192	0.14%	0.019%
90	14.017	2120	2121	2124	rBV2	181	228	0.03%	0.004%
91	14.133	2133	2140	2144	rBV	2589	3719	0.44%	0.060%
92	14.371	2177	2179	2181	rBV	298	305	0.04%	0.005%
93	14.639	2220	2223	2225	rBV2	192	252	0.03%	0.004%
94	14.694	2228	2232	2233	rBV2	369	397	0.05%	0.006%
95	14.755	2241	2242	2244	rBV2	354	225	0.03%	0.004%
96	15.535	2367	2370	2371	rBV2	297	402	0.05%	0.007%
97	15.987	2442	2444	2446	rVB2	441	272	0.03%	0.004%
98	16.529	2532	2533	2536	rBV3	514	354	0.04%	0.006%
99	16.614	2545	2547	2548	rBV2	477	362	0.04%	0.006%
100	16.730	2564	2566	2569	rBV2	381	361	0.04%	0.006%


Sum of corrected areas: 6159004

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026054.D
Acq On : 27 Dec 2021 12:17
Operator : JC/MD
Sample : M5121-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

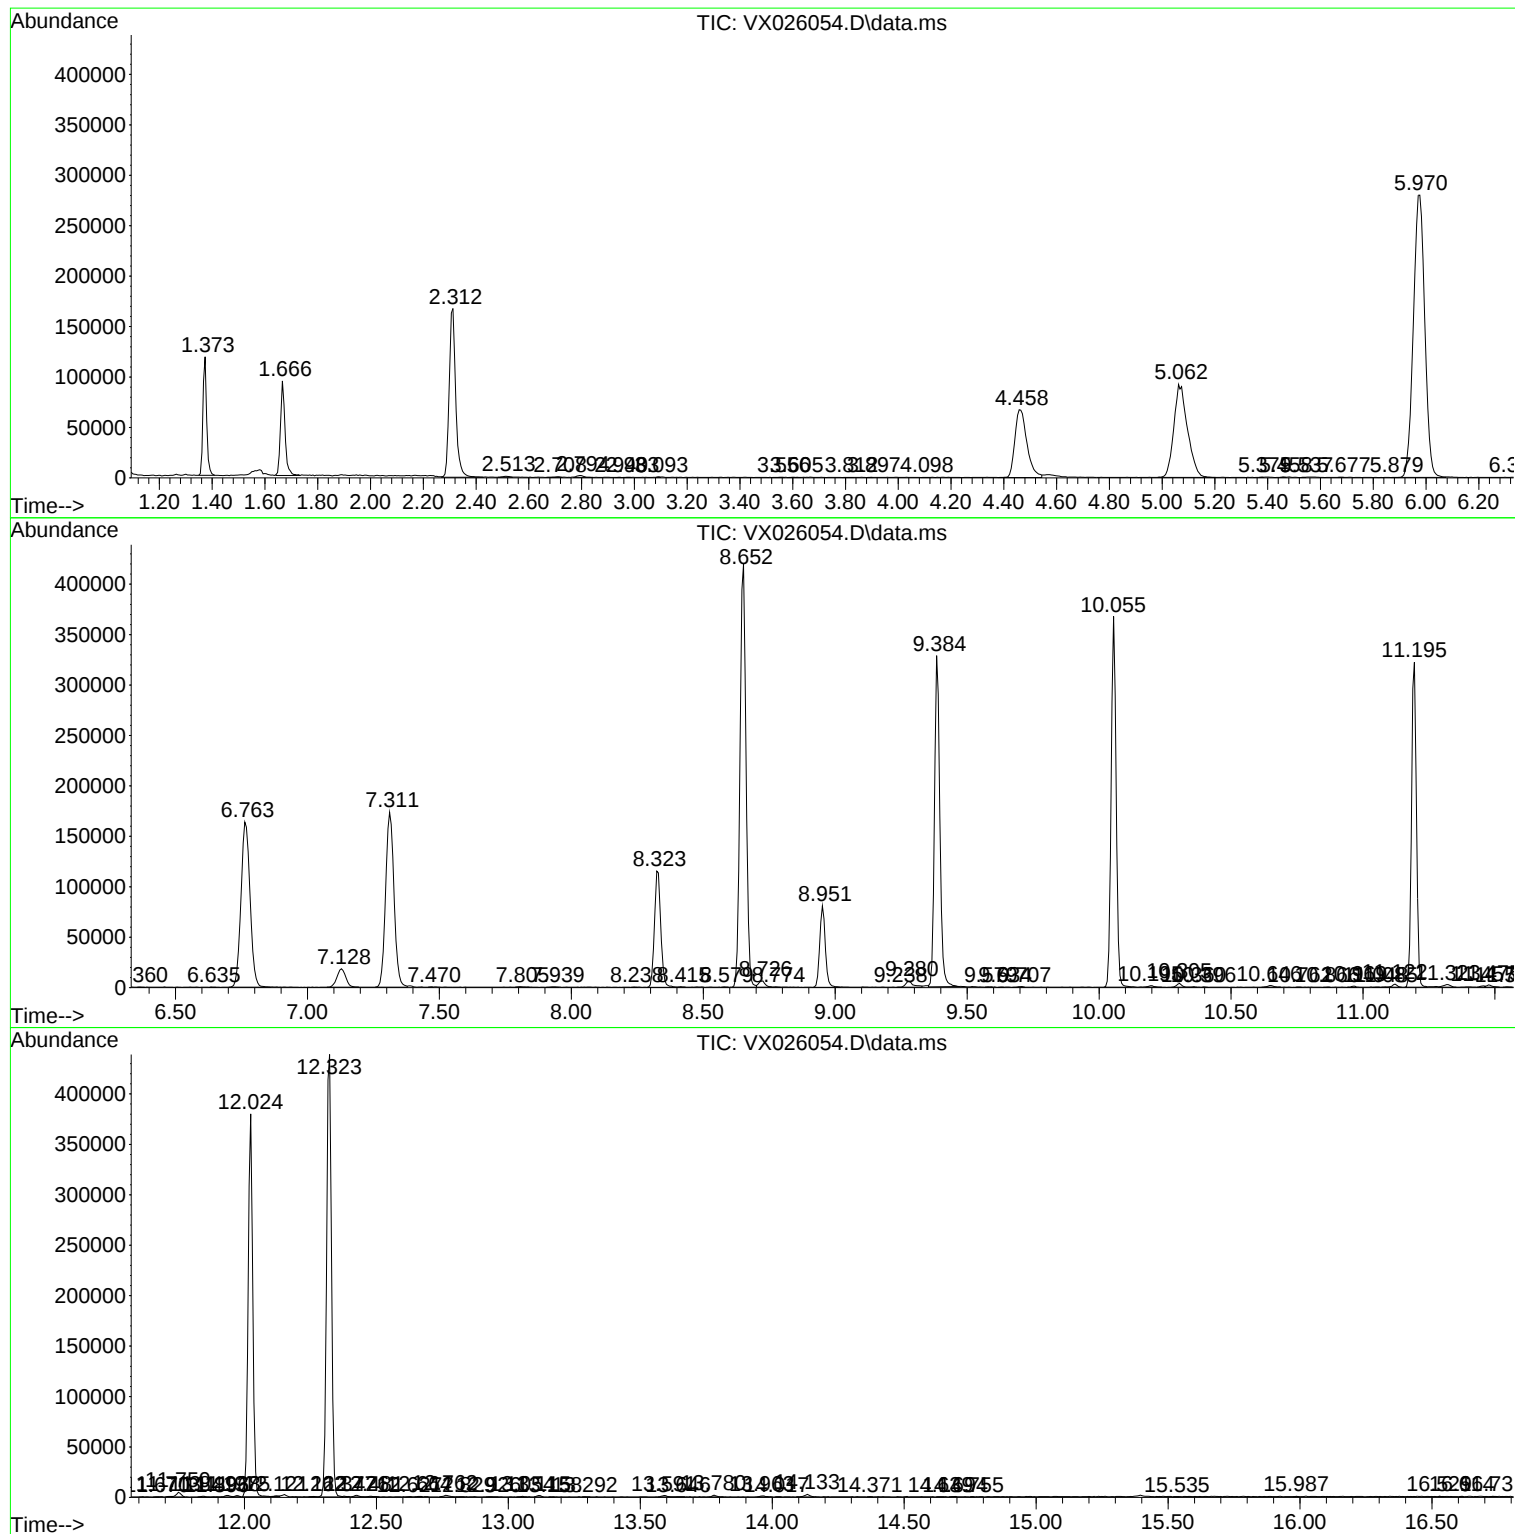

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026054.D
Acq On : 27 Dec 2021 12:17
Operator : JC/MD
Sample : M5121-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026054.D
Acq On : 27 Dec 2021 12:17
Operator : JC/MD
Sample : M5121-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc