

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026055.D
 Acq On : 27 Dec 2021 12:40
 Operator : JC/MD
 Sample : M5150-25DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBY1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026055.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	25	27	32	rBV	4818	5317	0.57%	0.069%
2	1.374	43	47	56	rVB	146001	147705	15.83%	1.909%
3	1.672	91	96	104	rVB	100198	131678	14.11%	1.702%
4	2.313	194	201	218	rVB	216598	346912	37.18%	4.484%
5	2.617	249	251	252	rBV2	257	253	0.03%	0.003%
6	2.715	262	267	268	rBV3	287	446	0.05%	0.006%
7	2.800	275	281	286	rVB3	1556	3078	0.33%	0.040%
8	2.873	290	293	295	rBV2	208	292	0.03%	0.004%
9	2.959	305	307	310	rVB2	390	339	0.04%	0.004%
10	3.008	310	315	316	rBV2	308	463	0.05%	0.006%
11	3.093	325	329	334	rVV3	628	991	0.11%	0.013%
12	3.190	341	345	346	rVB2	206	202	0.02%	0.003%
13	3.227	349	351	355	rVV2	244	371	0.04%	0.005%
14	4.001	476	478	479	rBV	318	211	0.02%	0.003%
15	4.227	512	515	516	rBV2	205	227	0.02%	0.003%
16	4.465	542	554	570	rBV3	72356	265070	28.41%	3.426%
17	4.684	588	590	593	rBV2	244	237	0.03%	0.003%
18	4.788	605	607	609	rBV2	212	221	0.02%	0.003%
19	5.068	639	653	673	rVB2	106736	369742	39.63%	4.779%
20	5.196	673	674	676	rBV	322	203	0.02%	0.003%
21	5.391	702	706	707	rBV3	455	502	0.05%	0.006%
22	5.489	721	722	726	rVB2	354	289	0.03%	0.004%
23	5.538	728	730	731	rBV	391	280	0.03%	0.004%
24	5.818	771	776	781	rVB2	191	437	0.05%	0.006%
25	5.977	787	802	819	rBV2	311547	932956	100.00%	12.060%
26	6.196	837	838	842	rVB2	260	224	0.02%	0.003%
27	6.495	885	887	891	rVB2	199	304	0.03%	0.004%
28	6.544	891	895	896	rBV2	219	302	0.03%	0.004%
29	6.763	922	931	947	rBV	211541	493671	52.91%	6.381%
30	7.129	982	991	1006	rVV	307274	657500	70.47%	8.499%
31	7.312	1012	1021	1036	rBV	191337	421462	45.17%	5.448%
32	7.470	1045	1047	1048	rBV	687	442	0.05%	0.006%
33	7.647	1075	1076	1081	rVB2	241	233	0.02%	0.003%
34	7.726	1088	1089	1093	rBV2	177	239	0.03%	0.003%
35	7.799	1098	1101	1102	rBV2	348	357	0.04%	0.005%
36	7.934	1120	1123	1126	rBV2	567	835	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026055.D
 Acq On : 27 Dec 2021 12:40
 Operator : JC/MD
 Sample : M5150-25DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBY1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	7.982	1130	1131	1134	rVB	340	258	0.03%	0.003%
38	8.055	1137	1143	1145	rVB3	354	723	0.08%	0.009%
39	8.074	1145	1146	1149	rBV	204	274	0.03%	0.004%
40	8.324	1181	1187	1199	rBV	123488	207018	22.19%	2.676%
41	8.421	1202	1203	1209	rVV2	283	369	0.04%	0.005%
42	8.482	1209	1213	1218	rVV2	416	618	0.07%	0.008%
43	8.653	1234	1241	1248	rBV	487251	764756	81.97%	9.885%
44	8.720	1248	1252	1263	rVB	6969	11964	1.28%	0.155%
45	8.909	1281	1283	1284	rBV	284	213	0.02%	0.003%
46	8.952	1284	1290	1300	rBV	89357	130182	13.95%	1.683%
47	9.281	1336	1344	1350	rBV3	5574	11036	1.18%	0.143%
48	9.384	1356	1361	1374	rVB	357140	481630	51.62%	6.226%
49	9.689	1408	1411	1412	rVB2	299	276	0.03%	0.004%
50	9.878	1440	1442	1445	rBV2	176	258	0.03%	0.003%
51	9.909	1445	1447	1450	rVB	278	270	0.03%	0.003%
52	9.939	1450	1452	1454	rBV	380	217	0.02%	0.003%
53	10.055	1465	1471	1481	rBV	464060	613569	65.77%	7.931%
54	10.201	1490	1495	1498	rBV3	998	1331	0.14%	0.017%
55	10.305	1508	1512	1518	rVB3	1956	2843	0.30%	0.037%
56	10.567	1553	1555	1557	rBV	318	325	0.03%	0.004%
57	10.646	1566	1568	1572	rVB2	784	804	0.09%	0.010%
58	10.860	1600	1603	1605	rBV2	218	290	0.03%	0.004%
59	10.921	1612	1613	1615	rBV	280	200	0.02%	0.003%
60	10.963	1617	1620	1622	rVV2	466	431	0.05%	0.006%
61	11.122	1641	1646	1652	rBV2	3764	4877	0.52%	0.063%
62	11.195	1652	1658	1666	rBV	342253	436711	46.81%	5.645%
63	11.378	1686	1688	1690	rBV2	285	263	0.03%	0.003%
64	11.445	1695	1699	1700	rBV2	469	437	0.05%	0.006%
65	11.482	1701	1705	1708	rVV4	855	1294	0.14%	0.017%
66	11.549	1714	1716	1719	rVB2	500	452	0.05%	0.006%
67	11.591	1721	1723	1725	rBV2	209	201	0.02%	0.003%
68	11.683	1735	1738	1741	rBV2	386	455	0.05%	0.006%
69	11.713	1741	1743	1744	rVV2	379	269	0.03%	0.003%
70	11.750	1745	1749	1756	rVB2	3988	4942	0.53%	0.064%
71	11.841	1762	1764	1769	rVB3	682	758	0.08%	0.010%
72	11.933	1773	1779	1782	rBV3	2004	2758	0.30%	0.036%
73	12.024	1788	1794	1806	rBV	496924	594740	63.75%	7.688%
74	12.122	1808	1810	1812	rBV	1044	1114	0.12%	0.014%
75	12.219	1824	1826	1830	rBV3	249	347	0.04%	0.004%
76	12.323	1835	1843	1850	rBV	494605	653339	70.03%	8.445%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026055.D
 Acq On : 27 Dec 2021 12:40
 Operator : JC/MD
 Sample : M5150-25DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBY1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	12.433	1856	1861	1863	rVB4	1172	1759	0.19%	0.023%
78	12.475	1863	1868	1875	rBV4	684	1271	0.14%	0.016%
79	12.579	1883	1885	1886	rBV	322	281	0.03%	0.004%
80	12.628	1891	1893	1894	rVV2	422	280	0.03%	0.004%
81	12.658	1896	1898	1906	rVB4	948	1755	0.19%	0.023%
82	12.768	1911	1916	1923	rVV3	1709	2820	0.30%	0.036%
83	12.823	1923	1925	1927	rVV2	524	399	0.04%	0.005%
84	12.847	1927	1929	1931	rVV	232	267	0.03%	0.003%
85	13.048	1959	1962	1966	rVB3	769	1025	0.11%	0.013%
86	13.116	1971	1973	1975	rVB	343	249	0.03%	0.003%
87	13.280	1998	2000	2003	rVB2	226	240	0.03%	0.003%
88	13.311	2003	2005	2008	rBV2	288	361	0.04%	0.005%
89	13.591	2049	2051	2054	rVV2	485	411	0.04%	0.005%
90	13.750	2074	2077	2079	rBV2	155	215	0.02%	0.003%
91	13.774	2079	2081	2086	rBV2	608	980	0.11%	0.013%
92	13.963	2110	2112	2116	rVB	626	485	0.05%	0.006%
93	14.134	2136	2140	2145	rVB3	2575	3884	0.42%	0.050%
94	14.231	2155	2156	2161	rVB2	268	344	0.04%	0.004%
95	14.286	2161	2165	2168	rBV2	289	408	0.04%	0.005%
96	14.871	2259	2261	2263	rBV	300	217	0.02%	0.003%
97	14.896	2263	2265	2270	rVV3	313	389	0.04%	0.005%
98	15.646	2385	2388	2389	rBV2	365	421	0.05%	0.005%
99	15.694	2394	2396	2399	rBV2	523	667	0.07%	0.009%
100	15.999	2444	2446	2448	rBV2	368	257	0.03%	0.003%




Sum of corrected areas: 7736188

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026055.D
Acq On : 27 Dec 2021 12:40
Operator : JC/MD
Sample : M5150-25DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBY1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

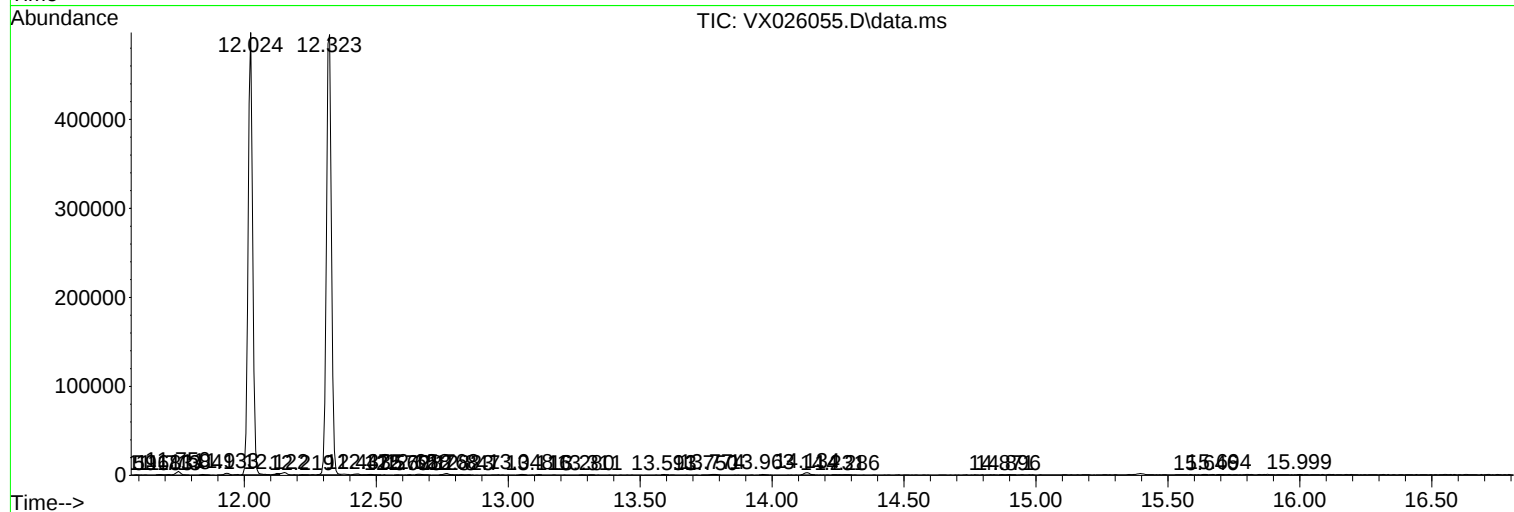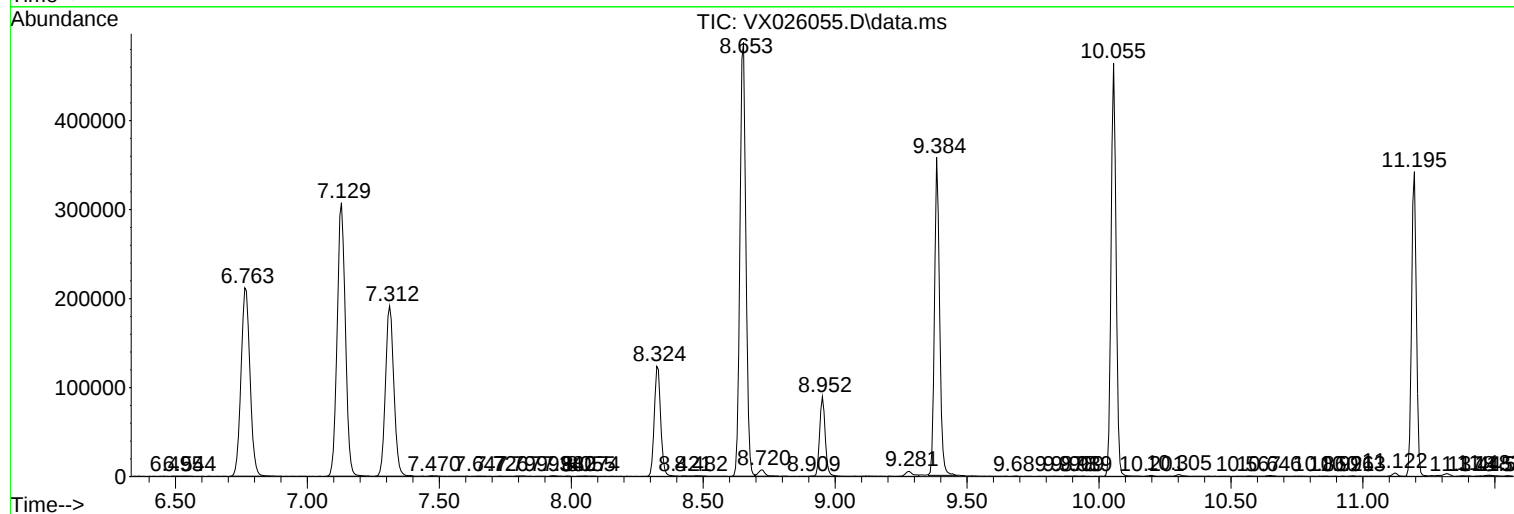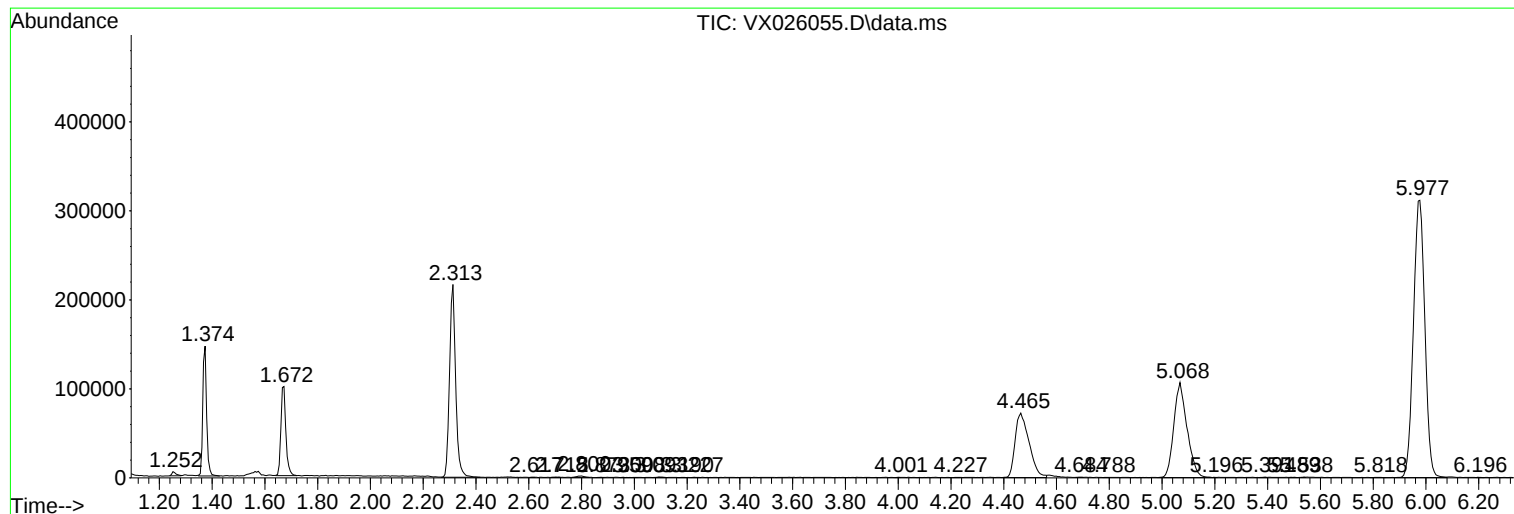

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026055.D
Acq On : 27 Dec 2021 12:40
Operator : JC/MD
Sample : M5150-25DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBY1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026055.D
Acq On : 27 Dec 2021 12:40
Operator : JC/MD
Sample : M5150-25DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBY1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc