

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026056.D
 Acq On : 27 Dec 2021 13:04
 Operator : JC/MD
 Sample : M5150-29
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026056.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	55	rVB	145107	147800	15.56%	2.108%
2	1.666	91	95	104	rVB	104927	132314	13.93%	1.887%
3	2.312	194	201	215	rVB	208403	347248	36.56%	4.953%
4	2.599	246	248	250	rVB	265	199	0.02%	0.003%
5	2.623	250	252	256	rBV3	182	260	0.03%	0.004%
6	2.690	261	263	264	rBV	223	217	0.02%	0.003%
7	2.733	269	270	273	rVB	394	238	0.03%	0.003%
8	2.794	276	280	286	rVB4	1848	3002	0.32%	0.043%
9	2.849	287	289	293	rVB2	252	287	0.03%	0.004%
10	3.050	321	322	326	rVB2	317	291	0.03%	0.004%
11	3.264	356	357	361	rVB	287	225	0.02%	0.003%
12	3.306	361	364	366	rBV	181	252	0.03%	0.004%
13	3.428	382	384	387	rVB2	318	290	0.03%	0.004%
14	3.721	429	432	435	rBV2	235	372	0.04%	0.005%
15	3.934	466	467	470	rVB3	198	210	0.02%	0.003%
16	4.105	493	495	498	rBV2	273	328	0.03%	0.005%
17	4.458	544	553	568	rBV2	69330	213463	22.47%	3.045%
18	5.068	641	653	671	rBV3	110119	372555	39.22%	5.314%
19	5.336	695	697	700	rBV2	261	251	0.03%	0.004%
20	5.403	703	708	711	rVB4	508	869	0.09%	0.012%
21	5.544	729	731	732	rBV	330	327	0.03%	0.005%
22	5.629	741	745	746	rBV2	133	189	0.02%	0.003%
23	5.659	748	750	755	rVB	386	401	0.04%	0.006%
24	5.976	789	802	824	rBV2	322327	949817	100.00%	13.548%
25	6.190	835	837	840	rBV2	189	192	0.02%	0.003%
26	6.763	922	931	946	rBV	187755	440697	46.40%	6.286%
27	6.915	954	956	960	rVB2	412	406	0.04%	0.006%
28	7.013	969	972	975	rBV	219	234	0.02%	0.003%
29	7.129	981	991	998	rVB6	7090	17347	1.83%	0.247%
30	7.312	1011	1021	1034	rBV	196588	432458	45.53%	6.168%
31	7.690	1081	1083	1087	rBV2	163	237	0.02%	0.003%
32	7.799	1100	1101	1103	rBV2	248	260	0.03%	0.004%
33	7.939	1119	1124	1127	rVV3	621	744	0.08%	0.011%
34	8.049	1140	1142	1145	rVB2	343	304	0.03%	0.004%
35	8.080	1145	1147	1151	rBV	252	263	0.03%	0.004%
36	8.147	1156	1158	1162	rBV2	174	216	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026056.D
 Acq On : 27 Dec 2021 13:04
 Operator : JC/MD
 Sample : M5150-29
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	8.196	1165	1166	1168	rBV2	260	248	0.03%	0.004%
38	8.238	1171	1173	1175	rVB	345	209	0.02%	0.003%
39	8.330	1181	1188	1200	rBV	127002	214704	22.60%	3.062%
40	8.476	1209	1212	1217	rVB3	522	883	0.09%	0.013%
41	8.567	1222	1227	1228	rBV2	305	394	0.04%	0.006%
42	8.653	1234	1241	1249	rBV	509768	794116	83.61%	11.327%
43	8.720	1249	1252	1257	rVB2	6816	10183	1.07%	0.145%
44	8.793	1262	1264	1266	rBV2	376	298	0.03%	0.004%
45	8.842	1270	1272	1273	rBV	288	190	0.02%	0.003%
46	8.952	1284	1290	1300	rVV	88517	131995	13.90%	1.883%
47	9.049	1304	1306	1311	rVB2	521	652	0.07%	0.009%
48	9.238	1335	1337	1338	rBV	301	314	0.03%	0.004%
49	9.281	1339	1344	1348	rBV2	4541	7807	0.82%	0.111%
50	9.384	1356	1361	1377	rVB	354125	503080	52.97%	7.176%
51	9.695	1409	1412	1418	rVB4	786	1332	0.14%	0.019%
52	10.055	1465	1471	1479	rBV	420600	552252	58.14%	7.877%
53	10.195	1491	1494	1501	rVB3	842	1228	0.13%	0.018%
54	10.256	1501	1504	1505	rBV	226	207	0.02%	0.003%
55	10.305	1508	1512	1516	rVV2	1924	2604	0.27%	0.037%
56	10.354	1518	1520	1522	rBV	245	208	0.02%	0.003%
57	10.561	1552	1554	1556	rVB2	219	192	0.02%	0.003%
58	10.591	1556	1559	1561	rBV2	230	224	0.02%	0.003%
59	10.622	1561	1564	1565	rVB	259	194	0.02%	0.003%
60	10.652	1565	1569	1575	rVB3	619	1293	0.14%	0.018%
61	10.756	1584	1586	1589	rBV2	170	201	0.02%	0.003%
62	11.122	1641	1646	1649	rBV	3905	4656	0.49%	0.066%
63	11.195	1652	1658	1666	rBV	359399	451481	47.53%	6.440%
64	11.311	1675	1677	1683	rVB3	2494	4020	0.42%	0.057%
65	11.457	1696	1701	1702	rBV3	499	643	0.07%	0.009%
66	11.482	1702	1705	1708	rVV3	1495	1683	0.18%	0.024%
67	11.549	1713	1716	1720	rVB2	580	645	0.07%	0.009%
68	11.664	1734	1735	1736	rBV	316	201	0.02%	0.003%
69	11.750	1745	1749	1755	rVB3	4139	5482	0.58%	0.078%
70	11.841	1761	1764	1769	rVB2	730	1083	0.11%	0.015%
71	11.933	1775	1779	1783	rVB2	1970	2439	0.26%	0.035%
72	11.969	1783	1785	1788	rBV2	681	705	0.07%	0.010%
73	12.024	1788	1794	1801	rBV	446864	548597	57.76%	7.825%
74	12.128	1808	1811	1812	rBV2	1256	1184	0.12%	0.017%
75	12.152	1812	1815	1819	rVB4	2705	3410	0.36%	0.049%
76	12.323	1836	1843	1849	rBV	534022	675142	71.08%	9.630%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026056.D
 Acq On : 27 Dec 2021 13:04
 Operator : JC/MD
 Sample : M5150-29
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	12.420	1856	1859	1865	rVB3	1262	1646	0.17%	0.023%
78	12.481	1865	1869	1872	rVV3	769	1031	0.11%	0.015%
79	12.512	1872	1874	1876	rVB	375	233	0.02%	0.003%
80	12.555	1879	1881	1884	rVB2	229	251	0.03%	0.004%
81	12.658	1896	1898	1903	rVB3	939	932	0.10%	0.013%
82	12.768	1911	1916	1919	rBV	2067	2643	0.28%	0.038%
83	12.987	1950	1952	1953	rBV	198	197	0.02%	0.003%
84	13.054	1960	1963	1966	rVB2	840	1049	0.11%	0.015%
85	13.591	2049	2051	2053	rVB	470	339	0.04%	0.005%
86	13.780	2079	2082	2086	rVV2	563	898	0.09%	0.013%
87	13.896	2099	2101	2102	rBV2	273	216	0.02%	0.003%
88	13.993	2115	2117	2119	rVV2	354	315	0.03%	0.004%
89	14.134	2135	2140	2146	rVB2	3024	4236	0.45%	0.060%
90	14.207	2150	2152	2153	rBV	361	215	0.02%	0.003%
91	14.633	2219	2222	2224	rBV2	302	257	0.03%	0.004%
92	14.700	2231	2233	2235	rBV2	220	219	0.02%	0.003%
93	15.048	2289	2290	2292	rVB	408	220	0.02%	0.003%
94	15.341	2336	2338	2341	rBV2	456	602	0.06%	0.009%
95	15.389	2343	2346	2354	rVB3	1438	2567	0.27%	0.037%
96	15.761	2406	2407	2409	rBV	426	275	0.03%	0.004%
97	15.786	2409	2411	2413	rVB2	442	357	0.04%	0.005%
98	16.005	2445	2447	2451	rBV4	347	385	0.04%	0.005%
99	16.279	2490	2492	2494	rVB	522	359	0.04%	0.005%
100	16.407	2511	2513	2514	rBV	357	300	0.03%	0.004%




Sum of corrected areas: 7010884

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026056.D
Acq On : 27 Dec 2021 13:04
Operator : JC/MD
Sample : M5150-29
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

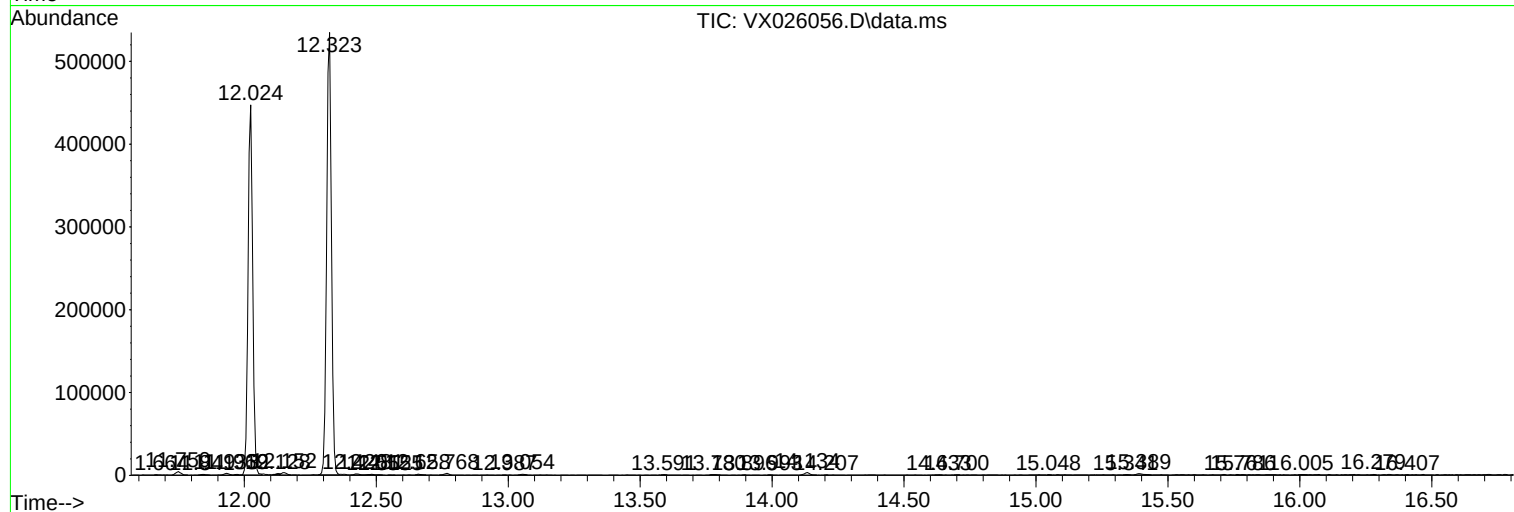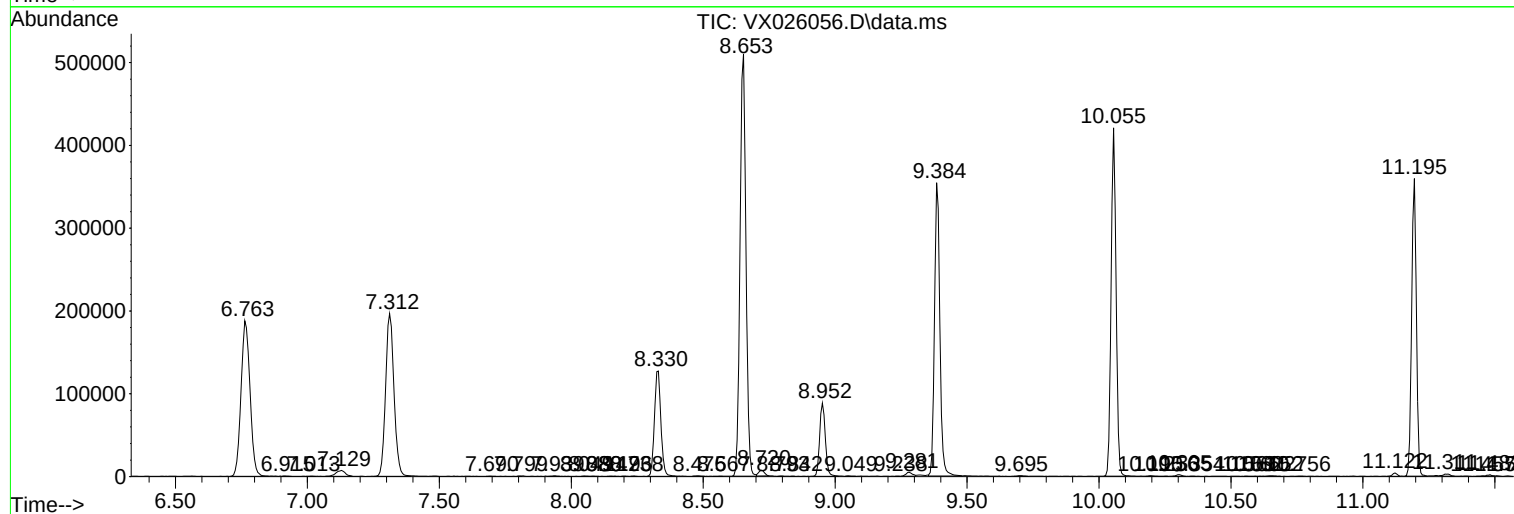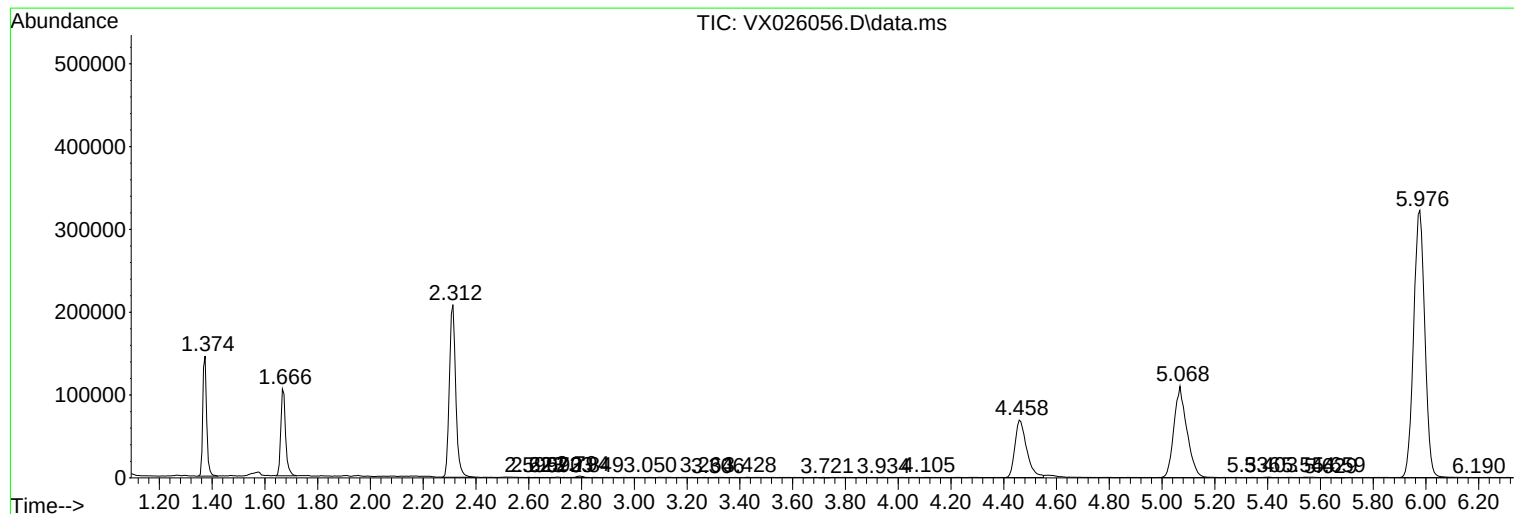

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026056.D
Acq On : 27 Dec 2021 13:04
Operator : JC/MD
Sample : M5150-29
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026056.D
Acq On : 27 Dec 2021 13:04
Operator : JC/MD
Sample : M5150-29
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc