

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026057.D
 Acq On : 27 Dec 2021 13:27
 Operator : JC/MD
 Sample : M5213-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGLD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026057.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	56	rVB	149526	151202	15.12%	2.072%
2	1.672	92	96	104	rVB	119333	138625	13.86%	1.899%
3	2.312	194	201	210	rBV	234603	369187	36.92%	5.059%
4	2.562	237	242	253	rBV3	2042	6319	0.63%	0.087%
5	2.788	275	279	287	rVB5	568	1306	0.13%	0.018%
6	2.959	305	307	310	rVV	402	404	0.04%	0.006%
7	3.440	384	386	390	rVV	247	336	0.03%	0.005%
8	3.483	390	393	394	rVB2	263	247	0.02%	0.003%
9	3.562	404	406	409	rVB	424	258	0.03%	0.004%
10	3.599	409	412	414	rBV	268	212	0.02%	0.003%
11	4.044	481	485	486	rBV	229	267	0.03%	0.004%
12	4.464	543	554	568	rBV	76192	221347	22.14%	3.033%
13	4.733	586	598	610	rBV2	5435	17388	1.74%	0.238%
14	5.062	640	652	668	rBV	127810	396116	39.61%	5.428%
15	5.342	697	698	700	rBV2	303	252	0.03%	0.003%
16	5.470	717	719	724	rVB	293	341	0.03%	0.005%
17	5.562	731	734	737	rVB2	383	470	0.05%	0.006%
18	5.751	763	765	767	rBV	259	240	0.02%	0.003%
19	5.806	773	774	779	rBV2	238	314	0.03%	0.004%
20	5.976	790	802	819	rBV2	348344	999972	100.00%	13.701%
21	6.543	893	895	899	rBV2	346	466	0.05%	0.006%
22	6.653	912	913	918	rVB2	246	231	0.02%	0.003%
23	6.769	921	932	943	rBV	196308	471992	47.20%	6.467%
24	6.940	959	960	967	rVB3	283	365	0.04%	0.005%
25	7.007	970	971	975	rVV2	302	242	0.02%	0.003%
26	7.129	982	991	999	rBV6	4546	11990	1.20%	0.164%
27	7.312	1012	1021	1038	rVV	215843	454732	45.47%	6.231%
28	7.427	1038	1040	1044	rVV2	446	520	0.05%	0.007%
29	7.476	1044	1048	1054	rVB4	759	1499	0.15%	0.021%
30	7.586	1064	1066	1068	rBV	354	226	0.02%	0.003%
31	7.824	1103	1105	1106	rVB	581	309	0.03%	0.004%
32	7.860	1109	1111	1115	rVB2	379	290	0.03%	0.004%
33	7.933	1120	1123	1124	rBV2	488	510	0.05%	0.007%
34	8.086	1145	1148	1149	rBV2	221	253	0.03%	0.003%
35	8.165	1158	1161	1163	rBV2	154	207	0.02%	0.003%
36	8.330	1180	1188	1197	rBV	136672	219956	22.00%	3.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026057.D
 Acq On : 27 Dec 2021 13:27
 Operator : JC/MD
 Sample : M5213-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGLD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	8.482	1210	1213	1216	rVB3	782	890	0.09%	0.012%
38	8.580	1225	1229	1231	rBV3	406	581	0.06%	0.008%
39	8.653	1234	1241	1249	rBV	520281	813444	81.35%	11.146%
40	8.720	1249	1252	1259	rVB	8230	13121	1.31%	0.180%
41	8.817	1265	1268	1272	rBV2	220	329	0.03%	0.005%
42	8.897	1280	1281	1284	rBV	319	272	0.03%	0.004%
43	8.951	1284	1290	1301	rBV	97434	138528	13.85%	1.898%
44	9.281	1338	1344	1348	rBV2	5623	9940	0.99%	0.136%
45	9.384	1356	1361	1374	rVB	370970	513710	51.37%	7.039%
46	9.525	1380	1384	1390	rVB2	3126	4485	0.45%	0.061%
47	9.622	1398	1400	1401	rVB2	482	268	0.03%	0.004%
48	9.915	1446	1448	1451	rVB2	276	285	0.03%	0.004%
49	10.055	1465	1471	1481	rVV	448284	581534	58.16%	7.968%
50	10.195	1490	1494	1500	rVB3	664	1180	0.12%	0.016%
51	10.305	1507	1512	1515	rBV2	1957	2765	0.28%	0.038%
52	10.396	1524	1527	1530	rBV2	227	300	0.03%	0.004%
53	10.451	1532	1536	1538	rVB2	219	294	0.03%	0.004%
54	10.476	1538	1540	1546	rVB2	279	328	0.03%	0.004%
55	10.652	1564	1569	1573	rBV5	930	1421	0.14%	0.019%
56	10.744	1579	1584	1585	rBV2	269	457	0.05%	0.006%
57	10.860	1600	1603	1607	rVB3	535	686	0.07%	0.009%
58	10.969	1618	1621	1623	rVB2	326	367	0.04%	0.005%
59	11.122	1641	1646	1652	rBV2	3923	4972	0.50%	0.068%
60	11.195	1652	1658	1667	rBV	363239	453280	45.33%	6.211%
61	11.323	1673	1679	1685	rVB3	4122	7494	0.75%	0.103%
62	11.390	1687	1690	1695	rBV3	411	502	0.05%	0.007%
63	11.457	1697	1701	1702	rBV2	678	730	0.07%	0.010%
64	11.475	1702	1704	1713	rVB2	1553	2514	0.25%	0.034%
65	11.542	1713	1715	1720	rVB2	414	419	0.04%	0.006%
66	11.750	1745	1749	1755	rVB3	4421	6384	0.64%	0.087%
67	11.841	1760	1764	1769	rBV3	1023	1534	0.15%	0.021%
68	11.933	1776	1779	1783	rBV3	2659	3346	0.33%	0.046%
69	11.969	1783	1785	1788	rBV2	453	394	0.04%	0.005%
70	12.024	1788	1794	1800	rBV	468790	563801	56.38%	7.725%
71	12.219	1822	1826	1830	rBV3	4023	6038	0.60%	0.083%
72	12.323	1837	1843	1849	rVB	530899	670612	67.06%	9.189%
73	12.426	1857	1860	1864	rVB4	1169	1593	0.16%	0.022%
74	12.762	1911	1915	1918	rBV2	1612	2196	0.22%	0.030%
75	12.859	1926	1931	1937	rVB2	2952	3496	0.35%	0.048%
76	12.920	1940	1941	1947	rVB3	322	347	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026057.D
 Acq On : 27 Dec 2021 13:27
 Operator : JC/MD
 Sample : M5213-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGLD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	12.963	1947	1948	1952	rBV	339	294	0.03%	0.004%
78	13.054	1960	1963	1967	rVB4	737	1009	0.10%	0.014%
79	13.103	1967	1971	1976	rBV4	1611	2166	0.22%	0.030%
80	13.573	2046	2048	2050	rVB2	250	207	0.02%	0.003%
81	13.597	2050	2052	2055	rBV	419	364	0.04%	0.005%
82	13.780	2079	2082	2086	rVB	1085	1306	0.13%	0.018%
83	13.957	2106	2111	2115	rBV	393	767	0.08%	0.011%
84	14.012	2118	2120	2122	rVV	267	319	0.03%	0.004%
85	14.048	2125	2126	2129	rVB2	377	225	0.02%	0.003%
86	14.133	2136	2140	2146	rBV2	1657	2711	0.27%	0.037%
87	14.597	2212	2216	2217	rBV3	245	345	0.03%	0.005%
88	14.639	2221	2223	2226	rVV3	257	304	0.03%	0.004%
89	14.902	2264	2266	2267	rBV	308	261	0.03%	0.004%
90	15.127	2302	2303	2306	rBV3	383	251	0.03%	0.003%
91	15.292	2328	2330	2332	rBV2	306	304	0.03%	0.004%
92	15.395	2343	2347	2352	rVB3	733	1355	0.14%	0.019%
93	15.493	2359	2363	2364	rBV3	281	349	0.03%	0.005%
94	15.780	2408	2410	2411	rBV	410	277	0.03%	0.004%
95	15.804	2413	2414	2416	rVB2	425	219	0.02%	0.003%
96	16.078	2457	2459	2461	rBV3	391	296	0.03%	0.004%
97	16.456	2519	2521	2523	rVB	731	535	0.05%	0.007%
98	16.487	2523	2526	2527	rBV2	455	458	0.05%	0.006%
99	16.578	2540	2541	2543	rBV	336	285	0.03%	0.004%
100	16.737	2564	2567	2568	rBV3	384	266	0.03%	0.004%




Sum of corrected areas: 7298301

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026057.D
Acq On : 27 Dec 2021 13:27
Operator : JC/MD
Sample : M5213-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGLD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

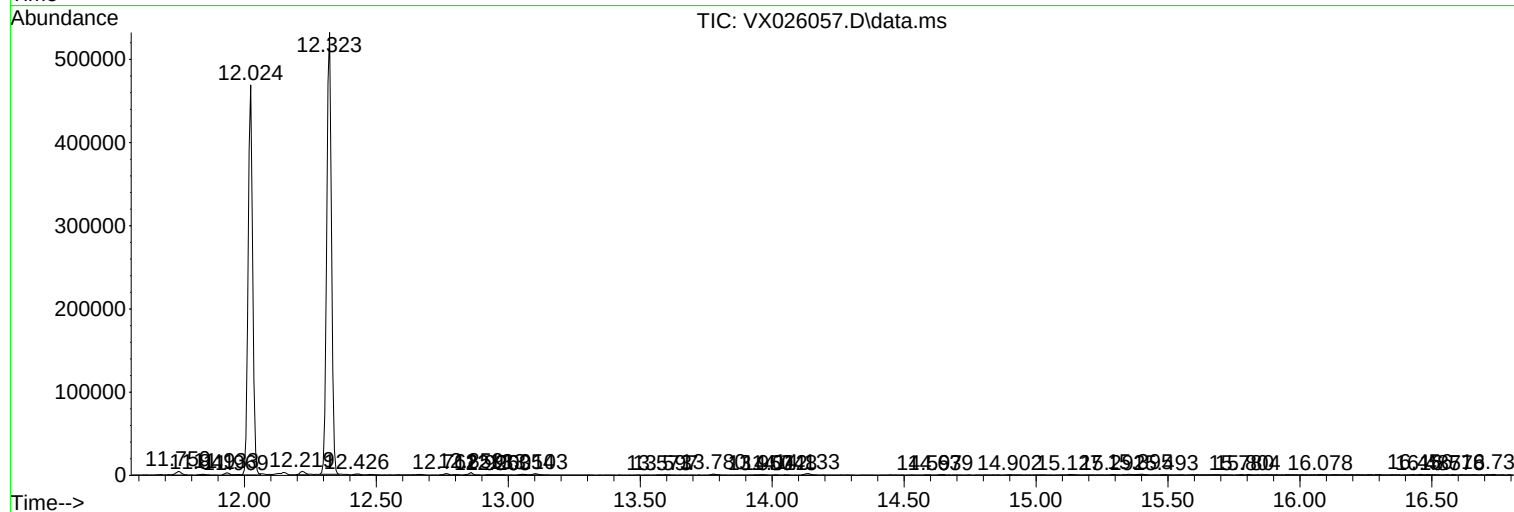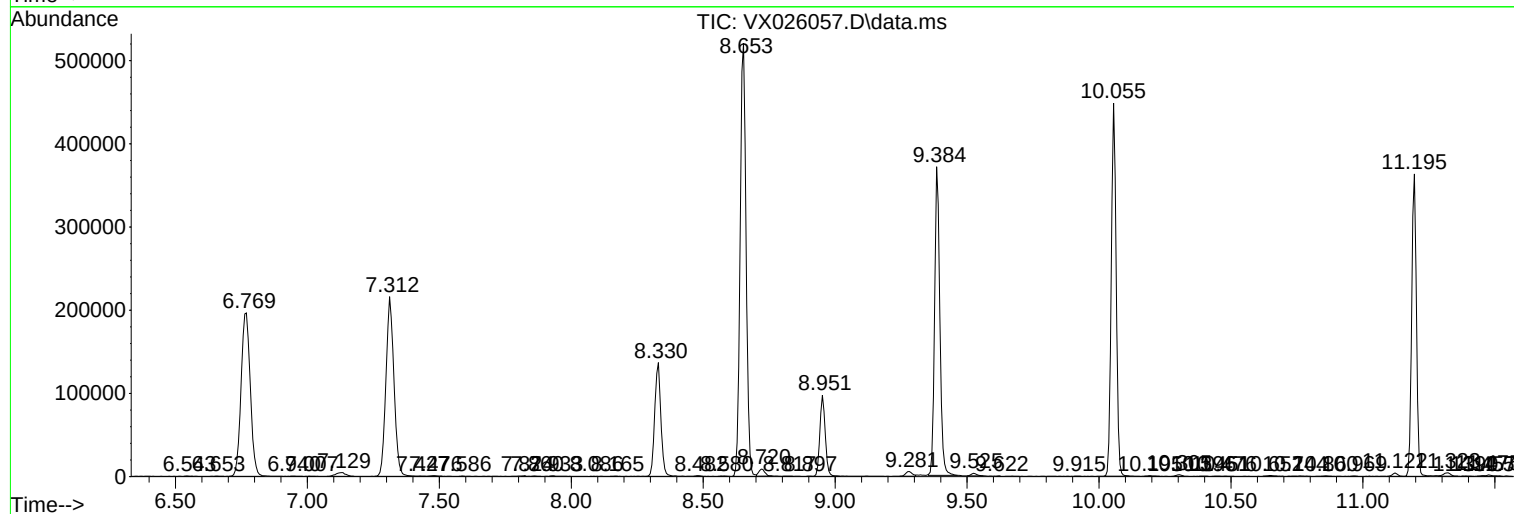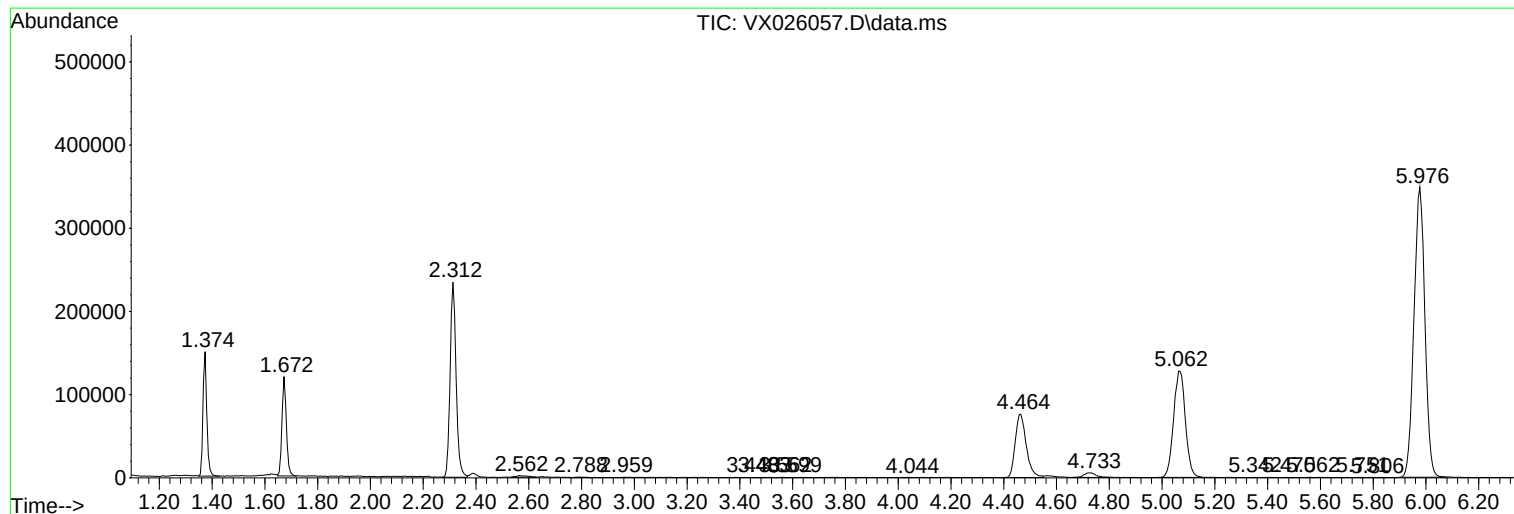

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026057.D
Acq On : 27 Dec 2021 13:27
Operator : JC/MD
Sample : M5213-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGLD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026057.D
Acq On : 27 Dec 2021 13:27
Operator : JC/MD
Sample : M5213-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGLD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
