

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026058.D
 Acq On : 27 Dec 2021 13:50
 Operator : JC/MD
 Sample : M5213-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026058.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	58	rVB	154077	156767	15.55%	2.128%
2	1.672	92	96	106	rVB	122773	144670	14.35%	1.964%
3	2.312	195	201	214	rBV	230614	369140	36.63%	5.011%
4	2.605	247	249	252	rBV	255	274	0.03%	0.004%
5	2.794	276	280	286	rVB2	1484	2516	0.25%	0.034%
6	2.904	293	298	300	rBV2	300	469	0.05%	0.006%
7	3.093	325	329	330	rBV2	181	207	0.02%	0.003%
8	3.117	330	333	334	rBV	241	225	0.02%	0.003%
9	3.355	370	372	377	rBV	205	339	0.03%	0.005%
10	3.422	380	383	385	rBV2	224	222	0.02%	0.003%
11	3.453	385	388	390	rBV2	228	343	0.03%	0.005%
12	3.611	413	414	417	rVB2	244	221	0.02%	0.003%
13	3.751	436	437	439	rBV	214	152	0.02%	0.002%
14	3.806	445	446	447	rBV	349	133	0.01%	0.002%
15	3.824	447	449	451	rBV2	144	145	0.01%	0.002%
16	3.940	467	468	470	rBV2	269	182	0.02%	0.002%
17	4.099	492	494	498	rVB	378	509	0.05%	0.007%
18	4.141	498	501	502	rBV2	344	353	0.04%	0.005%
19	4.458	543	553	567	rBV	71232	207764	20.61%	2.820%
20	4.800	608	609	611	rBV2	230	191	0.02%	0.003%
21	5.062	640	652	670	rBV	135257	406000	40.28%	5.511%
22	5.519	726	727	729	rBV2	263	215	0.02%	0.003%
23	5.556	731	733	735	rBV	233	159	0.02%	0.002%
24	5.605	740	741	744	rVB	205	165	0.02%	0.002%
25	5.672	750	752	753	rVB	362	188	0.02%	0.003%
26	5.976	789	802	817	rBV2	335405	1007838	100.00%	13.681%
27	6.464	880	882	884	rBV2	245	174	0.02%	0.002%
28	6.507	887	889	891	rVB	238	157	0.02%	0.002%
29	6.769	922	932	944	rBV	203468	480294	47.66%	6.520%
30	7.123	982	990	998	rBV5	4192	10513	1.04%	0.143%
31	7.208	1002	1004	1006	rVB	261	178	0.02%	0.002%
32	7.245	1006	1010	1012	rBV	201	297	0.03%	0.004%
33	7.312	1012	1021	1035	rBV	214441	465458	46.18%	6.318%
34	7.476	1044	1048	1049	rBV2	514	656	0.07%	0.009%
35	7.549	1059	1060	1063	rBV2	299	224	0.02%	0.003%
36	7.598	1066	1068	1072	rVB	251	264	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026058.D
 Acq On : 27 Dec 2021 13:50
 Operator : JC/MD
 Sample : M5213-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	7.629	1072	1073	1076	rBV2	194	204	0.02%	0.003%
38	7.714	1085	1087	1089	rBV2	224	263	0.03%	0.004%
39	7.738	1089	1091	1094	rVB2	257	196	0.02%	0.003%
40	7.769	1094	1096	1098	rBV2	239	247	0.02%	0.003%
41	7.940	1118	1124	1127	rBV4	609	965	0.10%	0.013%
42	8.019	1135	1137	1138	rBV	247	146	0.01%	0.002%
43	8.074	1144	1146	1150	rBV2	125	167	0.02%	0.002%
44	8.238	1171	1173	1176	rBV	233	134	0.01%	0.002%
45	8.330	1181	1188	1201	rBV	141394	228436	22.67%	3.101%
46	8.567	1225	1227	1229	rBV3	208	150	0.01%	0.002%
47	8.653	1234	1241	1249	rVV	519451	837590	83.11%	11.370%
48	8.720	1249	1252	1258	rVB2	7919	11782	1.17%	0.160%
49	8.860	1273	1275	1278	rVB	249	249	0.02%	0.003%
50	8.952	1284	1290	1298	rBV	93947	140353	13.93%	1.905%
51	9.134	1319	1320	1323	rBV	189	182	0.02%	0.002%
52	9.159	1323	1324	1327	rVB2	371	232	0.02%	0.003%
53	9.220	1333	1334	1337	rBV2	279	203	0.02%	0.003%
54	9.275	1338	1343	1348	rBV2	4134	7840	0.78%	0.106%
55	9.384	1356	1361	1377	rVB	349975	490312	48.65%	6.656%
56	9.878	1440	1442	1445	rBV2	160	142	0.01%	0.002%
57	9.903	1445	1446	1448	rBV	228	158	0.02%	0.002%
58	10.055	1465	1471	1487	rBV	474703	608955	60.42%	8.266%
59	10.195	1492	1494	1498	rVB3	506	589	0.06%	0.008%
60	10.305	1507	1512	1516	rVB4	1749	2588	0.26%	0.035%
61	10.610	1560	1562	1565	rVB	266	210	0.02%	0.003%
62	10.652	1565	1569	1572	rBV3	611	972	0.10%	0.013%
63	10.750	1584	1585	1588	rVB2	252	235	0.02%	0.003%
64	10.963	1619	1620	1622	rBV2	286	146	0.01%	0.002%
65	11.122	1642	1646	1650	rBV2	4253	5001	0.50%	0.068%
66	11.195	1652	1658	1666	rBV	343974	449047	44.56%	6.096%
67	11.317	1674	1678	1684	rVB2	3441	5706	0.57%	0.077%
68	11.482	1702	1705	1707	rBV2	918	966	0.10%	0.013%
69	11.543	1714	1715	1718	rBV	523	510	0.05%	0.007%
70	11.585	1720	1722	1724	rBV2	226	210	0.02%	0.003%
71	11.634	1729	1730	1732	rBV2	365	258	0.03%	0.004%
72	11.671	1734	1736	1738	rBV2	271	282	0.03%	0.004%
73	11.750	1745	1749	1754	rVB4	3910	5577	0.55%	0.076%
74	11.847	1760	1765	1767	rBV3	798	1118	0.11%	0.015%
75	11.933	1776	1779	1784	rVB3	1995	2241	0.22%	0.030%
76	12.024	1788	1794	1805	rBV	469673	587254	58.27%	7.972%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026058.D
 Acq On : 27 Dec 2021 13:50
 Operator : JC/MD
 Sample : M5213-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	12.152	1813	1815	1819	rVB2	3523	3478	0.35%	0.047%
78	12.219	1824	1826	1827	rBV	263	145	0.01%	0.002%
79	12.238	1827	1829	1831	rBV	240	157	0.02%	0.002%
80	12.262	1831	1833	1835	rBV2	393	348	0.03%	0.005%
81	12.323	1835	1843	1852	rBV	536266	698127	69.27%	9.477%
82	12.427	1858	1860	1864	rVB3	1409	1650	0.16%	0.022%
83	12.481	1866	1869	1875	rBV4	930	1457	0.14%	0.020%
84	12.628	1891	1893	1895	rBV2	314	270	0.03%	0.004%
85	12.664	1896	1899	1906	rVB5	1067	1580	0.16%	0.021%
86	12.768	1912	1916	1920	rVB	1620	2381	0.24%	0.032%
87	12.920	1939	1941	1945	rVB2	396	334	0.03%	0.005%
88	13.000	1952	1954	1958	rBV2	249	259	0.03%	0.004%
89	13.054	1959	1963	1967	rVV3	749	1204	0.12%	0.016%
90	13.115	1971	1973	1975	rVB	488	328	0.03%	0.004%
91	13.170	1980	1982	1984	rBV	250	188	0.02%	0.003%
92	13.353	2010	2012	2013	rBV	368	226	0.02%	0.003%
93	14.127	2136	2139	2146	rVB2	2486	3654	0.36%	0.050%
94	14.176	2146	2147	2148	rBV	335	195	0.02%	0.003%
95	14.310	2167	2169	2171	rBV	407	336	0.03%	0.005%
96	14.609	2217	2218	2220	rBV2	238	208	0.02%	0.003%
97	14.816	2250	2252	2254	rBV2	309	270	0.03%	0.004%
98	15.310	2331	2333	2336	rVB2	324	234	0.02%	0.003%
99	16.182	2475	2476	2477	rVB	500	183	0.02%	0.002%
100	16.548	2535	2536	2538	rBV	375	199	0.02%	0.003%




Sum of corrected areas: 7366829

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026058.D
Acq On : 27 Dec 2021 13:50
Operator : JC/MD
Sample : M5213-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

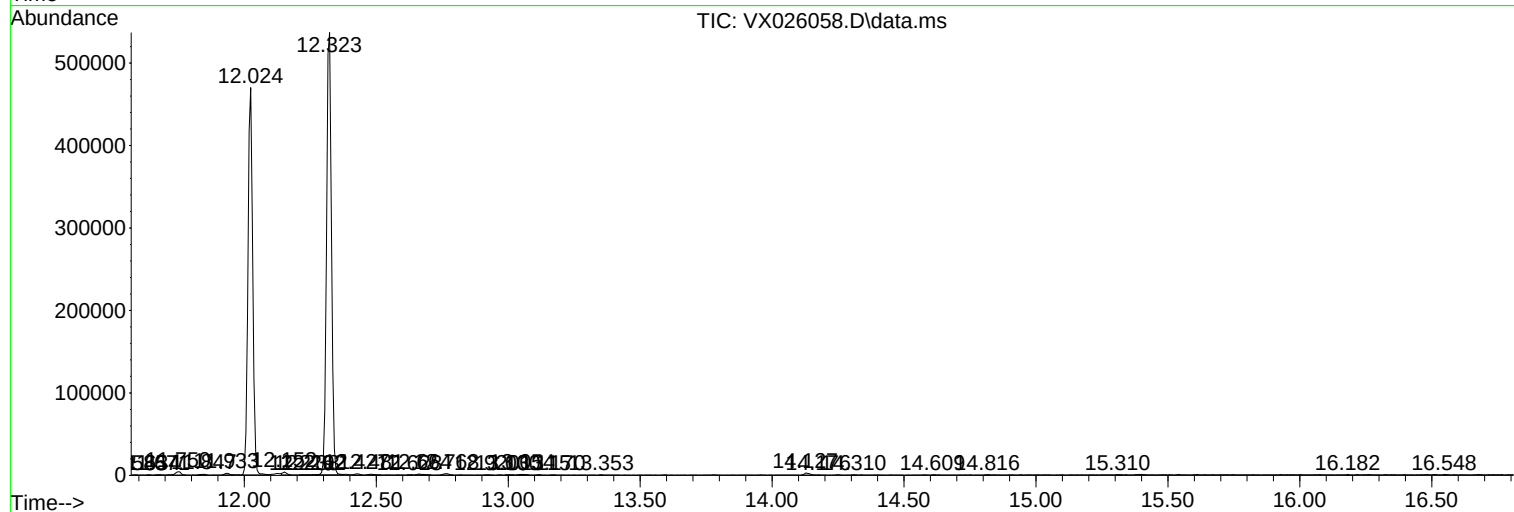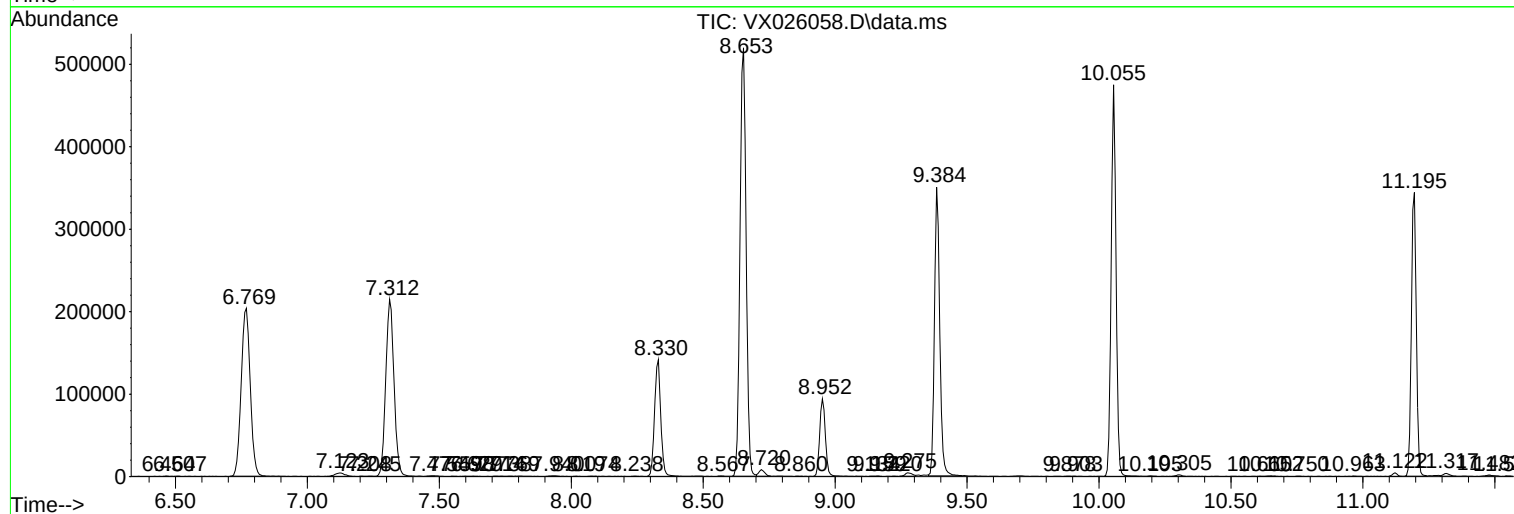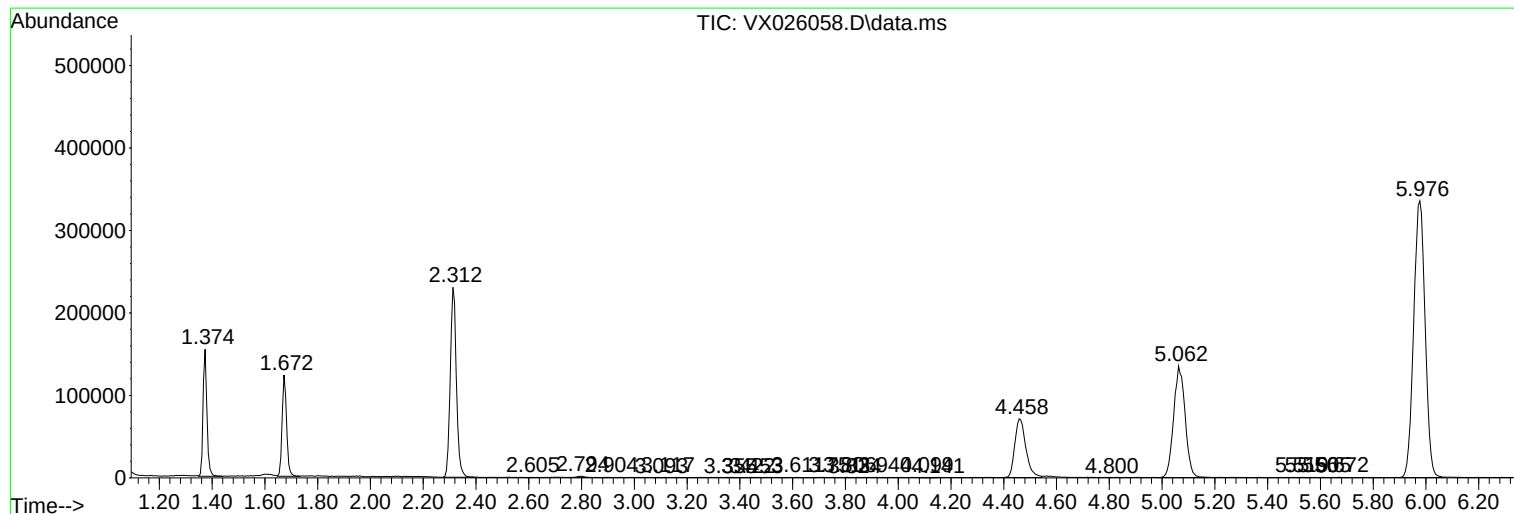

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026058.D
Acq On : 27 Dec 2021 13:50
Operator : JC/MD
Sample : M5213-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026058.D
Acq On : 27 Dec 2021 13:50
Operator : JC/MD
Sample : M5213-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc