

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026059.D
 Acq On : 27 Dec 2021 14:13
 Operator : JC/MD
 Sample : PB141697TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VLEB697

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	55	rVB	143683	146438	14.99%	2.086%
2	1.673	92	96	106	rVB	112120	133420	13.66%	1.901%
3	2.252	189	191	194	rBV2	291	338	0.03%	0.005%
4	2.313	194	201	212	rBV	220205	355558	36.40%	5.066%
5	2.502	231	232	233	rBV	393	207	0.02%	0.003%
6	2.703	262	265	268	rBV2	367	511	0.05%	0.007%
7	2.794	274	280	289	rVB	15335	26757	2.74%	0.381%
8	3.142	334	337	340	rBV2	191	253	0.03%	0.004%
9	3.617	414	415	419	rVV	301	240	0.02%	0.003%
10	3.666	419	423	426	rVV2	256	441	0.05%	0.006%
11	3.721	430	432	434	rBV	227	214	0.02%	0.003%
12	3.940	465	468	470	rVB2	194	224	0.02%	0.003%
13	4.465	543	554	578	rBV	74935	220487	22.57%	3.141%
14	4.916	627	628	630	rBV	258	227	0.02%	0.003%
15	4.971	634	637	638	rBV	195	229	0.02%	0.003%
16	5.062	640	652	669	rBV	132841	391402	40.07%	5.576%
17	5.276	684	687	689	rBV	210	230	0.02%	0.003%
18	5.660	745	750	754	rVB2	255	501	0.05%	0.007%
19	5.708	754	758	760	rBV2	300	412	0.04%	0.006%
20	5.977	787	802	818	rBV2	327589	976758	100.00%	13.916%
21	6.172	831	834	836	rBV3	163	256	0.03%	0.004%
22	6.361	863	865	869	rVB2	229	295	0.03%	0.004%
23	6.538	892	894	896	rBV	284	286	0.03%	0.004%
24	6.769	921	932	944	rBV	192153	465598	47.67%	6.634%
25	7.050	976	978	982	rBB2	248	289	0.03%	0.004%
26	7.123	982	990	998	rBV6	3780	9133	0.94%	0.130%
27	7.312	1012	1021	1032	rVV	202192	438887	44.93%	6.253%
28	7.452	1042	1044	1046	rBV	248	210	0.02%	0.003%
29	7.482	1046	1049	1054	rVV2	524	829	0.08%	0.012%
30	7.799	1098	1101	1102	rBV	305	263	0.03%	0.004%
31	7.928	1120	1122	1127	rVB3	546	655	0.07%	0.009%
32	8.043	1136	1141	1145	rVB2	162	348	0.04%	0.005%
33	8.330	1181	1188	1198	rVV	123313	207346	21.23%	2.954%
34	8.574	1224	1228	1231	rVV2	917	1085	0.11%	0.015%
35	8.653	1234	1241	1248	rVV	491118	779116	79.77%	11.100%
36	8.720	1248	1252	1257	rVV	6969	12253	1.25%	0.175%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026059.D
 Acq On : 27 Dec 2021 14:13
 Operator : JC/MD
 Sample : PB141697TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VLEB697

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	8.787	1261	1263	1266	rVB2	238	282	0.03%	0.004%
38	8.952	1284	1290	1301	rVV	89757	126899	12.99%	1.808%
39	9.275	1339	1343	1352	rBV2	4315	8791	0.90%	0.125%
40	9.385	1356	1361	1374	rVB	327708	472455	48.37%	6.731%
41	10.055	1465	1471	1480	rBV	432847	569510	58.31%	8.114%
42	10.153	1485	1487	1489	rBV	289	288	0.03%	0.004%
43	10.195	1492	1494	1497	rVB2	479	557	0.06%	0.008%
44	10.305	1508	1512	1516	rBV	1341	1809	0.19%	0.026%
45	10.537	1546	1550	1552	rBV2	225	372	0.04%	0.005%
46	10.573	1555	1556	1559	rVB2	248	217	0.02%	0.003%
47	10.640	1565	1567	1568	rBV	616	338	0.03%	0.005%
48	10.750	1583	1585	1586	rBV2	286	252	0.03%	0.004%
49	10.890	1606	1608	1610	rBV2	183	246	0.03%	0.004%
50	10.970	1617	1621	1623	rVB2	372	340	0.03%	0.005%
51	11.092	1639	1641	1642	rBV	238	211	0.02%	0.003%
52	11.122	1642	1646	1652	rBV	3683	4734	0.48%	0.067%
53	11.195	1652	1658	1666	rBV	339728	435382	44.57%	6.203%
54	11.317	1674	1678	1684	rVB5	2613	5194	0.53%	0.074%
55	11.378	1684	1688	1691	rBV2	380	424	0.04%	0.006%
56	11.476	1698	1704	1707	rBV7	1244	2039	0.21%	0.029%
57	11.628	1725	1729	1730	rBV2	256	311	0.03%	0.004%
58	11.689	1735	1739	1741	rVV2	447	508	0.05%	0.007%
59	11.750	1744	1749	1754	rBV3	3533	5009	0.51%	0.071%
60	11.841	1762	1764	1767	rVB3	583	633	0.06%	0.009%
61	11.933	1772	1779	1783	rBV3	2178	2882	0.30%	0.041%
62	11.963	1783	1784	1788	rVB2	414	439	0.04%	0.006%
63	12.024	1788	1794	1800	rBV	445517	546567	55.96%	7.787%
64	12.128	1807	1811	1812	rBV3	1195	1516	0.16%	0.022%
65	12.219	1824	1826	1831	rVV3	610	788	0.08%	0.011%
66	12.323	1835	1843	1850	rBV	483378	637049	65.22%	9.076%
67	12.421	1857	1859	1863	rVB2	961	1249	0.13%	0.018%
68	12.482	1864	1869	1872	rVB3	778	1161	0.12%	0.017%
69	12.628	1891	1893	1895	rBV	446	357	0.04%	0.005%
70	12.664	1896	1899	1902	rVV2	910	1136	0.12%	0.016%
71	12.762	1909	1915	1922	rBV	1349	2142	0.22%	0.031%
72	12.860	1930	1931	1935	rVB	291	243	0.02%	0.003%
73	12.933	1940	1943	1945	rBV2	192	242	0.02%	0.003%
74	12.969	1948	1949	1952	rVB2	295	262	0.03%	0.004%
75	12.994	1952	1953	1958	rBV3	297	398	0.04%	0.006%
76	13.049	1960	1962	1967	rVB2	769	1060	0.11%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026059.D
 Acq On : 27 Dec 2021 14:13
 Operator : JC/MD
 Sample : PB141697TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VLEB697

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	13.097	1967	1970	1971	rVB2	284	258	0.03%	0.004%
78	13.122	1971	1974	1977	rBV3	356	423	0.04%	0.006%
79	13.207	1983	1988	1990	rBV	245	316	0.03%	0.005%
80	13.311	2003	2005	2006	rBV2	264	210	0.02%	0.003%
81	13.603	2049	2053	2055	rBV	371	331	0.03%	0.005%
82	13.780	2079	2082	2084	rBV2	497	566	0.06%	0.008%
83	13.969	2111	2113	2117	rBV	336	384	0.04%	0.005%
84	14.012	2118	2120	2126	rVB2	268	356	0.04%	0.005%
85	14.134	2135	2140	2146	rVB	2329	3692	0.38%	0.053%
86	14.414	2185	2186	2188	rVB2	330	231	0.02%	0.003%
87	14.445	2188	2191	2193	rBV2	342	325	0.03%	0.005%
88	14.475	2193	2196	2198	rBV2	276	213	0.02%	0.003%
89	14.530	2203	2205	2206	rVV	367	210	0.02%	0.003%
90	14.573	2209	2212	2213	rBV2	284	348	0.04%	0.005%
91	14.628	2216	2221	2223	rBV3	201	280	0.03%	0.004%
92	14.695	2231	2232	2234	rBV2	196	212	0.02%	0.003%
93	15.121	2300	2302	2305	rBV2	285	297	0.03%	0.004%
94	15.341	2337	2338	2343	rVV2	433	262	0.03%	0.004%
95	15.396	2343	2347	2352	rVB4	1156	2018	0.21%	0.029%
96	15.499	2360	2364	2365	rVB2	483	498	0.05%	0.007%
97	15.518	2365	2367	2369	rBV2	486	281	0.03%	0.004%
98	15.798	2411	2413	2416	rBV	296	309	0.03%	0.004%
99	16.231	2482	2484	2486	rVB	729	536	0.05%	0.008%
100	16.280	2489	2492	2493	rBV3	298	315	0.03%	0.004%




Sum of corrected areas: 7018859

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026059.D
Acq On : 27 Dec 2021 14:13
Operator : JC/MD
Sample : PB141697TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VLEB697

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

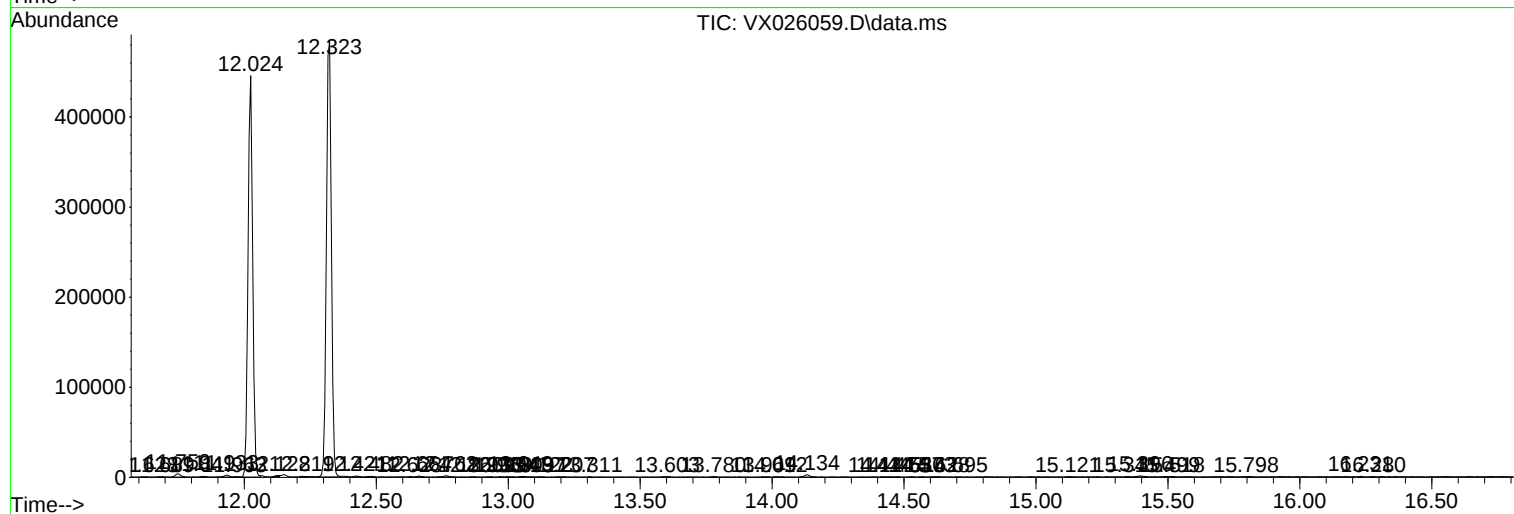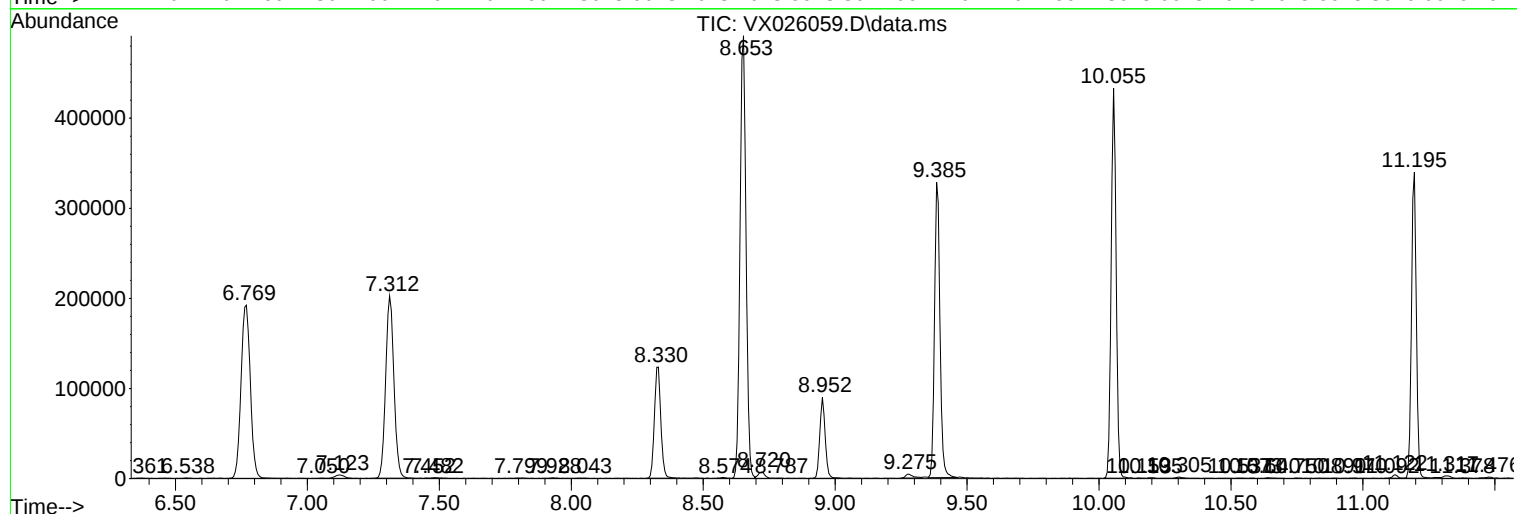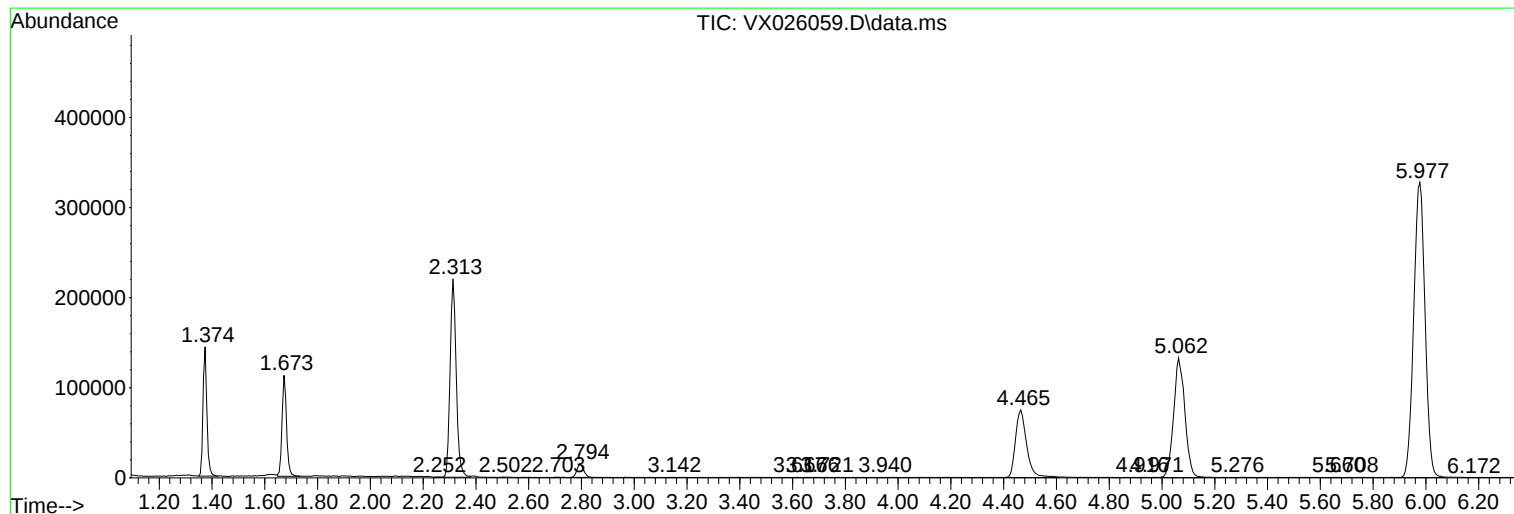

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026059.D
Acq On : 27 Dec 2021 14:13
Operator : JC/MD
Sample : PB141697TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VLEB697

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026059.D
Acq On : 27 Dec 2021 14:13
Operator : JC/MD
Sample : PB141697TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VLEB697

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc