

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026060.D
 Acq On : 27 Dec 2021 14:36
 Operator : JC/MD
 Sample : M5123-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGL60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M

Title : VOC Analysis

Signal : TIC: VX026060.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	59	rVB	167012	166664	16.02%	2.225%
2	1.673	92	96	105	rVB	124312	145189	13.96%	1.939%
3	2.313	195	201	209	rBV	233804	377557	36.29%	5.041%
4	2.386	209	213	227	rVB	25994	44862	4.31%	0.599%
5	2.520	230	235	241	rBV	3112	4642	0.45%	0.062%
6	2.709	265	266	274	rVB3	824	1037	0.10%	0.014%
7	2.794	274	280	288	rBV	11755	20733	1.99%	0.277%
8	3.788	440	443	446	rBV2	215	291	0.03%	0.004%
9	4.459	544	553	567	rBV	82501	239960	23.06%	3.204%
10	5.068	640	653	669	rBV	132463	411819	39.58%	5.499%
11	5.306	690	692	696	rVV2	247	314	0.03%	0.004%
12	5.404	704	708	710	rVB2	272	334	0.03%	0.004%
13	5.977	790	802	822	rVV2	349675	1040369	100.00%	13.891%
14	6.220	840	842	847	rVB2	250	300	0.03%	0.004%
15	6.269	847	850	854	rVB2	236	308	0.03%	0.004%
16	6.349	862	863	866	rBV3	386	414	0.04%	0.006%
17	6.769	922	932	945	rBV	192623	461822	44.39%	6.166%
18	7.123	983	990	997	rVB7	3472	8793	0.85%	0.117%
19	7.214	1001	1005	1007	rBV3	615	618	0.06%	0.008%
20	7.312	1012	1021	1032	rBV	213803	466362	44.83%	6.227%
21	7.476	1044	1048	1054	rBV2	979	1666	0.16%	0.022%
22	7.574	1060	1064	1066	rBV2	266	369	0.04%	0.005%
23	7.793	1098	1100	1101	rBV	409	309	0.03%	0.004%
24	7.934	1119	1123	1128	rVV3	619	1120	0.11%	0.015%
25	8.159	1157	1160	1164	rBV2	216	327	0.03%	0.004%
26	8.330	1178	1188	1197	rBV	136189	225221	21.65%	3.007%
27	8.476	1210	1212	1218	rVB4	425	627	0.06%	0.008%
28	8.580	1225	1229	1234	rVB3	2132	3181	0.31%	0.042%
29	8.653	1234	1241	1248	rVV	517018	819984	78.82%	10.949%
30	8.720	1249	1252	1259	rVV2	8698	12957	1.25%	0.173%
31	8.769	1259	1260	1263	rVV2	379	361	0.03%	0.005%
32	8.811	1265	1267	1271	rVB2	467	595	0.06%	0.008%
33	8.952	1284	1290	1300	rBV	94825	135980	13.07%	1.816%
34	9.244	1334	1338	1339	rBV2	330	399	0.04%	0.005%
35	9.281	1339	1344	1350	rVV3	4140	7139	0.69%	0.095%
36	9.385	1355	1361	1380	rVB	374614	525403	50.50%	7.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026060.D
 Acq On : 27 Dec 2021 14:36
 Operator : JC/MD
 Sample : M5123-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGL60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	9.604	1393	1397	1399	rBV2	187	309	0.03%	0.004%
38	9.628	1399	1401	1404	rVV	259	338	0.03%	0.005%
39	9.702	1408	1413	1416	rVB3	538	892	0.09%	0.012%
40	10.055	1465	1471	1487	rVV	417933	568973	54.69%	7.597%
41	10.195	1491	1494	1497	rVV2	954	948	0.09%	0.013%
42	10.244	1500	1502	1505	rVB3	572	532	0.05%	0.007%
43	10.305	1508	1512	1517	rVB2	1986	2543	0.24%	0.034%
44	10.390	1521	1526	1532	rVB3	493	1069	0.10%	0.014%
45	10.476	1536	1540	1543	rBV2	346	396	0.04%	0.005%
46	10.586	1556	1558	1561	rBV2	473	548	0.05%	0.007%
47	10.647	1564	1568	1572	rBV6	974	1592	0.15%	0.021%
48	10.689	1572	1575	1579	rVB3	1163	1583	0.15%	0.021%
49	10.781	1586	1590	1592	rVB2	350	391	0.04%	0.005%
50	10.970	1617	1621	1624	rVB	688	846	0.08%	0.011%
51	11.024	1626	1630	1636	rVB3	6480	8767	0.84%	0.117%
52	11.079	1636	1639	1641	rBV3	518	568	0.05%	0.008%
53	11.122	1641	1646	1652	rVB	5182	6615	0.64%	0.088%
54	11.195	1652	1658	1668	rBV	361612	463177	44.52%	6.185%
55	11.482	1699	1705	1707	rBV3	2101	3099	0.30%	0.041%
56	11.543	1713	1715	1721	rVB3	689	807	0.08%	0.011%
57	11.616	1723	1727	1728	rBV2	523	738	0.07%	0.010%
58	11.628	1728	1729	1732	rVB3	526	415	0.04%	0.006%
59	11.750	1745	1749	1756	rVB2	5353	7139	0.69%	0.095%
60	11.805	1756	1758	1761	rBV	251	300	0.03%	0.004%
61	11.841	1761	1764	1771	rBV4	1360	2082	0.20%	0.028%
62	11.933	1774	1779	1782	rBV3	2600	3290	0.32%	0.044%
63	11.969	1782	1785	1788	rVB3	1544	1784	0.17%	0.024%
64	12.024	1789	1794	1801	rBV	450820	544749	52.36%	7.274%
65	12.128	1808	1811	1812	rBV3	1408	1460	0.14%	0.019%
66	12.323	1835	1843	1849	rBV	514044	680031	65.36%	9.080%
67	12.427	1857	1860	1864	rVB4	2007	2655	0.26%	0.035%
68	12.488	1864	1870	1874	rVB6	1222	2152	0.21%	0.029%
69	12.530	1874	1877	1881	rBV3	393	620	0.06%	0.008%
70	12.579	1881	1885	1888	rBV3	1650	1987	0.19%	0.027%
71	12.634	1891	1894	1895	rBV2	597	430	0.04%	0.006%
72	12.658	1895	1898	1907	rVB6	1122	2265	0.22%	0.030%
73	12.768	1912	1916	1922	rVV2	1814	2807	0.27%	0.037%
74	12.817	1922	1924	1927	rVV2	513	456	0.04%	0.006%
75	13.000	1952	1954	1959	rVB2	423	492	0.05%	0.007%
76	13.055	1959	1963	1967	rBV5	751	1034	0.10%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026060.D
 Acq On : 27 Dec 2021 14:36
 Operator : JC/MD
 Sample : M5123-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGL60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	13.097	1967	1970	1975	rVB4	486	703	0.07%	0.009%
78	13.280	1998	2000	2004	rVB2	366	386	0.04%	0.005%
79	13.579	2046	2049	2050	rBV2	390	451	0.04%	0.006%
80	13.591	2050	2051	2054	rVB	458	332	0.03%	0.004%
81	13.683	2062	2066	2070	rBV4	407	662	0.06%	0.009%
82	13.780	2077	2082	2090	rBV	13293	16551	1.59%	0.221%
83	13.859	2093	2095	2098	rVB	666	536	0.05%	0.007%
84	14.134	2136	2140	2144	rVB2	1532	2179	0.21%	0.029%
85	14.189	2147	2149	2152	rBV2	243	301	0.03%	0.004%
86	14.323	2165	2171	2176	rBV3	992	1355	0.13%	0.018%
87	14.451	2190	2192	2196	rVB3	601	676	0.06%	0.009%
88	14.487	2196	2198	2199	rBV2	482	449	0.04%	0.006%
89	14.640	2221	2223	2227	rVB3	977	795	0.08%	0.011%
90	14.780	2241	2246	2251	rBV4	2403	3645	0.35%	0.049%
91	14.890	2260	2264	2266	rVB2	271	353	0.03%	0.005%
92	14.914	2266	2268	2269	rBV	418	305	0.03%	0.004%
93	15.152	2305	2307	2309	rVB	591	439	0.04%	0.006%
94	15.182	2309	2312	2314	rBV3	789	1002	0.10%	0.013%
95	15.255	2322	2324	2329	rVB5	667	682	0.07%	0.009%
96	15.323	2332	2335	2339	rVV3	2407	3149	0.30%	0.042%
97	15.603	2378	2381	2387	rBV3	555	1042	0.10%	0.014%
98	15.914	2430	2432	2435	rBV	401	381	0.04%	0.005%
99	16.091	2458	2461	2471	rVB7	1993	3628	0.35%	0.048%
100	16.639	2549	2551	2552	rBV	404	349	0.03%	0.005%




Sum of corrected areas: 7489256

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026060.D
Acq On : 27 Dec 2021 14:36
Operator : JC/MD
Sample : M5123-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGL60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

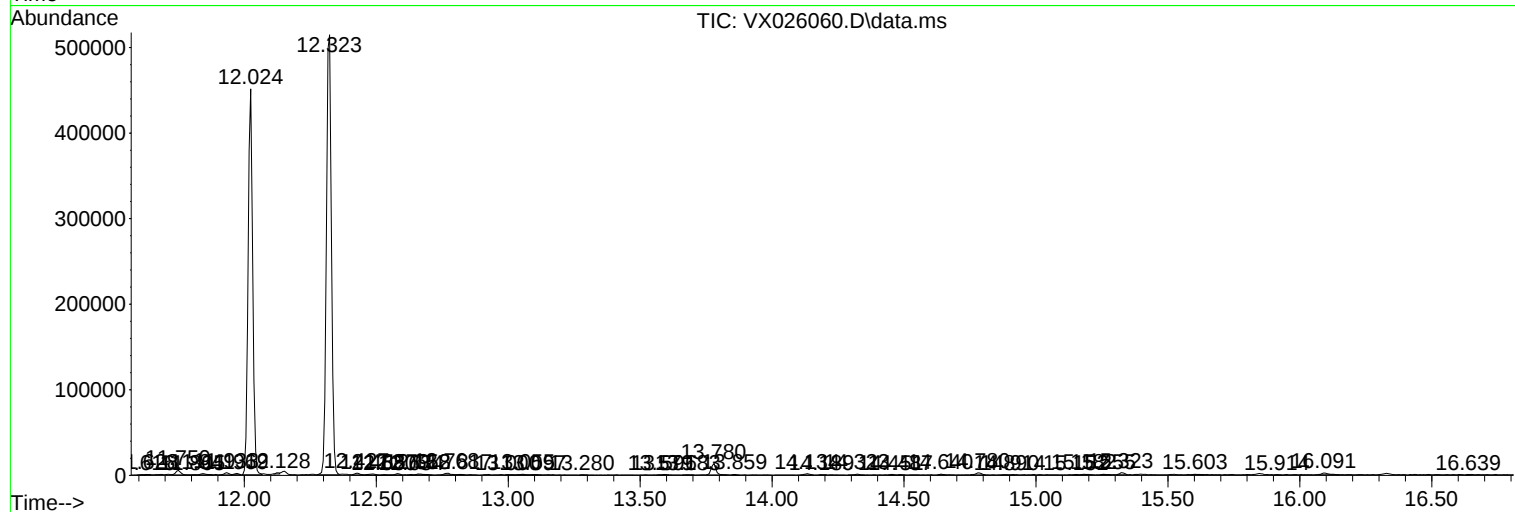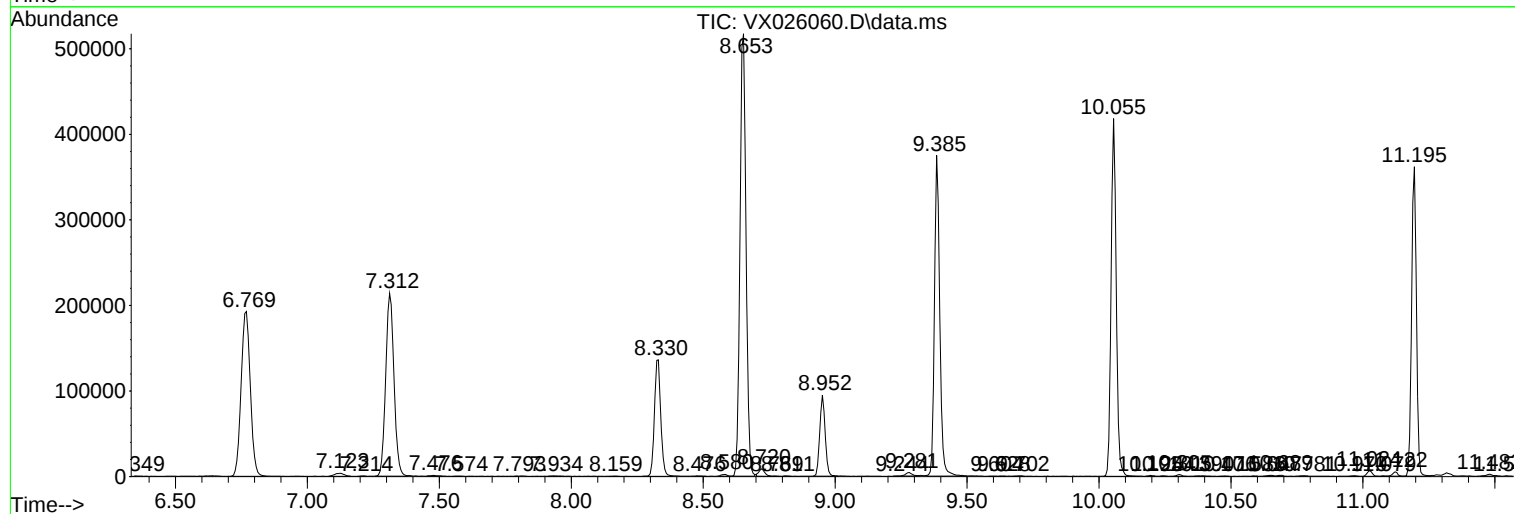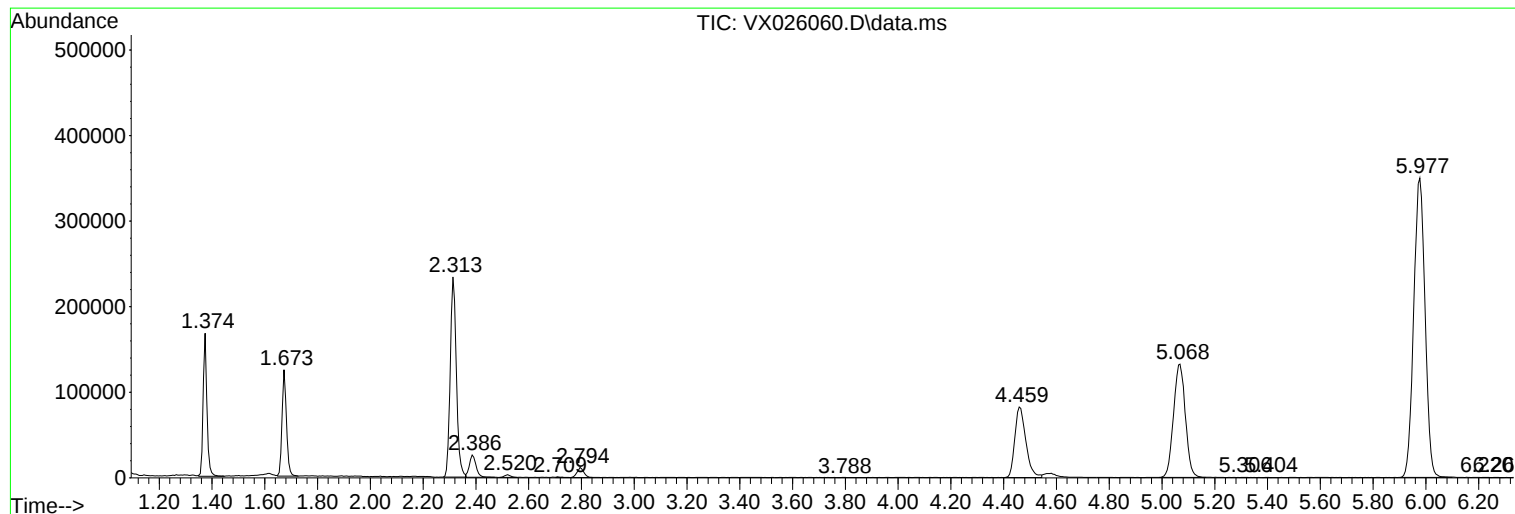

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026060.D
Acq On : 27 Dec 2021 14:36
Operator : JC/MD
Sample : M5123-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGL60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026060.D
Acq On : 27 Dec 2021 14:36
Operator : JC/MD
Sample : M5123-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGL60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc