

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026061.D
 Acq On : 27 Dec 2021 14:59
 Operator : JC/MD
 Sample : M5123-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026061.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	57	rVB	136187	145301	15.64%	2.191%
2	1.673	91	96	108	rVB	112622	132299	14.24%	1.995%
3	2.313	195	201	213	rVB	215284	337926	36.37%	5.095%
4	2.514	232	234	238	rVB2	585	652	0.07%	0.010%
5	2.587	243	246	247	rBV	285	248	0.03%	0.004%
6	2.611	247	250	254	rVB2	225	371	0.04%	0.006%
7	2.715	262	267	271	rBV2	401	693	0.07%	0.010%
8	2.794	275	280	285	rVB3	1541	2831	0.30%	0.043%
9	3.026	315	318	319	rVV	203	182	0.02%	0.003%
10	3.087	325	328	329	rBV2	191	231	0.02%	0.003%
11	3.117	332	333	335	rBV2	242	206	0.02%	0.003%
12	3.319	362	366	369	rVB2	180	218	0.02%	0.003%
13	3.349	369	371	375	rVB	302	334	0.04%	0.005%
14	3.678	422	425	427	rVB2	285	233	0.03%	0.004%
15	3.843	451	452	454	rVV	259	192	0.02%	0.003%
16	4.294	523	526	528	rBV2	264	311	0.03%	0.005%
17	4.459	544	553	565	rBV	70525	199658	21.49%	3.010%
18	4.830	610	614	617	rBV2	239	371	0.04%	0.006%
19	4.965	633	636	637	rBV	282	203	0.02%	0.003%
20	5.062	640	652	672	rVB	120122	371632	40.00%	5.603%
21	5.477	719	720	722	rBV	309	198	0.02%	0.003%
22	5.501	722	724	727	rVB	211	202	0.02%	0.003%
23	5.544	729	731	732	rBV2	187	181	0.02%	0.003%
24	5.708	755	758	760	rBV2	168	250	0.03%	0.004%
25	5.763	765	767	770	rVB2	248	267	0.03%	0.004%
26	5.794	770	772	775	rBV2	142	182	0.02%	0.003%
27	5.977	788	802	816	rBV2	317067	929024	100.00%	14.008%
28	6.092	819	821	824	rVV3	599	619	0.07%	0.009%
29	6.196	836	838	840	rVB2	245	193	0.02%	0.003%
30	6.409	872	873	875	rBV2	182	190	0.02%	0.003%
31	6.464	880	882	884	rVV	236	205	0.02%	0.003%
32	6.550	893	896	897	rBV2	242	181	0.02%	0.003%
33	6.763	922	931	946	rVV	183239	436182	46.95%	6.577%
34	6.915	954	956	958	rVB	343	240	0.03%	0.004%
35	7.111	983	988	989	rBV2	3078	3639	0.39%	0.055%
36	7.312	1012	1021	1038	rVB	193178	421326	45.35%	6.353%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026061.D
 Acq On : 27 Dec 2021 14:59
 Operator : JC/MD
 Sample : M5123-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	7.452	1041	1044	1045	rBV2	208	211	0.02%	0.003%
38	7.470	1045	1047	1049	rBV2	687	708	0.08%	0.011%
39	7.568	1061	1063	1064	rBV2	335	263	0.03%	0.004%
40	8.019	1136	1137	1140	rBV	190	207	0.02%	0.003%
41	8.220	1168	1170	1173	rBV2	250	266	0.03%	0.004%
42	8.330	1181	1188	1201	rBV	118918	200430	21.57%	3.022%
43	8.476	1210	1212	1214	rBV	433	381	0.04%	0.006%
44	8.574	1226	1228	1229	rBV	343	309	0.03%	0.005%
45	8.653	1234	1241	1248	rVV	470218	742106	79.88%	11.190%
46	8.720	1248	1252	1258	rVB	6476	10348	1.11%	0.156%
47	8.952	1284	1290	1301	rVV	83532	122859	13.22%	1.852%
48	9.110	1313	1316	1319	rBV2	252	418	0.04%	0.006%
49	9.141	1319	1321	1323	rVB2	201	180	0.02%	0.003%
50	9.165	1323	1325	1327	rBV	221	211	0.02%	0.003%
51	9.281	1338	1344	1350	rBV2	4037	8098	0.87%	0.122%
52	9.385	1356	1361	1373	rVB	311673	438637	47.21%	6.614%
53	9.506	1380	1381	1385	rVB2	613	536	0.06%	0.008%
54	9.635	1398	1402	1405	rVB2	345	478	0.05%	0.007%
55	9.665	1405	1407	1409	rBV	231	230	0.02%	0.003%
56	9.695	1409	1412	1418	rVB4	807	1188	0.13%	0.018%
57	9.756	1420	1422	1424	rVB	330	195	0.02%	0.003%
58	9.860	1437	1439	1441	rBV2	176	198	0.02%	0.003%
59	10.055	1465	1471	1481	rBV	399064	530977	57.15%	8.006%
60	10.189	1491	1493	1495	rBV2	351	329	0.04%	0.005%
61	10.305	1507	1512	1517	rBV3	925	1423	0.15%	0.021%
62	10.567	1553	1555	1558	rVB	276	190	0.02%	0.003%
63	10.616	1559	1563	1564	rVB2	278	266	0.03%	0.004%
64	10.817	1594	1596	1599	rVB	325	253	0.03%	0.004%
65	10.848	1599	1601	1602	rBV	404	210	0.02%	0.003%
66	10.970	1616	1621	1625	rVB2	473	701	0.08%	0.011%
67	11.012	1625	1628	1629	rBV	229	223	0.02%	0.003%
68	11.122	1640	1646	1649	rBV	3798	4308	0.46%	0.065%
69	11.195	1652	1658	1665	rBV	323551	416506	44.83%	6.280%
70	11.323	1675	1679	1686	rVB3	2983	4942	0.53%	0.075%
71	11.384	1687	1689	1693	rVB2	353	393	0.04%	0.006%
72	11.451	1699	1700	1701	rBV	460	318	0.03%	0.005%
73	11.476	1702	1704	1707	rVV2	1002	1118	0.12%	0.017%
74	11.549	1713	1716	1720	rVB2	491	680	0.07%	0.010%
75	11.585	1720	1722	1725	rBV	178	281	0.03%	0.004%
76	11.616	1725	1727	1729	rVB	379	267	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026061.D
 Acq On : 27 Dec 2021 14:59
 Operator : JC/MD
 Sample : M5123-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	11.671	1732	1736	1739	rBV3	378	652	0.07%	0.010%
78	11.750	1745	1749	1757	rVB4	3008	4327	0.47%	0.065%
79	11.841	1761	1764	1769	rVB	654	621	0.07%	0.009%
80	11.927	1776	1778	1784	rBV4	1300	2019	0.22%	0.030%
81	12.024	1788	1794	1803	rVV	428640	517259	55.68%	7.799%
82	12.128	1806	1811	1812	rVV3	1461	2074	0.22%	0.031%
83	12.152	1812	1815	1821	rVB4	2580	3317	0.36%	0.050%
84	12.323	1837	1843	1849	rBV	462041	611812	65.86%	9.225%
85	12.427	1858	1860	1864	rVB2	1444	1355	0.15%	0.020%
86	12.463	1864	1866	1867	rBV	294	222	0.02%	0.003%
87	12.524	1874	1876	1878	rVB	258	272	0.03%	0.004%
88	12.664	1896	1899	1902	rVB4	464	564	0.06%	0.009%
89	12.768	1911	1916	1920	rBV3	1456	2089	0.22%	0.031%
90	12.890	1933	1936	1937	rBV	218	239	0.03%	0.004%
91	13.055	1961	1963	1965	rVB2	603	451	0.05%	0.007%
92	13.189	1983	1985	1987	rVB	287	222	0.02%	0.003%
93	13.213	1987	1989	1990	rBV	302	182	0.02%	0.003%
94	13.225	1990	1991	1993	rBV	221	180	0.02%	0.003%
95	13.780	2080	2082	2088	rVB2	542	692	0.07%	0.010%
96	14.134	2136	2140	2144	rBV2	2183	2962	0.32%	0.045%
97	14.548	2206	2208	2210	rVB2	266	198	0.02%	0.003%
98	15.304	2329	2332	2333	rBV2	286	311	0.03%	0.005%
99	15.396	2343	2347	2352	rBV3	518	778	0.08%	0.012%
100	15.908	2430	2431	2433	rBV2	372	339	0.04%	0.005%


Sum of corrected areas: 6632150

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026061.D
Acq On : 27 Dec 2021 14:59
Operator : JC/MD
Sample : M5123-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

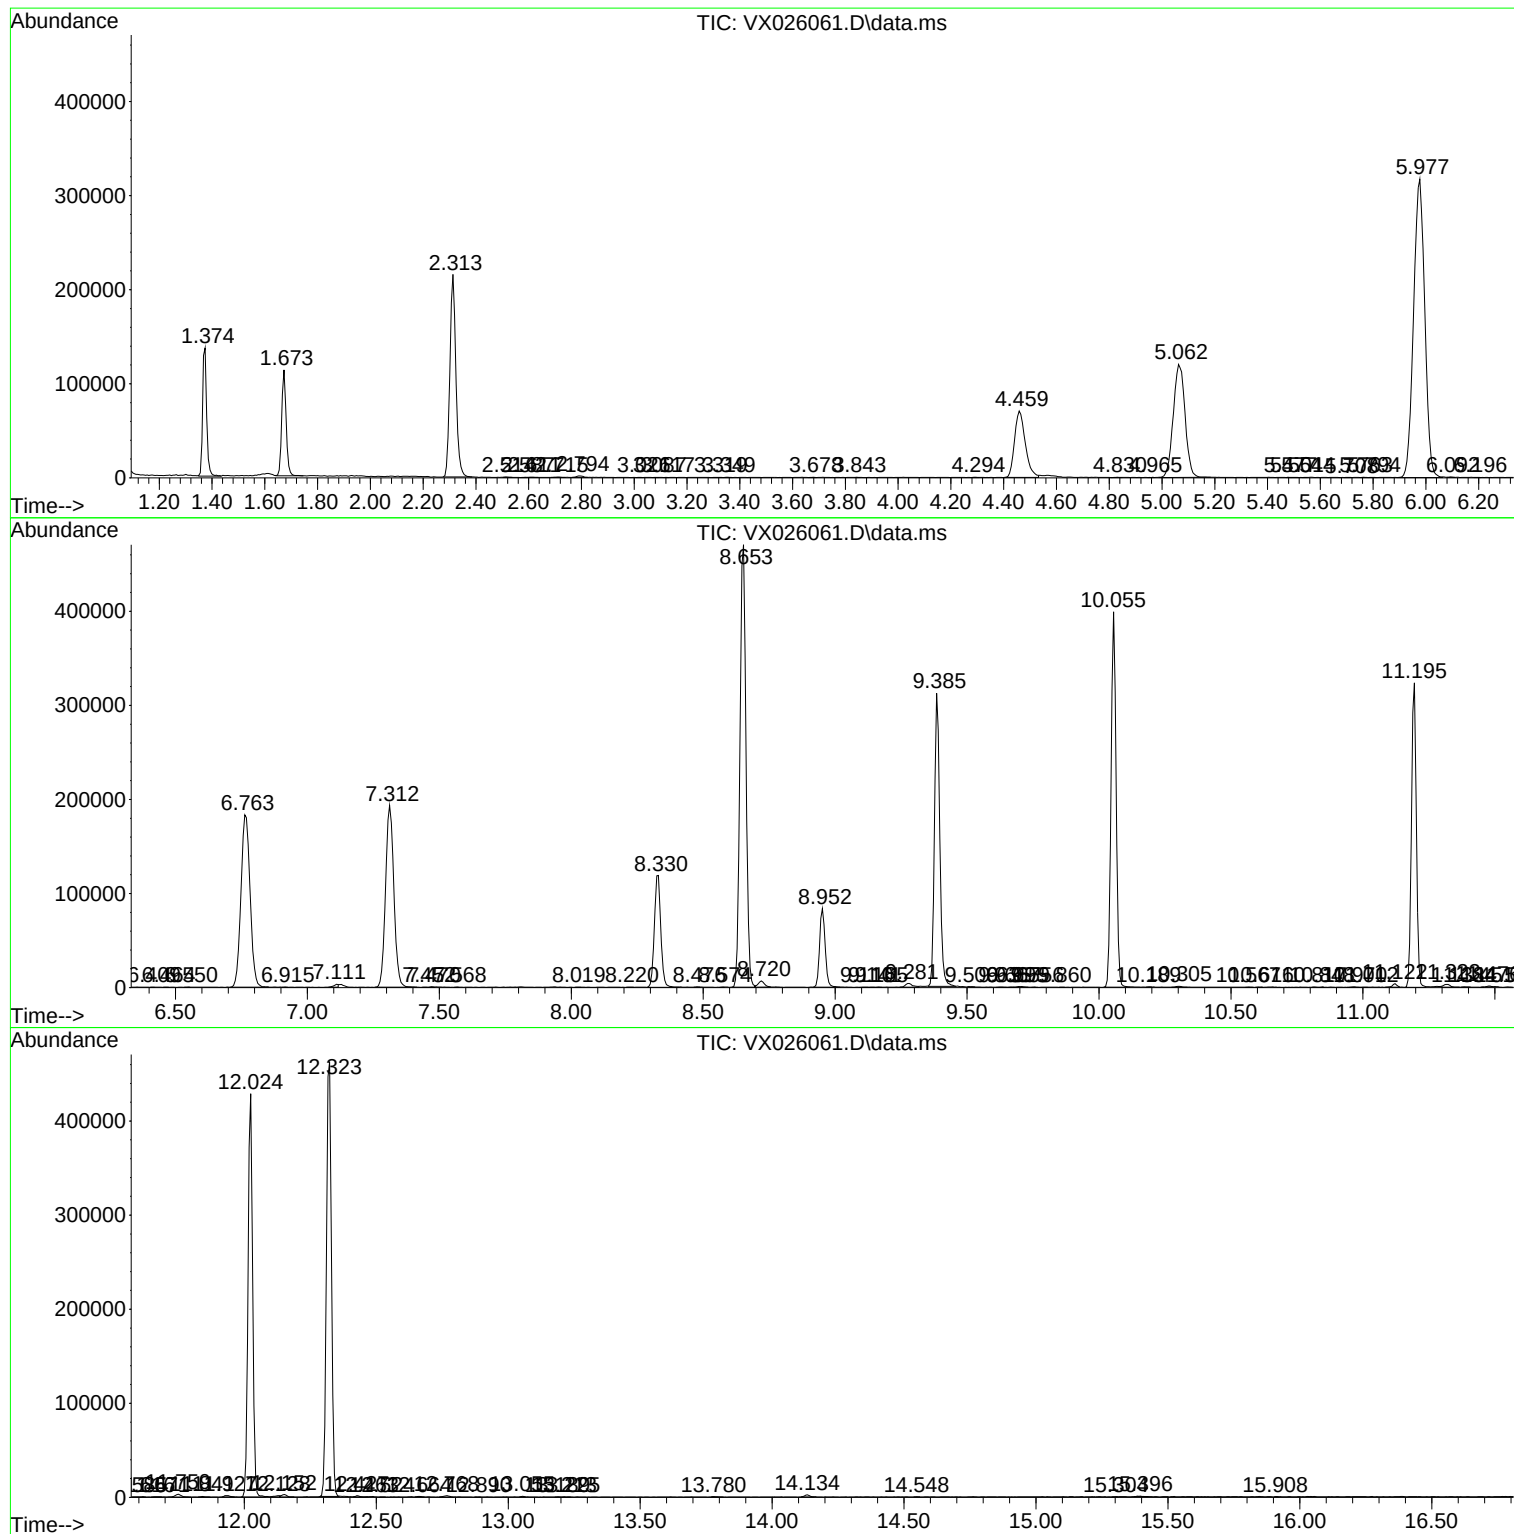

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026061.D
Acq On : 27 Dec 2021 14:59
Operator : JC/MD
Sample : M5123-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026061.D
Acq On : 27 Dec 2021 14:59
Operator : JC/MD
Sample : M5123-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc