

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026062.D
 Acq On : 27 Dec 2021 15:22
 Operator : JC/MD
 Sample : M5126-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026062.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	54	rVB	141555	146843	14.88%	2.068%
2	1.672	92	96	106	rVB	118181	137991	13.98%	1.943%
3	2.313	194	201	210	rBV	233896	363682	36.86%	5.122%
4	2.800	276	281	286	rVB3	826	1467	0.15%	0.021%
5	2.910	297	299	302	rBV2	344	427	0.04%	0.006%
6	3.331	366	368	372	rBV3	412	642	0.07%	0.009%
7	3.501	395	396	401	rBV2	184	230	0.02%	0.003%
8	4.062	484	488	489	rBV2	278	301	0.03%	0.004%
9	4.196	507	510	512	rBV2	397	515	0.05%	0.007%
10	4.221	512	514	517	rVV3	518	611	0.06%	0.009%
11	4.465	542	554	567	rBV	71618	210625	21.35%	2.966%
12	4.769	602	604	606	rBV2	325	367	0.04%	0.005%
13	5.062	640	652	669	rBV	123129	389745	39.50%	5.489%
14	5.385	702	705	710	rVB4	214	409	0.04%	0.006%
15	5.452	714	716	720	rBV	317	297	0.03%	0.004%
16	5.550	728	732	733	rBV2	270	400	0.04%	0.006%
17	5.617	740	743	744	rBV	255	225	0.02%	0.003%
18	5.653	747	749	754	rVB	369	423	0.04%	0.006%
19	5.757	764	766	769	rVB	306	276	0.03%	0.004%
20	5.976	787	802	820	rBV2	332723	986712	100.00%	13.896%
21	6.458	878	881	882	rBV2	237	296	0.03%	0.004%
22	6.678	915	917	919	rVB2	229	227	0.02%	0.003%
23	6.763	919	931	944	rBV	200393	479054	48.55%	6.747%
24	7.123	983	990	998	rVB6	2849	7225	0.73%	0.102%
25	7.177	998	999	1005	rBV2	209	332	0.03%	0.005%
26	7.312	1012	1021	1032	rBV	206649	444297	45.03%	6.257%
27	7.476	1044	1048	1050	rBV3	825	943	0.10%	0.013%
28	7.586	1062	1066	1073	rVV3	1985	4009	0.41%	0.056%
29	7.702	1083	1085	1088	rVB2	258	268	0.03%	0.004%
30	7.854	1106	1110	1117	rVB4	2281	4613	0.47%	0.065%
31	8.281	1178	1180	1181	rVB	327	222	0.02%	0.003%
32	8.324	1181	1187	1201	rBV	129386	215107	21.80%	3.029%
33	8.580	1225	1229	1234	rVV2	549	819	0.08%	0.012%
34	8.653	1234	1241	1248	rVV	508145	787973	79.86%	11.097%
35	8.726	1248	1253	1260	rVB	6959	12255	1.24%	0.173%
36	8.872	1275	1277	1280	rVB	287	254	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026062.D
 Acq On : 27 Dec 2021 15:22
 Operator : JC/MD
 Sample : M5126-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	8.952	1284	1290	1300	rVV	92628	131810	13.36%	1.856%
38	9.281	1338	1344	1348	rBV	6923	10885	1.10%	0.153%
39	9.384	1356	1361	1375	rVB	330003	467869	47.42%	6.589%
40	9.531	1380	1385	1389	rVB3	1455	2373	0.24%	0.033%
41	9.915	1446	1448	1451	rBV	216	239	0.02%	0.003%
42	10.055	1465	1471	1485	rVV	435641	576424	58.42%	8.118%
43	10.201	1489	1495	1497	rVV3	531	858	0.09%	0.012%
44	10.244	1497	1502	1507	rVV2	1637	2276	0.23%	0.032%
45	10.305	1508	1512	1516	rVB3	1644	2174	0.22%	0.031%
46	10.378	1522	1524	1529	rVV2	227	367	0.04%	0.005%
47	10.451	1532	1536	1538	rBV2	259	373	0.04%	0.005%
48	10.652	1564	1569	1572	rVB4	611	851	0.09%	0.012%
49	10.817	1594	1596	1598	rBV2	304	263	0.03%	0.004%
50	10.860	1601	1603	1606	rVB	691	542	0.05%	0.008%
51	10.902	1609	1610	1614	rBV2	305	348	0.04%	0.005%
52	11.030	1627	1631	1638	rBV3	1359	2233	0.23%	0.031%
53	11.122	1642	1646	1650	rVB3	3773	4718	0.48%	0.066%
54	11.195	1652	1658	1666	rVV	350184	439628	44.55%	6.191%
55	11.280	1669	1672	1674	rVV3	1057	1490	0.15%	0.021%
56	11.317	1674	1678	1684	rVB	5204	7873	0.80%	0.111%
57	11.476	1697	1704	1713	rBV5	1613	4025	0.41%	0.057%
58	11.549	1713	1716	1720	rVB2	449	566	0.06%	0.008%
59	11.616	1723	1727	1728	rBV2	414	330	0.03%	0.005%
60	11.671	1735	1736	1739	rBV2	512	541	0.05%	0.008%
61	11.750	1744	1749	1756	rVB3	3996	6117	0.62%	0.086%
62	11.841	1761	1764	1771	rVB3	768	1058	0.11%	0.015%
63	11.933	1775	1779	1783	rBV2	1941	2507	0.25%	0.035%
64	11.969	1783	1785	1788	rVB2	369	394	0.04%	0.006%
65	12.024	1788	1794	1801	rBV	448907	553007	56.05%	7.788%
66	12.128	1808	1811	1812	rBV3	1076	1405	0.14%	0.020%
67	12.152	1813	1815	1818	rVB	3249	2758	0.28%	0.039%
68	12.219	1822	1826	1835	rBV2	7074	10832	1.10%	0.153%
69	12.323	1837	1843	1850	rVV	504387	641778	65.04%	9.038%
70	12.378	1850	1852	1856	rVV4	1026	1195	0.12%	0.017%
71	12.433	1857	1861	1864	rVB3	1132	1473	0.15%	0.021%
72	12.488	1864	1870	1873	rBV5	758	1561	0.16%	0.022%
73	12.634	1891	1894	1896	rBV2	297	382	0.04%	0.005%
74	12.725	1907	1909	1911	rVB2	303	262	0.03%	0.004%
75	12.768	1911	1916	1920	rBV2	1760	2751	0.28%	0.039%
76	12.865	1928	1932	1937	rVB2	542	800	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026062.D
 Acq On : 27 Dec 2021 15:22
 Operator : JC/MD
 Sample : M5126-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	12.902	1937	1938	1941	rBV	235	292	0.03%	0.004%
78	12.933	1941	1943	1946	rVB2	288	271	0.03%	0.004%
79	12.969	1946	1949	1952	rBV	468	592	0.06%	0.008%
80	13.054	1959	1963	1966	rBV3	736	1163	0.12%	0.016%
81	13.128	1974	1975	1978	rVB2	296	259	0.03%	0.004%
82	13.384	2016	2017	2022	rBV2	226	309	0.03%	0.004%
83	13.591	2048	2051	2054	rBV2	310	461	0.05%	0.006%
84	13.621	2054	2056	2059	rVB2	200	207	0.02%	0.003%
85	13.780	2077	2082	2087	rBV3	495	885	0.09%	0.012%
86	14.134	2136	2140	2144	rVB	1809	2643	0.27%	0.037%
87	14.371	2178	2179	2183	rVB2	324	238	0.02%	0.003%
88	14.457	2190	2193	2195	rBV3	218	365	0.04%	0.005%
89	14.505	2199	2201	2202	rBV	261	212	0.02%	0.003%
90	14.999	2280	2282	2286	rBV2	341	344	0.03%	0.005%
91	15.139	2303	2305	2306	rVB	399	216	0.02%	0.003%
92	15.304	2331	2332	2333	rBV	407	206	0.02%	0.003%
93	15.353	2338	2340	2343	rVB2	394	258	0.03%	0.004%
94	15.396	2343	2347	2352	rBV5	505	1157	0.12%	0.016%
95	15.524	2366	2368	2371	rBV3	316	421	0.04%	0.006%
96	15.731	2398	2402	2403	rBV	603	703	0.07%	0.010%
97	16.060	2454	2456	2461	rVB3	416	585	0.06%	0.008%
98	16.115	2461	2465	2467	rBV3	442	554	0.06%	0.008%
99	16.334	2499	2501	2503	rBV3	408	429	0.04%	0.006%
100	16.560	2536	2538	2539	rBV	406	323	0.03%	0.005%


Sum of corrected areas: 7100511

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026062.D
Acq On : 27 Dec 2021 15:22
Operator : JC/MD
Sample : M5126-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

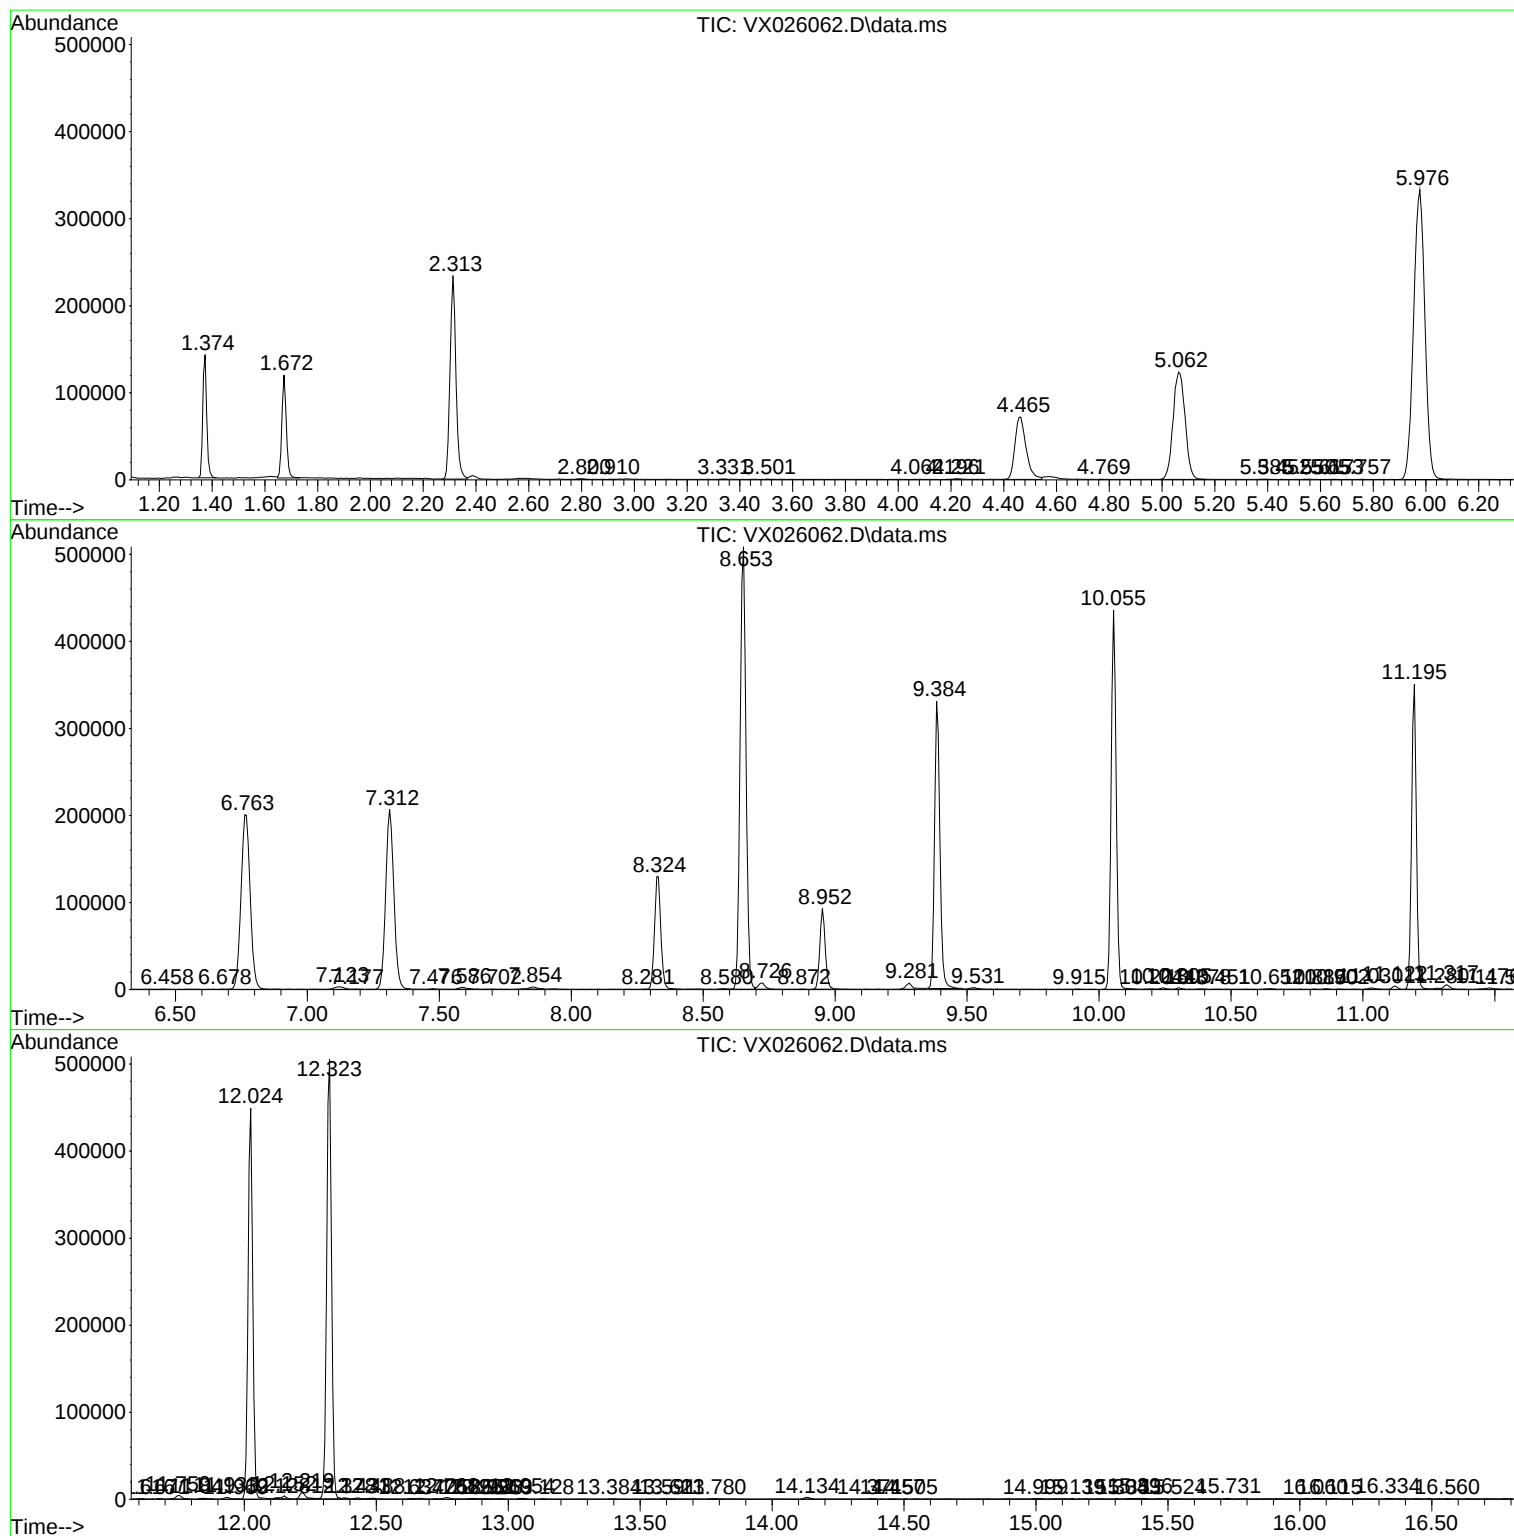

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026062.D
Acq On : 27 Dec 2021 15:22
Operator : JC/MD
Sample : M5126-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026062.D
Acq On : 27 Dec 2021 15:22
Operator : JC/MD
Sample : M5126-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------