

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026063.D
 Acq On : 27 Dec 2021 15:45
 Operator : JC/MD
 Sample : M5126-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026063.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	57	rVB	133505	141313	15.21%	2.129%
2	1.672	92	96	106	rVB	111396	131017	14.10%	1.974%
3	2.312	195	201	211	rBV	219325	338548	36.43%	5.101%
4	2.453	222	224	228	rVB2	346	318	0.03%	0.005%
5	2.703	262	265	270	rVB3	438	588	0.06%	0.009%
6	2.794	276	280	285	rVB4	891	1599	0.17%	0.024%
7	2.861	285	291	293	rBV2	221	378	0.04%	0.006%
8	3.099	327	330	332	rVB2	351	388	0.04%	0.006%
9	3.123	332	334	335	rBV2	232	245	0.03%	0.004%
10	3.257	354	356	359	rBV	170	217	0.02%	0.003%
11	3.452	386	388	391	rVB2	237	262	0.03%	0.004%
12	4.123	495	498	500	rVB2	296	367	0.04%	0.006%
13	4.147	500	502	503	rBV	259	205	0.02%	0.003%
14	4.227	512	515	516	rBV	292	247	0.03%	0.004%
15	4.458	544	553	569	rBV	65819	194280	20.91%	2.927%
16	4.910	623	627	628	rBV	191	225	0.02%	0.003%
17	5.062	640	652	667	rVV	119835	362166	38.97%	5.457%
18	5.391	696	706	715	rVB5	2113	6490	0.70%	0.098%
19	5.861	780	783	787	rVB2	199	284	0.03%	0.004%
20	5.976	788	802	818	rBV2	309864	929333	100.00%	14.002%
21	6.214	838	841	843	rBV	306	313	0.03%	0.005%
22	6.592	899	903	906	rBV2	202	386	0.04%	0.006%
23	6.763	922	931	946	rBV	183807	437281	47.05%	6.588%
24	7.129	983	991	999	rVB2	17955	39071	4.20%	0.589%
25	7.312	1012	1021	1036	rBV	196194	416273	44.79%	6.272%
26	7.482	1044	1049	1050	rBV3	588	854	0.09%	0.013%
27	7.818	1098	1104	1109	rVV3	420	1020	0.11%	0.015%
28	7.933	1118	1123	1127	rBV2	466	639	0.07%	0.010%
29	8.025	1136	1138	1140	rBV	207	199	0.02%	0.003%
30	8.074	1143	1146	1147	rVB2	244	217	0.02%	0.003%
31	8.263	1174	1177	1179	rVB2	224	204	0.02%	0.003%
32	8.324	1181	1187	1198	rVV	122647	198482	21.36%	2.990%
33	8.421	1202	1203	1208	rVB	446	373	0.04%	0.006%
34	8.470	1208	1211	1212	rBV	229	260	0.03%	0.004%
35	8.488	1212	1214	1217	rVB2	531	478	0.05%	0.007%
36	8.653	1234	1241	1249	rBV	461017	732824	78.85%	11.041%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026063.D
 Acq On : 27 Dec 2021 15:45
 Operator : JC/MD
 Sample : M5126-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	8.720	1249	1252	1262	rVB	6056	10711	1.15%	0.161%
38	8.951	1284	1290	1300	rBV	83416	121326	13.06%	1.828%
39	9.079	1309	1311	1314	rBV2	310	346	0.04%	0.005%
40	9.122	1316	1318	1320	rBV2	317	283	0.03%	0.004%
41	9.214	1332	1333	1335	rBV	301	196	0.02%	0.003%
42	9.275	1337	1343	1349	rBV2	26431	39009	4.20%	0.588%
43	9.384	1356	1361	1374	rVB	297178	419987	45.19%	6.328%
44	9.549	1387	1388	1391	rVB	330	223	0.02%	0.003%
45	9.592	1393	1395	1399	rVV2	296	398	0.04%	0.006%
46	9.720	1415	1416	1420	rBV	220	286	0.03%	0.004%
47	10.055	1466	1471	1482	rVB	399850	526327	56.63%	7.930%
48	10.201	1493	1495	1496	rVV2	510	348	0.04%	0.005%
49	10.244	1499	1502	1508	rVB2	1131	1495	0.16%	0.023%
50	10.299	1508	1511	1519	rBV3	978	1602	0.17%	0.024%
51	10.384	1523	1525	1528	rBV	258	271	0.03%	0.004%
52	10.640	1564	1567	1574	rBV4	544	1146	0.12%	0.017%
53	10.750	1582	1585	1586	rBV2	278	356	0.04%	0.005%
54	10.963	1618	1620	1623	rBV2	340	259	0.03%	0.004%
55	11.073	1637	1638	1641	rBV2	219	237	0.03%	0.004%
56	11.122	1641	1646	1652	rVV2	3291	4398	0.47%	0.066%
57	11.195	1652	1658	1667	rVV	314954	406404	43.73%	6.123%
58	11.286	1669	1673	1674	rVV2	703	863	0.09%	0.013%
59	11.317	1674	1678	1685	rVB	4647	7476	0.80%	0.113%
60	11.482	1702	1705	1707	rVB2	836	793	0.09%	0.012%
61	11.579	1720	1721	1724	rBV2	278	233	0.03%	0.004%
62	11.652	1729	1733	1735	rBV2	303	418	0.04%	0.006%
63	11.677	1735	1737	1739	rBV2	290	198	0.02%	0.003%
64	11.750	1745	1749	1756	rVB3	3122	4387	0.47%	0.066%
65	11.841	1762	1764	1768	rBV4	645	759	0.08%	0.011%
66	11.896	1771	1773	1776	rBV2	202	294	0.03%	0.004%
67	11.933	1776	1779	1784	rBV3	1598	1894	0.20%	0.029%
68	12.024	1788	1794	1805	rBV	411437	505026	54.34%	7.609%
69	12.122	1808	1810	1812	rBV3	1028	900	0.10%	0.014%
70	12.152	1812	1815	1821	rVB3	2624	3388	0.36%	0.051%
71	12.219	1821	1826	1831	rBV2	14508	20186	2.17%	0.304%
72	12.323	1837	1843	1850	rVB	464546	596716	64.21%	8.990%
73	12.426	1857	1860	1867	rVV3	1309	1687	0.18%	0.025%
74	12.481	1867	1869	1873	rVB3	807	946	0.10%	0.014%
75	12.579	1884	1885	1887	rBV2	249	211	0.02%	0.003%
76	12.658	1896	1898	1902	rBV2	586	735	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026063.D
 Acq On : 27 Dec 2021 15:45
 Operator : JC/MD
 Sample : M5126-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	12.762	1910	1915	1923	rBV3	1561	2692	0.29%	0.041%
78	12.853	1929	1930	1933	rVB2	314	207	0.02%	0.003%
79	12.926	1940	1942	1944	rBV2	283	269	0.03%	0.004%
80	12.981	1949	1951	1952	rBV	290	272	0.03%	0.004%
81	13.042	1959	1961	1964	rBV3	423	516	0.06%	0.008%
82	13.280	1996	2000	2001	rBV2	230	219	0.02%	0.003%
83	13.481	2031	2033	2035	rVB2	339	269	0.03%	0.004%
84	13.634	2057	2058	2060	rBV	291	235	0.03%	0.004%
85	13.780	2079	2082	2083	rBV	242	271	0.03%	0.004%
86	13.877	2096	2098	2101	rVB2	260	265	0.03%	0.004%
87	13.914	2101	2104	2107	rBV2	297	449	0.05%	0.007%
88	14.127	2136	2139	2146	rVB	1557	2599	0.28%	0.039%
89	14.182	2146	2148	2150	rBV2	176	219	0.02%	0.003%
90	14.298	2164	2167	2171	rBV2	274	365	0.04%	0.005%
91	14.457	2188	2193	2194	rBV3	298	421	0.05%	0.006%
92	14.554	2207	2209	2213	rBV2	308	367	0.04%	0.006%
93	14.896	2264	2265	2270	rBV2	415	513	0.06%	0.008%
94	14.993	2278	2281	2288	rBV5	3448	5382	0.58%	0.081%
95	15.078	2293	2295	2296	rBV	290	199	0.02%	0.003%
96	15.158	2306	2308	2311	rBV	274	198	0.02%	0.003%
97	15.395	2345	2347	2349	rBV2	534	508	0.05%	0.008%
98	15.706	2397	2398	2401	rVB2	512	298	0.03%	0.004%
99	15.908	2430	2431	2432	rBV	447	211	0.02%	0.003%
100	16.542	2534	2535	2537	rBV	355	208	0.02%	0.003%




Sum of corrected areas: 6637214

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026063.D
Acq On : 27 Dec 2021 15:45
Operator : JC/MD
Sample : M5126-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

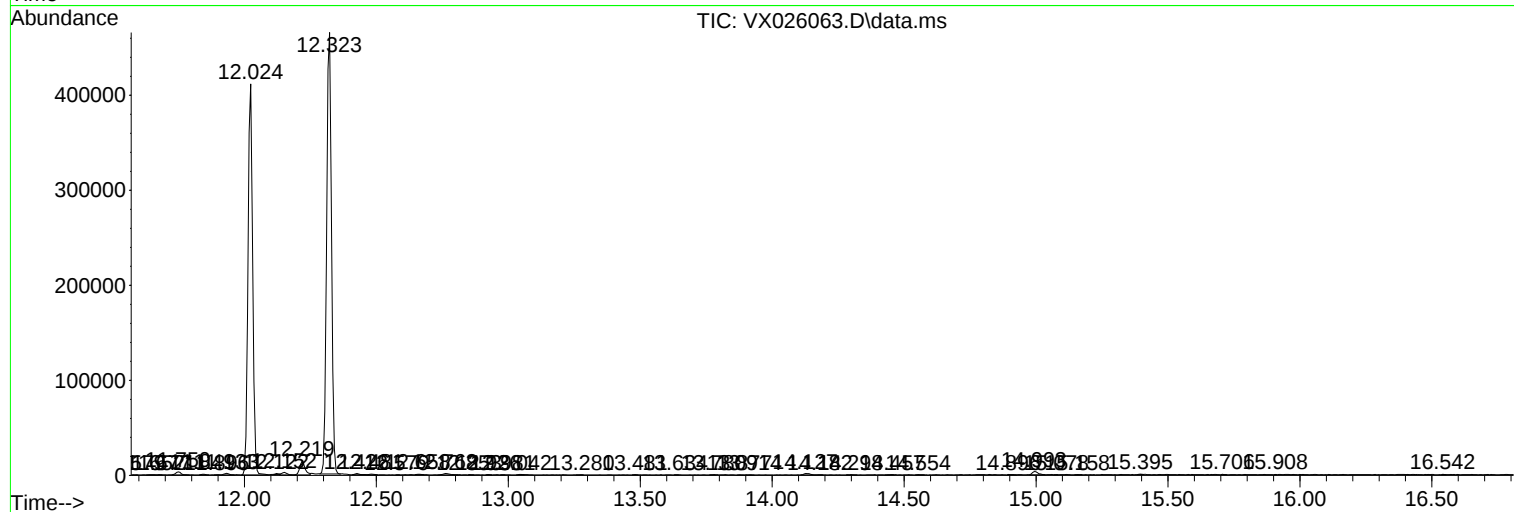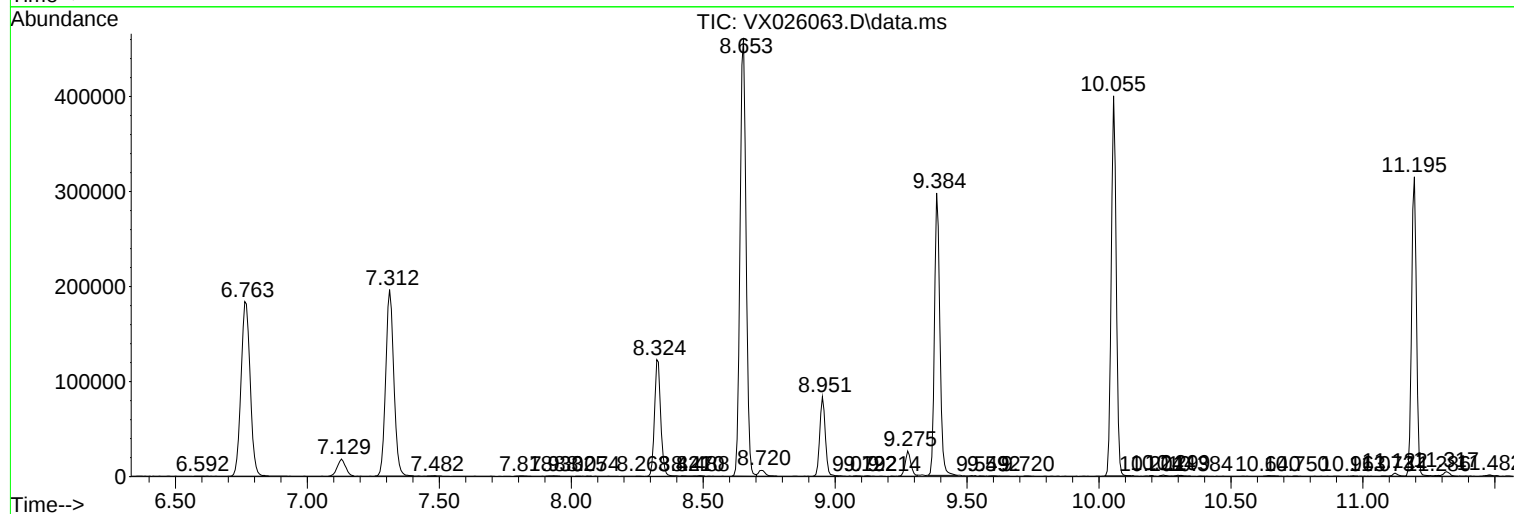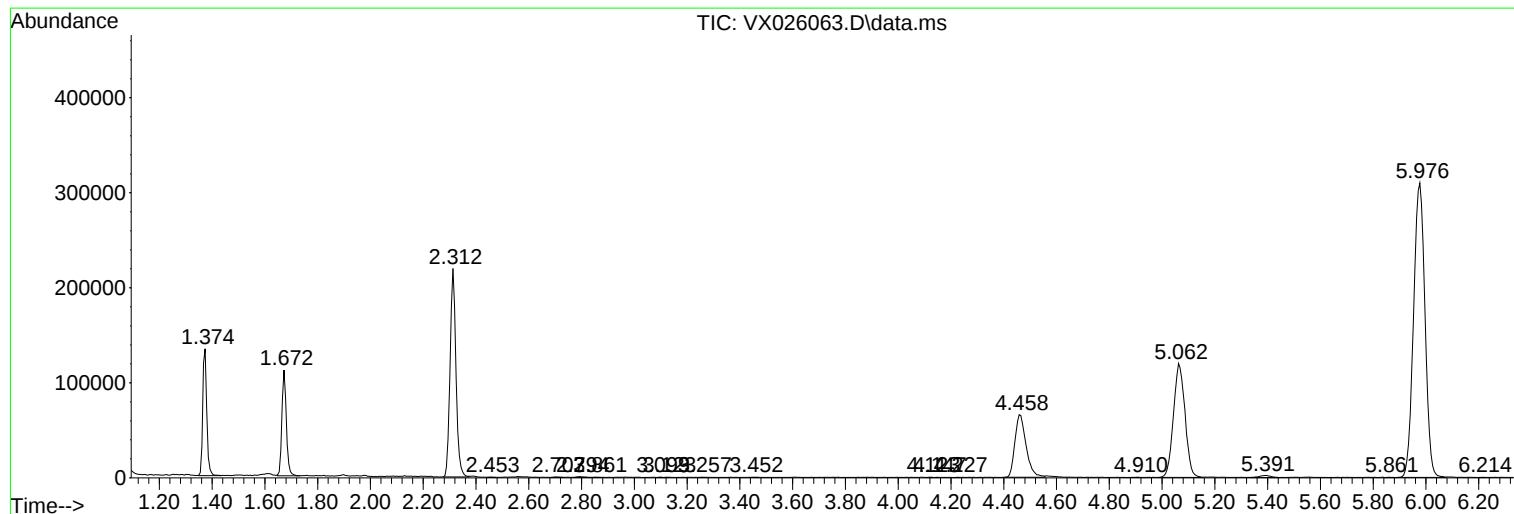

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026063.D
Acq On : 27 Dec 2021 15:45
Operator : JC/MD
Sample : M5126-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026063.D
Acq On : 27 Dec 2021 15:45
Operator : JC/MD
Sample : M5126-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------