

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026064.D
 Acq On : 27 Dec 2021 16:08
 Operator : JC/MD
 Sample : M5126-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026064.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	55	rVB	125563	124345	15.18%	2.058%
2	1.672	92	96	103	rVB	96450	110979	13.55%	1.836%
3	2.312	195	201	212	rBV	185316	297002	36.26%	4.914%
4	2.508	230	233	237	rBV2	320	549	0.07%	0.009%
5	2.788	275	279	286	rBV4	1571	3104	0.38%	0.051%
6	2.959	306	307	310	rVB	370	239	0.03%	0.004%
7	3.081	324	327	331	rBV	278	431	0.05%	0.007%
8	3.123	331	334	336	rBV2	310	247	0.03%	0.004%
9	3.568	406	407	412	rBV2	214	311	0.04%	0.005%
10	3.648	419	420	426	rVV2	249	288	0.04%	0.005%
11	3.733	432	434	437	rBV2	300	241	0.03%	0.004%
12	3.904	459	462	465	rVB2	255	262	0.03%	0.004%
13	3.940	465	468	469	rBV	180	180	0.02%	0.003%
14	4.312	527	529	532	rBV	249	211	0.03%	0.003%
15	4.458	544	553	568	rBV	62566	183016	22.34%	3.028%
16	4.818	611	612	615	rBV2	273	262	0.03%	0.004%
17	5.068	639	653	667	rBV	111379	328029	40.05%	5.428%
18	5.251	681	683	684	rBV2	373	180	0.02%	0.003%
19	5.281	685	688	691	rVB2	322	428	0.05%	0.007%
20	5.318	691	694	696	rBV2	225	270	0.03%	0.004%
21	5.342	696	698	702	rBV2	199	248	0.03%	0.004%
22	5.397	704	707	709	rBV2	203	226	0.03%	0.004%
23	5.562	731	734	735	rVB2	401	318	0.04%	0.005%
24	5.635	745	746	751	rVB2	324	338	0.04%	0.006%
25	5.678	751	753	756	rBV2	273	281	0.03%	0.005%
26	5.806	772	774	776	rBV	273	271	0.03%	0.004%
27	5.879	784	786	789	rBV	249	325	0.04%	0.005%
28	5.976	790	802	819	rVV2	272986	819105	100.00%	13.554%
29	6.458	879	881	883	rBV	256	225	0.03%	0.004%
30	6.629	905	909	913	rBV2	183	310	0.04%	0.005%
31	6.763	921	931	943	rBV	182150	437857	53.46%	7.245%
32	7.116	984	989	996	rBV7	2818	5614	0.69%	0.093%
33	7.226	1003	1007	1009	rVB2	193	208	0.03%	0.003%
34	7.312	1012	1021	1032	rBV	167954	370864	45.28%	6.137%
35	7.433	1039	1041	1043	rVB2	375	290	0.04%	0.005%
36	7.574	1060	1064	1067	rBV	233	356	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026064.D
 Acq On : 27 Dec 2021 16:08
 Operator : JC/MD
 Sample : M5126-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	7.641	1071	1075	1077	rBV2	151	195	0.02%	0.003%
38	7.708	1084	1086	1089	rBV2	344	415	0.05%	0.007%
39	7.793	1097	1100	1101	rBV2	225	234	0.03%	0.004%
40	7.866	1110	1112	1114	rVB	356	323	0.04%	0.005%
41	7.891	1114	1116	1117	rBV	281	229	0.03%	0.004%
42	7.982	1130	1131	1134	rVB2	210	196	0.02%	0.003%
43	8.013	1134	1136	1137	rBV	281	192	0.02%	0.003%
44	8.031	1137	1139	1142	rVB2	293	306	0.04%	0.005%
45	8.202	1164	1167	1170	rBV2	291	480	0.06%	0.008%
46	8.244	1170	1174	1180	rVV2	7538	11871	1.45%	0.196%
47	8.330	1181	1188	1198	rVB	103290	172132	21.01%	2.848%
48	8.470	1209	1211	1217	rBV	410	702	0.09%	0.012%
49	8.653	1234	1241	1249	rBV	417031	651727	79.57%	10.784%
50	8.720	1249	1252	1259	rVB	6080	9097	1.11%	0.151%
51	8.951	1284	1290	1304	rVV	73093	106621	13.02%	1.764%
52	9.140	1319	1321	1324	rVB2	317	343	0.04%	0.006%
53	9.183	1327	1328	1332	rVB2	237	243	0.03%	0.004%
54	9.281	1338	1344	1348	rBV	4253	6632	0.81%	0.110%
55	9.384	1356	1361	1377	rVB	280124	404078	49.33%	6.686%
56	9.610	1394	1398	1399	rBV2	331	308	0.04%	0.005%
57	9.701	1411	1413	1416	rVB	543	534	0.07%	0.009%
58	9.903	1444	1446	1448	rVB2	259	182	0.02%	0.003%
59	10.055	1465	1471	1481	rBV	399217	532160	64.97%	8.806%
60	10.195	1490	1494	1496	rBV2	386	536	0.07%	0.009%
61	10.299	1509	1511	1515	rVB3	1230	1388	0.17%	0.023%
62	10.591	1558	1559	1563	rBV2	210	255	0.03%	0.004%
63	10.640	1565	1567	1569	rBV2	405	377	0.05%	0.006%
64	10.854	1600	1602	1606	rBV2	265	363	0.04%	0.006%
65	10.939	1613	1616	1617	rBV2	334	249	0.03%	0.004%
66	10.963	1617	1620	1622	rBV2	330	327	0.04%	0.005%
67	11.122	1642	1646	1652	rVB2	2945	3956	0.48%	0.065%
68	11.195	1652	1658	1665	rBV	285038	370667	45.25%	6.133%
69	11.323	1674	1679	1684	rVB3	2462	4650	0.57%	0.077%
70	11.378	1684	1688	1690	rBV3	301	404	0.05%	0.007%
71	11.475	1698	1704	1707	rBV4	941	1545	0.19%	0.026%
72	11.713	1741	1743	1745	rBV3	330	387	0.05%	0.006%
73	11.750	1745	1749	1756	rVB4	2453	3724	0.45%	0.062%
74	11.841	1762	1764	1767	rBV	603	537	0.07%	0.009%
75	11.933	1776	1779	1782	rVB3	1188	1567	0.19%	0.026%
76	12.024	1788	1794	1799	rBV	413108	513368	62.67%	8.495%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026064.D
 Acq On : 27 Dec 2021 16:08
 Operator : JC/MD
 Sample : M5126-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	12.128	1807	1811	1812	rBV3	1046	1092	0.13%	0.018%
78	12.231	1826	1828	1830	rBV	269	265	0.03%	0.004%
79	12.323	1837	1843	1850	rBV	419309	539385	65.85%	8.925%
80	12.426	1857	1860	1863	rVB2	825	923	0.11%	0.015%
81	12.536	1876	1878	1881	rBV2	378	350	0.04%	0.006%
82	12.658	1897	1898	1901	rBV3	446	410	0.05%	0.007%
83	12.762	1912	1915	1920	rVB2	1543	1862	0.23%	0.031%
84	12.902	1937	1938	1940	rVB	475	234	0.03%	0.004%
85	13.054	1960	1963	1967	rVB4	545	682	0.08%	0.011%
86	13.195	1984	1986	1991	rBB	265	248	0.03%	0.004%
87	13.280	1999	2000	2002	rBV2	296	218	0.03%	0.004%
88	13.359	2009	2013	2014	rBV2	176	224	0.03%	0.004%
89	13.780	2080	2082	2086	rVB	373	263	0.03%	0.004%
90	13.884	2096	2099	2102	rBV2	246	364	0.04%	0.006%
91	14.133	2134	2140	2148	rBV	1826	3137	0.38%	0.052%
92	14.207	2148	2152	2153	rBV2	252	217	0.03%	0.004%
93	14.280	2162	2164	2167	rBV2	231	197	0.02%	0.003%
94	14.420	2185	2187	2189	rBV	264	204	0.02%	0.003%
95	14.444	2189	2191	2194	rBV2	272	311	0.04%	0.005%
96	14.859	2258	2259	2262	rBV2	303	271	0.03%	0.004%
97	14.944	2271	2273	2276	rBV2	282	367	0.04%	0.006%
98	15.066	2290	2293	2297	rBV2	409	657	0.08%	0.011%
99	15.310	2332	2333	2336	rVB	313	311	0.04%	0.005%
100	16.474	2523	2524	2527	rBV3	436	336	0.04%	0.006%


Sum of corrected areas: 6043438

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026064.D
Acq On : 27 Dec 2021 16:08
Operator : JC/MD
Sample : M5126-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

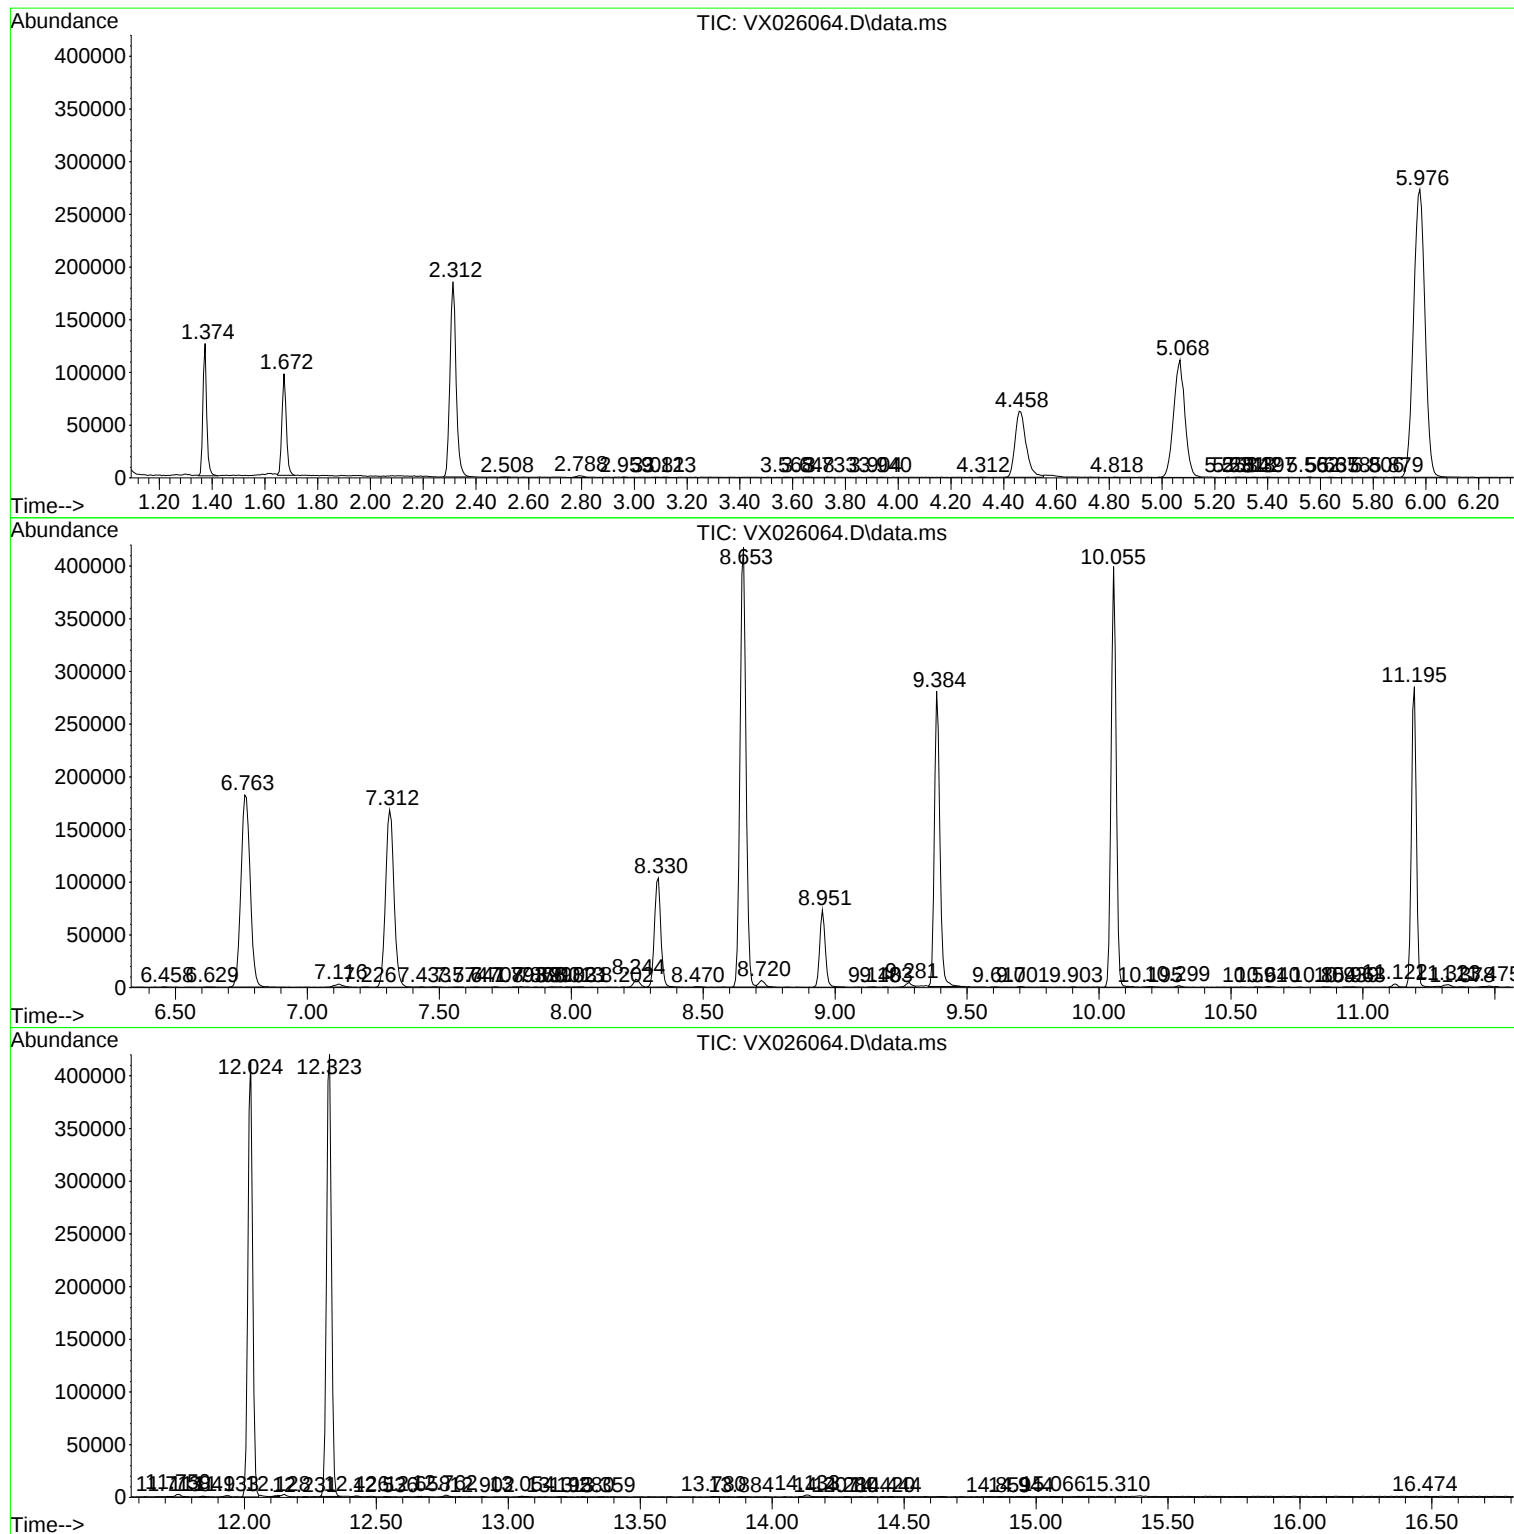

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026064.D
Acq On : 27 Dec 2021 16:08
Operator : JC/MD
Sample : M5126-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026064.D
Acq On : 27 Dec 2021 16:08
Operator : JC/MD
Sample : M5126-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc