

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026065.D
 Acq On : 27 Dec 2021 16:31
 Operator : JC/MD
 Sample : M5154-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026065.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	56	rVB	112760	121882	14.94%	2.035%
2	1.672	92	96	105	rVB	91908	112611	13.81%	1.880%
3	2.313	194	201	216	rBV	182753	295703	36.25%	4.937%
4	2.508	230	233	239	rVB3	275	496	0.06%	0.008%
5	2.715	263	267	268	rBV2	261	408	0.05%	0.007%
6	2.794	274	280	286	rVB4	1627	3084	0.38%	0.051%
7	2.959	302	307	309	rBV3	277	534	0.07%	0.009%
8	3.123	333	334	337	rBV	320	245	0.03%	0.004%
9	3.239	350	353	355	rBV	413	338	0.04%	0.006%
10	3.398	375	379	380	rBV2	184	247	0.03%	0.004%
11	3.422	380	383	386	rVV2	255	260	0.03%	0.004%
12	4.245	514	518	519	rVB2	264	275	0.03%	0.005%
13	4.459	543	553	568	rBV	62376	181999	22.31%	3.039%
14	4.879	620	622	625	rVB2	208	255	0.03%	0.004%
15	4.952	630	634	635	rBV2	351	342	0.04%	0.006%
16	5.068	640	653	670	rBV	108142	328025	40.21%	5.477%
17	5.282	685	688	692	rBV	180	244	0.03%	0.004%
18	5.355	697	700	703	rBV2	214	276	0.03%	0.005%
19	5.568	730	735	737	rBV3	432	776	0.10%	0.013%
20	5.623	742	744	746	rBV2	187	236	0.03%	0.004%
21	5.690	751	755	756	rBV2	230	282	0.03%	0.005%
22	5.739	761	763	767	rVB2	312	284	0.03%	0.005%
23	5.977	788	802	818	rBV2	272712	815699	100.00%	13.619%
24	6.208	838	840	842	rBV	325	267	0.03%	0.004%
25	6.361	862	865	866	rBV	298	311	0.04%	0.005%
26	6.763	922	931	950	rVV	184711	439631	53.90%	7.340%
27	7.117	979	989	996	rVB6	2842	6480	0.79%	0.108%
28	7.312	1011	1021	1032	rBV	173645	371960	45.60%	6.210%
29	7.476	1045	1048	1053	rBV3	396	759	0.09%	0.013%
30	7.586	1065	1066	1071	rBV2	199	330	0.04%	0.006%
31	7.690	1081	1083	1086	rVV	364	334	0.04%	0.006%
32	7.927	1119	1122	1124	rBV	443	578	0.07%	0.010%
33	8.324	1180	1187	1200	rBV	103843	172610	21.16%	2.882%
34	8.433	1204	1205	1208	rBV	269	301	0.04%	0.005%
35	8.476	1210	1212	1213	rVV2	486	356	0.04%	0.006%
36	8.586	1227	1230	1232	rBV2	243	289	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026065.D
 Acq On : 27 Dec 2021 16:31
 Operator : JC/MD
 Sample : M5154-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	8.653	1234	1241	1248	rBV	401412	640837	78.56%	10.699%
38	8.720	1248	1252	1258	rVB	5716	9058	1.11%	0.151%
39	8.830	1267	1270	1274	rBV2	253	297	0.04%	0.005%
40	8.909	1279	1283	1284	rBV2	224	280	0.03%	0.005%
41	8.952	1284	1290	1302	rBV	72302	104399	12.80%	1.743%
42	9.080	1308	1311	1314	rBV2	283	381	0.05%	0.006%
43	9.275	1338	1343	1348	rBV2	3765	6592	0.81%	0.110%
44	9.385	1356	1361	1375	rVB	280744	394728	48.39%	6.590%
45	9.628	1400	1401	1405	rVB2	414	375	0.05%	0.006%
46	9.659	1405	1406	1409	rBV2	386	348	0.04%	0.006%
47	9.702	1409	1413	1416	rBV2	783	910	0.11%	0.015%
48	9.805	1428	1430	1436	rBV2	204	300	0.04%	0.005%
49	9.982	1456	1459	1462	rBV2	257	435	0.05%	0.007%
50	10.055	1465	1471	1483	rVV	402101	530298	65.01%	8.854%
51	10.195	1492	1494	1495	rBV	353	255	0.03%	0.004%
52	10.305	1509	1512	1517	rVB3	1014	1326	0.16%	0.022%
53	10.537	1547	1550	1554	rBV2	247	401	0.05%	0.007%
54	10.616	1560	1563	1565	rBV2	214	278	0.03%	0.005%
55	10.640	1565	1567	1570	rBV2	364	554	0.07%	0.009%
56	10.707	1573	1578	1579	rBV2	190	285	0.03%	0.005%
57	10.793	1590	1592	1595	rVB2	249	298	0.04%	0.005%
58	10.835	1595	1599	1600	rBV2	225	271	0.03%	0.005%
59	10.884	1604	1607	1611	rBV2	340	620	0.08%	0.010%
60	10.939	1613	1616	1618	rBV2	210	278	0.03%	0.005%
61	10.970	1618	1621	1623	rBV2	301	287	0.04%	0.005%
62	11.122	1643	1646	1649	rVB2	2635	3219	0.39%	0.054%
63	11.195	1652	1658	1666	rBV	287714	365296	44.78%	6.099%
64	11.317	1675	1678	1684	rVB5	2601	4110	0.50%	0.069%
65	11.482	1702	1705	1708	rBV2	1101	1195	0.15%	0.020%
66	11.689	1731	1739	1740	rBV2	504	771	0.09%	0.013%
67	11.750	1744	1749	1752	rBV3	3060	3873	0.47%	0.065%
68	11.847	1762	1765	1767	rBV2	432	339	0.04%	0.006%
69	11.933	1776	1779	1785	rVB3	1382	1675	0.21%	0.028%
70	12.024	1789	1794	1800	rVV	419215	509347	62.44%	8.504%
71	12.122	1807	1810	1813	rVV3	1022	1670	0.20%	0.028%
72	12.152	1813	1815	1818	rVB2	1982	1976	0.24%	0.033%
73	12.232	1824	1828	1830	rBV2	535	638	0.08%	0.011%
74	12.323	1837	1843	1852	rVB	418256	528066	64.74%	8.817%
75	12.427	1856	1860	1864	rVB3	781	1040	0.13%	0.017%
76	12.482	1865	1869	1874	rVV3	341	608	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026065.D
 Acq On : 27 Dec 2021 16:31
 Operator : JC/MD
 Sample : M5154-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	12.616	1888	1891	1894	rBV	200	323	0.04%	0.005%
78	12.671	1896	1900	1901	rVB2	509	527	0.06%	0.009%
79	12.762	1911	1915	1920	rVB2	1408	2048	0.25%	0.034%
80	12.811	1920	1923	1928	rBV2	330	487	0.06%	0.008%
81	12.872	1930	1933	1936	rVB	291	319	0.04%	0.005%
82	12.902	1936	1938	1942	rBV2	217	296	0.04%	0.005%
83	13.000	1953	1954	1957	rBV2	228	240	0.03%	0.004%
84	13.061	1960	1964	1965	rVB	450	545	0.07%	0.009%
85	13.079	1965	1967	1969	rBV	260	255	0.03%	0.004%
86	13.207	1985	1988	1992	rBV2	206	325	0.04%	0.005%
87	13.676	2063	2065	2067	rBV	231	264	0.03%	0.004%
88	13.841	2089	2092	2094	rBV2	265	318	0.04%	0.005%
89	14.134	2136	2140	2144	rVB	1942	2554	0.31%	0.043%
90	14.243	2155	2158	2160	rBV2	285	389	0.05%	0.006%
91	14.597	2213	2216	2219	rBV3	260	392	0.05%	0.007%
92	14.670	2226	2228	2231	rVV2	251	262	0.03%	0.004%
93	14.957	2274	2275	2278	rBV3	316	253	0.03%	0.004%
94	15.292	2328	2330	2332	rBV2	296	312	0.04%	0.005%
95	15.847	2419	2421	2423	rVB	415	326	0.04%	0.005%
96	16.231	2482	2484	2488	rBV2	274	379	0.05%	0.006%
97	16.292	2491	2494	2500	rVB2	456	931	0.11%	0.016%
98	16.334	2500	2501	2503	rBV	554	414	0.05%	0.007%
99	16.426	2513	2516	2518	rBV2	410	464	0.06%	0.008%
100	16.651	2551	2553	2555	rBV2	288	255	0.03%	0.004%




Sum of corrected areas: 5989499

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026065.D
Acq On : 27 Dec 2021 16:31
Operator : JC/MD
Sample : M5154-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

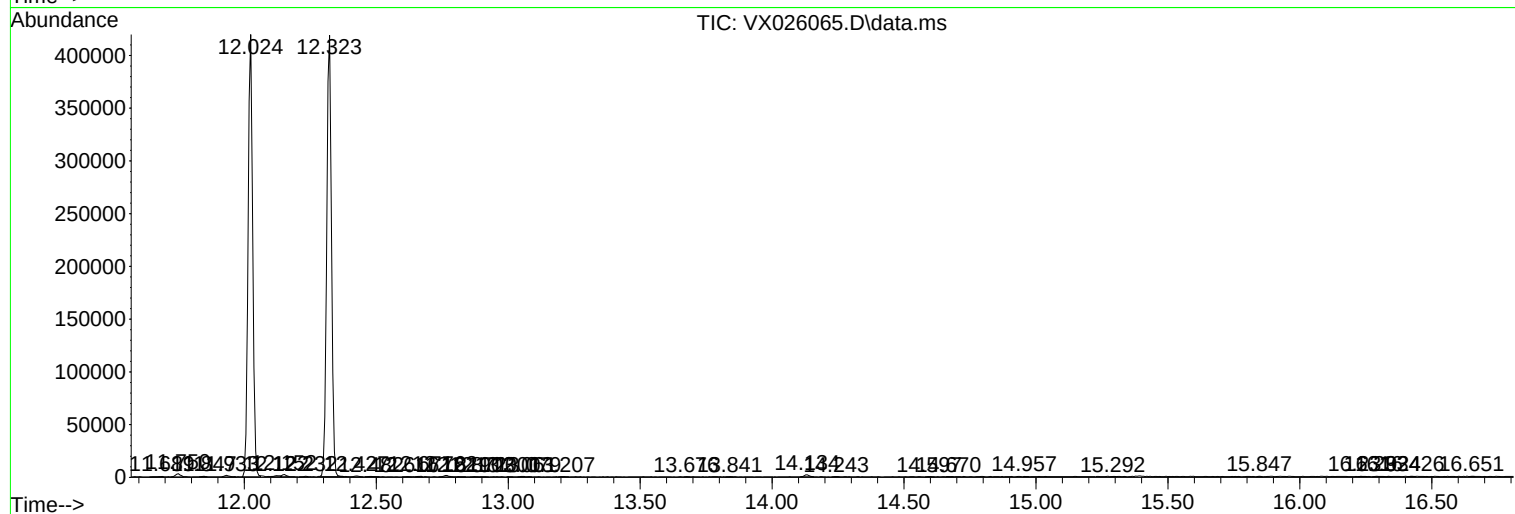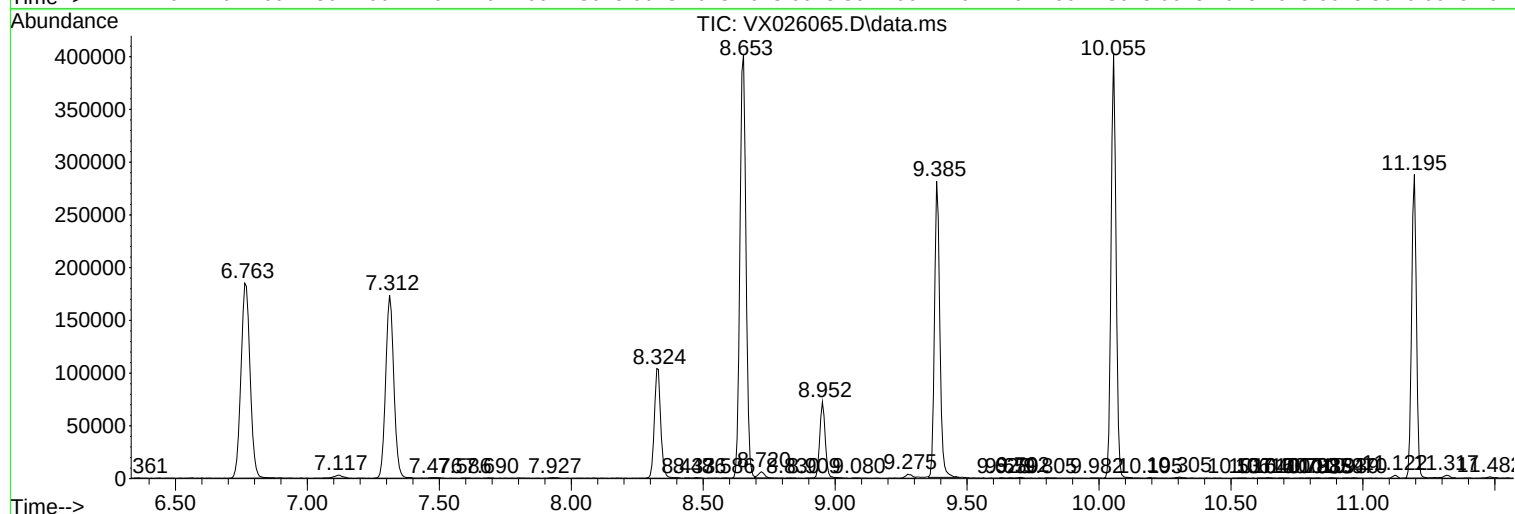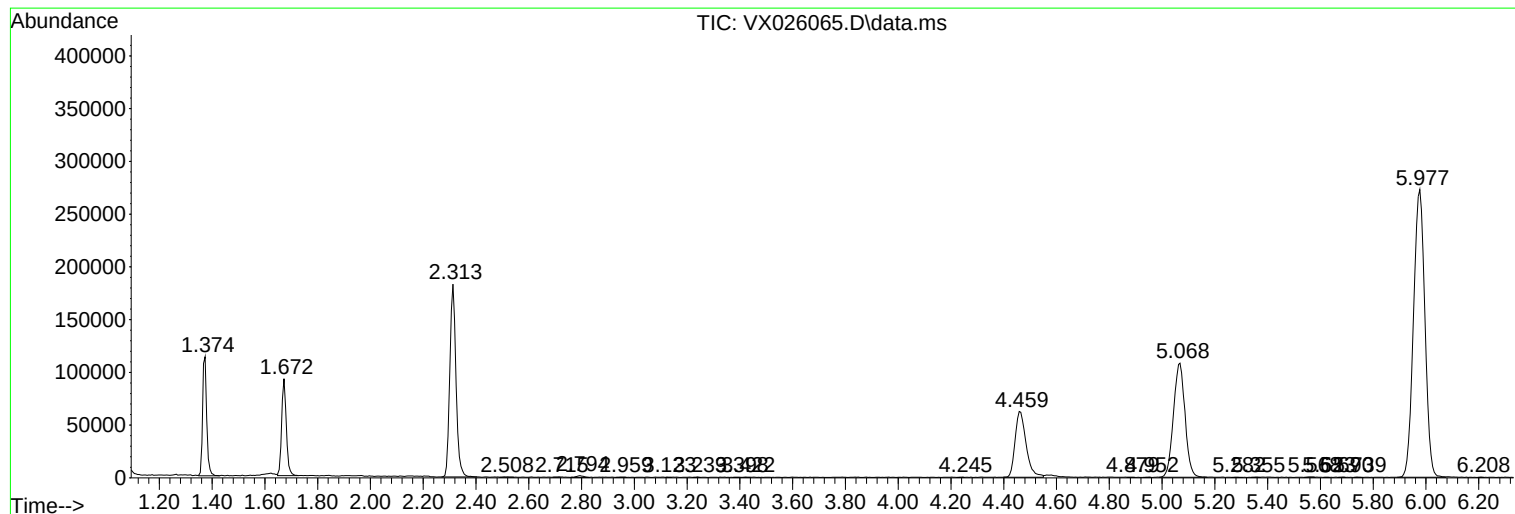

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026065.D
Acq On : 27 Dec 2021 16:31
Operator : JC/MD
Sample : M5154-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026065.D
Acq On : 27 Dec 2021 16:31
Operator : JC/MD
Sample : M5154-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc