

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026067.D
 Acq On : 27 Dec 2021 17:17
 Operator : JC/MD
 Sample : M5150-26 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M

Title : VOC Analysis

Signal : TIC: VX026067.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	33	rVB	19418	16970	1.39%	0.211%
2	1.374	43	47	57	rVB	145609	155676	12.72%	1.933%
3	1.672	92	96	103	rVB	107304	124180	10.15%	1.542%
4	2.312	195	201	214	rBV	213489	355135	29.01%	4.411%
5	2.514	233	234	238	rVB3	432	500	0.04%	0.006%
6	2.660	256	258	262	rVB2	454	500	0.04%	0.006%
7	2.703	262	265	267	rBV2	425	596	0.05%	0.007%
8	2.751	272	273	275	rVV2	360	281	0.02%	0.003%
9	2.794	275	280	288	rVV3	1800	3555	0.29%	0.044%
10	2.873	291	293	297	rVB2	190	261	0.02%	0.003%
11	2.953	302	306	309	rVV3	244	360	0.03%	0.004%
12	3.014	315	316	318	rBV	293	248	0.02%	0.003%
13	3.099	325	330	338	rVB4	2725	5310	0.43%	0.066%
14	3.215	346	349	350	rBV	269	232	0.02%	0.003%
15	3.282	359	360	363	rBV2	251	272	0.02%	0.003%
16	3.367	373	374	376	rBV2	255	194	0.02%	0.002%
17	3.416	379	382	383	rVB2	278	248	0.02%	0.003%
18	3.434	383	385	387	rBV2	283	244	0.02%	0.003%
19	3.452	387	388	390	rVB	375	188	0.02%	0.002%
20	3.489	390	394	397	rBV2	215	285	0.02%	0.004%
21	3.971	471	473	475	rBV2	217	233	0.02%	0.003%
22	4.056	486	487	489	rBV	231	205	0.02%	0.003%
23	4.221	513	514	517	rBV	217	226	0.02%	0.003%
24	4.391	539	542	543	rBV	239	241	0.02%	0.003%
25	4.489	544	558	580	rVV2	124883	480761	39.28%	5.971%
26	5.062	640	652	671	rBV	119325	365073	29.83%	4.534%
27	5.220	675	678	680	rBV2	195	210	0.02%	0.003%
28	5.281	687	688	691	rVB	291	191	0.02%	0.002%
29	5.379	702	704	707	rBV3	368	298	0.02%	0.004%
30	5.550	729	732	734	rBV	576	672	0.05%	0.008%
31	5.763	766	767	770	rBV	307	308	0.03%	0.004%
32	5.976	789	802	818	rBV2	302380	909888	74.33%	11.300%
33	6.196	837	838	840	rVB	307	194	0.02%	0.002%
34	6.458	879	881	885	rVB2	201	222	0.02%	0.003%
35	6.531	890	893	894	rBV2	357	315	0.03%	0.004%
36	6.763	922	931	945	rVV	179820	434047	35.46%	5.391%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026067.D
 Acq On : 27 Dec 2021 17:17
 Operator : JC/MD
 Sample : M5150-26 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	6.921	955	957	960	rBV3	232	339	0.03%	0.004%
38	7.129	980	991	1009	rBV	568750	1224045	100.00%	15.202%
39	7.312	1012	1021	1036	rVB	189858	412350	33.69%	5.121%
40	7.482	1045	1049	1051	rBV4	678	894	0.07%	0.011%
41	7.549	1056	1060	1062	rVB2	269	304	0.02%	0.004%
42	7.787	1097	1099	1101	rBV	354	386	0.03%	0.005%
43	7.915	1119	1120	1121	rBV	316	190	0.02%	0.002%
44	7.933	1121	1123	1124	rVV	461	388	0.03%	0.005%
45	8.098	1149	1150	1153	rBV	262	286	0.02%	0.004%
46	8.330	1181	1188	1199	rBV	119248	194020	15.85%	2.410%
47	8.482	1208	1213	1217	rBV3	366	638	0.05%	0.008%
48	8.653	1234	1241	1248	rVV	458137	724350	59.18%	8.996%
49	8.720	1248	1252	1265	rVB	6684	12070	0.99%	0.150%
50	8.951	1284	1290	1301	rVV	83088	119143	9.73%	1.480%
51	9.183	1327	1328	1332	rVB	285	325	0.03%	0.004%
52	9.281	1339	1344	1347	rBV	3734	6201	0.51%	0.077%
53	9.384	1356	1361	1381	rVB	307714	442833	36.18%	5.500%
54	9.756	1419	1422	1424	rBV2	220	278	0.02%	0.003%
55	9.854	1436	1438	1442	rBV	274	259	0.02%	0.003%
56	9.994	1459	1461	1465	rVB	273	210	0.02%	0.003%
57	10.055	1465	1471	1480	rBV	394714	523161	42.74%	6.497%
58	10.195	1492	1494	1500	rBV4	450	796	0.07%	0.010%
59	10.244	1500	1502	1505	rBV2	278	374	0.03%	0.005%
60	10.299	1509	1511	1517	rVB2	1142	1470	0.12%	0.018%
61	10.476	1538	1540	1545	rBV2	208	285	0.02%	0.004%
62	10.646	1562	1568	1571	rVB3	464	746	0.06%	0.009%
63	10.713	1576	1579	1581	rBV2	162	228	0.02%	0.003%
64	11.122	1641	1646	1652	rVV3	2952	4255	0.35%	0.053%
65	11.195	1652	1658	1668	rBV	321893	406249	33.19%	5.045%
66	11.323	1676	1679	1685	rVB2	2710	3714	0.30%	0.046%
67	11.475	1701	1704	1708	rVV3	1244	1542	0.13%	0.019%
68	11.555	1714	1717	1720	rVB3	577	673	0.05%	0.008%
69	11.622	1725	1728	1729	rBV2	232	219	0.02%	0.003%
70	11.671	1735	1736	1740	rVB3	451	474	0.04%	0.006%
71	11.719	1742	1744	1745	rVV	350	271	0.02%	0.003%
72	11.750	1745	1749	1755	rVB3	3037	4369	0.36%	0.054%
73	11.835	1760	1763	1769	rVB3	671	992	0.08%	0.012%
74	11.933	1776	1779	1784	rBV5	1640	2318	0.19%	0.029%
75	12.024	1789	1794	1800	rBV	413697	497120	40.61%	6.174%
76	12.146	1812	1814	1818	rVB3	2394	2994	0.24%	0.037%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026067.D
 Acq On : 27 Dec 2021 17:17
 Operator : JC/MD
 Sample : M5150-26 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

77	12.244	1826	1830	1833	rBV3	497	828	0.07%	0.010%
78	12.323	1836	1843	1849	rBV	457815	588809	48.10%	7.313%
79	12.426	1856	1860	1864	rVB3	1156	1595	0.13%	0.020%
80	12.481	1866	1869	1872	rVV	602	816	0.07%	0.010%
81	12.664	1897	1899	1902	rBV	523	512	0.04%	0.006%
82	12.768	1912	1916	1919	rVB3	1071	1386	0.11%	0.017%
83	12.878	1932	1934	1935	rVB	380	239	0.02%	0.003%
84	12.896	1935	1937	1938	rBV2	381	320	0.03%	0.004%
85	13.054	1959	1963	1967	rVB3	626	1015	0.08%	0.013%
86	13.237	1992	1993	1996	rVV	234	196	0.02%	0.002%
87	13.310	2003	2005	2008	rBV2	225	214	0.02%	0.003%
88	13.341	2008	2010	2014	rBV2	148	190	0.02%	0.002%
89	13.749	2076	2077	2080	rBV2	242	249	0.02%	0.003%
90	14.060	2126	2128	2130	rVB	292	234	0.02%	0.003%
91	14.097	2130	2134	2135	rBV2	286	342	0.03%	0.004%
92	14.133	2135	2140	2144	rBV	2145	2556	0.21%	0.032%
93	14.201	2149	2151	2154	rBV	349	371	0.03%	0.005%
94	14.322	2169	2171	2173	rBV	292	206	0.02%	0.003%
95	14.444	2190	2191	2193	rBV2	347	247	0.02%	0.003%
96	14.524	2200	2204	2205	rBV2	261	324	0.03%	0.004%
97	14.633	2220	2222	2224	rBV	414	245	0.02%	0.003%
98	14.914	2265	2268	2272	rBV2	343	434	0.04%	0.005%
99	15.085	2294	2296	2297	rBV	387	238	0.02%	0.003%
100	15.700	2395	2397	2399	rBV	334	347	0.03%	0.004%




Sum of corrected areas: 8051991

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026067.D
Acq On : 27 Dec 2021 17:17
Operator : JC/MD
Sample : M5150-26 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

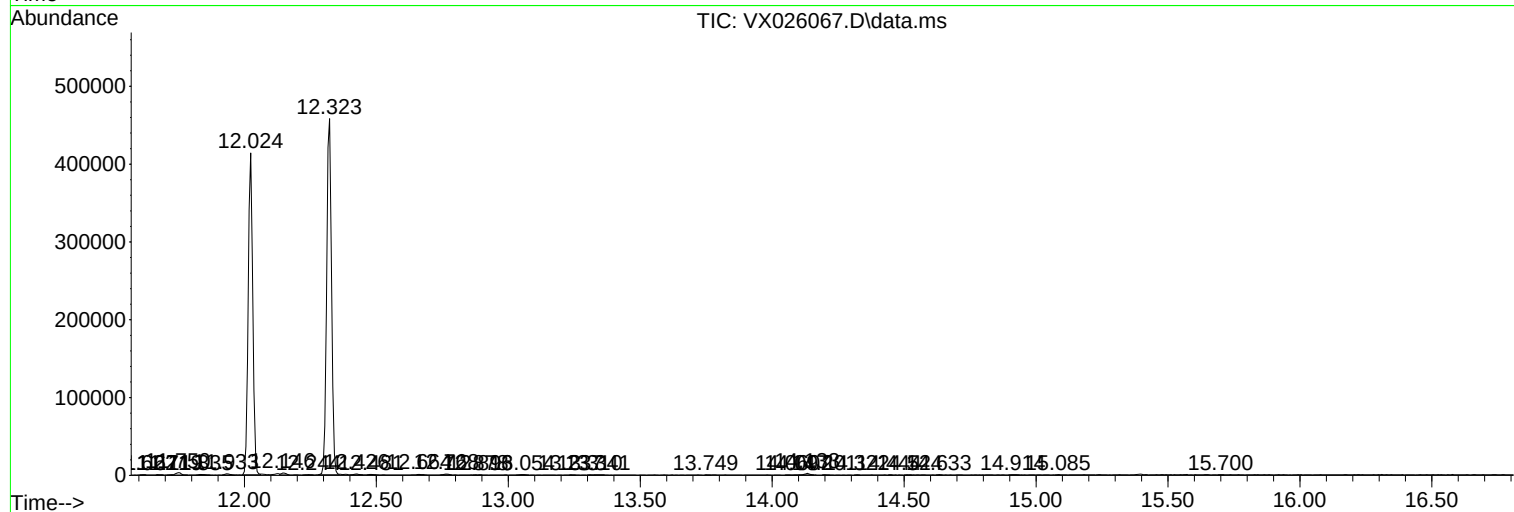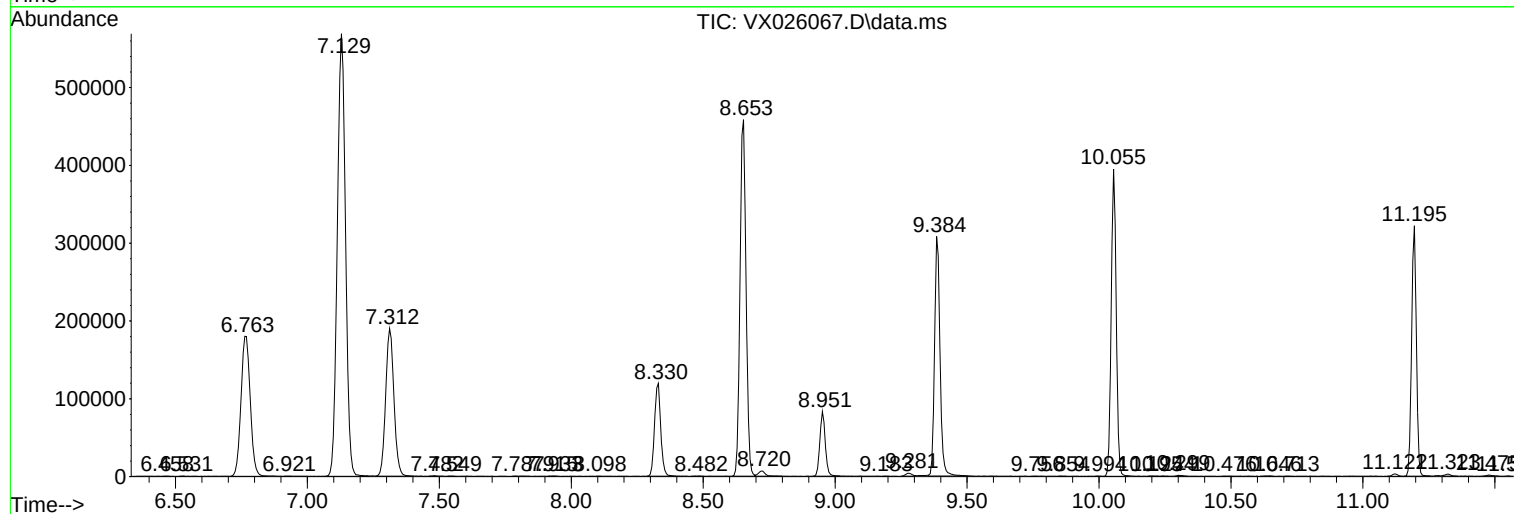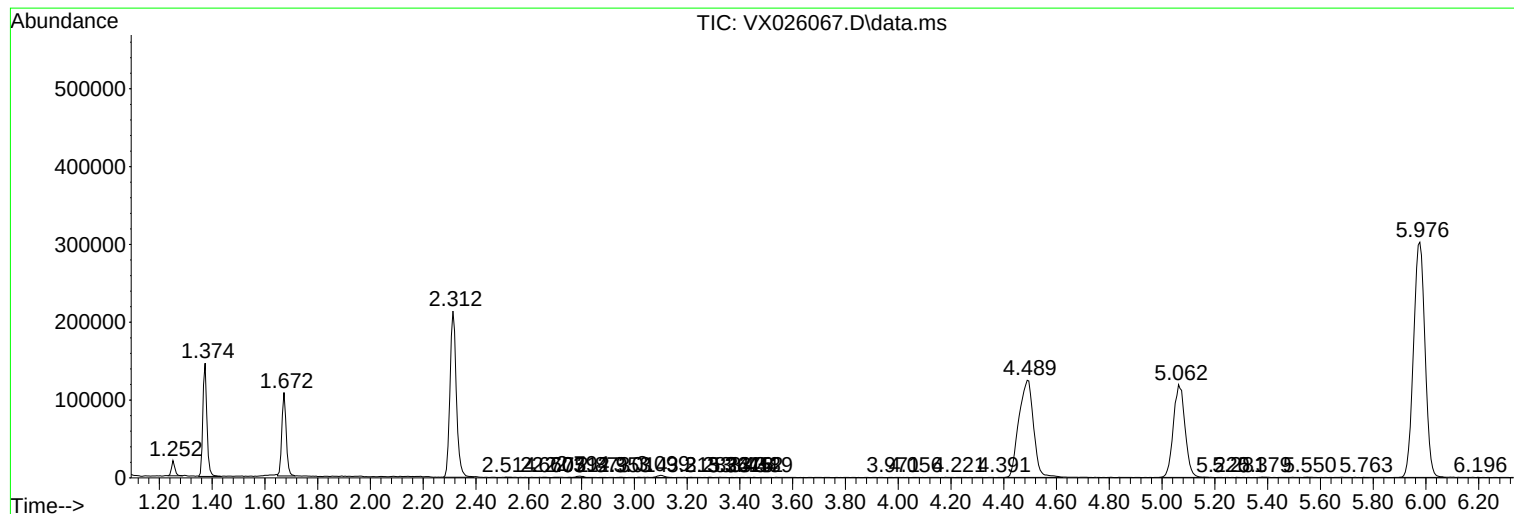

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026067.D
Acq On : 27 Dec 2021 17:17
Operator : JC/MD
Sample : M5150-26 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026067.D
Acq On : 27 Dec 2021 17:17
Operator : JC/MD
Sample : M5150-26 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc