

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026069.D
 Acq On : 27 Dec 2021 18:04
 Operator : JC/MD
 Sample : M5150-29
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026069.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	55	rVB	113572	119470	14.81%	2.017%
2	1.672	92	96	107	rVB	95026	113052	14.02%	1.908%
3	2.313	194	201	215	rVB	179385	290658	36.04%	4.906%
4	2.556	239	241	243	rBV2	297	365	0.05%	0.006%
5	2.794	276	280	288	rVB3	1400	2648	0.33%	0.045%
6	2.947	304	305	309	rBV2	265	316	0.04%	0.005%
7	3.014	312	316	318	rBV2	143	225	0.03%	0.004%
8	3.203	345	347	350	rBV	181	211	0.03%	0.004%
9	3.404	379	380	384	rBV	251	284	0.04%	0.005%
10	3.910	460	463	465	rVB2	256	261	0.03%	0.004%
11	3.934	465	467	469	rBV	369	298	0.04%	0.005%
12	4.196	509	510	515	rBV2	170	223	0.03%	0.004%
13	4.459	543	553	568	rBV	61674	179586	22.26%	3.031%
14	4.861	615	619	620	rBV2	170	240	0.03%	0.004%
15	5.068	640	653	670	rBV2	108663	324061	40.18%	5.470%
16	5.245	679	682	684	rBV	294	353	0.04%	0.006%
17	5.403	704	708	712	rBV3	285	441	0.05%	0.007%
18	5.519	726	727	730	rBV2	186	242	0.03%	0.004%
19	5.690	753	755	757	rVB2	276	282	0.03%	0.005%
20	5.781	767	770	771	rBV2	233	275	0.03%	0.005%
21	5.830	775	778	783	rBV2	197	373	0.05%	0.006%
22	5.977	787	802	816	rBV2	269496	806588	100.00%	13.615%
23	6.196	836	838	842	rVB2	417	385	0.05%	0.006%
24	6.458	875	881	882	rBV2	255	370	0.05%	0.006%
25	6.489	884	886	889	rVB	320	229	0.03%	0.004%
26	6.519	889	891	894	rBV	244	245	0.03%	0.004%
27	6.763	922	931	945	rBV	179126	425753	52.78%	7.187%
28	6.970	961	965	967	rBV2	295	434	0.05%	0.007%
29	7.056	976	979	980	rBV2	202	237	0.03%	0.004%
30	7.110	982	988	997	rVB5	2943	7448	0.92%	0.126%
31	7.312	1012	1021	1036	rVV	170029	369011	45.75%	6.229%
32	7.470	1044	1047	1048	rBV2	533	467	0.06%	0.008%
33	7.537	1054	1058	1059	rBV	223	258	0.03%	0.004%
34	7.812	1099	1103	1106	rVB3	357	636	0.08%	0.011%
35	7.854	1106	1110	1114	rVB2	228	323	0.04%	0.005%
36	7.940	1118	1124	1126	rBV3	422	685	0.08%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026069.D
 Acq On : 27 Dec 2021 18:04
 Operator : JC/MD
 Sample : M5150-29
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	8.013	1133	1136	1138	rBV	257	305	0.04%	0.005%
38	8.062	1141	1144	1147	rBV2	204	285	0.04%	0.005%
39	8.159	1157	1160	1161	rVB2	258	258	0.03%	0.004%
40	8.202	1165	1167	1170	rBV	312	397	0.05%	0.007%
41	8.324	1181	1187	1200	rBV	107517	171958	21.32%	2.903%
42	8.452	1205	1208	1210	rBV2	271	318	0.04%	0.005%
43	8.476	1210	1212	1217	rBV3	351	479	0.06%	0.008%
44	8.580	1226	1229	1232	rVB2	527	518	0.06%	0.009%
45	8.653	1234	1241	1248	rVV	397915	639435	79.28%	10.794%
46	8.720	1248	1252	1261	rVB	5578	10057	1.25%	0.170%
47	8.952	1284	1290	1298	rBV	72704	103124	12.79%	1.741%
48	9.220	1331	1334	1339	rVB2	172	285	0.04%	0.005%
49	9.281	1339	1344	1349	rBV3	3278	6296	0.78%	0.106%
50	9.384	1356	1361	1374	rVB	276625	389457	48.28%	6.574%
51	9.537	1385	1386	1389	rVB	491	270	0.03%	0.005%
52	9.647	1401	1404	1405	rVB2	270	272	0.03%	0.005%
53	9.695	1411	1412	1415	rVB2	334	293	0.04%	0.005%
54	9.799	1426	1429	1434	rBV2	223	379	0.05%	0.006%
55	9.842	1434	1436	1439	rVB	227	233	0.03%	0.004%
56	10.055	1465	1471	1485	rVV	396158	518423	64.27%	8.751%
57	10.195	1492	1494	1496	rBV2	387	330	0.04%	0.006%
58	10.305	1508	1512	1517	rBV3	1036	1538	0.19%	0.026%
59	10.409	1526	1529	1532	rBV2	144	223	0.03%	0.004%
60	10.640	1565	1567	1568	rBV	407	268	0.03%	0.005%
61	10.963	1618	1620	1621	rVB	316	216	0.03%	0.004%
62	11.122	1642	1646	1652	rVV	2600	3477	0.43%	0.059%
63	11.195	1652	1658	1667	rVV	285770	367300	45.54%	6.200%
64	11.256	1667	1668	1670	rVV2	622	648	0.08%	0.011%
65	11.317	1674	1678	1683	rVB3	2705	4697	0.58%	0.079%
66	11.390	1688	1690	1693	rVB2	415	472	0.06%	0.008%
67	11.421	1693	1695	1697	rBV	235	229	0.03%	0.004%
68	11.451	1698	1700	1702	rVV	510	330	0.04%	0.006%
69	11.482	1702	1705	1707	rVV2	1241	1308	0.16%	0.022%
70	11.549	1714	1716	1718	rVV	316	228	0.03%	0.004%
71	11.671	1735	1736	1739	rBV	250	270	0.03%	0.005%
72	11.750	1745	1749	1753	rVB3	2824	3357	0.42%	0.057%
73	11.841	1759	1764	1769	rBV4	569	923	0.11%	0.016%
74	11.933	1775	1779	1785	rBV3	1194	1888	0.23%	0.032%
75	12.024	1789	1794	1805	rVV	408927	495373	61.42%	8.362%
76	12.122	1807	1810	1812	rVV2	866	1188	0.15%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026069.D
 Acq On : 27 Dec 2021 18:04
 Operator : JC/MD
 Sample : M5150-29
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	12.152	1812	1815	1818	rVB	1874	2111	0.26%	0.036%
78	12.323	1835	1843	1850	rBV	415307	535469	66.39%	9.039%
79	12.427	1858	1860	1864	rVB4	823	711	0.09%	0.012%
80	12.488	1866	1870	1872	rBV2	584	653	0.08%	0.011%
81	12.640	1893	1895	1896	rBV	239	238	0.03%	0.004%
82	12.768	1912	1916	1919	rVB3	1500	2144	0.27%	0.036%
83	12.853	1926	1930	1932	rBV	261	487	0.06%	0.008%
84	13.359	2010	2013	2016	rVB2	296	414	0.05%	0.007%
85	13.506	2035	2037	2039	rBV2	265	224	0.03%	0.004%
86	13.530	2039	2041	2044	rVV2	207	252	0.03%	0.004%
87	13.573	2046	2048	2051	rVV	310	277	0.03%	0.005%
88	13.615	2053	2055	2058	rBV	237	242	0.03%	0.004%
89	13.701	2066	2069	2072	rBV2	340	371	0.05%	0.006%
90	14.128	2135	2139	2143	rBV2	1809	2591	0.32%	0.044%
91	14.188	2148	2149	2154	rVB2	303	317	0.04%	0.005%
92	14.621	2216	2220	2221	rBV	297	252	0.03%	0.004%
93	14.688	2229	2231	2235	rBV2	218	266	0.03%	0.004%
94	15.213	2315	2317	2318	rBV2	384	293	0.04%	0.005%
95	15.310	2331	2333	2334	rBV2	272	269	0.03%	0.005%
96	15.396	2343	2347	2351	rBV3	558	1013	0.13%	0.017%
97	15.871	2423	2425	2427	rVB2	446	350	0.04%	0.006%
98	15.963	2439	2440	2445	rBV2	264	305	0.04%	0.005%
99	16.109	2463	2464	2467	rBV2	627	365	0.05%	0.006%
100	16.767	2570	2572	2575	rBV3	319	338	0.04%	0.006%




Sum of corrected areas: 5924190

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026069.D
Acq On : 27 Dec 2021 18:04
Operator : JC/MD
Sample : M5150-29
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

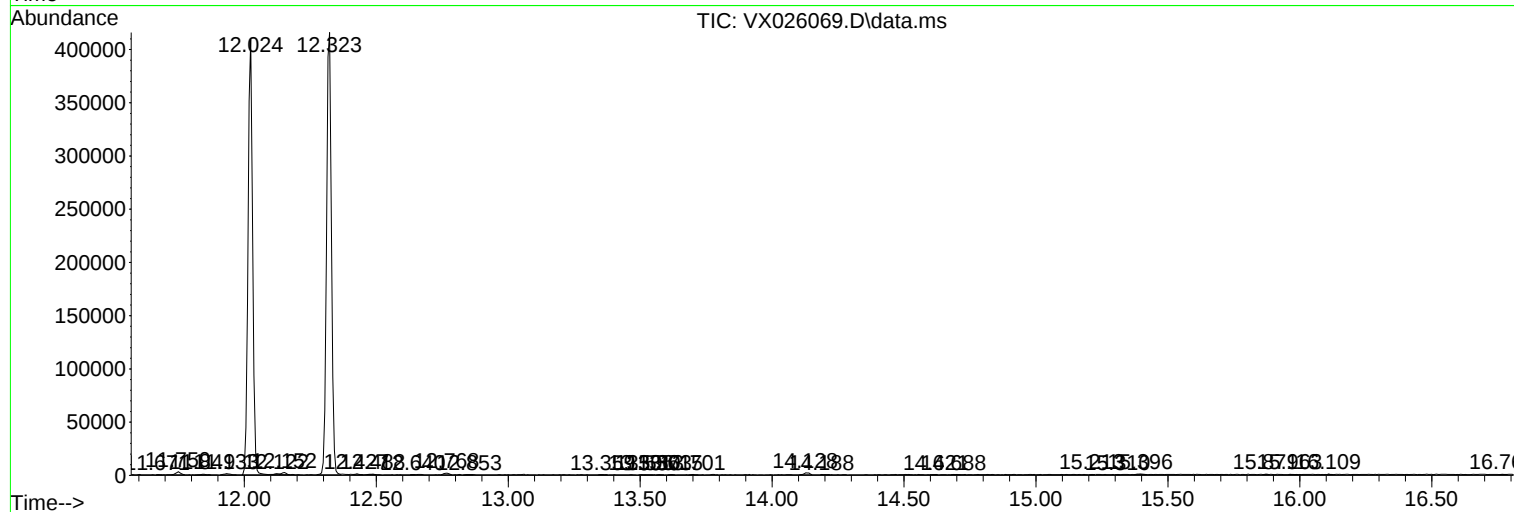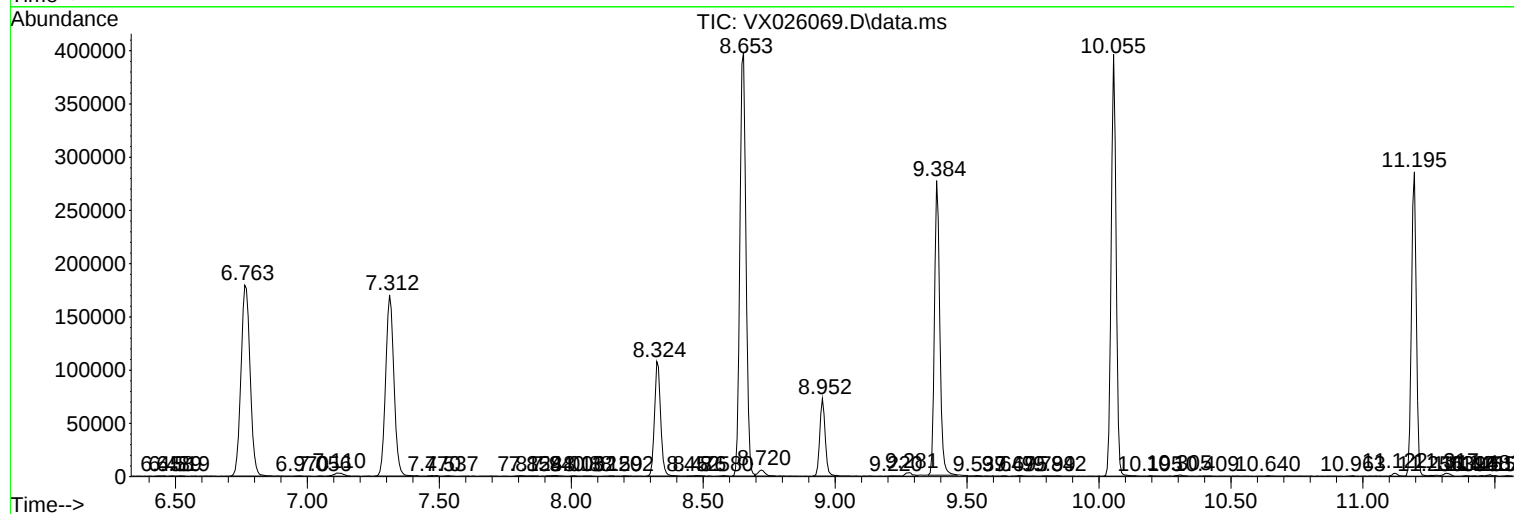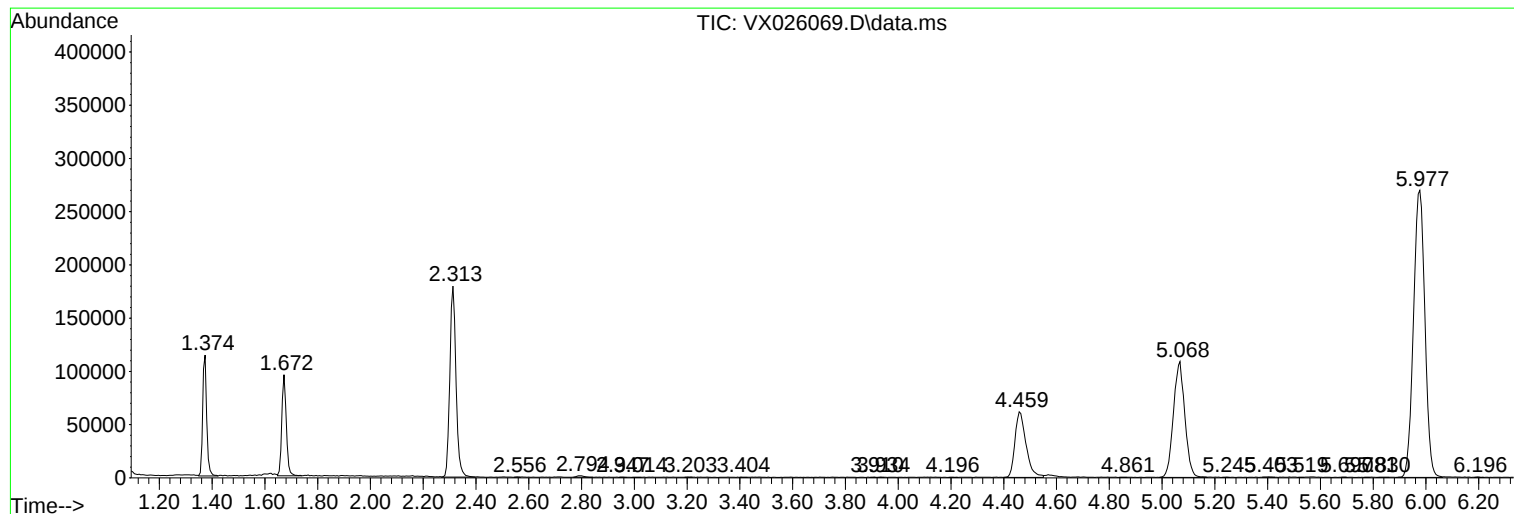

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026069.D
Acq On : 27 Dec 2021 18:04
Operator : JC/MD
Sample : M5150-29
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026069.D
Acq On : 27 Dec 2021 18:04
Operator : JC/MD
Sample : M5150-29
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc