

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026076.D
 Acq On : 27 Dec 2021 21:31
 Operator : JC/MD
 Sample : VX1227WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK663

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026076.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.197	16	18	20	rBV2	1373	1746	0.21%	0.028%
2	1.227	21	23	25	rVV2	785	829	0.10%	0.013%
3	1.374	43	47	55	rVB	116445	124613	14.96%	1.981%
4	1.526	70	72	74	rBV2	883	876	0.11%	0.014%
5	1.612	80	86	87	rBV4	2574	3645	0.44%	0.058%
6	1.673	91	96	105	rVB	96857	114617	13.76%	1.822%
7	2.014	149	152	155	rVB3	844	1037	0.12%	0.016%
8	2.124	166	170	172	rBV	590	827	0.10%	0.013%
9	2.209	182	184	187	rVB3	1027	895	0.11%	0.014%
10	2.313	192	201	214	rBV	185926	302306	36.30%	4.806%
11	2.520	230	235	237	rBV2	1521	1801	0.22%	0.029%
12	2.721	264	268	270	rVB2	700	824	0.10%	0.013%
13	2.794	276	280	285	rVB3	2694	4529	0.54%	0.072%
14	2.837	285	287	289	rBV	913	850	0.10%	0.014%
15	2.959	303	307	308	rBV2	838	1096	0.13%	0.017%
16	3.087	323	328	329	rVV3	815	1195	0.14%	0.019%
17	3.105	329	331	335	rVV3	798	1210	0.15%	0.019%
18	3.154	338	339	341	rBV	989	793	0.10%	0.013%
19	3.282	357	360	361	rBV	1028	761	0.09%	0.012%
20	3.556	403	405	409	rVV	785	890	0.11%	0.014%
21	3.660	419	422	424	rBV	804	979	0.12%	0.016%
22	3.703	428	429	431	rBV	1096	841	0.10%	0.013%
23	3.983	473	475	478	rVB	931	913	0.11%	0.015%
24	4.111	495	496	500	rVB	1127	989	0.12%	0.016%
25	4.178	504	507	509	rBV	1116	1320	0.16%	0.021%
26	4.209	509	512	514	rVB2	1146	1306	0.16%	0.021%
27	4.459	544	553	566	rBV	65368	190899	22.92%	3.035%
28	4.812	609	611	613	rBV	973	864	0.10%	0.014%
29	4.855	615	618	621	rBV	1096	1616	0.19%	0.026%
30	5.062	639	652	667	rBV	110580	343319	41.23%	5.458%
31	5.318	690	694	698	rVB	1006	1888	0.23%	0.030%
32	5.465	716	718	720	rBV	834	821	0.10%	0.013%
33	5.489	720	722	725	rVB	1041	871	0.10%	0.014%
34	5.599	739	740	745	rBV2	1090	1457	0.17%	0.023%
35	5.806	772	774	777	rVB	876	921	0.11%	0.015%
36	5.977	789	802	816	rBV2	280251	832771	100.00%	13.240%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026076.D
 Acq On : 27 Dec 2021 21:31
 Operator : JC/MD
 Sample : VX1227WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK663

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	6.763	923	931	943	rBV	195799	473123	56.81%	7.522%
38	7.037	974	976	979	rBV	968	1075	0.13%	0.017%
39	7.117	983	989	996	rBV7	4018	10633	1.28%	0.169%
40	7.312	1013	1021	1031	rBV	173115	382099	45.88%	6.075%
41	7.409	1036	1037	1040	rVB	1116	1033	0.12%	0.016%
42	7.598	1065	1068	1069	rBV	1394	1372	0.16%	0.022%
43	7.757	1091	1094	1096	rBV	783	1149	0.14%	0.018%
44	7.806	1099	1102	1109	rVB4	836	1771	0.21%	0.028%
45	7.970	1127	1129	1133	rVB	875	954	0.11%	0.015%
46	8.147	1155	1158	1159	rBV	950	1162	0.14%	0.018%
47	8.324	1181	1187	1199	rBV	119058	194662	23.38%	3.095%
48	8.653	1234	1241	1248	rBV	412747	643876	77.32%	10.237%
49	8.720	1249	1252	1259	rVB3	6628	10901	1.31%	0.173%
50	8.836	1269	1271	1274	rVB	1170	1061	0.13%	0.017%
51	8.952	1285	1290	1299	rBV	83379	118159	14.19%	1.879%
52	9.037	1301	1304	1307	rVB	1478	1817	0.22%	0.029%
53	9.068	1307	1309	1312	rBV	964	1050	0.13%	0.017%
54	9.275	1340	1343	1349	rVV3	3585	5558	0.67%	0.088%
55	9.385	1356	1361	1371	rBV	281147	397692	47.76%	6.323%
56	9.500	1379	1380	1383	rBV2	739	766	0.09%	0.012%
57	9.653	1403	1405	1408	rVB	1083	817	0.10%	0.013%
58	9.732	1417	1418	1421	rBV	1703	1489	0.18%	0.024%
59	9.842	1432	1436	1438	rBV	802	1103	0.13%	0.018%
60	9.952	1451	1454	1457	rVB	1189	1722	0.21%	0.027%
61	10.006	1459	1463	1465	rVV	1015	1346	0.16%	0.021%
62	10.055	1465	1471	1479	rVV	422473	565724	67.93%	8.994%
63	10.201	1491	1495	1497	rBV2	968	1076	0.13%	0.017%
64	10.232	1499	1500	1504	rBV2	704	872	0.10%	0.014%
65	10.409	1527	1529	1533	rBV2	823	775	0.09%	0.012%
66	10.653	1567	1569	1572	rVV3	1212	1505	0.18%	0.024%
67	11.122	1641	1646	1650	rBV3	2865	3952	0.47%	0.063%
68	11.195	1652	1658	1667	rVV	297891	381751	45.84%	6.069%
69	11.274	1669	1671	1672	rVV2	1103	775	0.09%	0.012%
70	11.317	1676	1678	1683	rVV3	3092	5119	0.61%	0.081%
71	11.537	1712	1714	1718	rVB2	682	986	0.12%	0.016%
72	11.750	1746	1749	1753	rVB2	3581	4719	0.57%	0.075%
73	11.969	1784	1785	1789	rBV2	898	1131	0.14%	0.018%
74	12.024	1789	1794	1800	rBV	448138	545135	65.46%	8.667%
75	12.122	1809	1810	1812	rBV2	996	800	0.10%	0.013%
76	12.158	1812	1816	1820	rVB3	2217	2831	0.34%	0.045%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026076.D
 Acq On : 27 Dec 2021 21:31
 Operator : JC/MD
 Sample : VX1227WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK663

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	12.323	1837	1843	1848	rBV	428012	539599	64.80%	8.579%
78	12.427	1859	1860	1863	rVB2	1230	930	0.11%	0.015%
79	12.475	1866	1868	1871	rVB	1216	1226	0.15%	0.019%
80	12.762	1913	1915	1921	rVB3	2314	3258	0.39%	0.052%
81	12.823	1924	1925	1928	rBV2	789	831	0.10%	0.013%
82	12.908	1938	1939	1941	rBV	916	797	0.10%	0.013%
83	13.122	1972	1974	1977	rVB3	1059	1019	0.12%	0.016%
84	13.591	2049	2051	2056	rVB2	1379	1583	0.19%	0.025%
85	13.780	2079	2082	2086	rVB	1473	1678	0.20%	0.027%
86	13.957	2109	2111	2114	rBV3	1110	1469	0.18%	0.023%
87	14.042	2121	2125	2127	rBV2	886	889	0.11%	0.014%
88	14.073	2127	2130	2132	rBV2	768	842	0.10%	0.013%
89	14.134	2136	2140	2143	rBV	2728	3004	0.36%	0.048%
90	14.652	2224	2225	2229	rBV2	675	1076	0.13%	0.017%
91	15.127	2300	2303	2305	rBV2	911	1055	0.13%	0.017%
92	15.152	2305	2307	2310	rVV2	906	906	0.11%	0.014%
93	15.768	2403	2408	2410	rVB	1368	1833	0.22%	0.029%
94	15.798	2410	2413	2415	rBV	716	925	0.11%	0.015%
95	15.822	2415	2417	2423	rVB	793	896	0.11%	0.014%
96	16.243	2483	2486	2487	rVB	1016	899	0.11%	0.014%
97	16.267	2487	2490	2493	rBV2	797	1525	0.18%	0.024%
98	16.310	2495	2497	2499	rBV	1031	821	0.10%	0.013%
99	16.591	2542	2543	2546	rBV	903	1099	0.13%	0.017%
100	16.700	2560	2561	2563	rBV2	1013	934	0.11%	0.015%


Sum of corrected areas: 6289750

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026076.D
Acq On : 27 Dec 2021 21:31
Operator : JC/MD
Sample : VX1227WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK663

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

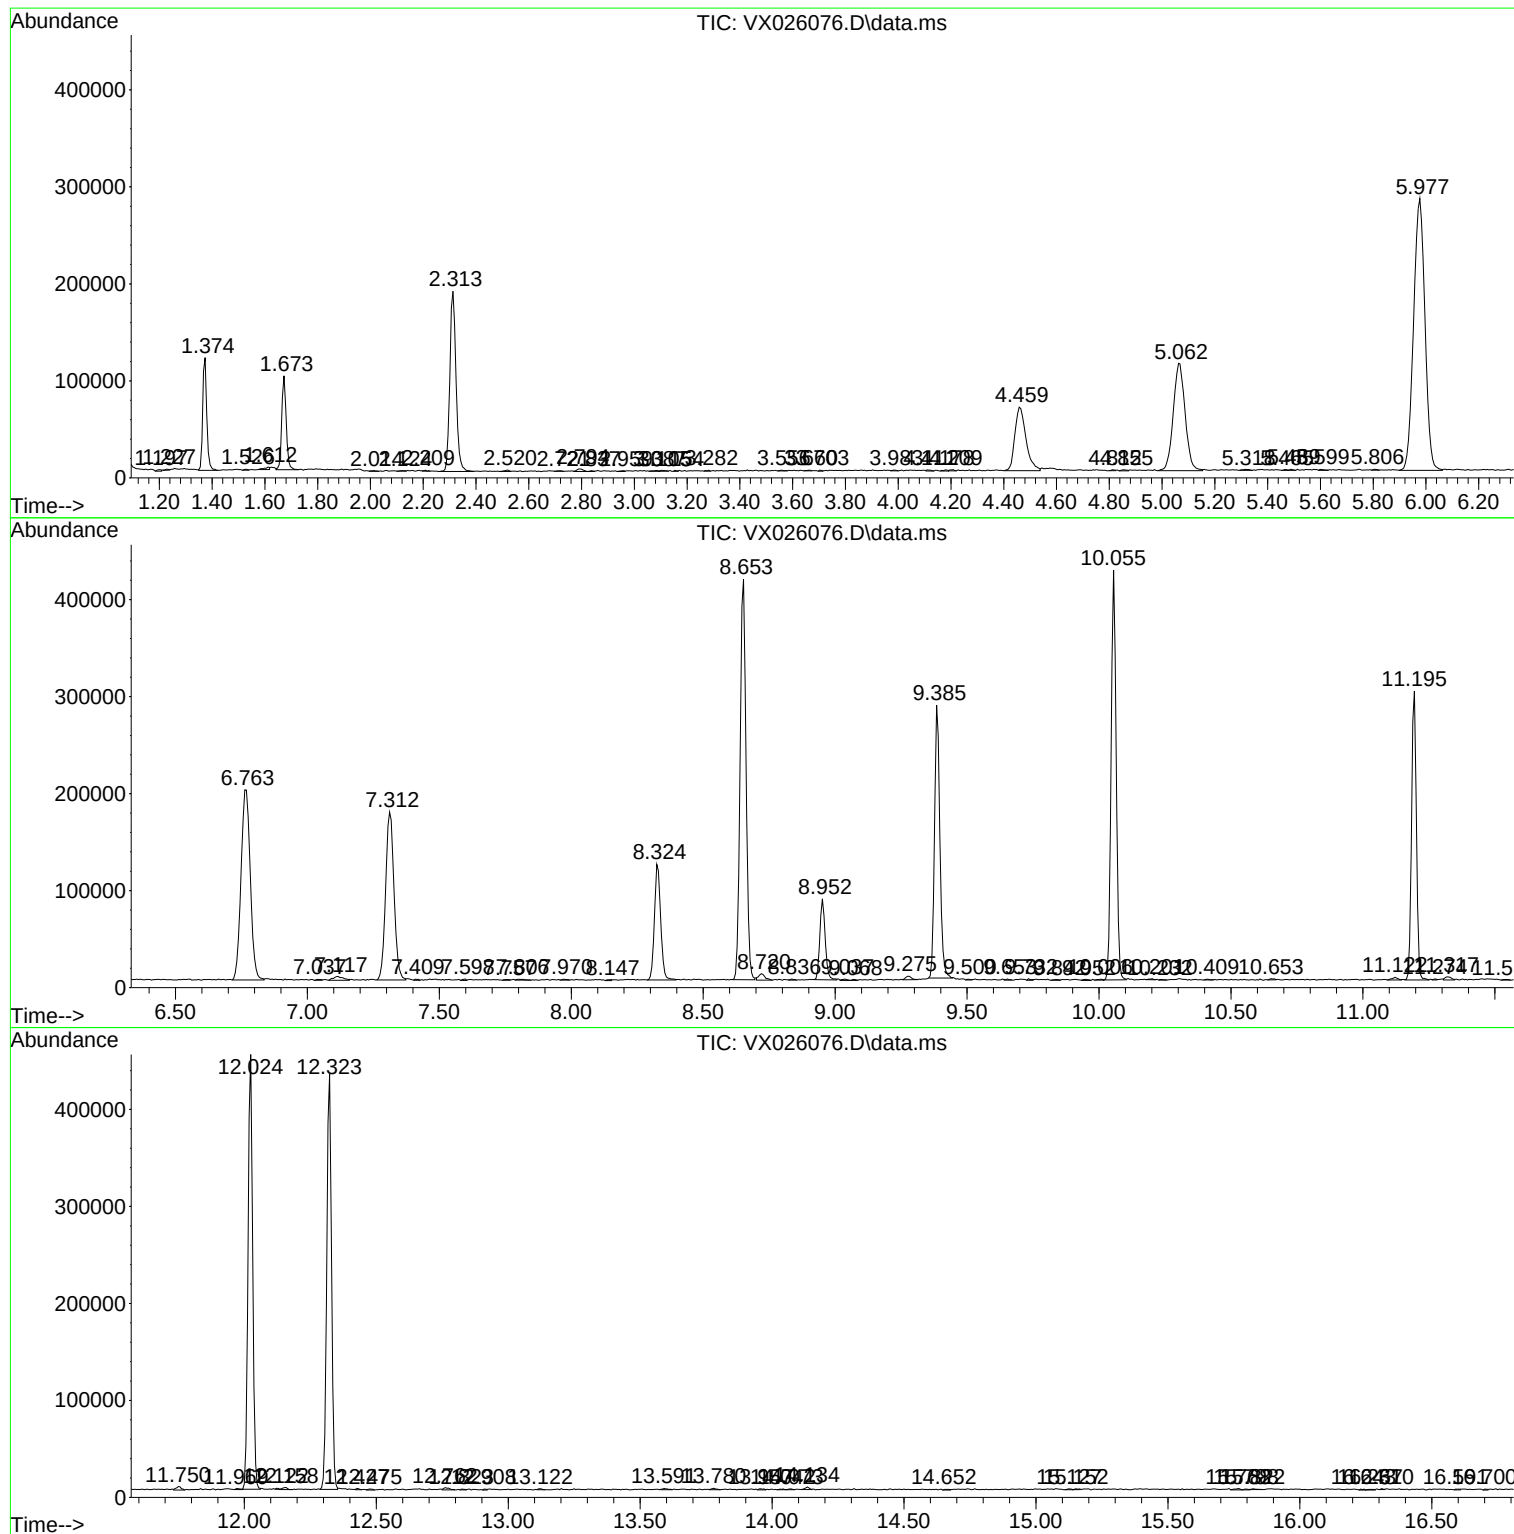

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026076.D
Acq On : 27 Dec 2021 21:31
Operator : JC/MD
Sample : VX1227WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK663

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026076.D
Acq On : 27 Dec 2021 21:31
Operator : JC/MD
Sample : VX1227WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK663

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc