
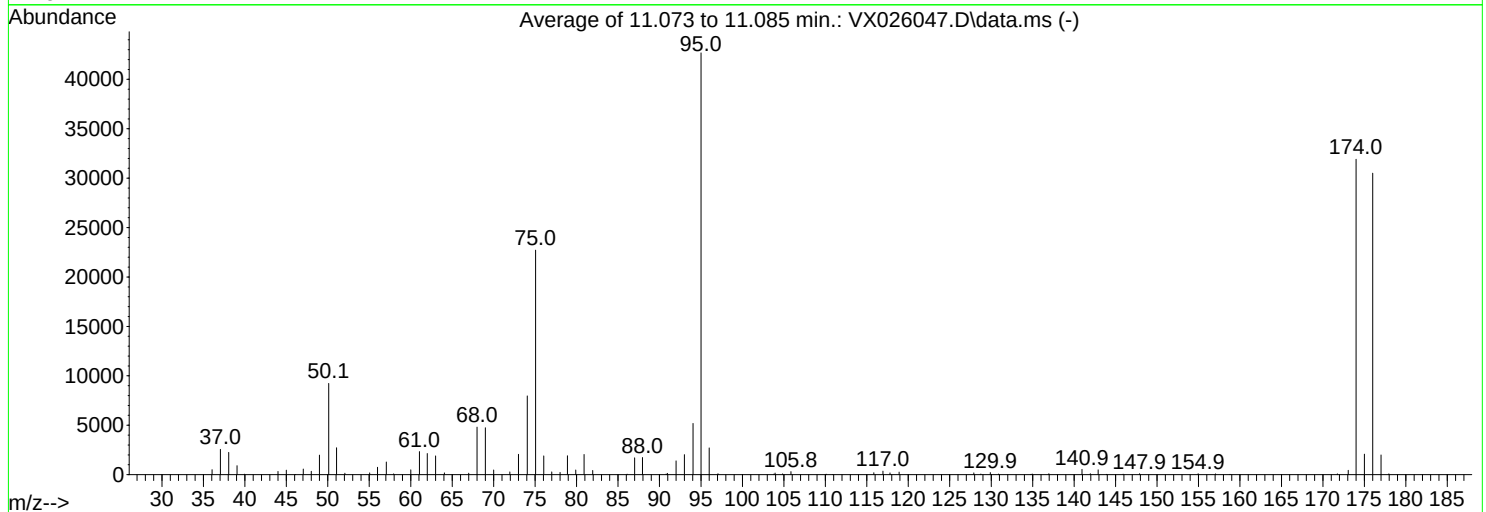


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026047.D
 Acq On : 27 Dec 2021 08:56
 Operator : JC/MD
 Sample : BFB631
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB631

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis
 Last Update : Tue Dec 28 02:17:03 2021

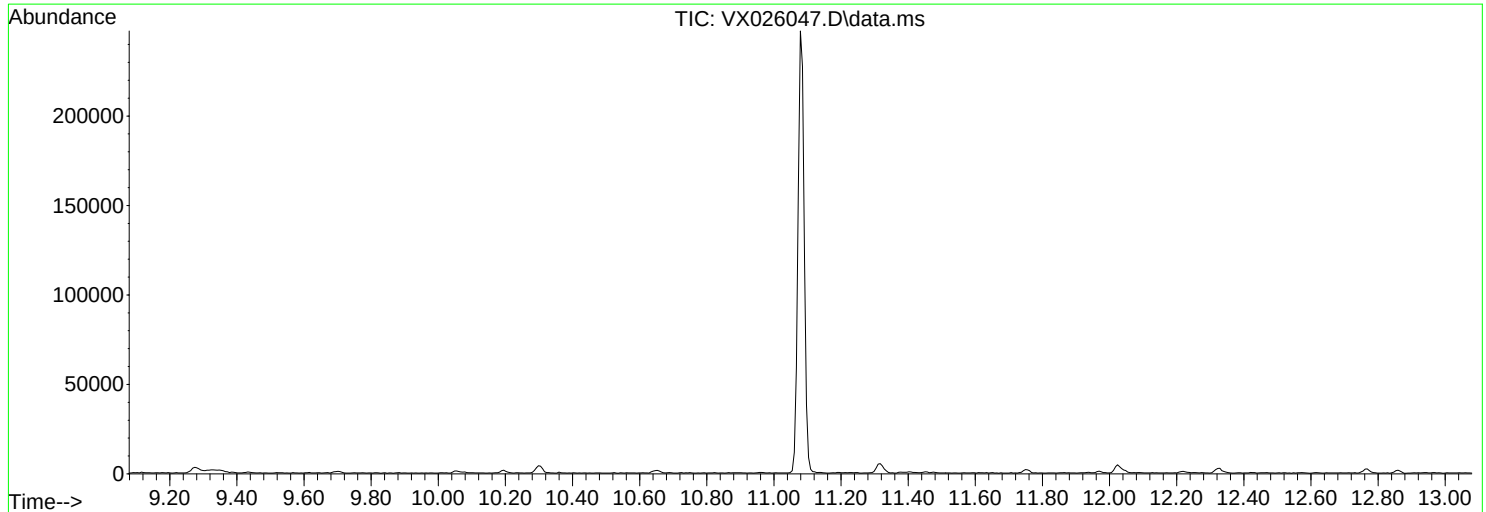

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	9237	PASS
75	95	30	80	53.2	22717	PASS
95	95	100	100	100.0	42683	PASS
96	95	5	9	6.3	2701	PASS
173	174	0.00	2	1.3	430	PASS
174	95	50	120	74.8	31909	PASS
175	174	5	9	6.5	2081	PASS
176	174	95	101	95.6	30509	PASS
177	176	5	9	6.6	1999	PASS

m/z	Abundance
40.00	283.0
44.00	236.0

Instrument :
MSVOA_X
ClientSampleId :
BFB631

m/z	Abundance
36.00	361.0
37.10	2241.0
38.10	1899.0
39.10	1005.0
40.00	348.0
44.00	622.0
45.00	399.0
47.10	493.0
48.10	262.0
49.00	1623.0
50.10	8185.0
51.00	2442.0
52.00	174.0
55.10	162.0
56.00	587.0
57.00	995.0
58.00	92.0
60.00	356.0
61.00	1764.0
62.00	1851.0
63.00	1509.0
64.10	196.0
67.10	77.0
68.00	4137.0
69.00	4049.0
70.00	495.0
71.90	214.0
73.00	1490.0
74.10	6039.0
75.00	18328.0
76.00	1498.0
77.10	237.0
78.00	167.0
78.90	1577.0
79.90	364.0
80.90	1653.0
82.00	311.0
87.00	1079.0
87.90	1291.0
90.80	180.0
92.00	1158.0
93.00	1405.0
94.10	3997.0
95.00	32448.0
96.00	2052.0
97.10	58.0
103.80	182.0
104.90	71.0
105.80	261.0
116.00	105.0
116.90	301.0
117.80	118.0
118.90	221.0
128.00	109.0
128.70	65.0
129.90	146.0
134.80	77.0
137.00	77.0
141.00	302.0
142.00	90.0
142.80	423.0
154.90	63.0
171.80	64.0
173.10	298.0
174.00	20248.0
175.00	1457.0
176.00	20032.0
177.00	1338.0
177.90	63.0

Instrument :
MSVOA_X
ClientSampleId :
BFB631

m/z	Abundance
36.10	680.0
37.00	3217.0
38.10	2477.0
39.00	1017.0
39.90	352.0
43.90	586.0
45.00	488.0
46.10	75.0
47.10	611.0
47.90	431.0
49.00	2314.0
50.10	10667.0
51.10	3055.0
52.00	140.0
54.90	237.0
56.00	855.0
57.10	1634.0
60.00	661.0
61.00	3034.0
62.00	2576.0
63.00	2409.0
64.10	157.0
66.90	199.0
68.00	5563.0
69.00	5278.0
70.00	527.0
72.00	364.0
73.00	2539.0
74.00	9518.0
75.00	27168.0
76.10	2300.0
77.00	308.0
78.10	234.0
78.90	2305.0
79.90	507.0
80.90	2315.0
81.90	535.0
86.10	107.0
87.00	1955.0
88.00	2264.0
91.00	242.0
92.00	1617.0
93.00	2581.0
94.00	5889.0
95.00	50272.0
96.00	3251.0
97.00	102.0
104.00	229.0
104.80	82.0
105.80	304.0
110.10	56.0
110.90	71.0
115.80	285.0
116.90	386.0
117.80	213.0
118.90	302.0
128.00	150.0
128.80	80.0
129.90	242.0
130.90	91.0
135.00	99.0
136.90	144.0
140.90	697.0
142.00	70.0
142.90	510.0
143.90	56.0
146.00	81.0
147.90	139.0
154.90	101.0
157.10	80.0
171.70	99.0
173.00	400.0
174.00	37200.0
175.00	2384.0
176.00	35104.0
177.00	2201.0
177.90	61.0

Instrument :
MSVOA_X
ClientSampleId :
BFB631

m/z	Abundance
36.00	446.0
37.10	2237.0
38.00	2391.0
39.10	711.0
40.00	302.0
44.10	482.0
45.00	495.0
47.00	604.0
48.00	324.0
49.00	1986.0
50.10	8859.0
51.10	2686.0
52.10	115.0
55.10	158.0
56.00	779.0
57.00	1233.0
57.90	134.0
60.00	439.0
61.10	2200.0
62.00	1972.0
63.00	1747.0
63.90	180.0
67.10	146.0
68.00	4719.0
69.00	4892.0
70.00	408.0
71.90	227.0
73.00	2126.0
74.00	8350.0
75.10	22656.0
76.00	1905.0
76.90	286.0
77.90	267.0
78.90	1876.0
79.90	516.0
80.90	2162.0
81.90	439.0
86.10	59.0
87.00	2061.0
88.00	1626.0
90.90	165.0
92.00	1387.0
93.00	2076.0
94.10	5643.0
95.00	45328.0
96.00	2800.0
97.00	123.0
103.90	265.0
104.90	98.0
105.90	355.0
110.10	94.0
115.90	204.0
117.00	369.0
117.80	203.0
118.90	262.0
127.80	257.0
128.70	69.0
129.90	230.0
130.90	91.0
134.90	114.0
136.90	78.0
140.90	597.0
141.90	150.0
143.00	508.0
143.90	63.0
145.80	79.0
147.90	141.0
155.00	145.0
157.00	144.0
158.80	81.0
171.70	98.0
173.00	591.0
174.00	38280.0
175.00	2403.0
176.00	36392.0
177.00	2457.0
178.00	99.0

Instrument :
MSVOA_X
ClientSampleId :
BFB631