

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122722\
 Data File : VX033567.D
 Acq On : 27 Dec 2022 15:34
 Operator : JC/MD
 Sample : VIBLK604
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK604

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122722WMA.M
 Title : VOC Analysis

Signal : TIC: VX033567.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	11	13	18	rVB2	1685	1977	0.28%	0.037%
2	1.294	32	34	38	rVB3	749	917	0.13%	0.017%
3	1.368	42	46	64	rVV	63534	84256	11.97%	1.563%
4	1.672	92	96	111	rVB	51977	74857	10.63%	1.389%
5	1.886	129	131	136	rVB	1552	2280	0.32%	0.042%
6	2.075	160	162	166	rBV2	307	265	0.04%	0.005%
7	2.142	172	173	174	rBV	410	195	0.03%	0.004%
8	2.306	194	200	210	rVB	115820	184116	26.15%	3.416%
9	2.514	229	234	242	rBV	4686	7429	1.06%	0.138%
10	2.617	249	251	254	rBV	101	121	0.02%	0.002%
11	2.709	262	266	271	rVV2	446	640	0.09%	0.012%
12	2.794	275	280	289	rBB2	1812	3519	0.50%	0.065%
13	2.867	289	292	293	rBV2	231	214	0.03%	0.004%
14	2.947	296	305	311	rVB2	1859	3898	0.55%	0.072%
15	3.105	324	331	339	rVB5	2230	5442	0.77%	0.101%
16	3.178	341	343	347	rVB	131	184	0.03%	0.003%
17	3.270	356	358	361	rBV	114	171	0.02%	0.003%
18	3.611	410	414	419	rBB2	610	1216	0.17%	0.023%
19	3.672	420	424	427	rBV	169	237	0.03%	0.004%
20	3.794	442	444	448	rVV	155	153	0.02%	0.003%
21	4.081	487	491	493	rBV	181	236	0.03%	0.004%
22	4.135	497	500	503	rBV	109	188	0.03%	0.003%
23	4.239	515	517	522	rBV	204	364	0.05%	0.007%
24	4.300	525	527	529	rVB	151	133	0.02%	0.002%
25	4.465	545	554	567	rBV	40203	123282	17.51%	2.287%
26	4.702	590	593	595	rBV3	150	181	0.03%	0.003%
27	4.904	621	626	632	rBV4	883	2088	0.30%	0.039%
28	5.062	638	652	670	rBV	92776	294135	41.77%	5.457%
29	5.214	675	677	683	rVB2	183	253	0.04%	0.005%
30	5.330	693	696	697	rBV2	135	125	0.02%	0.002%
31	5.391	700	706	712	rVB4	1003	2439	0.35%	0.045%
32	5.464	713	718	727	rVB5	1649	4538	0.64%	0.084%
33	5.550	727	732	733	rBV3	471	679	0.10%	0.013%
34	5.672	746	752	762	rVB3	1023	2958	0.42%	0.055%
35	5.812	773	775	777	rVB	196	153	0.02%	0.003%
36	5.842	777	780	783	rBV	156	255	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122722\
 Data File : VX033567.D
 Acq On : 27 Dec 2022 15:34
 Operator : JC/MD
 Sample : VIBLK604
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK604

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122722WMA.M
 Title : VOC Analysis

37	5.970	789	801	818	rBV2	237727	704150	100.00%	13.064%
38	6.269	848	850	852	rBV	127	137	0.02%	0.003%
39	6.592	900	903	907	rBV2	140	257	0.04%	0.005%
40	6.659	910	914	917	rBV	144	243	0.03%	0.005%
41	6.763	921	931	946	rBV	186115	435811	61.89%	8.086%
42	7.123	983	990	999	rVB5	3244	8402	1.19%	0.156%
43	7.312	1011	1021	1029	rBV	140983	307940	43.73%	5.713%
44	7.482	1047	1049	1052	rVB2	289	248	0.04%	0.005%
45	7.598	1066	1068	1070	rBV	109	127	0.02%	0.002%
46	7.641	1073	1075	1077	rBV	123	113	0.02%	0.002%
47	7.824	1099	1105	1111	rBV2	1050	1870	0.27%	0.035%
48	7.940	1119	1124	1132	rVB3	1066	2143	0.30%	0.040%
49	8.153	1157	1159	1164	rVB2	138	179	0.03%	0.003%
50	8.324	1181	1187	1200	rBV	100723	166024	23.58%	3.080%
51	8.440	1205	1206	1207	rBV	228	131	0.02%	0.002%
52	8.482	1210	1213	1219	rVB3	755	1144	0.16%	0.021%
53	8.580	1224	1229	1234	rBV2	1829	2954	0.42%	0.055%
54	8.647	1234	1240	1248	rBV	383238	594075	84.37%	11.022%
55	8.720	1248	1252	1258	rVB	4068	6960	0.99%	0.129%
56	8.811	1265	1267	1269	rBV	224	204	0.03%	0.004%
57	8.952	1284	1290	1303	rVB	72089	108592	15.42%	2.015%
58	9.159	1320	1324	1329	rVB2	1735	2501	0.36%	0.046%
59	9.275	1338	1343	1348	rVB2	4959	6733	0.96%	0.125%
60	9.311	1348	1349	1353	rBV2	149	172	0.02%	0.003%
61	9.384	1356	1361	1380	rVV	195992	277306	39.38%	5.145%
62	9.525	1380	1384	1388	rVB4	1272	2005	0.28%	0.037%
63	9.616	1395	1399	1404	rVB	1295	1838	0.26%	0.034%
64	9.701	1409	1413	1417	rVV2	1319	1797	0.26%	0.033%
65	9.976	1457	1458	1460	rBV	145	120	0.02%	0.002%
66	10.055	1465	1471	1484	rVV	376119	505141	71.74%	9.372%
67	10.195	1490	1494	1502	rVB	5415	7599	1.08%	0.141%
68	10.305	1507	1512	1516	rBV2	5078	7144	1.01%	0.133%
69	10.433	1531	1533	1538	rBV2	114	178	0.03%	0.003%
70	10.592	1557	1559	1562	rVB	233	182	0.03%	0.003%
71	10.653	1562	1569	1576	rBV4	6757	13471	1.91%	0.250%
72	10.768	1586	1588	1590	rBV	160	179	0.03%	0.003%
73	10.799	1590	1593	1599	rVB2	1183	1651	0.23%	0.031%
74	10.963	1616	1620	1628	rVB	6224	7750	1.10%	0.144%
75	11.110	1642	1644	1645	rBV	141	117	0.02%	0.002%
76	11.189	1652	1657	1664	rBV	241263	323693	45.97%	6.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122722\
 Data File : VX033567.D
 Acq On : 27 Dec 2022 15:34
 Operator : JC/MD
 Sample : VIBLK604
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK604

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122722WMA.M
 Title : VOC Analysis

77	11.354	1682	1684	1685	rBV	163	104	0.01%	0.002%
78	11.427	1693	1696	1697	rBV	169	167	0.02%	0.003%
79	11.451	1697	1700	1708	rVB	6415	8073	1.15%	0.150%
80	11.707	1740	1742	1743	rBV	168	167	0.02%	0.003%
81	11.756	1745	1750	1755	rVB	6573	8014	1.14%	0.149%
82	11.854	1764	1766	1769	rBV	155	183	0.03%	0.003%
83	11.969	1781	1785	1789	rBV	7384	9422	1.34%	0.175%
84	12.024	1789	1794	1804	rVB	376368	485405	68.93%	9.006%
85	12.262	1832	1833	1837	rBV2	151	155	0.02%	0.003%
86	12.323	1837	1843	1853	rBV	384999	514812	73.11%	9.551%
87	12.652	1895	1897	1900	rVB	176	173	0.02%	0.003%
88	12.725	1907	1909	1911	rBV	114	108	0.02%	0.002%
89	12.817	1922	1924	1926	rBV	153	105	0.01%	0.002%
90	12.859	1929	1931	1932	rBV	197	116	0.02%	0.002%
91	12.945	1942	1945	1950	rVB2	728	981	0.14%	0.018%
92	13.116	1969	1973	1978	rVB	10637	12360	1.76%	0.229%
93	13.451	2027	2028	2031	rVB	127	126	0.02%	0.002%
94	13.591	2046	2051	2061	rVB	11832	14575	2.07%	0.270%
95	13.780	2077	2082	2088	rVB	10556	13868	1.97%	0.257%
96	13.963	2107	2112	2119	rVB	11513	14674	2.08%	0.272%
97	14.121	2136	2138	2143	rVB2	236	317	0.05%	0.006%
98	14.225	2154	2155	2158	rBV2	201	194	0.03%	0.004%
99	14.438	2188	2190	2191	rBV2	237	176	0.02%	0.003%
100	14.652	2222	2225	2226	rBV2	245	272	0.04%	0.005%




Sum of corrected areas: 5389922

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122722\
Data File : VX033567.D
Acq On : 27 Dec 2022 15:34
Operator : JC/MD
Sample : VIBLK604
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK604

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

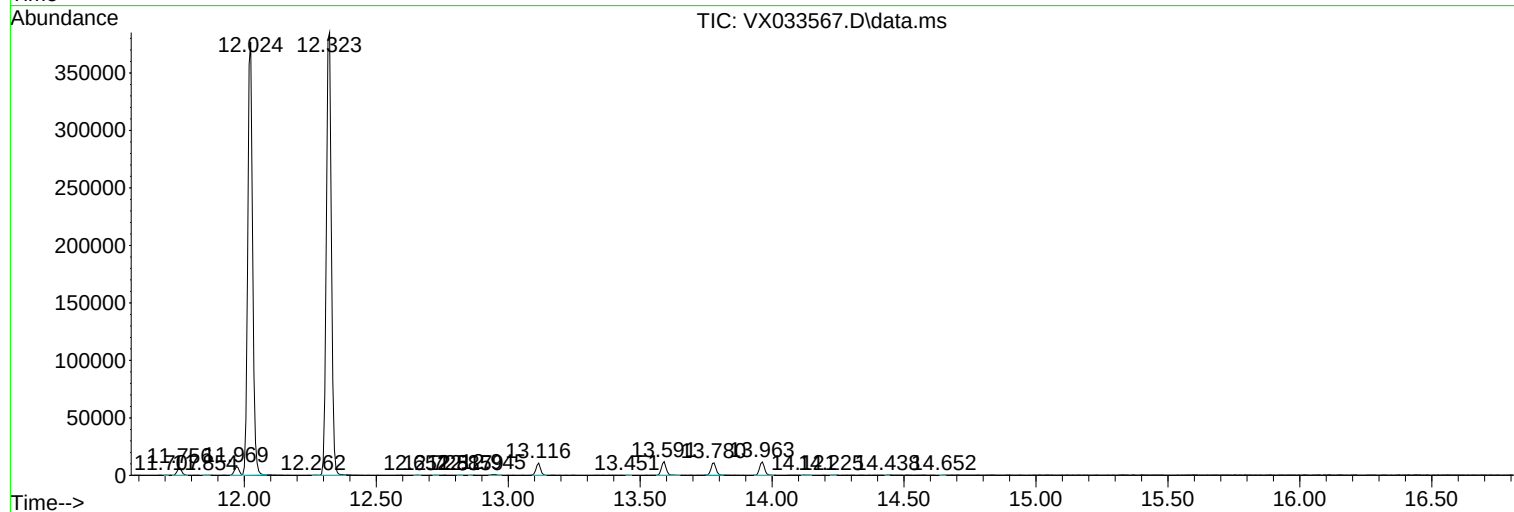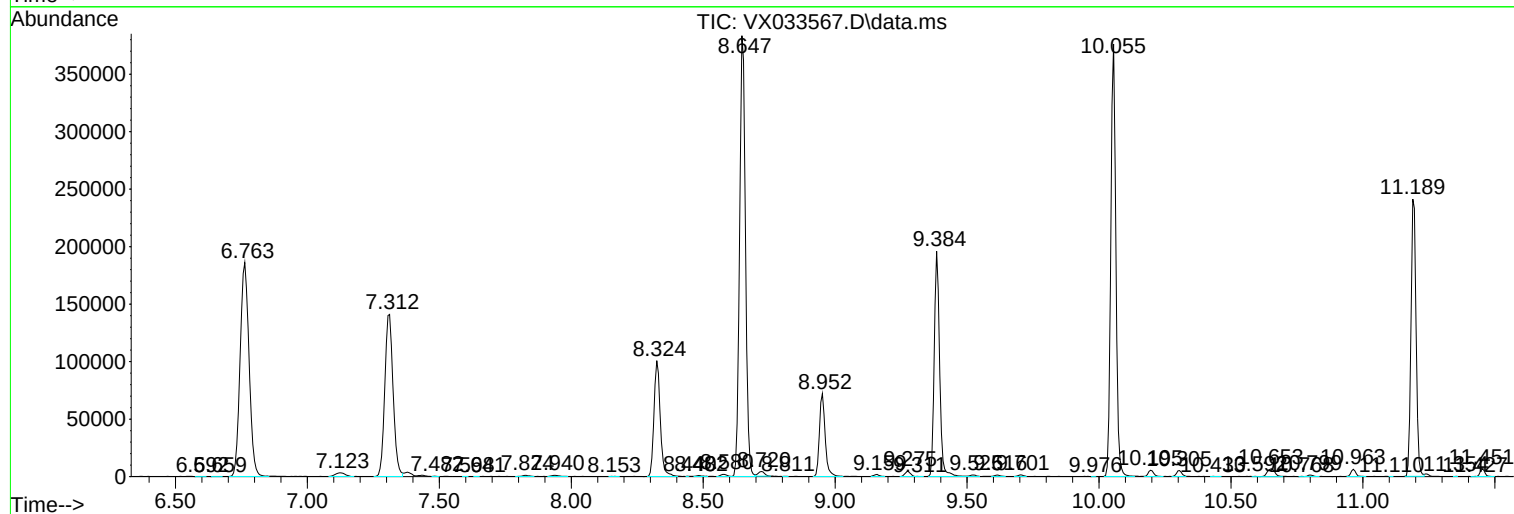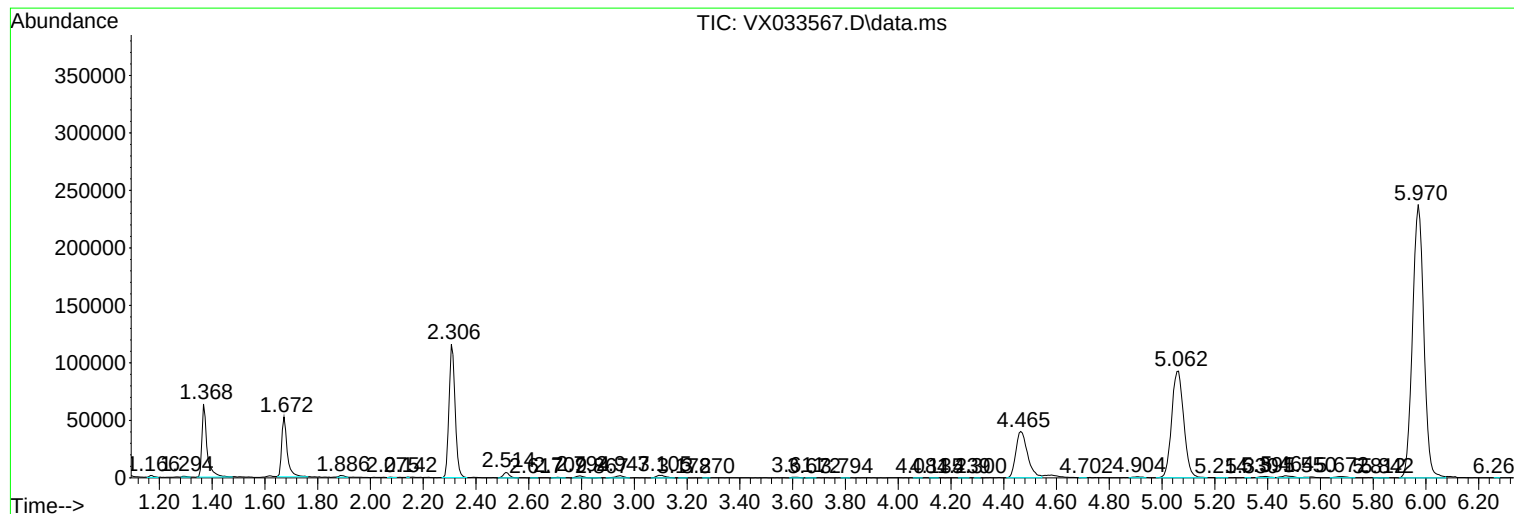

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122722\
Data File : VX033567.D
Acq On : 27 Dec 2022 15:34
Operator : JC/MD
Sample : VIBLK604
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK604

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122722\
Data File : VX033567.D
Acq On : 27 Dec 2022 15:34
Operator : JC/MD
Sample : VIBLK604
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK604

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc