
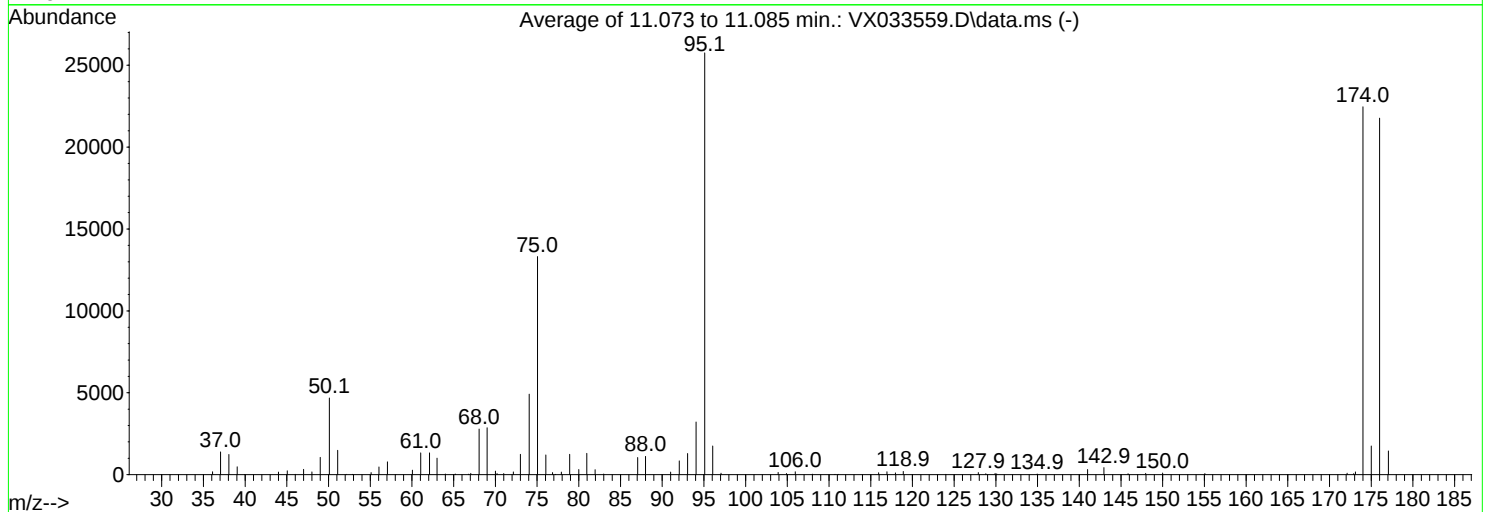


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122722\
Data File : VX033559.D
Acq On : 27 Dec 2022 09:19
Operator : JC/MD
Sample : BFB603
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB603

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122722WMA.M
Title : VOC Analysis
Last Update : Wed Dec 28 01:59:02 2022

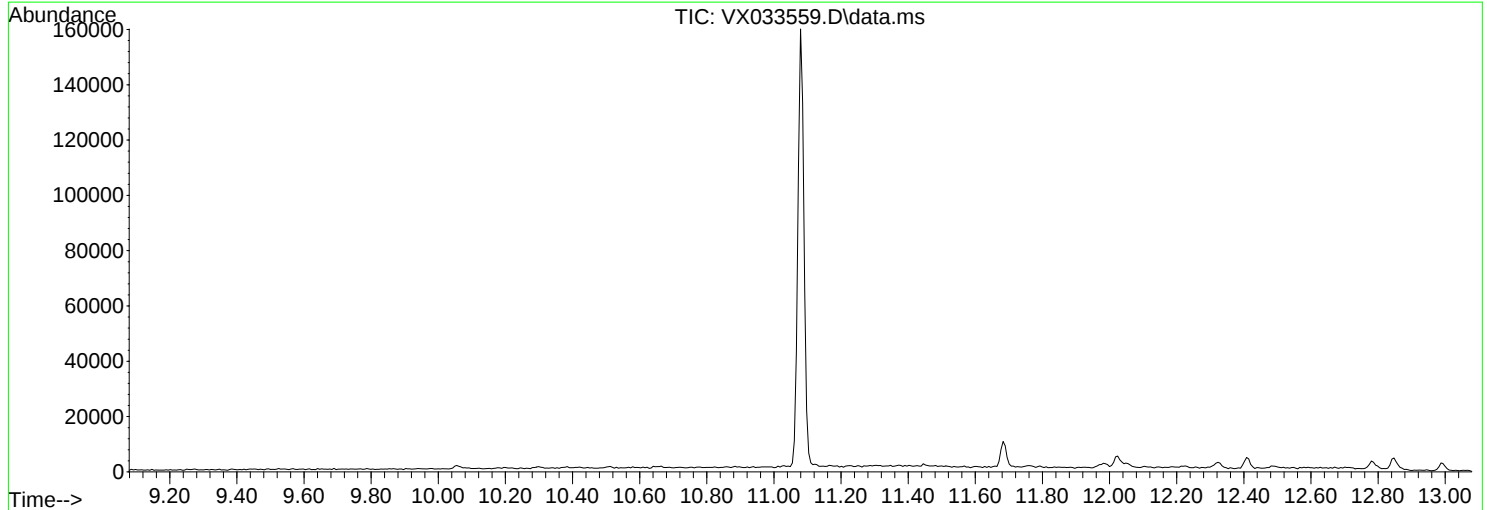

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	4678	PASS
75	95	30	80	51.7	13315	PASS
95	95	100	100	100.0	25757	PASS
96	95	5	9	6.8	1749	PASS
173	174	0.00	2	0.7	168	PASS
174	95	50	120	87.2	22466	PASS
175	174	5	9	7.8	1754	PASS
176	174	95	101	96.9	21766	PASS
177	176	5	9	6.7	1448	PASS

m/z	Abundance
39.10	147.0
39.90	89.0
41.10	373.0
41.90	54.0
43.00	214.0
44.00	163.0
45.20	60.0
55.00	71.0
56.20	129.0
57.00	339.0
58.00	86.0
64.10	57.0
69.10	50.0
71.10	131.0
89.00	97.0

Instrument :
MSVOA_X
ClientSampleId :
BFB603

m/z	Abundance
36.10	159.0
37.10	1289.0
38.00	1154.0
39.10	574.0
40.10	124.0
41.00	285.0
42.10	64.0
43.10	242.0
44.00	281.0
45.10	271.0
46.00	52.0
47.00	367.0
48.00	159.0
49.00	1006.0
50.10	4222.0
51.10	1441.0
55.20	188.0
56.10	624.0
57.10	1086.0
58.10	144.0
60.00	204.0
61.00	1043.0
62.10	1113.0
63.00	891.0
63.90	66.0
65.20	54.0
67.00	98.0
68.00	2535.0
69.00	2851.0
70.00	260.0
71.00	185.0
72.10	107.0
73.00	1060.0
74.00	4235.0
75.10	11975.0
76.10	1044.0
76.80	97.0
77.90	203.0
78.90	1111.0
80.00	280.0
80.90	1202.0
81.90	287.0
87.10	900.0
88.00	1159.0
89.30	53.0
91.10	92.0
92.00	746.0
93.10	988.0
94.10	2827.0
95.10	21600.0
96.10	1664.0
97.10	84.0
103.90	89.0
105.00	61.0
106.00	134.0
108.00	74.0
110.70	50.0
116.00	115.0
116.90	157.0
117.90	74.0
118.90	194.0
127.90	98.0
129.90	120.0
141.00	147.0
142.90	287.0
148.00	52.0
150.00	89.0
172.00	55.0
172.90	174.0
174.00	15863.0
175.00	1410.0
176.00	15385.0
177.10	1002.0

Instrument :
MSVOA_X
ClientSampleId :
BFB603

m/z	Abundance
36.10	253.0
37.10	1561.0
38.10	1437.0
39.10	805.0
40.00	105.0
41.00	288.0
43.10	168.0
44.10	408.0
45.00	321.0
46.90	379.0
48.00	225.0
49.00	1287.0
50.10	5589.0
51.10	1812.0
55.10	214.0
56.00	757.0
57.10	1248.0
58.10	97.0
60.10	363.0
61.00	1674.0
62.10	1516.0
63.00	1280.0
64.00	140.0
65.20	54.0
67.10	143.0
68.00	3325.0
69.00	3368.0
70.00	394.0
71.00	200.0
72.20	217.0
73.00	1597.0
74.00	5847.0
75.10	15808.0
76.00	1484.0
76.90	181.0
77.90	186.0
78.90	1385.0
80.10	344.0
80.90	1554.0
82.00	330.0
83.00	58.0
87.10	1295.0
88.00	1278.0
89.10	97.0
91.00	210.0
92.00	1013.0
93.00	1587.0
94.00	3785.0
95.10	31224.0
96.00	2039.0
97.00	90.0
103.80	157.0
104.80	73.0
105.90	213.0
111.10	52.0
116.00	104.0
117.00	200.0
117.90	146.0
118.90	257.0
124.00	50.0
127.80	180.0
128.80	116.0
130.10	137.0
135.00	68.0
141.00	420.0
143.00	550.0
145.80	98.0
147.90	87.0
150.00	78.0
155.00	108.0
172.10	90.0
173.10	270.0
174.00	26464.0
175.00	2096.0
176.00	25384.0
177.00	1732.0

Instrument :
MSVOA_X
ClientSampleId :
BFB603

m/z	Abundance
36.10	116.0
37.00	1309.0
38.10	1092.0
39.00	502.0
40.10	65.0
41.10	284.0
43.10	227.0
44.00	268.0
45.00	287.0
47.10	221.0
48.00	114.0
49.00	876.0
50.10	4224.0
51.10	1194.0
52.10	51.0
52.90	53.0
55.10	184.0
56.10	410.0
57.10	1037.0
58.10	60.0
60.10	255.0
61.10	1274.0
62.10	1352.0
63.00	840.0
64.00	97.0
66.80	89.0
68.10	2506.0
69.00	2511.0
70.20	214.0
71.00	223.0
72.20	178.0
73.00	1081.0
74.10	4672.0
75.00	12162.0
76.00	1079.0
76.80	104.0
77.20	62.0
77.90	80.0
78.90	1229.0
79.90	325.0
81.00	1142.0
82.00	279.0
83.00	60.0
87.00	948.0
88.00	912.0
89.00	119.0
90.90	159.0
92.10	748.0
93.00	1291.0
94.10	3022.0
95.10	24448.0
96.10	1544.0
97.00	106.0
104.00	175.0
104.90	81.0
105.90	171.0
115.90	126.0
116.90	181.0
118.00	117.0
119.00	148.0
128.00	115.0
128.80	69.0
129.90	114.0
134.90	51.0
141.00	379.0
143.00	449.0
145.90	80.0
147.90	92.0
150.00	114.0
155.10	93.0
172.20	110.0
173.10	233.0
174.00	25072.0
175.00	1756.0
176.00	24528.0
177.00	1611.0

Instrument :
MSVOA_X
ClientSampleId :
BFB603