

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039487.D
 Acq On : 27 Dec 2023 11:19
 Operator : JC/MD
 Sample : VX1227WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK659

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.245	23	26	33	rBV2	2763	5839	0.69%	0.086%
2	1.367	42	46	57	rBV	88926	95571	11.27%	1.413%
3	1.666	91	95	113	rVB	62777	94959	11.20%	1.404%
4	2.306	194	200	210	rVB	167182	262485	30.96%	3.880%
5	2.459	224	225	227	rBV2	370	247	0.03%	0.004%
6	2.501	231	232	235	rBV3	304	285	0.03%	0.004%
7	2.574	243	244	246	rBV	315	221	0.03%	0.003%
8	2.678	259	261	262	rBV	258	165	0.02%	0.002%
9	2.782	276	278	282	rBV2	618	789	0.09%	0.012%
10	2.849	287	289	293	rBV	337	326	0.04%	0.005%
11	2.940	301	304	305	rBV2	639	733	0.09%	0.011%
12	3.111	331	332	335	rBV2	217	264	0.03%	0.004%
13	3.221	348	350	351	rBV	422	214	0.03%	0.003%
14	3.513	396	398	401	rBV2	198	231	0.03%	0.003%
15	3.635	416	418	419	rBV	234	166	0.02%	0.002%
16	3.934	465	467	470	rVB	293	332	0.04%	0.005%
17	3.964	470	472	474	rBV2	277	337	0.04%	0.005%
18	4.147	501	502	505	rVB	275	206	0.02%	0.003%
19	4.446	542	551	570	rBV	91167	262610	30.98%	3.882%
20	4.934	629	631	633	rBV	164	183	0.02%	0.003%
21	5.056	637	651	666	rBV	110071	340484	40.16%	5.033%
22	5.287	686	689	690	rVB2	248	187	0.02%	0.003%
23	5.373	699	703	704	rBV	663	655	0.08%	0.010%
24	5.964	789	800	818	rBV3	279852	847716	100.00%	12.531%
25	6.202	837	839	840	rVB	311	176	0.02%	0.003%
26	6.275	848	851	852	rVB	208	198	0.02%	0.003%
27	6.299	852	855	857	rBV2	414	409	0.05%	0.006%
28	6.348	861	863	866	rVV	330	301	0.04%	0.004%
29	6.385	868	869	872	rVB	247	182	0.02%	0.003%
30	6.464	881	882	884	rBV	451	236	0.03%	0.003%
31	6.604	902	905	907	rBV	169	195	0.02%	0.003%
32	6.757	920	930	946	rBV	227045	543857	64.16%	8.039%
33	7.001	968	970	973	rBV3	300	300	0.04%	0.004%
34	7.110	981	988	994	rBV6	1491	3090	0.36%	0.046%
35	7.177	997	999	1001	rVB2	170	158	0.02%	0.002%
36	7.220	1004	1006	1007	rBV2	232	170	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039487.D
 Acq On : 27 Dec 2023 11:19
 Operator : JC/MD
 Sample : VX1227WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK659

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.305	1011	1020	1033	rBV	178426	394539	46.54%	5.832%
38	7.476	1045	1048	1049	rBV3	383	393	0.05%	0.006%
39	7.622	1070	1072	1077	rVV	175	285	0.03%	0.004%
40	7.781	1096	1098	1100	rVB	240	186	0.02%	0.003%
41	7.805	1100	1102	1104	rBV2	182	219	0.03%	0.003%
42	7.945	1123	1125	1128	rBV3	409	399	0.05%	0.006%
43	8.262	1172	1177	1180	rBV2	644	783	0.09%	0.012%
44	8.323	1180	1187	1199	rBV	115191	194939	23.00%	2.882%
45	8.451	1206	1208	1210	rBV	310	162	0.02%	0.002%
46	8.647	1233	1240	1250	rBV	421093	651161	76.81%	9.625%
47	8.945	1284	1289	1301	rBV	83492	129088	15.23%	1.908%
48	9.098	1312	1314	1315	rBV2	270	240	0.03%	0.004%
49	9.232	1333	1336	1338	rBV	199	242	0.03%	0.004%
50	9.281	1340	1344	1347	rVB3	337	506	0.06%	0.007%
51	9.378	1355	1360	1378	rBV	410766	603624	71.21%	8.923%
52	9.701	1410	1413	1418	rVB3	795	1095	0.13%	0.016%
53	9.805	1429	1430	1434	rBV2	183	261	0.03%	0.004%
54	9.963	1453	1456	1458	rBV	253	239	0.03%	0.004%
55	10.000	1460	1462	1465	rBV	175	206	0.02%	0.003%
56	10.055	1465	1471	1486	rBV	461167	662444	78.14%	9.792%
57	10.256	1502	1504	1506	rVV	181	214	0.03%	0.003%
58	10.311	1509	1513	1516	rVB3	295	449	0.05%	0.007%
59	10.335	1516	1517	1524	rBV2	195	428	0.05%	0.006%
60	10.390	1524	1526	1527	rVB	222	159	0.02%	0.002%
61	10.482	1540	1541	1544	rVB	316	161	0.02%	0.002%
62	10.561	1552	1554	1556	rBV2	225	220	0.03%	0.003%
63	10.719	1577	1580	1582	rBV2	278	245	0.03%	0.004%
64	10.835	1596	1599	1601	rBV2	154	183	0.02%	0.003%
65	11.085	1636	1640	1649	rBV3	1844	3199	0.38%	0.047%
66	11.189	1652	1657	1666	rVV	348861	454115	53.57%	6.713%
67	11.347	1681	1683	1686	rBV	273	162	0.02%	0.002%
68	11.390	1688	1690	1692	rVB	224	169	0.02%	0.002%
69	11.652	1731	1733	1735	rVB2	221	184	0.02%	0.003%
70	11.762	1749	1751	1752	rVV2	419	226	0.03%	0.003%
71	11.975	1784	1786	1788	rBV2	436	396	0.05%	0.006%
72	12.024	1788	1794	1805	rBV	457550	610642	72.03%	9.026%
73	12.317	1837	1842	1851	rBV	444073	581145	68.55%	8.590%
74	12.573	1882	1884	1886	rBV2	141	166	0.02%	0.002%
75	12.768	1912	1916	1919	rBV2	199	297	0.04%	0.004%
76	12.951	1944	1946	1949	rBV2	157	181	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039487.D
 Acq On : 27 Dec 2023 11:19
 Operator : JC/MD
 Sample : VX1227WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK659

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.993	1952	1953	1957	rBV2	254	209	0.02%	0.003%
78	13.121	1973	1974	1976	rBV2	217	209	0.02%	0.003%
79	13.188	1983	1985	1989	rVB	280	209	0.02%	0.003%
80	13.432	2023	2025	2026	rBV	248	176	0.02%	0.003%
81	13.512	2036	2038	2041	rBV2	159	174	0.02%	0.003%
82	13.560	2044	2046	2048	rVB2	195	160	0.02%	0.002%
83	13.597	2048	2052	2055	rVB3	459	695	0.08%	0.010%
84	13.627	2055	2057	2058	rBV	214	185	0.02%	0.003%
85	13.713	2069	2071	2073	rBV2	200	201	0.02%	0.003%
86	13.786	2080	2083	2092	rVB3	502	1028	0.12%	0.015%
87	14.042	2123	2125	2129	rBV2	134	158	0.02%	0.002%
88	14.121	2135	2138	2140	rBV3	185	285	0.03%	0.004%
89	14.182	2147	2148	2151	rVB2	283	249	0.03%	0.004%
90	14.444	2189	2191	2193	rVB2	258	188	0.02%	0.003%
91	14.463	2193	2194	2196	rBV	263	206	0.02%	0.003%
92	14.536	2204	2206	2209	rVB2	269	224	0.03%	0.003%
93	14.639	2220	2223	2226	rBV2	182	235	0.03%	0.003%
94	14.713	2233	2235	2237	rBV2	224	224	0.03%	0.003%
95	15.206	2314	2316	2321	rBV3	359	524	0.06%	0.008%
96	15.718	2398	2400	2401	rBV	265	158	0.02%	0.002%
97	16.121	2463	2466	2467	rBV2	259	195	0.02%	0.003%
98	16.206	2478	2480	2481	rBV2	261	161	0.02%	0.002%
99	16.328	2498	2500	2502	rVB2	323	197	0.02%	0.003%
100	16.706	2559	2562	2564	rBV2	397	358	0.04%	0.005%




Sum of corrected areas: 6765037

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039487.D
Acq On : 27 Dec 2023 11:19
Operator : JC/MD
Sample : VX1227WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK659

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

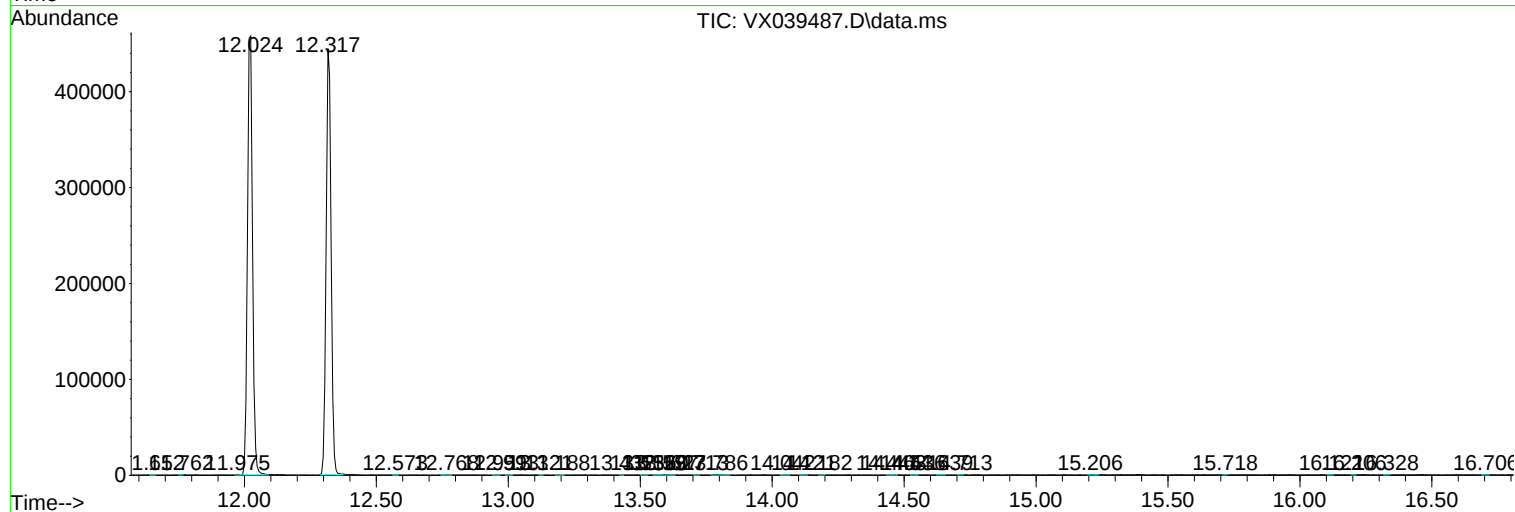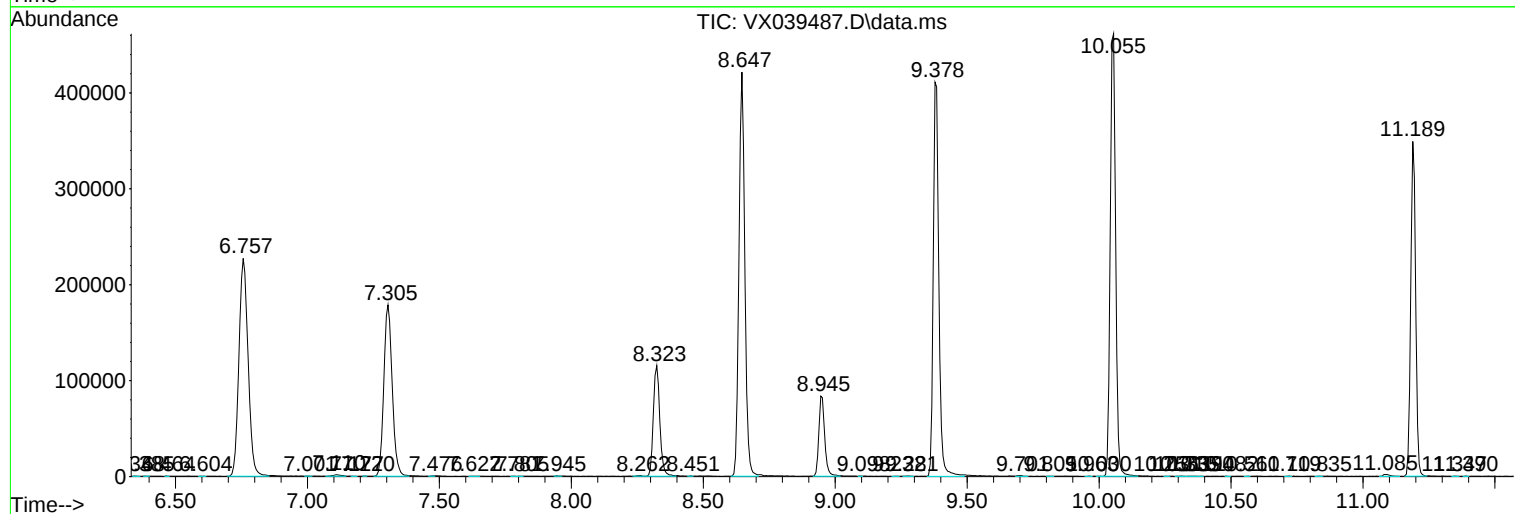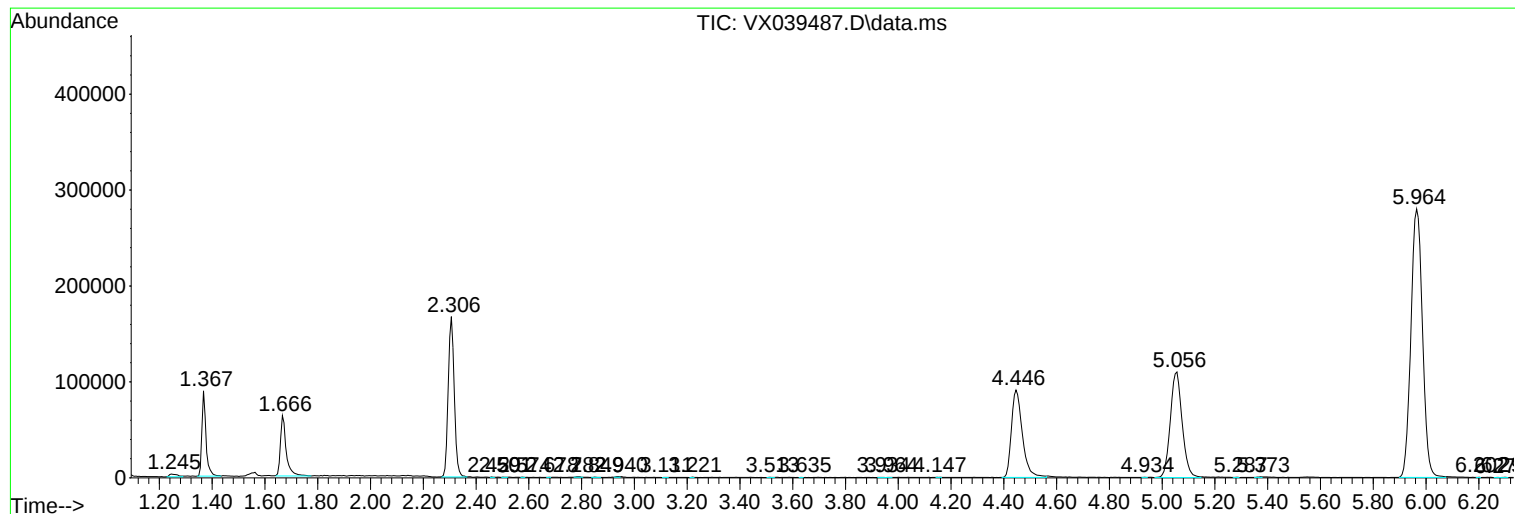

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039487.D
Acq On : 27 Dec 2023 11:19
Operator : JC/MD
Sample : VX1227WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK659

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039487.D
Acq On : 27 Dec 2023 11:19
Operator : JC/MD
Sample : VX1227WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK659

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc