

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039492.D
 Acq On : 27 Dec 2023 13:29
 Operator : JC/MD
 Sample : 05989-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7A78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	32	rBV	8172	17120	2.29%	0.278%
2	1.368	42	46	54	rBV	77694	81193	10.88%	1.320%
3	1.666	91	95	111	rVB	52518	81568	10.93%	1.326%
4	2.306	194	200	207	rBV	145715	225714	30.24%	3.669%
5	2.380	207	212	219	rVB	18375	30508	4.09%	0.496%
6	2.532	228	237	246	rBV3	4227	9436	1.26%	0.153%
7	2.648	252	256	260	rBV2	389	379	0.05%	0.006%
8	2.788	276	279	283	rVB3	474	611	0.08%	0.010%
9	2.940	299	304	312	rVV2	1804	3794	0.51%	0.062%
10	3.014	315	316	320	rVV2	229	292	0.04%	0.005%
11	3.050	320	322	323	rVV2	224	197	0.03%	0.003%
12	3.154	337	339	340	rVB	442	222	0.03%	0.004%
13	3.428	381	384	387	rBV2	298	413	0.06%	0.007%
14	3.568	406	407	410	rVB2	317	249	0.03%	0.004%
15	3.757	435	438	439	rBV	241	220	0.03%	0.004%
16	3.818	446	448	449	rVV	256	195	0.03%	0.003%
17	3.861	453	455	457	rVV2	211	219	0.03%	0.004%
18	3.983	473	475	476	rVV	398	266	0.04%	0.004%
19	4.001	476	478	479	rVV2	248	215	0.03%	0.003%
20	4.135	498	500	503	rVB	386	308	0.04%	0.005%
21	4.215	510	513	514	rBV	238	224	0.03%	0.004%
22	4.288	523	525	526	rBV	461	206	0.03%	0.003%
23	4.379	538	540	543	rVB	265	199	0.03%	0.003%
24	4.452	543	552	568	rBV	81922	226857	30.39%	3.688%
25	4.745	598	600	603	rBV	298	199	0.03%	0.003%
26	4.879	621	622	624	rBV	351	252	0.03%	0.004%
27	5.056	638	651	669	rBV2	95529	303851	40.70%	4.940%
28	5.367	700	702	703	rBV	319	280	0.04%	0.005%
29	5.556	728	733	734	rBV4	488	721	0.10%	0.012%
30	5.623	741	744	745	rBV	209	230	0.03%	0.004%
31	5.970	789	801	819	rBV2	246054	746476	100.00%	12.136%
32	6.172	832	834	838	rVB2	368	327	0.04%	0.005%
33	6.294	851	854	855	rVB	315	276	0.04%	0.004%
34	6.440	875	878	879	rBV2	284	306	0.04%	0.005%
35	6.684	916	918	921	rBB2	191	226	0.03%	0.004%
36	6.763	921	931	947	rBV	212723	518861	69.51%	8.435%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039492.D
 Acq On : 27 Dec 2023 13:29
 Operator : JC/MD
 Sample : 05989-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7A78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	7.098	984	986	989	rBV	295	238	0.03%	0.004%
38	7.306	1012	1020	1033	rBV	156972	346577	46.43%	5.634%
39	7.458	1043	1045	1046	rBV2	357	250	0.03%	0.004%
40	7.598	1067	1068	1070	rBV	280	198	0.03%	0.003%
41	7.635	1073	1074	1079	rVB2	264	279	0.04%	0.005%
42	7.860	1109	1111	1115	rBV	436	417	0.06%	0.007%
43	7.903	1115	1118	1121	rVB2	388	479	0.06%	0.008%
44	7.952	1121	1126	1131	rBV3	673	1469	0.20%	0.024%
45	8.135	1152	1156	1158	rBV2	300	387	0.05%	0.006%
46	8.183	1160	1164	1167	rBV2	145	218	0.03%	0.004%
47	8.263	1174	1177	1178	rBV	194	250	0.03%	0.004%
48	8.324	1181	1187	1203	rVV	103122	171337	22.95%	2.785%
49	8.500	1214	1216	1219	rBV2	268	405	0.05%	0.007%
50	8.580	1227	1229	1231	rBV	509	283	0.04%	0.005%
51	8.647	1234	1240	1249	rBV	355831	568782	76.20%	9.247%
52	8.842	1270	1272	1273	rBV	270	200	0.03%	0.003%
53	8.952	1284	1290	1301	rBV	75494	114859	15.39%	1.867%
54	9.269	1339	1342	1350	rBV4	1438	2404	0.32%	0.039%
55	9.384	1355	1361	1375	rBV	360236	523643	70.15%	8.513%
56	9.903	1444	1446	1449	rBV2	193	210	0.03%	0.003%
57	9.939	1451	1452	1457	rVB3	531	608	0.08%	0.010%
58	10.000	1460	1462	1465	rBV2	230	303	0.04%	0.005%
59	10.055	1465	1471	1487	rBV	447493	632004	84.67%	10.275%
60	10.305	1509	1512	1517	rBV2	824	1071	0.14%	0.017%
61	10.360	1519	1521	1523	rBV2	237	237	0.03%	0.004%
62	10.476	1538	1540	1542	rBV2	188	198	0.03%	0.003%
63	10.659	1565	1570	1573	rVB2	499	888	0.12%	0.014%
64	10.713	1577	1579	1584	rVB2	196	243	0.03%	0.004%
65	10.841	1598	1600	1603	rVB2	241	244	0.03%	0.004%
66	10.884	1605	1607	1609	rVB2	234	198	0.03%	0.003%
67	10.988	1621	1624	1629	rBV2	204	368	0.05%	0.006%
68	11.085	1637	1640	1645	rBV4	1745	2317	0.31%	0.038%
69	11.189	1652	1657	1666	rBV	320904	404434	54.18%	6.575%
70	11.311	1673	1677	1682	rBV4	2076	3048	0.41%	0.050%
71	11.390	1686	1690	1693	rVV3	346	604	0.08%	0.010%
72	11.451	1695	1700	1703	rBV2	268	502	0.07%	0.008%
73	11.482	1703	1705	1707	rVB2	361	283	0.04%	0.005%
74	11.604	1722	1725	1729	rBV3	1273	1866	0.25%	0.030%
75	11.707	1741	1742	1744	rBV	216	203	0.03%	0.003%
76	11.762	1747	1751	1756	rVB4	2317	3411	0.46%	0.055%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039492.D
 Acq On : 27 Dec 2023 13:29
 Operator : JC/MD
 Sample : 05989-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7A78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	11.811	1756	1759	1761	rBV	323	307	0.04%	0.005%
78	11.854	1761	1766	1771	rVB4	828	1281	0.17%	0.021%
79	11.951	1778	1782	1783	rVB2	284	242	0.03%	0.004%
80	12.018	1788	1793	1804	rBV	434763	580986	77.83%	9.445%
81	12.219	1821	1826	1833	rBV4	2117	3776	0.51%	0.061%
82	12.317	1837	1842	1852	rVV	403514	517048	69.27%	8.406%
83	12.512	1869	1874	1876	rBV2	188	318	0.04%	0.005%
84	12.579	1882	1885	1889	rBV3	1106	1371	0.18%	0.022%
85	12.634	1892	1894	1896	rVB2	266	207	0.03%	0.003%
86	12.768	1911	1916	1921	rBV3	1157	1963	0.26%	0.032%
87	12.841	1925	1928	1929	rBV2	283	274	0.04%	0.004%
88	12.859	1929	1931	1932	rVV	441	364	0.05%	0.006%
89	12.945	1944	1945	1950	rBV	281	320	0.04%	0.005%
90	12.994	1952	1953	1956	rBV2	277	238	0.03%	0.004%
91	13.067	1962	1965	1966	rVB	277	231	0.03%	0.004%
92	13.079	1966	1967	1969	rBV2	191	196	0.03%	0.003%
93	13.268	1997	1998	2001	rBV2	219	241	0.03%	0.004%
94	13.298	2001	2003	2005	rVV2	222	210	0.03%	0.003%
95	13.329	2007	2008	2011	rVV2	306	262	0.04%	0.004%
96	13.585	2048	2050	2055	rVB4	892	1264	0.17%	0.021%
97	13.737	2073	2075	2077	rVB	360	263	0.04%	0.004%
98	13.780	2080	2082	2086	rVB2	536	579	0.08%	0.009%
99	13.890	2098	2100	2101	rBV2	271	210	0.03%	0.003%
100	13.993	2114	2117	2120	rBV	433	480	0.06%	0.008%




Sum of corrected areas: 6151156

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039492.D
Acq On : 27 Dec 2023 13:29
Operator : JC/MD
Sample : 05989-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7A78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

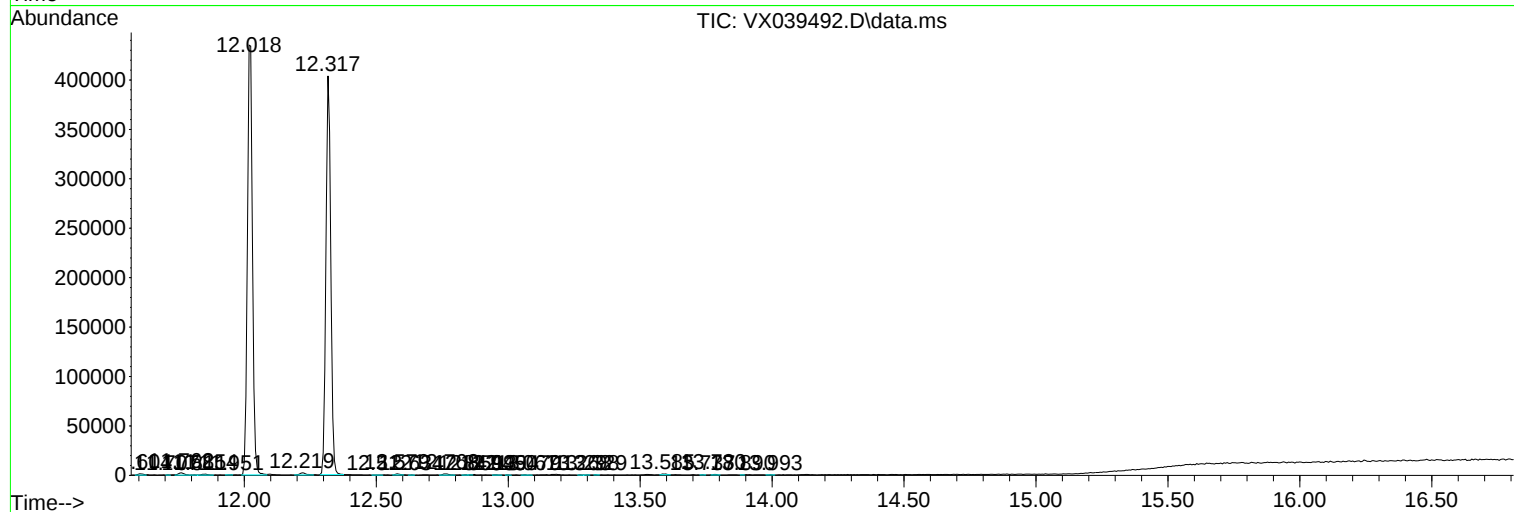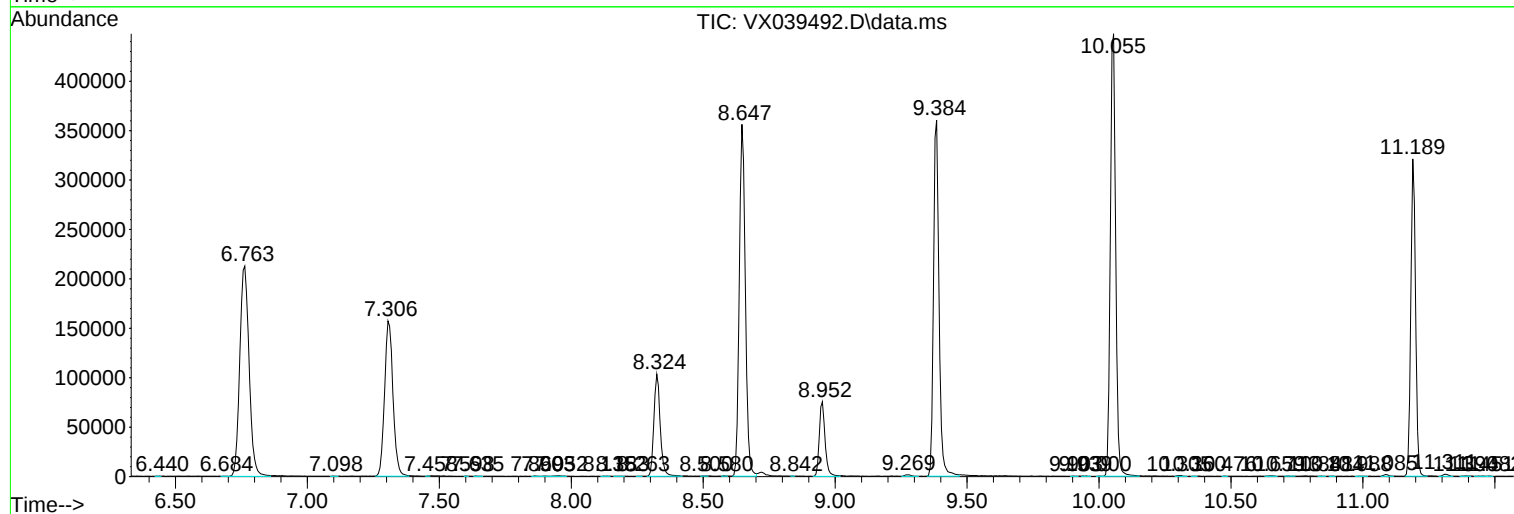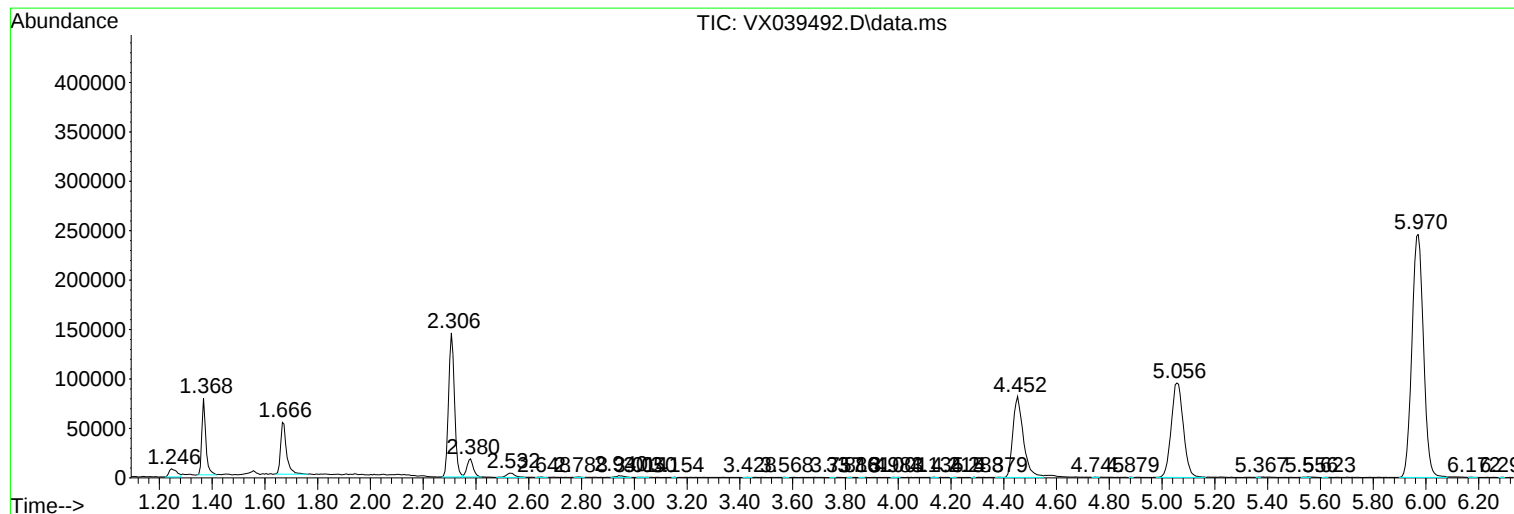

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039492.D
Acq On : 27 Dec 2023 13:29
Operator : JC/MD
Sample : 05989-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7A78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039492.D
Acq On : 27 Dec 2023 13:29
Operator : JC/MD
Sample : 05989-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7A78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc