

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039493.D
 Acq On : 27 Dec 2023 13:51
 Operator : JC/MD
 Sample : 05989-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7A82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M

Title : VOC Analysis

Signal : TIC: VX039493.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	53	rBV	73957	77410	10.89%	1.328%
2	1.672	92	96	106	rVB	52057	76252	10.73%	1.308%
3	2.306	195	200	207	rBV	135563	211474	29.74%	3.629%
4	2.380	208	212	222	rVB	19471	31619	4.45%	0.543%
5	4.452	544	552	566	rBV	78023	216126	30.40%	3.709%
6	5.056	640	651	668	rVB	93641	291988	41.07%	5.010%
7	5.684	752	754	756	rBV	417	297	0.04%	0.005%
8	5.800	771	773	775	rVB	487	395	0.06%	0.007%
9	5.970	789	801	817	rBV2	237304	710960	100.00%	12.200%
10	6.220	840	842	844	rBV2	380	375	0.05%	0.006%
11	6.245	844	846	848	rVV	419	365	0.05%	0.006%
12	6.507	888	889	891	rBV	471	310	0.04%	0.005%
13	6.763	921	931	943	rBV	200986	477955	67.23%	8.201%
14	7.306	1012	1020	1039	rBV	151917	333596	46.92%	5.724%
15	7.836	1105	1107	1109	rBV2	312	307	0.04%	0.005%
16	7.854	1109	1110	1112	rVV	434	228	0.03%	0.004%
17	7.946	1123	1125	1128	rVB3	594	705	0.10%	0.012%
18	8.324	1181	1187	1201	rBV	103380	171409	24.11%	2.941%
19	8.647	1234	1240	1249	rBV	345980	539956	75.95%	9.265%
20	8.952	1284	1290	1300	rBV	74914	113590	15.98%	1.949%
21	9.092	1312	1313	1316	rBV3	271	241	0.03%	0.004%
22	9.208	1331	1332	1335	rBV2	369	449	0.06%	0.008%
23	9.275	1340	1343	1348	rVB3	1360	1831	0.26%	0.031%
24	9.384	1355	1361	1378	rBV	353686	506820	71.29%	8.697%
25	9.775	1422	1425	1426	rBV	354	322	0.05%	0.006%
26	9.817	1431	1432	1435	rVV	323	271	0.04%	0.005%
27	9.872	1437	1441	1444	rVV2	234	292	0.04%	0.005%
28	10.055	1465	1471	1489	rBV	416157	589740	82.95%	10.120%
29	10.299	1509	1511	1517	rVB4	924	1438	0.20%	0.025%
30	10.348	1517	1519	1522	rVB	440	407	0.06%	0.007%
31	10.457	1534	1537	1538	rBV	268	272	0.04%	0.005%
32	10.524	1546	1548	1550	rBV	315	265	0.04%	0.005%
33	10.799	1592	1593	1595	rVB	373	241	0.03%	0.004%
34	10.854	1599	1602	1603	rBV	225	259	0.04%	0.004%
35	10.921	1612	1613	1615	rBV	278	227	0.03%	0.004%
36	11.085	1637	1640	1644	rBV3	1249	1662	0.23%	0.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039493.D
 Acq On : 27 Dec 2023 13:51
 Operator : JC/MD
 Sample : 05989-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7A82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	11.122	1644	1646	1647	rVB	398	249	0.04%	0.004%
38	11.189	1652	1657	1668	rVB	310722	391067	55.01%	6.710%
39	11.311	1673	1677	1683	rVB3	2028	2824	0.40%	0.048%
40	11.421	1693	1695	1698	rVB2	291	246	0.03%	0.004%
41	11.604	1723	1725	1731	rVB3	988	1491	0.21%	0.026%
42	11.762	1747	1751	1754	rBV3	1258	1710	0.24%	0.029%
43	11.811	1757	1759	1761	rVB2	440	354	0.05%	0.006%
44	11.829	1761	1762	1764	rBV	267	235	0.03%	0.004%
45	11.982	1784	1787	1788	rVB2	350	234	0.03%	0.004%
46	12.018	1788	1793	1804	rBV	418853	551823	77.62%	9.469%
47	12.219	1821	1826	1829	rBV2	2912	3997	0.56%	0.069%
48	12.317	1837	1842	1857	rVB	381826	493068	69.35%	8.461%
49	12.548	1877	1880	1881	rVB	380	236	0.03%	0.004%
50	12.579	1881	1885	1890	rVB3	1292	1857	0.26%	0.032%
51	12.652	1895	1897	1901	rVB2	300	337	0.05%	0.006%
52	12.719	1906	1908	1910	rBV	201	225	0.03%	0.004%
53	12.762	1911	1915	1919	rVV3	1053	1690	0.24%	0.029%
54	12.859	1928	1931	1934	rVV	748	730	0.10%	0.013%
55	12.902	1934	1938	1939	rVB2	233	227	0.03%	0.004%
56	13.213	1985	1989	1990	rBV2	290	261	0.04%	0.004%
57	13.292	1999	2002	2004	rVB	468	428	0.06%	0.007%
58	13.317	2004	2006	2009	rBV2	276	258	0.04%	0.004%
59	13.408	2019	2021	2024	rBV2	253	265	0.04%	0.005%
60	13.439	2024	2026	2029	rVB	308	309	0.04%	0.005%
61	13.469	2029	2031	2033	rBB2	348	270	0.04%	0.005%
62	13.597	2049	2052	2056	rVB2	1159	1421	0.20%	0.024%
63	13.634	2056	2058	2060	rBV2	309	241	0.03%	0.004%
64	13.731	2072	2074	2078	rVB	174	225	0.03%	0.004%
65	13.786	2080	2083	2084	rVV2	383	385	0.05%	0.007%
66	13.847	2090	2093	2094	rVB2	284	259	0.04%	0.004%
67	13.896	2098	2101	2105	rBV2	178	285	0.04%	0.005%
68	14.030	2121	2123	2126	rVV2	238	247	0.03%	0.004%
69	14.134	2135	2140	2142	rBV2	395	547	0.08%	0.009%
70	14.219	2153	2154	2156	rBV2	351	237	0.03%	0.004%
71	14.420	2186	2187	2191	rBV	243	347	0.05%	0.006%
72	14.597	2214	2216	2217	rBV2	335	282	0.04%	0.005%
73	14.615	2217	2219	2225	rVV2	367	573	0.08%	0.010%
74	14.847	2254	2257	2259	rBV2	223	359	0.05%	0.006%
75	14.902	2265	2266	2270	rBV2	271	290	0.04%	0.005%
76	14.957	2273	2275	2277	rBV2	239	260	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039493.D
 Acq On : 27 Dec 2023 13:51
 Operator : JC/MD
 Sample : 05989-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7A82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	15.036	2287	2288	2291	rBV2	266	231	0.03%	0.004%
78	15.280	2326	2328	2331	rBV	257	259	0.04%	0.004%
79	15.365	2338	2342	2344	rVB2	320	292	0.04%	0.005%
80	15.438	2352	2354	2356	rBV2	283	316	0.04%	0.005%
81	15.487	2360	2362	2364	rVV2	316	249	0.04%	0.004%
82	15.542	2370	2371	2373	rVB2	314	224	0.03%	0.004%
83	15.566	2373	2375	2378	rBV3	295	287	0.04%	0.005%
84	15.597	2378	2380	2383	rBV2	491	529	0.07%	0.009%
85	15.694	2394	2396	2399	rVB	301	288	0.04%	0.005%
86	15.725	2399	2401	2404	rBV2	178	238	0.03%	0.004%
87	15.755	2404	2406	2409	rVB2	551	532	0.07%	0.009%
88	15.798	2409	2413	2414	rVB2	267	225	0.03%	0.004%
89	15.816	2414	2416	2419	rBV	421	314	0.04%	0.005%
90	15.895	2428	2429	2432	rVB2	421	338	0.05%	0.006%
91	15.938	2432	2436	2437	rBV3	329	296	0.04%	0.005%
92	15.999	2444	2446	2448	rBV	338	335	0.05%	0.006%
93	16.048	2451	2454	2455	rBV2	334	308	0.04%	0.005%
94	16.091	2458	2461	2463	rVV2	204	222	0.03%	0.004%
95	16.145	2468	2470	2472	rVB2	320	267	0.04%	0.005%
96	16.164	2472	2473	2477	rBV2	313	484	0.07%	0.008%
97	16.267	2488	2490	2491	rBV	368	306	0.04%	0.005%
98	16.395	2508	2511	2512	rBV2	203	282	0.04%	0.005%
99	16.408	2512	2513	2516	rVV2	365	283	0.04%	0.005%
100	16.493	2525	2527	2528	rBV3	241	225	0.03%	0.004%




Sum of corrected areas: 5827733

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039493.D
Acq On : 27 Dec 2023 13:51
Operator : JC/MD
Sample : 05989-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7A82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

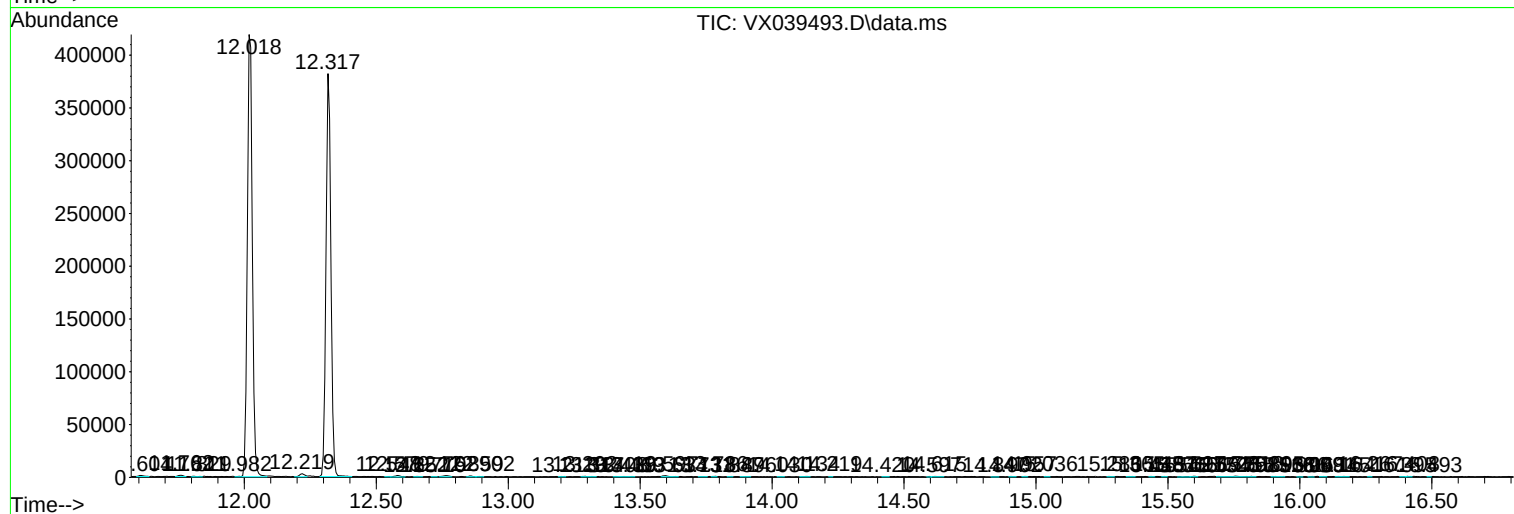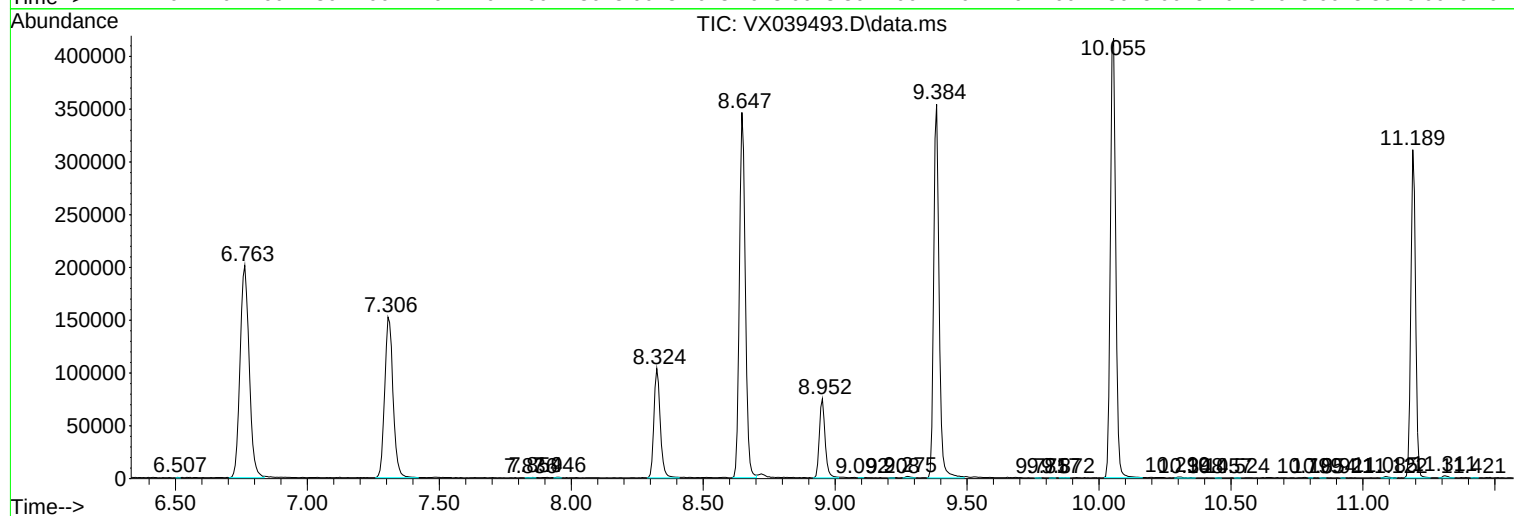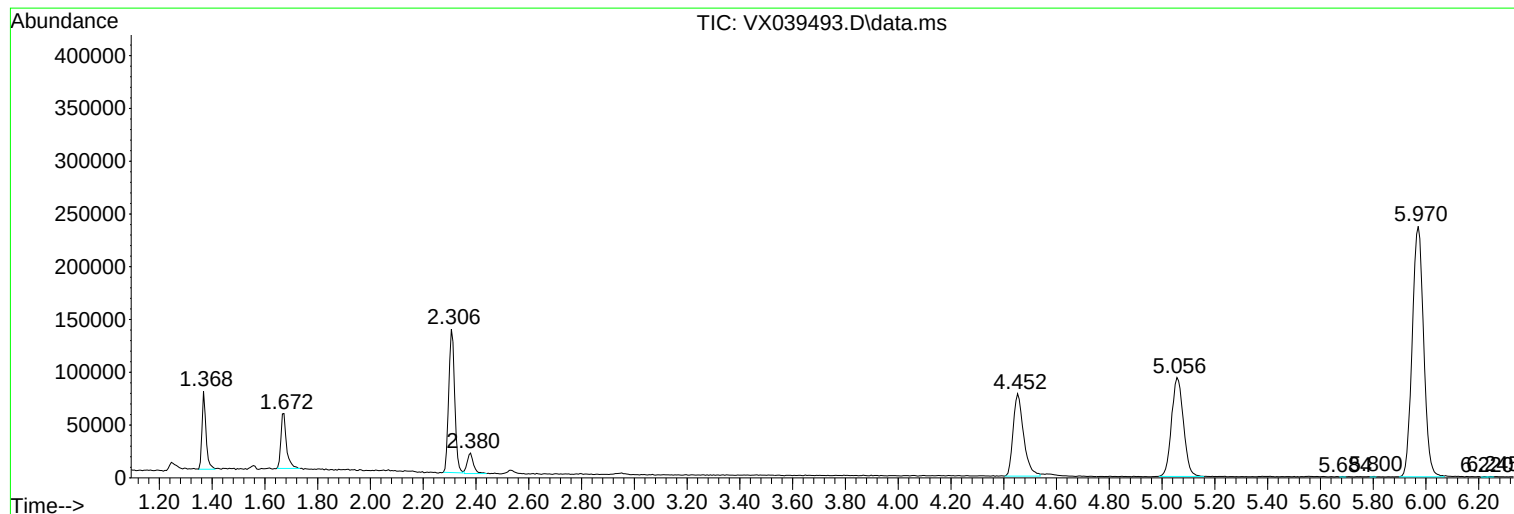

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039493.D
Acq On : 27 Dec 2023 13:51
Operator : JC/MD
Sample : 05989-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7A82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039493.D
Acq On : 27 Dec 2023 13:51
Operator : JC/MD
Sample : 05989-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7A82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc