

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039494.D
 Acq On : 27 Dec 2023 14:14
 Operator : JC/MD
 Sample : 05988-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0Q55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039494.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	32	rBV	7818	16730	2.33%	0.279%
2	1.368	42	46	58	rVB	74104	80645	11.25%	1.345%
3	1.666	91	95	107	rVB	56205	79387	11.07%	1.324%
4	2.306	194	200	209	rBV	141683	219629	30.64%	3.664%
5	2.373	209	211	220	rVB2	2203	3863	0.54%	0.064%
6	2.508	230	233	235	rBV3	402	472	0.07%	0.008%
7	2.788	276	279	283	rVB3	451	688	0.10%	0.011%
8	2.940	301	304	310	rBV2	470	854	0.12%	0.014%
9	3.264	354	357	358	rBV	238	203	0.03%	0.003%
10	3.556	403	405	407	rBV2	190	171	0.02%	0.003%
11	3.666	422	423	425	rBV	281	188	0.03%	0.003%
12	3.776	438	441	442	rBV2	241	193	0.03%	0.003%
13	3.940	465	468	470	rBV2	207	239	0.03%	0.004%
14	3.959	470	471	475	rVB2	210	215	0.03%	0.004%
15	4.068	487	489	491	rBV2	251	255	0.04%	0.004%
16	4.227	513	515	518	rVB2	303	386	0.05%	0.006%
17	4.257	518	520	521	rVB	337	170	0.02%	0.003%
18	4.276	521	523	525	rBV2	277	232	0.03%	0.004%
19	4.312	525	529	530	rBV2	273	268	0.04%	0.004%
20	4.373	537	539	542	rVB2	198	229	0.03%	0.004%
21	4.452	543	552	569	rBV	78631	223715	31.21%	3.732%
22	4.708	591	594	598	rBV2	205	299	0.04%	0.005%
23	4.922	626	629	630	rBV2	248	218	0.03%	0.004%
24	5.062	639	652	666	rBV	95818	289551	40.39%	4.831%
25	5.245	681	682	686	rVB2	300	204	0.03%	0.003%
26	5.275	686	687	691	rVB2	165	184	0.03%	0.003%
27	5.324	694	695	698	rVB2	255	185	0.03%	0.003%
28	5.470	717	719	722	rBV	247	305	0.04%	0.005%
29	5.519	725	727	729	rBV	203	245	0.03%	0.004%
30	5.550	729	732	735	rVV3	432	703	0.10%	0.012%
31	5.720	758	760	763	rVB2	158	202	0.03%	0.003%
32	5.970	789	801	821	rBV2	238644	716858	100.00%	11.960%
33	6.586	900	902	905	rVB2	330	372	0.05%	0.006%
34	6.610	905	906	908	rBV2	303	262	0.04%	0.004%
35	6.641	908	911	913	rVB	253	264	0.04%	0.004%
36	6.671	913	916	918	rBV	291	286	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039494.D
 Acq On : 27 Dec 2023 14:14
 Operator : JC/MD
 Sample : 05988-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0Q55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	6.763	920	931	951	rBV	206601	497124	69.35%	8.294%
38	7.074	980	982	983	rBV	340	240	0.03%	0.004%
39	7.305	1012	1020	1037	rBV	152054	334433	46.65%	5.580%
40	7.494	1046	1051	1054	rBV3	510	813	0.11%	0.014%
41	7.531	1056	1057	1062	rVB2	350	357	0.05%	0.006%
42	7.946	1121	1125	1127	rBV2	408	606	0.08%	0.010%
43	8.324	1180	1187	1201	rBV	101953	169277	23.61%	2.824%
44	8.488	1211	1214	1216	rBV2	223	305	0.04%	0.005%
45	8.647	1234	1240	1255	rBV	354513	551091	76.88%	9.194%
46	8.952	1285	1290	1303	rBV	74716	111764	15.59%	1.865%
47	9.080	1309	1311	1313	rVB2	388	285	0.04%	0.005%
48	9.110	1313	1316	1318	rBV2	392	424	0.06%	0.007%
49	9.134	1318	1320	1321	rVV2	269	186	0.03%	0.003%
50	9.269	1340	1342	1344	rBV2	568	537	0.07%	0.009%
51	9.384	1355	1361	1374	rBV	365964	522021	72.82%	8.709%
52	9.622	1398	1400	1404	rBV2	280	305	0.04%	0.005%
53	9.860	1437	1439	1441	rBV	310	199	0.03%	0.003%
54	10.055	1465	1471	1487	rBV	435555	673504	93.95%	11.237%
55	10.244	1498	1502	1507	rVB4	379	582	0.08%	0.010%
56	10.530	1546	1549	1552	rVB2	209	266	0.04%	0.004%
57	10.707	1577	1578	1581	rBV2	253	227	0.03%	0.004%
58	10.750	1581	1585	1586	rVV2	183	202	0.03%	0.003%
59	10.866	1602	1604	1607	rBV2	252	209	0.03%	0.003%
60	10.963	1618	1620	1623	rBV	205	179	0.02%	0.003%
61	11.085	1637	1640	1644	rBV3	1368	1800	0.25%	0.030%
62	11.146	1648	1650	1652	rBV2	215	207	0.03%	0.003%
63	11.189	1652	1657	1665	rBV	307358	394109	54.98%	6.575%
64	11.311	1674	1677	1682	rVB2	1161	1472	0.21%	0.025%
65	11.378	1687	1688	1690	rBV2	262	193	0.03%	0.003%
66	11.457	1699	1701	1703	rVB	410	377	0.05%	0.006%
67	11.488	1703	1706	1707	rBV2	265	215	0.03%	0.004%
68	11.610	1721	1726	1728	rBV5	800	1009	0.14%	0.017%
69	11.634	1728	1730	1731	rVB	358	258	0.04%	0.004%
70	11.707	1739	1742	1745	rBV2	288	354	0.05%	0.006%
71	11.756	1747	1750	1754	rVB4	704	1126	0.16%	0.019%
72	11.811	1754	1759	1761	rBV2	362	532	0.07%	0.009%
73	11.853	1763	1766	1768	rBV2	263	295	0.04%	0.005%
74	11.969	1782	1785	1788	rVV3	1572	2071	0.29%	0.035%
75	12.024	1788	1794	1807	rVB	419030	563373	78.59%	9.399%
76	12.183	1817	1820	1821	rVB2	276	216	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039494.D
 Acq On : 27 Dec 2023 14:14
 Operator : JC/MD
 Sample : 05988-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0Q55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.219	1823	1826	1833	rVV3	2690	3831	0.53%	0.064%
78	12.317	1837	1842	1854	rVV	387809	509097	71.02%	8.494%
79	12.561	1881	1882	1885	rVB	329	231	0.03%	0.004%
80	12.591	1885	1887	1889	rBV	241	263	0.04%	0.004%
81	12.756	1910	1914	1919	rBV3	459	746	0.10%	0.012%
82	12.890	1935	1936	1940	rVB	286	312	0.04%	0.005%
83	12.926	1940	1942	1943	rBV2	260	193	0.03%	0.003%
84	13.164	1980	1981	1984	rBV	196	212	0.03%	0.004%
85	13.591	2047	2051	2055	rVV2	1421	1577	0.22%	0.026%
86	13.670	2062	2064	2067	rBV2	279	308	0.04%	0.005%
87	13.816	2086	2088	2089	rBV	214	202	0.03%	0.003%
88	13.926	2104	2106	2108	rVV2	220	241	0.03%	0.004%
89	13.963	2108	2112	2115	rVV2	1591	1924	0.27%	0.032%
90	14.121	2136	2138	2141	rVB2	298	248	0.03%	0.004%
91	14.347	2174	2175	2178	rBV	310	221	0.03%	0.004%
92	14.652	2223	2225	2227	rBV	334	339	0.05%	0.006%
93	14.700	2232	2233	2236	rBV2	252	232	0.03%	0.004%
94	14.755	2241	2242	2245	rBV2	385	394	0.05%	0.007%
95	14.847	2254	2257	2258	rBV2	397	334	0.05%	0.006%
96	14.908	2266	2267	2269	rBV2	223	182	0.03%	0.003%
97	14.999	2280	2282	2283	rBV	343	314	0.04%	0.005%
98	15.475	2358	2360	2365	rBV3	248	348	0.05%	0.006%
99	15.664	2389	2391	2393	rBV2	272	285	0.04%	0.005%
100	16.042	2452	2453	2455	rBV2	194	199	0.03%	0.003%




Sum of corrected areas: 5993846

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039494.D
Acq On : 27 Dec 2023 14:14
Operator : JC/MD
Sample : 05988-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0Q55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

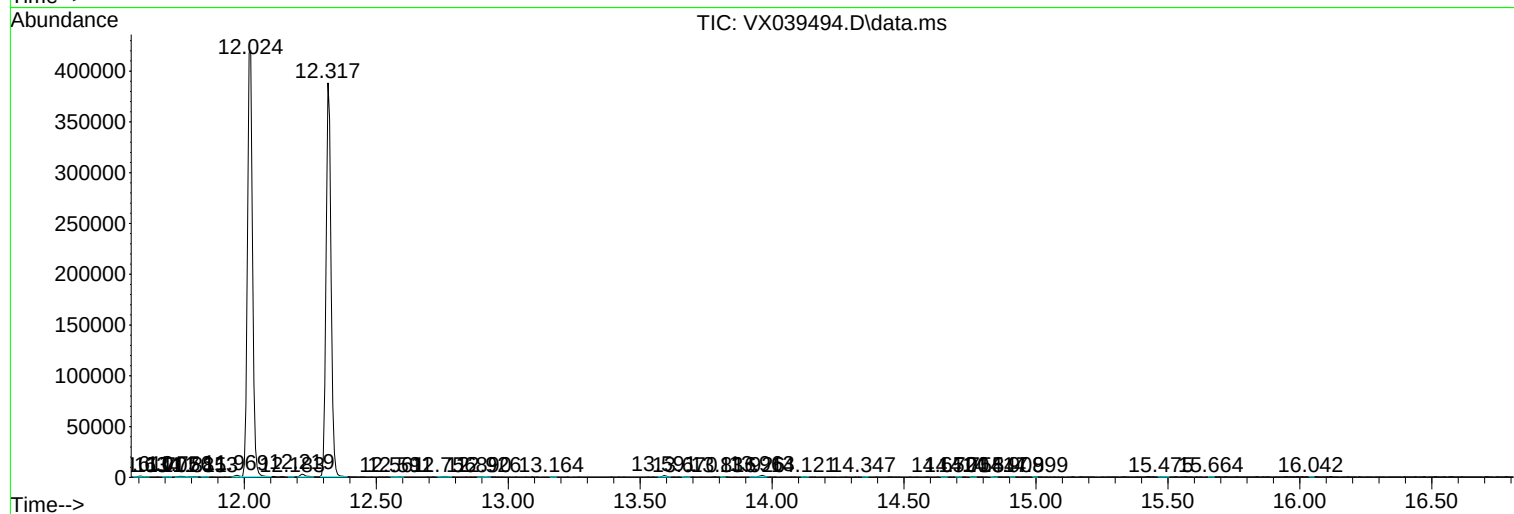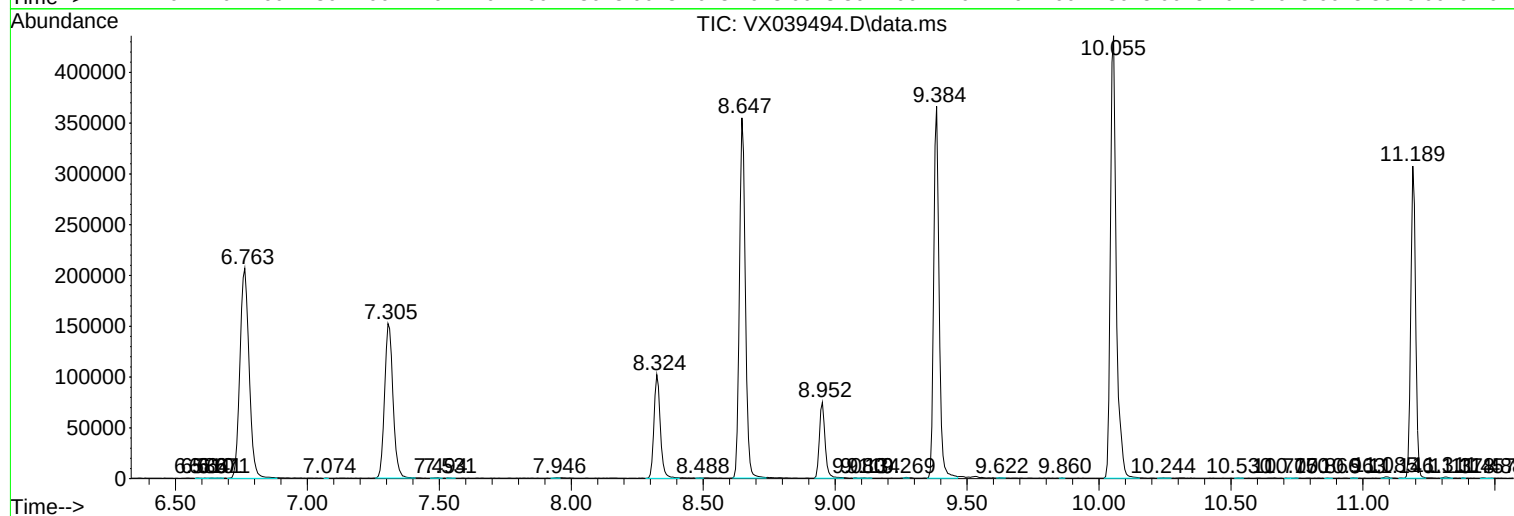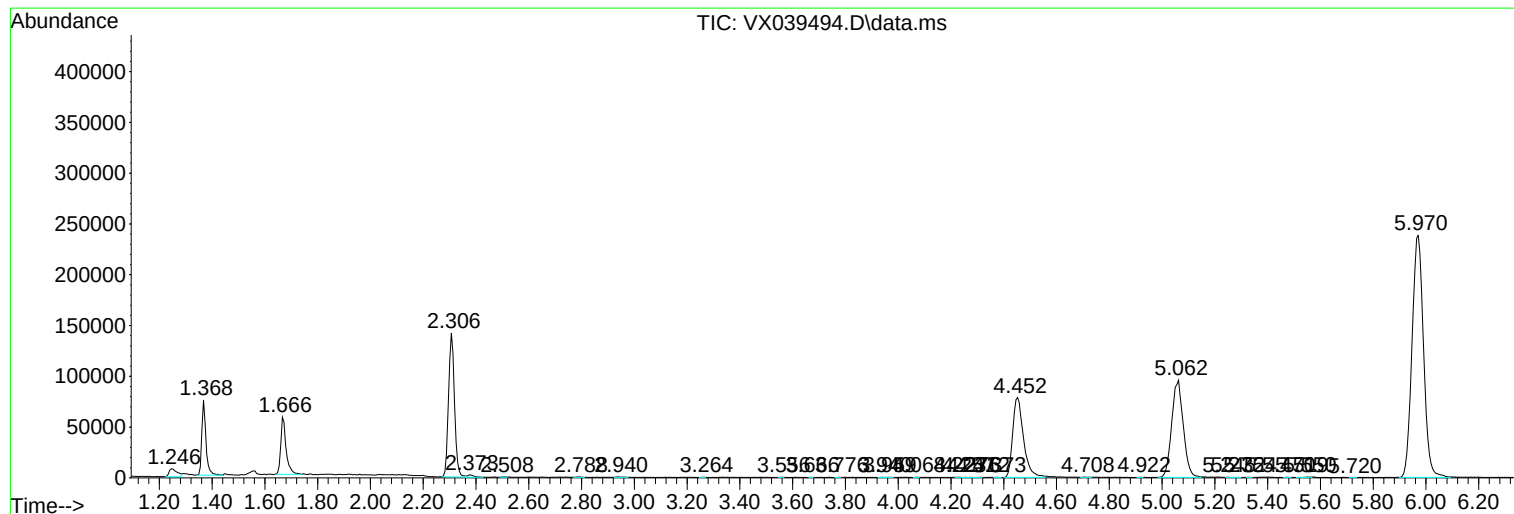

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039494.D
Acq On : 27 Dec 2023 14:14
Operator : JC/MD
Sample : 05988-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0Q55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039494.D
Acq On : 27 Dec 2023 14:14
Operator : JC/MD
Sample : 05988-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0Q55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc