

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039495.D
 Acq On : 27 Dec 2023 14:37
 Operator : JC/MD
 Sample : 05988-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0Q56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039495.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	31	rBV	8204	14536	1.99%	0.244%
2	1.368	43	46	56	rVB	73351	77039	10.57%	1.296%
3	1.666	91	95	108	rBV	54649	80009	10.98%	1.346%
4	2.306	194	200	208	rBV	139120	219454	30.11%	3.691%
5	2.373	208	211	218	rVB	3760	6272	0.86%	0.105%
6	2.532	231	237	246	rBV	4260	8695	1.19%	0.146%
7	2.934	299	303	304	rBV	1566	1590	0.22%	0.027%
8	3.117	330	333	334	rBV	237	249	0.03%	0.004%
9	3.331	362	368	374	rVB4	816	1985	0.27%	0.033%
10	3.733	432	434	440	rVV	167	196	0.03%	0.003%
11	3.861	454	455	459	rVV2	175	236	0.03%	0.004%
12	3.959	469	471	472	rBV	245	176	0.02%	0.003%
13	4.184	506	508	509	rVB	365	194	0.03%	0.003%
14	4.361	535	537	541	rVB	289	325	0.04%	0.005%
15	4.452	543	552	567	rBV2	77085	223127	30.61%	3.753%
16	4.843	614	616	618	rVB2	350	253	0.03%	0.004%
17	4.971	635	637	639	rBV	235	218	0.03%	0.004%
18	5.056	639	651	666	rVV	95938	299988	41.16%	5.046%
19	5.251	681	683	686	rBV3	314	434	0.06%	0.007%
20	5.385	700	705	708	rBV4	483	959	0.13%	0.016%
21	5.507	722	725	726	rBV2	247	273	0.04%	0.005%
22	5.605	740	741	744	rBV2	210	277	0.04%	0.005%
23	5.763	765	767	769	rVB	303	214	0.03%	0.004%
24	5.800	769	773	775	rBV2	137	226	0.03%	0.004%
25	5.970	789	801	817	rBV2	238365	728835	100.00%	12.258%
26	6.300	853	855	858	rBV	254	290	0.04%	0.005%
27	6.592	902	903	905	rBV	208	205	0.03%	0.003%
28	6.647	908	912	916	rBV3	284	530	0.07%	0.009%
29	6.763	921	931	948	rBV	205039	491896	67.49%	8.273%
30	6.958	961	963	964	rVB2	294	173	0.02%	0.003%
31	7.117	987	989	994	rVB2	413	538	0.07%	0.009%
32	7.202	1000	1003	1008	rBV4	322	549	0.08%	0.009%
33	7.312	1012	1021	1041	rVV	149879	338081	46.39%	5.686%
34	7.470	1045	1047	1049	rBV2	263	260	0.04%	0.004%
35	7.623	1071	1072	1075	rVB	343	225	0.03%	0.004%
36	7.799	1098	1101	1104	rVB2	199	260	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039495.D
 Acq On : 27 Dec 2023 14:37
 Operator : JC/MD
 Sample : 05988-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0Q56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	7.897	1113	1117	1123	rBV4	1737	3526	0.48%	0.059%
38	8.025	1136	1138	1140	rVB2	292	256	0.04%	0.004%
39	8.049	1140	1142	1143	rBV	322	180	0.02%	0.003%
40	8.092	1145	1149	1153	rVV2	242	393	0.05%	0.007%
41	8.324	1181	1187	1202	rBV	105207	169651	23.28%	2.853%
42	8.488	1209	1214	1221	rVB6	1467	2656	0.36%	0.045%
43	8.574	1227	1228	1233	rVB2	603	648	0.09%	0.011%
44	8.647	1234	1240	1250	rBV	348602	559324	76.74%	9.407%
45	8.897	1279	1281	1284	rVB	281	181	0.02%	0.003%
46	8.952	1284	1290	1304	rBV	72800	112365	15.42%	1.890%
47	9.275	1339	1343	1350	rVB2	1159	1809	0.25%	0.030%
48	9.384	1355	1361	1374	rBV	361160	515482	70.73%	8.670%
49	9.829	1433	1434	1435	rBV	381	188	0.03%	0.003%
50	9.909	1445	1447	1449	rBV	228	189	0.03%	0.003%
51	10.055	1465	1471	1484	rBV	429447	601667	82.55%	10.120%
52	10.153	1485	1487	1492	rVB3	1387	1387	0.19%	0.023%
53	10.195	1492	1494	1496	rBV	555	440	0.06%	0.007%
54	10.293	1507	1510	1511	rBV2	671	806	0.11%	0.014%
55	10.470	1537	1539	1541	rBV2	217	220	0.03%	0.004%
56	10.604	1560	1561	1563	rVB	379	213	0.03%	0.004%
57	10.622	1563	1564	1565	rBV	243	175	0.02%	0.003%
58	10.799	1590	1593	1595	rVB2	330	433	0.06%	0.007%
59	10.969	1619	1621	1623	rBV2	246	178	0.02%	0.003%
60	11.085	1637	1640	1645	rBV3	1247	1684	0.23%	0.028%
61	11.189	1652	1657	1666	rVB	309445	393491	53.99%	6.618%
62	11.280	1670	1672	1673	rBV	220	169	0.02%	0.003%
63	11.317	1674	1678	1683	rVB3	1515	1770	0.24%	0.030%
64	11.390	1686	1690	1693	rBV3	564	828	0.11%	0.014%
65	11.451	1698	1700	1704	rBV3	301	341	0.05%	0.006%
66	11.524	1711	1712	1716	rVV	248	183	0.03%	0.003%
67	11.616	1723	1727	1730	rVB3	594	926	0.13%	0.016%
68	11.756	1746	1750	1753	rVB3	825	1014	0.14%	0.017%
69	12.018	1788	1793	1804	rBV	412559	549223	75.36%	9.238%
70	12.219	1821	1826	1837	rBV2	8401	14763	2.03%	0.248%
71	12.317	1837	1842	1855	rVB	389878	503514	69.08%	8.469%
72	12.451	1862	1864	1865	rBV2	269	186	0.03%	0.003%
73	12.591	1885	1887	1888	rBV2	276	175	0.02%	0.003%
74	12.762	1912	1915	1918	rVV2	516	609	0.08%	0.010%
75	12.884	1932	1935	1936	rBV	185	181	0.02%	0.003%
76	13.103	1969	1971	1973	rVB2	328	273	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039495.D
 Acq On : 27 Dec 2023 14:37
 Operator : JC/MD
 Sample : 05988-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0Q56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.140	1973	1977	1978	rBV	188	268	0.04%	0.005%
78	13.280	1998	2000	2001	rBV	294	183	0.03%	0.003%
79	13.439	2024	2026	2028	rBV	189	200	0.03%	0.003%
80	13.646	2057	2060	2064	rVB2	206	261	0.04%	0.004%
81	13.682	2064	2066	2068	rBV	205	169	0.02%	0.003%
82	14.085	2130	2132	2133	rBV	297	184	0.03%	0.003%
83	14.286	2164	2165	2166	rBV	255	170	0.02%	0.003%
84	14.365	2177	2178	2181	rVV2	204	218	0.03%	0.004%
85	14.414	2184	2186	2187	rVV	317	181	0.02%	0.003%
86	14.463	2191	2194	2197	rVB2	233	315	0.04%	0.005%
87	14.597	2214	2216	2219	rVV	374	293	0.04%	0.005%
88	14.670	2227	2228	2231	rBV2	219	208	0.03%	0.003%
89	15.060	2290	2292	2294	rBV2	182	182	0.02%	0.003%
90	15.194	2313	2314	2317	rVB	281	201	0.03%	0.003%
91	15.353	2339	2340	2343	rVB2	321	249	0.03%	0.004%
92	15.456	2355	2357	2358	rBV2	365	178	0.02%	0.003%
93	15.517	2366	2367	2369	rVB	320	176	0.02%	0.003%
94	15.603	2379	2381	2383	rBV2	253	203	0.03%	0.003%
95	15.944	2435	2437	2438	rBV2	283	192	0.03%	0.003%
96	15.993	2443	2445	2447	rVV	249	191	0.03%	0.003%
97	16.054	2453	2455	2456	rBV	328	253	0.03%	0.004%
98	16.267	2488	2490	2491	rBV	386	240	0.03%	0.004%
99	16.292	2492	2494	2497	rBV2	239	210	0.03%	0.004%
100	16.597	2542	2544	2545	rBV	248	169	0.02%	0.003%

Sum of corrected areas: 5945558




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039495.D
Acq On : 27 Dec 2023 14:37
Operator : JC/MD
Sample : 05988-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0Q56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

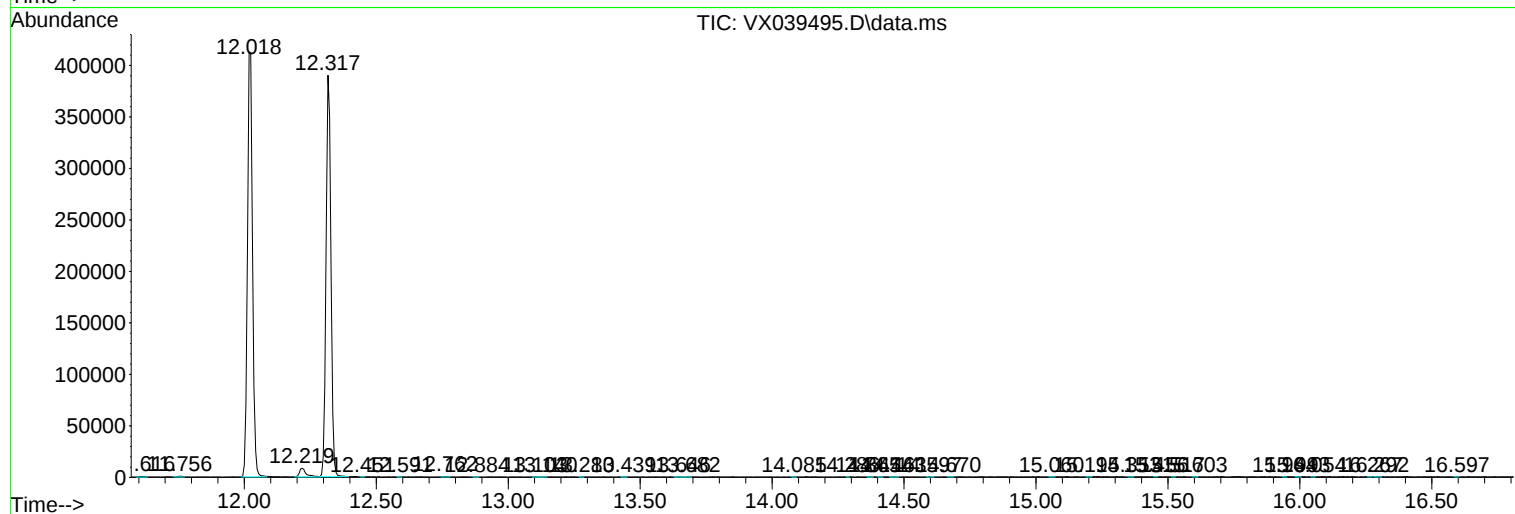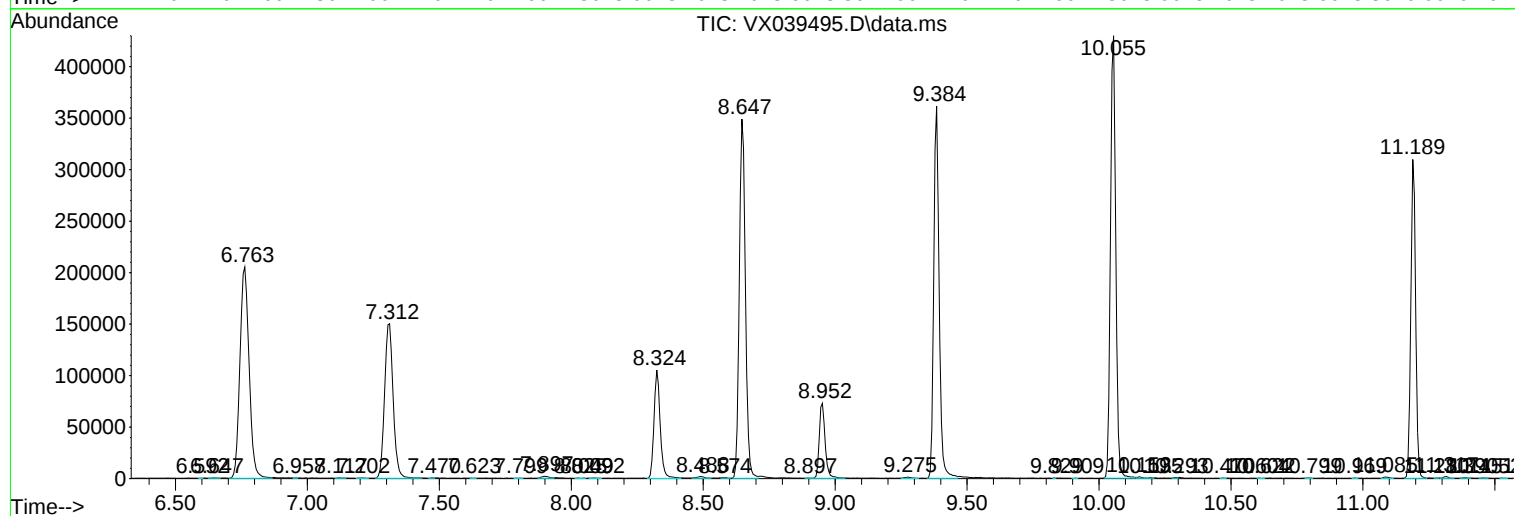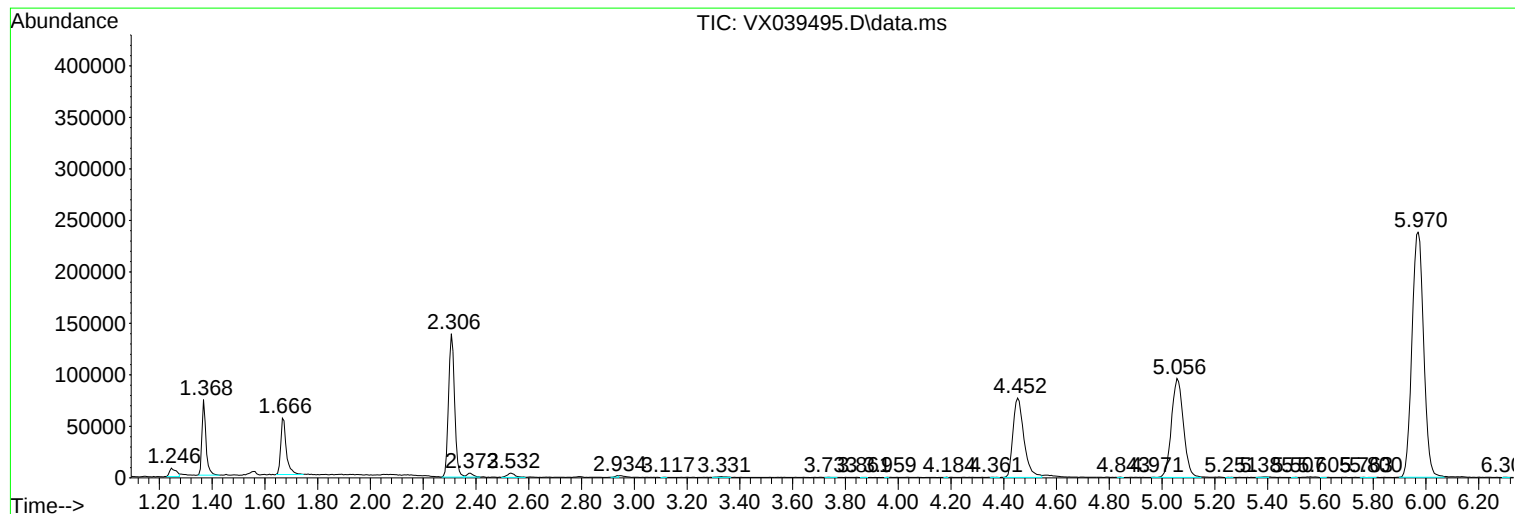

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039495.D
Acq On : 27 Dec 2023 14:37
Operator : JC/MD
Sample : 05988-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0Q56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039495.D
Acq On : 27 Dec 2023 14:37
Operator : JC/MD
Sample : 05988-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0Q56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------