

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039496.D
 Acq On : 27 Dec 2023 15:00
 Operator : JC/MD
 Sample : 05988-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0Q57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039496.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	32	rBV	7771	16055	2.24%	0.275%
2	1.368	42	46	56	rVB	72265	77279	10.80%	1.322%
3	1.666	91	95	107	rBV	51638	77315	10.80%	1.323%
4	2.307	194	200	208	rBV	138109	215982	30.18%	3.695%
5	2.374	209	211	218	rVB	2536	3813	0.53%	0.065%
6	2.867	291	292	295	rVB2	262	198	0.03%	0.003%
7	2.941	302	304	307	rBV3	376	381	0.05%	0.007%
8	3.026	316	318	320	rVB2	259	253	0.04%	0.004%
9	3.264	356	357	360	rBV2	201	188	0.03%	0.003%
10	3.355	370	372	374	rBV	293	330	0.05%	0.006%
11	3.587	409	410	412	rBV2	207	219	0.03%	0.004%
12	3.733	432	434	437	rVB	258	207	0.03%	0.004%
13	3.855	452	454	456	rBV	251	180	0.03%	0.003%
14	3.977	472	474	477	rBV2	268	309	0.04%	0.005%
15	4.014	478	480	486	rVV	370	413	0.06%	0.007%
16	4.233	514	516	519	rBV2	174	196	0.03%	0.003%
17	4.270	521	522	525	rBV2	314	238	0.03%	0.004%
18	4.453	543	552	573	rBV	77122	224436	31.36%	3.839%
19	4.642	581	583	584	rVB	429	218	0.03%	0.004%
20	4.885	620	623	626	rBV2	232	312	0.04%	0.005%
21	4.916	626	628	630	rVB	235	237	0.03%	0.004%
22	5.056	637	651	672	rBV	97779	293119	40.95%	5.014%
23	5.483	718	721	724	rBV2	164	213	0.03%	0.004%
24	5.544	726	731	732	rBV	530	588	0.08%	0.010%
25	5.666	748	751	752	rBV	222	225	0.03%	0.004%
26	5.806	772	774	775	rBV2	181	172	0.02%	0.003%
27	5.971	789	801	817	rBV2	238626	715734	100.00%	12.244%
28	6.263	846	849	855	rVB2	227	500	0.07%	0.009%
29	6.470	879	883	887	rBV	189	384	0.05%	0.007%
30	6.544	893	895	897	rVV2	318	254	0.04%	0.004%
31	6.617	905	907	910	rBV2	277	247	0.03%	0.004%
32	6.763	922	931	948	rBV	206228	488712	68.28%	8.360%
33	7.306	1011	1020	1037	rBV	150681	335840	46.92%	5.745%
34	7.482	1045	1049	1052	rBV2	568	723	0.10%	0.012%
35	7.940	1122	1124	1125	rBV2	521	437	0.06%	0.007%
36	8.074	1143	1146	1149	rVB2	269	253	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039496.D
 Acq On : 27 Dec 2023 15:00
 Operator : JC/MD
 Sample : 05988-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0Q57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	8.159	1156	1160	1162	rBV	217	248	0.03%	0.004%
38	8.324	1181	1187	1200	rBV	98201	164532	22.99%	2.815%
39	8.507	1215	1217	1219	rVB	433	320	0.04%	0.005%
40	8.647	1234	1240	1251	rBV	342696	547833	76.54%	9.372%
41	8.903	1280	1282	1284	rBV2	279	233	0.03%	0.004%
42	8.952	1284	1290	1304	rVV	72734	109066	15.24%	1.866%
43	9.086	1311	1312	1315	rBV3	298	221	0.03%	0.004%
44	9.171	1324	1326	1328	rBV	206	188	0.03%	0.003%
45	9.281	1339	1344	1347	rBV	848	1112	0.16%	0.019%
46	9.385	1356	1361	1378	rVV	354212	509086	71.13%	8.709%
47	9.641	1402	1403	1407	rVB2	186	179	0.03%	0.003%
48	9.945	1450	1453	1454	rBV	260	228	0.03%	0.004%
49	10.055	1465	1471	1485	rBV	425618	597206	83.44%	10.216%
50	10.195	1492	1494	1499	rVB3	595	771	0.11%	0.013%
51	10.244	1499	1502	1505	rBV3	481	651	0.09%	0.011%
52	10.269	1505	1506	1510	rVV2	234	243	0.03%	0.004%
53	10.299	1510	1511	1512	rVV	339	173	0.02%	0.003%
54	10.390	1523	1526	1527	rBV2	179	185	0.03%	0.003%
55	10.476	1539	1540	1545	rBV2	248	301	0.04%	0.005%
56	10.695	1573	1576	1579	rBV3	187	239	0.03%	0.004%
57	10.768	1584	1588	1590	rVB2	242	235	0.03%	0.004%
58	10.970	1619	1621	1625	rBV2	328	416	0.06%	0.007%
59	11.037	1630	1632	1636	rBV2	232	270	0.04%	0.005%
60	11.085	1637	1640	1646	rVB4	1215	1820	0.25%	0.031%
61	11.189	1652	1657	1667	rBV	300895	387529	54.14%	6.629%
62	11.317	1674	1678	1681	rVB	763	991	0.14%	0.017%
63	11.451	1698	1700	1702	rVB	255	181	0.03%	0.003%
64	11.616	1724	1727	1730	rVB2	425	559	0.08%	0.010%
65	11.665	1733	1735	1739	rVB2	256	261	0.04%	0.004%
66	11.713	1741	1743	1745	rVB	270	176	0.02%	0.003%
67	11.756	1748	1750	1754	rVV2	375	405	0.06%	0.007%
68	11.817	1757	1760	1762	rBV2	316	365	0.05%	0.006%
69	11.866	1766	1768	1771	rVB2	214	208	0.03%	0.004%
70	11.890	1771	1772	1774	rBV	315	255	0.04%	0.004%
71	12.024	1788	1794	1803	rBV	414659	551467	77.05%	9.434%
72	12.219	1822	1826	1831	rBV2	3842	4957	0.69%	0.085%
73	12.317	1837	1842	1857	rVB	384387	498406	69.64%	8.526%
74	12.482	1868	1869	1872	rVB	158	173	0.02%	0.003%
75	12.530	1875	1877	1879	rBV2	309	328	0.05%	0.006%
76	12.683	1899	1902	1905	rBV2	267	352	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039496.D
 Acq On : 27 Dec 2023 15:00
 Operator : JC/MD
 Sample : 05988-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0Q57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.768	1912	1916	1920	rVB3	642	870	0.12%	0.015%
78	13.085	1965	1968	1969	rVB	284	228	0.03%	0.004%
79	13.506	2036	2037	2039	rBV	312	172	0.02%	0.003%
80	13.585	2048	2050	2054	rBV2	453	489	0.07%	0.008%
81	13.774	2079	2081	2083	rBV2	232	247	0.03%	0.004%
82	13.939	2106	2108	2113	rBV2	153	230	0.03%	0.004%
83	14.000	2116	2118	2125	rVB2	160	191	0.03%	0.003%
84	14.067	2127	2129	2131	rVB2	282	180	0.03%	0.003%
85	14.103	2134	2135	2138	rBV2	243	247	0.03%	0.004%
86	14.128	2138	2139	2142	rBV	225	219	0.03%	0.004%
87	14.213	2151	2153	2154	rBV	370	179	0.03%	0.003%
88	14.542	2205	2207	2211	rBV2	212	188	0.03%	0.003%
89	14.664	2225	2227	2230	rVB2	325	323	0.05%	0.006%
90	14.859	2257	2259	2261	rVB	317	229	0.03%	0.004%
91	14.890	2261	2264	2269	rBV3	347	532	0.07%	0.009%
92	14.951	2272	2274	2276	rBV2	204	198	0.03%	0.003%
93	14.981	2276	2279	2283	rVB2	277	379	0.05%	0.006%
94	15.048	2286	2290	2291	rBV2	243	281	0.04%	0.005%
95	15.792	2410	2412	2415	rBV2	263	248	0.03%	0.004%
96	15.944	2436	2437	2439	rBV	315	202	0.03%	0.003%
97	16.194	2476	2478	2479	rBV	457	237	0.03%	0.004%
98	16.231	2479	2484	2485	rVV3	372	404	0.06%	0.007%
99	16.469	2520	2523	2524	rBV	263	227	0.03%	0.004%
100	16.731	2563	2566	2568	rBV	285	320	0.04%	0.005%




Sum of corrected areas: 5845549

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039496.D
Acq On : 27 Dec 2023 15:00
Operator : JC/MD
Sample : 05988-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0Q57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

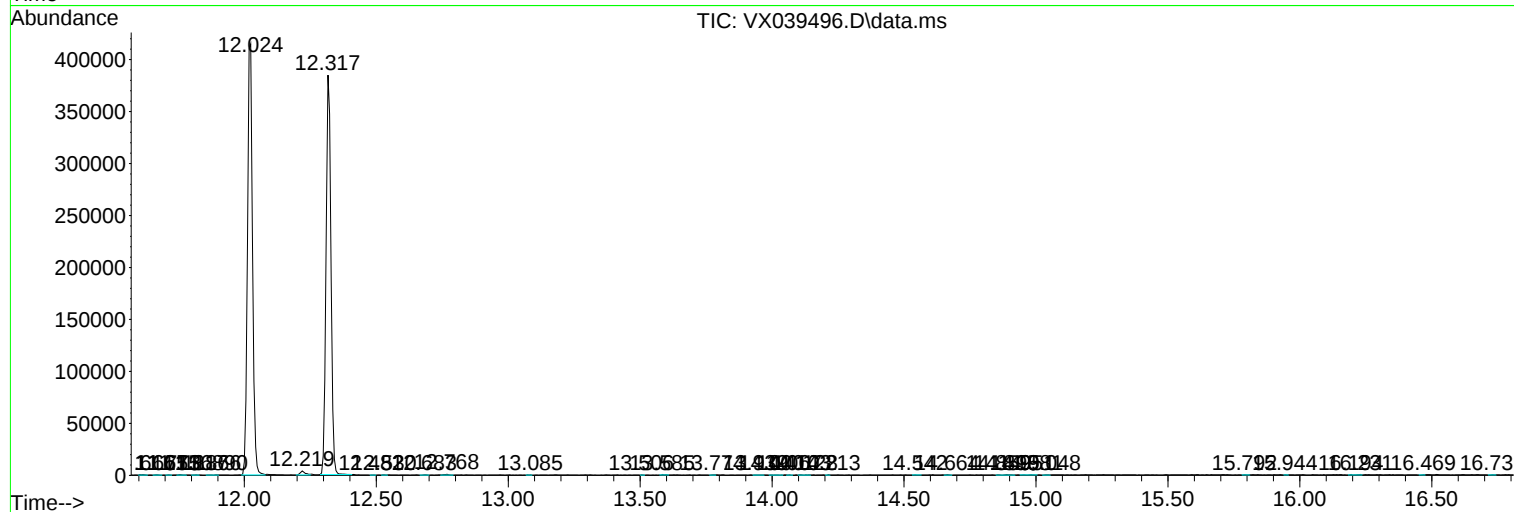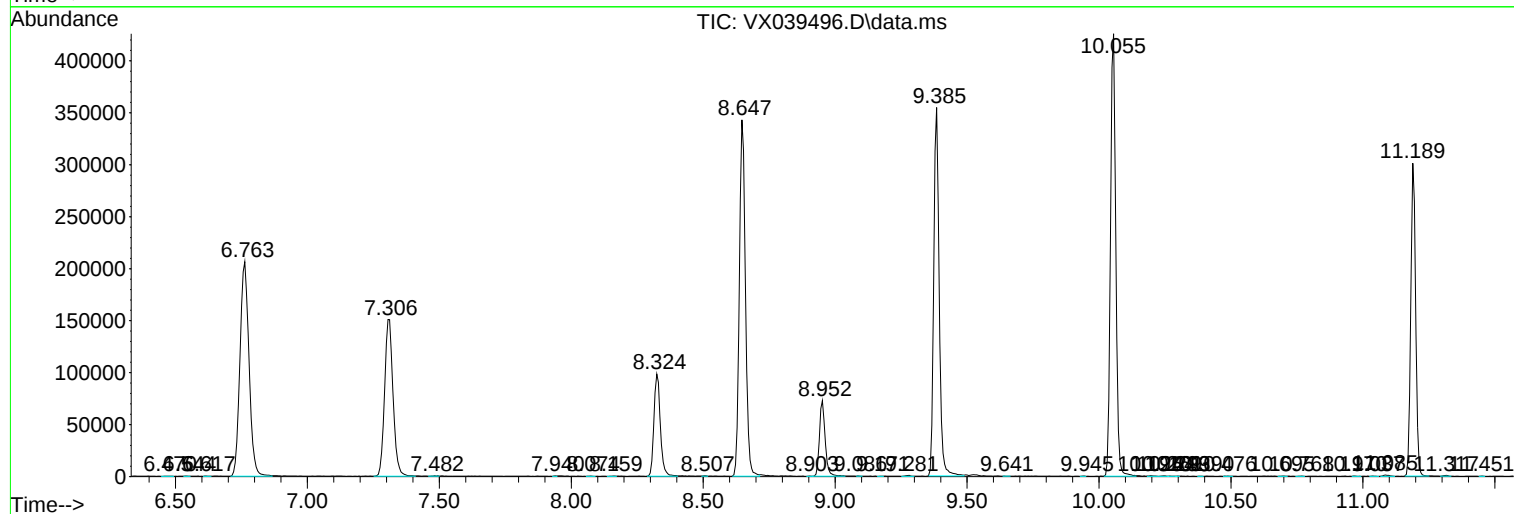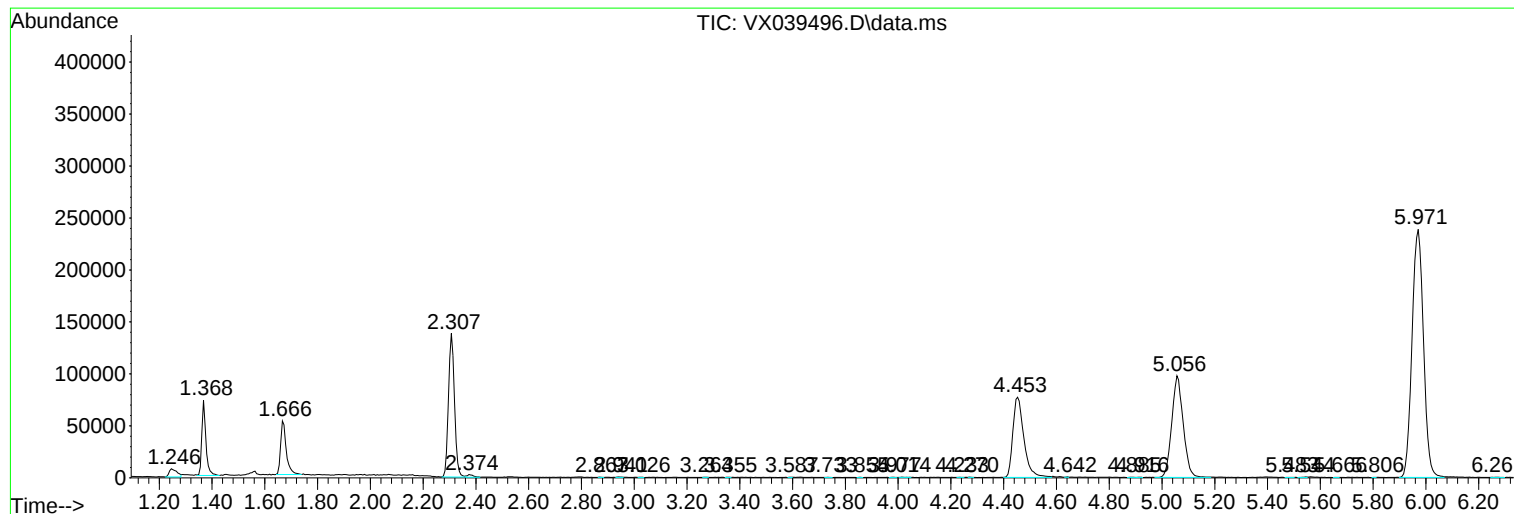

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039496.D
Acq On : 27 Dec 2023 15:00
Operator : JC/MD
Sample : 05988-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0Q57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039496.D
Acq On : 27 Dec 2023 15:00
Operator : JC/MD
Sample : 05988-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0Q57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc