

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039499.D
 Acq On : 27 Dec 2023 17:08
 Operator : JC/MD
 Sample : 05988-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039499.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	35	rBV	4487	11616	1.38%	0.181%
2	1.368	42	46	59	rBV	110346	118769	14.12%	1.849%
3	1.666	91	95	109	rBV	67838	100361	11.93%	1.562%
4	2.306	194	200	210	rVB	189074	290853	34.57%	4.527%
5	2.428	219	220	223	rVB	324	253	0.03%	0.004%
6	2.752	270	273	275	rBV	187	223	0.03%	0.003%
7	2.788	275	279	284	rVB4	1018	1786	0.21%	0.028%
8	2.886	293	295	298	rBV2	176	240	0.03%	0.004%
9	2.947	298	305	312	rVB2	3216	6828	0.81%	0.106%
10	3.069	323	325	328	rVB2	287	322	0.04%	0.005%
11	3.099	328	330	331	rBV	224	200	0.02%	0.003%
12	3.111	331	332	337	rVB	288	248	0.03%	0.004%
13	3.184	343	344	347	rBB	238	188	0.02%	0.003%
14	3.355	370	372	375	rVV	206	210	0.02%	0.003%
15	3.398	375	379	381	rVV2	213	255	0.03%	0.004%
16	3.514	397	398	401	rVB	435	210	0.02%	0.003%
17	3.642	417	419	421	rVV2	170	199	0.02%	0.003%
18	3.696	425	428	431	rBV2	197	280	0.03%	0.004%
19	3.812	444	447	451	rBV	164	243	0.03%	0.004%
20	3.873	454	457	459	rVV2	162	190	0.02%	0.003%
21	4.446	543	551	565	rBV2	76348	212864	25.30%	3.313%
22	4.763	601	603	607	rBV3	260	319	0.04%	0.005%
23	4.824	611	613	614	rBV	366	284	0.03%	0.004%
24	4.861	617	619	621	rBV2	228	233	0.03%	0.004%
25	5.056	637	651	670	rVV	104414	326402	38.80%	5.081%
26	5.391	701	706	707	rVV2	493	726	0.09%	0.011%
27	5.538	727	730	731	rBV2	331	302	0.04%	0.005%
28	5.727	757	761	764	rBV2	152	255	0.03%	0.004%
29	5.964	787	800	821	rVV2	280981	841260	100.00%	13.095%
30	6.105	821	823	826	rVV2	272	210	0.02%	0.003%
31	6.275	849	851	855	rBV2	159	271	0.03%	0.004%
32	6.489	885	886	891	rBB2	142	181	0.02%	0.003%
33	6.556	895	897	900	rVB2	249	197	0.02%	0.003%
34	6.592	902	903	906	rBV2	232	235	0.03%	0.004%
35	6.757	920	930	947	rBV	205043	491516	58.43%	7.651%
36	7.031	973	975	976	rBV	331	231	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039499.D
 Acq On : 27 Dec 2023 17:08
 Operator : JC/MD
 Sample : 05988-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.110	983	988	990	rBV3	1163	1899	0.23%	0.030%
38	7.306	1011	1020	1038	rBV	171161	377138	44.83%	5.870%
39	7.482	1046	1049	1053	rBV	771	828	0.10%	0.013%
40	7.556	1058	1061	1064	rVB	401	413	0.05%	0.006%
41	7.592	1064	1067	1070	rBV	229	274	0.03%	0.004%
42	7.897	1114	1117	1120	rBV	169	243	0.03%	0.004%
43	7.946	1123	1125	1129	rVB2	314	266	0.03%	0.004%
44	8.159	1157	1160	1165	rVB	207	251	0.03%	0.004%
45	8.208	1165	1168	1171	rBV2	184	245	0.03%	0.004%
46	8.257	1171	1176	1181	rBV3	1696	2651	0.32%	0.041%
47	8.324	1181	1187	1202	rVV	116433	189583	22.54%	2.951%
48	8.500	1214	1216	1218	rBV2	279	198	0.02%	0.003%
49	8.647	1233	1240	1255	rBV	421427	662717	78.78%	10.316%
50	8.885	1277	1279	1282	rBV	243	249	0.03%	0.004%
51	8.946	1284	1289	1301	rBV	79371	123984	14.74%	1.930%
52	9.128	1317	1319	1321	rBV2	274	251	0.03%	0.004%
53	9.195	1328	1330	1335	rBV2	167	212	0.03%	0.003%
54	9.281	1342	1344	1347	rVB2	199	224	0.03%	0.003%
55	9.384	1355	1361	1375	rBV	338873	505969	60.14%	7.876%
56	9.689	1410	1411	1416	rVB3	609	827	0.10%	0.013%
57	9.732	1416	1418	1420	rVB	375	211	0.03%	0.003%
58	10.055	1465	1471	1490	rBV	423099	604029	71.80%	9.402%
59	10.360	1518	1521	1525	rBV2	186	211	0.03%	0.003%
60	10.445	1533	1535	1540	rBV2	173	265	0.03%	0.004%
61	10.598	1559	1560	1565	rBV2	120	203	0.02%	0.003%
62	10.659	1569	1570	1573	rBV	245	203	0.02%	0.003%
63	10.732	1579	1582	1585	rBV3	339	409	0.05%	0.006%
64	10.927	1611	1614	1617	rBV	245	253	0.03%	0.004%
65	10.963	1617	1620	1623	rBV2	265	313	0.04%	0.005%
66	11.091	1638	1641	1645	rBV3	770	1187	0.14%	0.018%
67	11.189	1652	1657	1665	rBV	326445	405864	48.24%	6.318%
68	11.469	1701	1703	1706	rVV2	151	217	0.03%	0.003%
69	11.597	1720	1724	1726	rBV2	240	341	0.04%	0.005%
70	11.799	1754	1757	1760	rBV2	190	224	0.03%	0.003%
71	11.975	1782	1786	1788	rBV	207	238	0.03%	0.004%
72	12.018	1788	1793	1801	rBV	427300	563988	67.04%	8.779%
73	12.225	1824	1827	1828	rBV2	292	216	0.03%	0.003%
74	12.317	1837	1842	1851	rBV	445833	560861	66.67%	8.730%
75	12.597	1887	1888	1891	rBV2	160	195	0.02%	0.003%
76	12.664	1897	1899	1903	rVB	245	335	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039499.D
 Acq On : 27 Dec 2023 17:08
 Operator : JC/MD
 Sample : 05988-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.756	1913	1914	1920	rVV3	509	726	0.09%	0.011%
78	13.024	1955	1958	1960	rBV2	201	198	0.02%	0.003%
79	13.262	1994	1997	1998	rBV	248	260	0.03%	0.004%
80	13.579	2046	2049	2050	rBV2	243	229	0.03%	0.004%
81	13.701	2067	2069	2071	rBV	151	193	0.02%	0.003%
82	13.871	2095	2097	2098	rVV	327	195	0.02%	0.003%
83	14.054	2126	2127	2130	rBV2	171	192	0.02%	0.003%
84	14.134	2135	2140	2142	rVB2	355	549	0.07%	0.009%
85	14.256	2157	2160	2162	rVB2	246	237	0.03%	0.004%
86	14.280	2162	2164	2167	rBV2	353	345	0.04%	0.005%
87	14.353	2174	2176	2180	rBV2	244	235	0.03%	0.004%
88	14.621	2219	2220	2223	rVB	295	182	0.02%	0.003%
89	14.658	2223	2226	2227	rBV2	271	243	0.03%	0.004%
90	14.810	2249	2251	2253	rBV	230	286	0.03%	0.004%
91	15.018	2283	2285	2288	rBV2	260	352	0.04%	0.005%
92	15.097	2296	2298	2301	rVB2	298	265	0.03%	0.004%
93	15.450	2354	2356	2361	rBV2	264	305	0.04%	0.005%
94	15.591	2376	2379	2381	rBV2	383	409	0.05%	0.006%
95	15.749	2402	2405	2407	rBV2	406	351	0.04%	0.005%
96	15.810	2413	2415	2419	rVB3	235	272	0.03%	0.004%
97	16.176	2474	2475	2478	rBV2	259	255	0.03%	0.004%
98	16.237	2483	2485	2488	rBV2	288	350	0.04%	0.005%
99	16.328	2498	2500	2501	rBV2	240	202	0.02%	0.003%
100	16.426	2514	2516	2518	rVB2	383	380	0.05%	0.006%




Sum of corrected areas: 6424356

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039499.D
Acq On : 27 Dec 2023 17:08
Operator : JC/MD
Sample : 05988-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

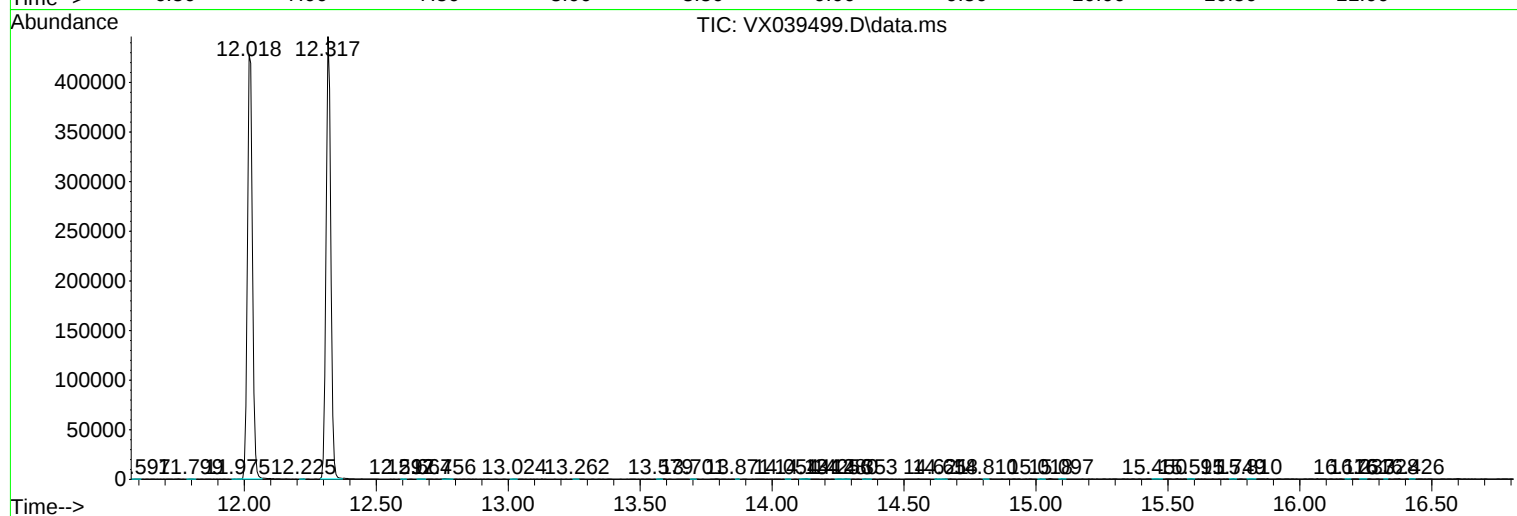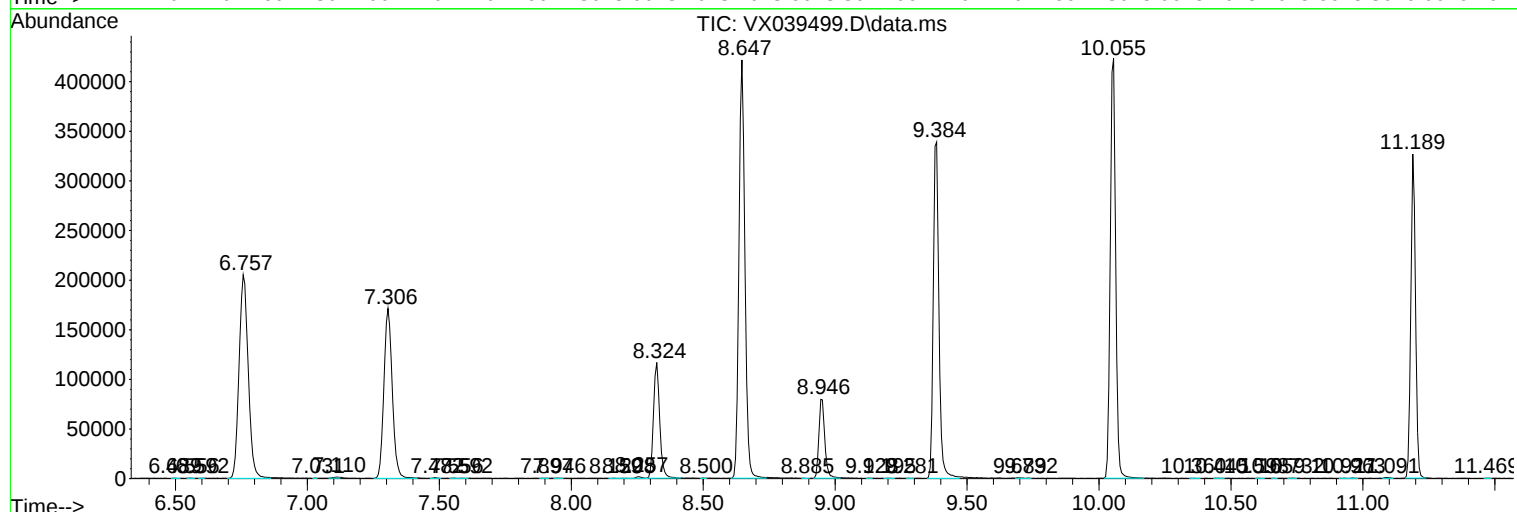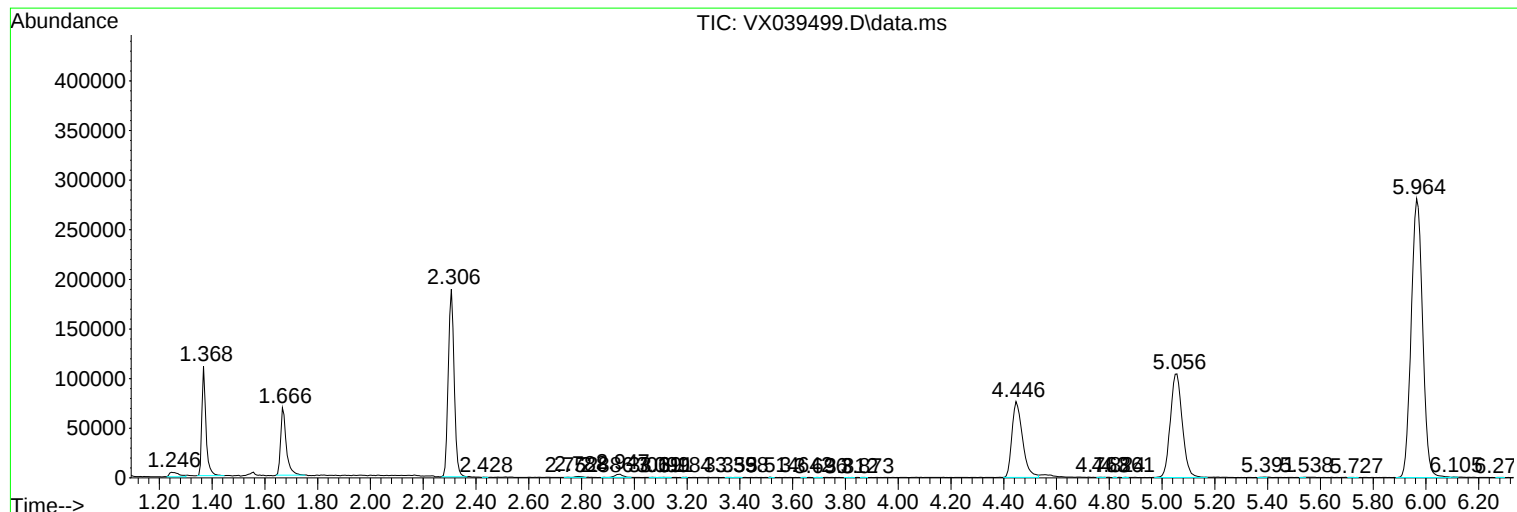

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039499.D
Acq On : 27 Dec 2023 17:08
Operator : JC/MD
Sample : 05988-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039499.D
Acq On : 27 Dec 2023 17:08
Operator : JC/MD
Sample : 05988-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc