

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039500.D
 Acq On : 27 Dec 2023 17:30
 Operator : JC/MD
 Sample : 05989-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M

Title : VOC Analysis

Signal : TIC: VX039500.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.251	22	27	34	rBV3	4199	10718	1.27%	0.168%
2	1.367	42	46	58	rBV	107565	116907	13.85%	1.830%
3	1.666	91	95	107	rBV	69388	102851	12.18%	1.610%
4	2.306	194	200	212	rVB	186808	287317	34.03%	4.498%
5	2.452	223	224	228	rVB2	361	302	0.04%	0.005%
6	2.519	232	235	239	rBV2	645	914	0.11%	0.014%
7	2.788	275	279	285	rVB3	1170	2179	0.26%	0.034%
8	2.946	294	305	314	rBV	3689	9271	1.10%	0.145%
9	3.086	326	328	331	rBV2	337	268	0.03%	0.004%
10	3.196	345	346	350	rVB2	223	218	0.03%	0.003%
11	3.324	364	367	369	rBV	275	262	0.03%	0.004%
12	3.367	372	374	375	rBV	296	237	0.03%	0.004%
13	3.788	440	443	444	rBV2	219	168	0.02%	0.003%
14	3.867	454	456	461	rVB2	268	353	0.04%	0.006%
15	4.025	480	482	484	rVB	208	167	0.02%	0.003%
16	4.050	484	486	490	rVB2	289	439	0.05%	0.007%
17	4.080	490	491	495	rBV	184	273	0.03%	0.004%
18	4.117	495	497	500	rVV	237	204	0.02%	0.003%
19	4.202	507	511	512	rVB2	161	173	0.02%	0.003%
20	4.452	543	552	564	rBV	77261	221763	26.27%	3.472%
21	5.056	638	651	670	rBV	104252	324731	38.46%	5.084%
22	5.202	673	675	677	rVV3	516	578	0.07%	0.009%
23	5.239	679	681	687	rVB2	452	714	0.08%	0.011%
24	5.330	694	696	701	rBV2	241	337	0.04%	0.005%
25	5.391	701	706	708	rBV3	426	708	0.08%	0.011%
26	5.458	714	717	720	rVB2	182	170	0.02%	0.003%
27	5.556	730	733	736	rBV2	453	753	0.09%	0.012%
28	5.970	789	801	822	rBV2	280373	844252	100.00%	13.217%
29	6.153	829	831	832	rBV	242	243	0.03%	0.004%
30	6.366	863	866	867	rBV	293	192	0.02%	0.003%
31	6.452	877	880	884	rVB	266	352	0.04%	0.006%
32	6.482	884	885	887	rBV	298	168	0.02%	0.003%
33	6.763	922	931	945	rBV	198696	469922	55.66%	7.357%
34	6.915	952	956	957	rBB	359	243	0.03%	0.004%
35	7.055	978	979	982	rVB	281	181	0.02%	0.003%
36	7.104	982	987	988	rBV2	1236	1406	0.17%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039500.D
 Acq On : 27 Dec 2023 17:30
 Operator : JC/MD
 Sample : 05989-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.305	1012	1020	1035	rVV	172205	380108	45.02%	5.951%
38	7.488	1046	1050	1053	rBV2	589	843	0.10%	0.013%
39	7.604	1067	1069	1071	rBV2	168	210	0.02%	0.003%
40	7.951	1124	1126	1129	rBV	285	349	0.04%	0.005%
41	8.262	1172	1177	1181	rBV2	1430	2205	0.26%	0.035%
42	8.323	1181	1187	1200	rBV	116974	191524	22.69%	2.998%
43	8.512	1215	1218	1222	rVB2	359	526	0.06%	0.008%
44	8.646	1234	1240	1254	rBV	425430	659851	78.16%	10.330%
45	8.793	1262	1264	1267	rBV2	309	262	0.03%	0.004%
46	8.890	1278	1280	1282	rBV	356	269	0.03%	0.004%
47	8.951	1284	1290	1303	rVV	81512	125224	14.83%	1.960%
48	9.195	1328	1330	1334	rVB2	243	338	0.04%	0.005%
49	9.317	1348	1350	1353	rBV	247	206	0.02%	0.003%
50	9.384	1355	1361	1376	rBV	367002	526322	62.34%	8.240%
51	9.701	1407	1413	1416	rBV4	949	1605	0.19%	0.025%
52	9.902	1443	1446	1449	rVV2	180	209	0.02%	0.003%
53	9.982	1456	1459	1461	rVB	249	241	0.03%	0.004%
54	10.012	1461	1464	1465	rBV	278	272	0.03%	0.004%
55	10.055	1465	1471	1487	rVV	413557	577337	68.38%	9.039%
56	10.183	1491	1492	1496	rVB3	401	350	0.04%	0.005%
57	10.250	1501	1503	1504	rBV2	418	258	0.03%	0.004%
58	10.299	1510	1511	1515	rVB2	140	181	0.02%	0.003%
59	10.573	1553	1556	1557	rBV2	190	177	0.02%	0.003%
60	11.000	1625	1626	1629	rVB2	197	174	0.02%	0.003%
61	11.091	1637	1641	1646	rBV3	679	1225	0.15%	0.019%
62	11.189	1652	1657	1665	rBV	317393	406788	48.18%	6.369%
63	11.402	1690	1692	1695	rBV	197	172	0.02%	0.003%
64	11.439	1695	1698	1702	rVB2	166	202	0.02%	0.003%
65	11.530	1711	1713	1719	rVV2	167	247	0.03%	0.004%
66	11.609	1724	1726	1728	rVV2	269	193	0.02%	0.003%
67	11.682	1734	1738	1739	rBV2	250	233	0.03%	0.004%
68	11.841	1761	1764	1767	rBV2	162	206	0.02%	0.003%
69	12.024	1788	1794	1805	rBV	414610	540388	64.01%	8.460%
70	12.231	1826	1828	1831	rBV	164	188	0.02%	0.003%
71	12.317	1837	1842	1851	rBV	432857	560296	66.37%	8.772%
72	12.487	1868	1870	1872	rBV2	230	229	0.03%	0.004%
73	12.737	1908	1911	1913	rBV2	187	233	0.03%	0.004%
74	12.829	1924	1926	1927	rBV2	213	170	0.02%	0.003%
75	12.981	1949	1951	1953	rBV	185	169	0.02%	0.003%
76	13.438	2025	2026	2029	rBV2	157	178	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
 Data File : VX039500.D
 Acq On : 27 Dec 2023 17:30
 Operator : JC/MD
 Sample : 05989-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.518	2036	2039	2041	rVB2	182	170	0.02%	0.003%
78	13.725	2071	2073	2075	rVB	290	202	0.02%	0.003%
79	14.005	2116	2119	2124	rBV2	206	353	0.04%	0.006%
80	14.127	2135	2139	2143	rVB2	622	962	0.11%	0.015%
81	14.615	2217	2219	2220	rBV	380	243	0.03%	0.004%
82	14.633	2220	2222	2224	rBV2	177	210	0.02%	0.003%
83	14.694	2230	2232	2236	rBV2	211	280	0.03%	0.004%
84	14.731	2236	2238	2242	rVB2	249	315	0.04%	0.005%
85	14.779	2242	2246	2249	rBV	356	369	0.04%	0.006%
86	14.853	2255	2258	2261	rVB3	271	390	0.05%	0.006%
87	14.883	2261	2263	2264	rBV	245	180	0.02%	0.003%
88	14.981	2277	2279	2282	rVV3	222	220	0.03%	0.003%
89	15.176	2308	2311	2312	rBV	261	317	0.04%	0.005%
90	15.218	2317	2318	2319	rBV	291	186	0.02%	0.003%
91	15.383	2344	2345	2349	rBV3	276	340	0.04%	0.005%
92	15.444	2352	2355	2357	rBV2	247	258	0.03%	0.004%
93	15.523	2366	2368	2369	rBV	295	194	0.02%	0.003%
94	15.560	2373	2374	2378	rBV3	458	588	0.07%	0.009%
95	15.657	2388	2390	2393	rBV2	234	241	0.03%	0.004%
96	15.840	2418	2420	2421	rBV	248	178	0.02%	0.003%
97	15.956	2437	2439	2441	rVB2	306	185	0.02%	0.003%
98	15.999	2445	2446	2448	rBV2	225	176	0.02%	0.003%
99	16.426	2514	2516	2518	rVB2	293	234	0.03%	0.004%
100	16.456	2518	2521	2524	rBV2	355	531	0.06%	0.008%




Sum of corrected areas: 6387414

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039500.D
Acq On : 27 Dec 2023 17:30
Operator : JC/MD
Sample : 05989-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

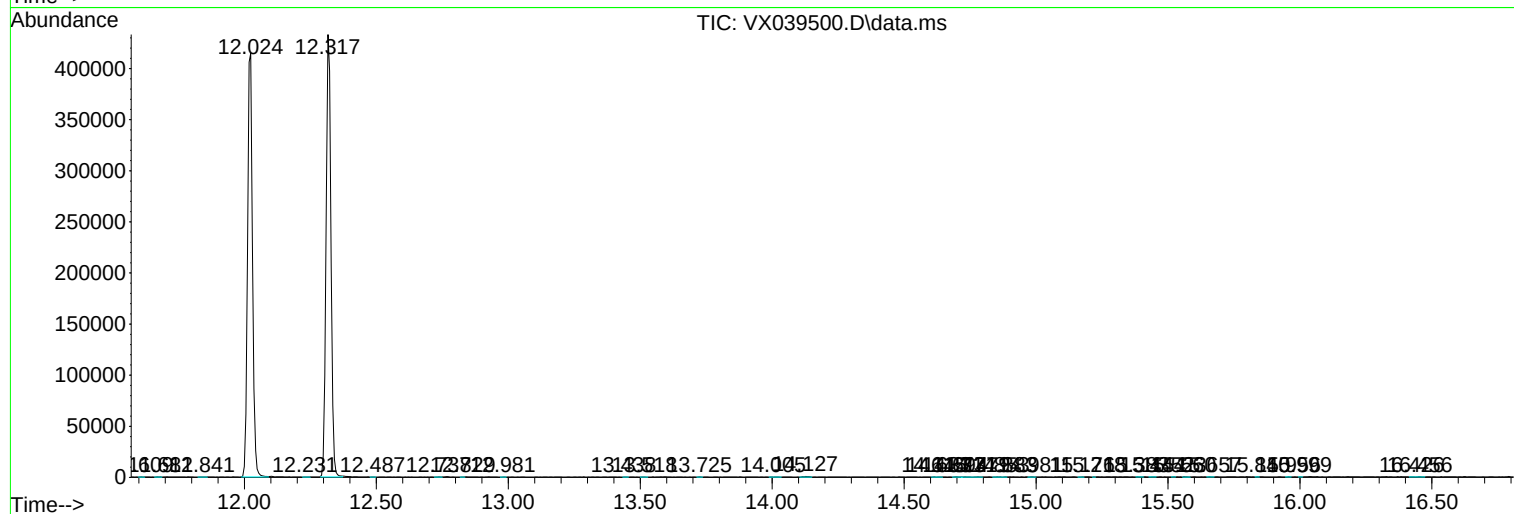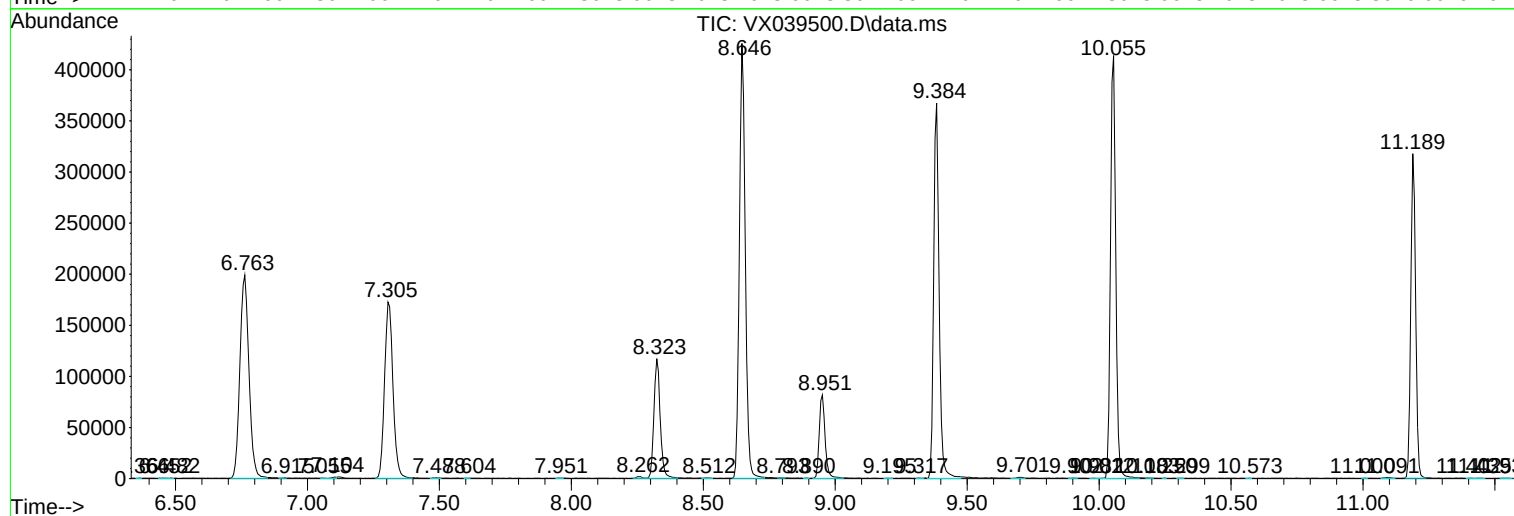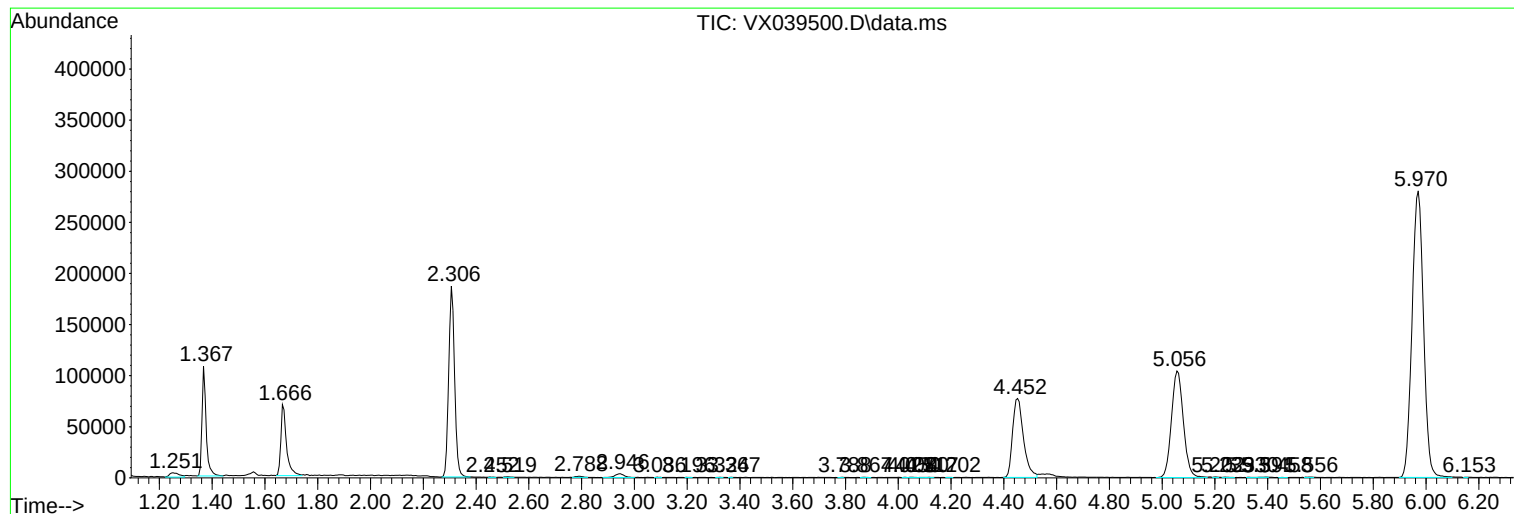

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039500.D
Acq On : 27 Dec 2023 17:30
Operator : JC/MD
Sample : 05989-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039500.D
Acq On : 27 Dec 2023 17:30
Operator : JC/MD
Sample : 05989-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------