
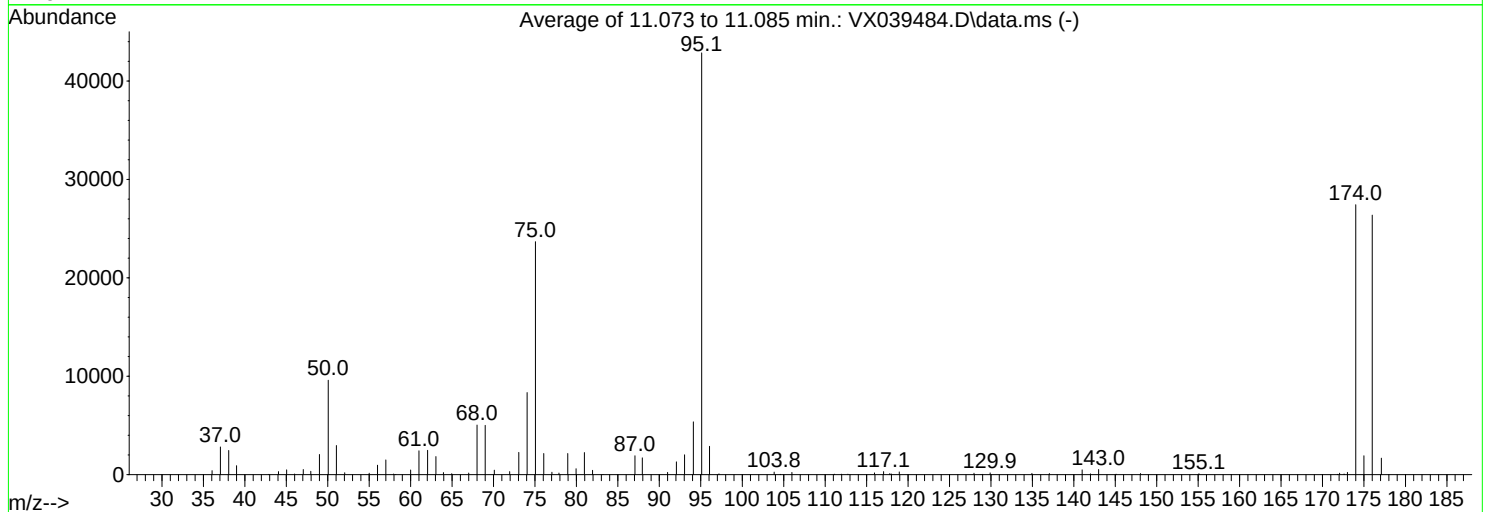


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122723\
Data File : VX039484.D
Acq On : 27 Dec 2023 08:25
Operator : JC/MD
Sample : BFB660
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB660

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Title : VOC Analysis
Last Update : Thu Dec 28 04:06:47 2023

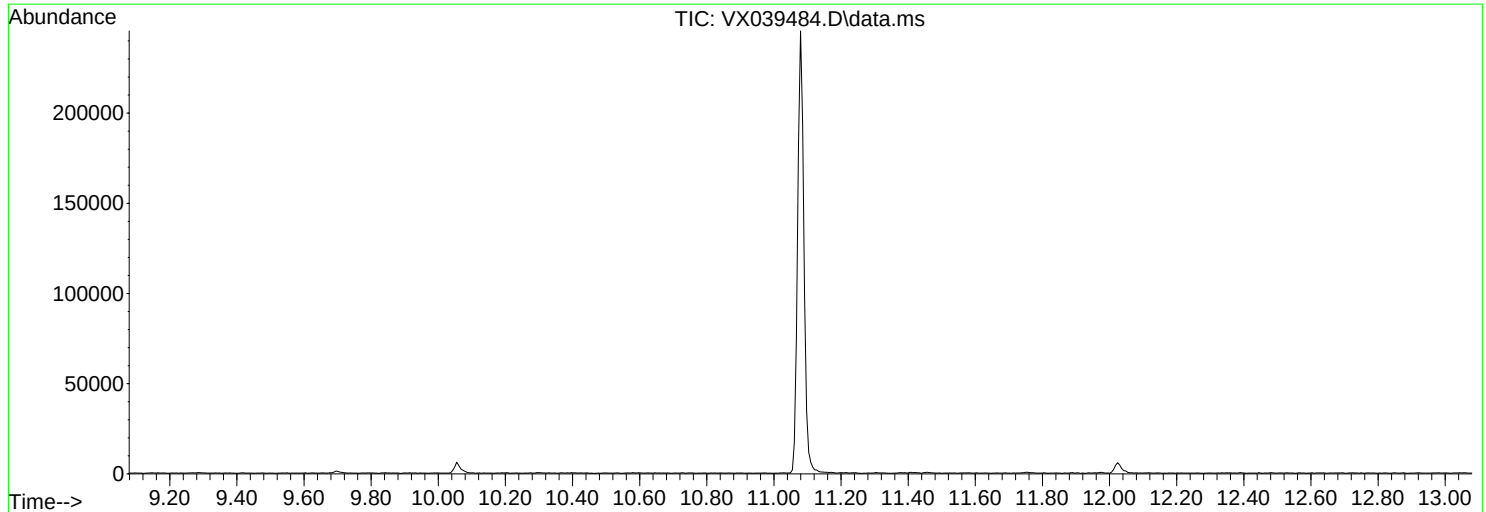

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	9587	PASS
75	95	30	80	55.2	23677	PASS
95	95	100	100	100.0	42859	PASS
96	95	5	9	6.7	2881	PASS
173	174	0.00	2	0.8	223	PASS
174	95	50	120	64.0	27427	PASS
175	174	5	9	7.0	1922	PASS
176	174	95	101	96.2	26379	PASS
177	176	5	9	6.4	1680	PASS

m/z	Abundance
39.00	57.0
40.00	368.0
44.10	143.0

Instrument :
MSVOA_X
ClientSampleId :
BFB660

m/z	Abundance
36.10	339.0
37.00	2818.0
38.00	2429.0
39.00	999.0
40.00	315.0
42.90	115.0
44.20	374.0
45.10	429.0
46.10	68.0
47.10	465.0
47.90	396.0
49.00	1932.0
50.00	9259.0
51.00	2721.0
52.10	179.0
55.00	124.0
56.00	926.0
57.00	1640.0
58.20	67.0
60.00	430.0
61.00	2152.0
62.10	2247.0
63.00	1668.0
64.00	215.0
67.10	174.0
68.00	4694.0
69.00	4955.0
70.10	357.0
72.00	289.0
73.00	2063.0
74.10	7641.0
75.00	22872.0
76.10	2184.0
77.00	261.0
77.80	137.0
78.90	1953.0
80.00	519.0
81.00	2254.0
81.90	401.0
83.20	70.0
87.00	1968.0
88.00	1602.0
91.10	204.0
92.00	1236.0
93.10	1865.0
94.10	4414.0
95.10	36832.0
96.10	2830.0
97.20	135.0
103.80	221.0
106.00	272.0
111.10	57.0
116.00	159.0
117.10	283.0
117.80	173.0
119.00	192.0
127.90	96.0
128.80	66.0
130.10	145.0
135.00	93.0
137.20	76.0
141.00	488.0
142.00	67.0
143.00	310.0
145.10	57.0
148.10	91.0
155.10	110.0
171.80	114.0
173.00	189.0
174.00	21272.0
175.00	1544.0
176.00	20064.0
177.10	1294.0

Instrument :
MSVOA_X
ClientSampleId :
BFB660

m/z	Abundance
36.00	546.0
37.10	3279.0
38.00	2920.0
39.10	1060.0
40.00	361.0
44.00	594.0
45.00	604.0
46.00	80.0
47.10	643.0
48.00	382.0
49.00	2517.0
50.10	11450.0
51.10	3746.0
52.00	241.0
55.00	185.0
55.90	1145.0
57.00	1599.0
57.90	103.0
60.00	559.0
61.00	3201.0
62.00	2856.0
63.10	2298.0
63.90	245.0
65.00	129.0
66.90	192.0
68.00	6071.0
69.00	5741.0
70.10	582.0
71.90	370.0
73.10	2501.0
74.00	9797.0
75.10	27464.0
76.10	2474.0
77.10	268.0
77.90	154.0
79.00	2560.0
80.00	741.0
80.90	2512.0
81.90	522.0
87.10	2369.0
87.90	2220.0
91.00	238.0
92.10	1258.0
93.10	2327.0
94.10	6292.0
95.10	52120.0
96.10	3350.0
97.20	123.0
103.90	332.0
104.60	81.0
106.00	244.0
111.10	81.0
111.90	85.0
112.70	100.0
116.00	178.0
117.10	401.0
118.00	210.0
118.90	366.0
127.80	114.0
129.00	77.0
129.90	178.0
135.00	137.0
137.00	149.0
140.90	492.0
142.00	95.0
143.00	653.0
145.10	51.0
148.10	130.0
155.10	108.0
172.10	178.0
173.00	257.0
174.00	32952.0
175.00	2293.0
176.00	30632.0
177.10	1929.0

Instrument :
MSVOA_X
ClientSampleId :
BFB660

m/z	Abundance
36.00	318.0
37.00	2344.0
38.10	2013.0
39.10	865.0
40.00	388.0
44.00	402.0
45.00	444.0
45.90	54.0
47.00	474.0
47.90	254.0
49.00	1713.0
50.10	8051.0
51.10	2408.0
52.00	156.0
55.00	144.0
56.10	799.0
57.00	1256.0
58.00	77.0
60.00	439.0
61.00	1923.0
62.10	2296.0
63.10	1551.0
64.00	196.0
64.90	143.0
67.00	107.0
68.00	4372.0
69.00	4345.0
70.10	444.0
72.00	266.0
73.00	2218.0
74.00	7579.0
75.10	20696.0
76.00	1788.0
77.00	223.0
78.00	220.0
79.00	1910.0
79.90	527.0
81.00	1979.0
82.00	389.0
87.00	1406.0
88.00	1318.0
90.90	234.0
92.00	1433.0
93.00	1880.0
94.10	5380.0
95.10	39624.0
96.00	2462.0
103.80	209.0
106.00	190.0
112.00	64.0
112.80	53.0
115.90	195.0
117.00	266.0
117.80	195.0
118.90	277.0
128.00	221.0
129.80	201.0
134.90	150.0
137.00	125.0
141.10	481.0
142.00	86.0
143.00	597.0
145.10	57.0
148.00	120.0
155.10	100.0
159.00	62.0
172.00	245.0
172.60	189.0
173.00	224.0
174.00	28056.0
175.00	1930.0
176.00	28440.0
177.10	1816.0
178.00	55.0

Instrument :
MSVOA_X
ClientSampleId :
BFB660