

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044511.D
 Acq On : 27 Dec 2024 10:58
 Operator : JC/MD
 Sample : VX1227WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 27 22:11:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 27 22:07:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	214198	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	184007	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	82693	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	86665	44.213	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	88.420%		
7) Chloroethane-d5	1.648	69	63548	41.851	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	83.700%		
11) 1,1-Dichloroethene-d2	2.294	65	37406	44.621	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.240%		
21) 2-Butanone-d5	4.459	46	94825	79.014	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	79.010%		
24) Chloroform-d	5.056	84	161716	43.452	ug/L	0.01
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.900%		
26) 1,2-Dichloroethane-d4	5.952	65	112508	42.747	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.500%		
32) Benzene-d6	5.964	84	316533	49.785	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.580%		
36) 1,2-Dichloropropane-d6	7.299	67	97548	49.411	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	98.820%		
41) Toluene-d8	8.647	98	274276	46.655	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.320%		
43) trans-1,3-Dichloroprop...	8.946	79	38460	40.539	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	81.080%		
47) 2-Hexanone-d5	9.384	63	64383	83.640	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	83.640%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	132731	50.140	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	100.280%		
66) 1,2-Dichlorobenzene-d4	12.317	152	92926	48.230	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.460%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	8.324	75	3022	1.286	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044511.D
Acq On : 27 Dec 2024 10:58
Operator : JC/MD
Sample : VX1227WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Dec 27 22:11:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 27 22:07:46 2024
Response via : Initial Calibration

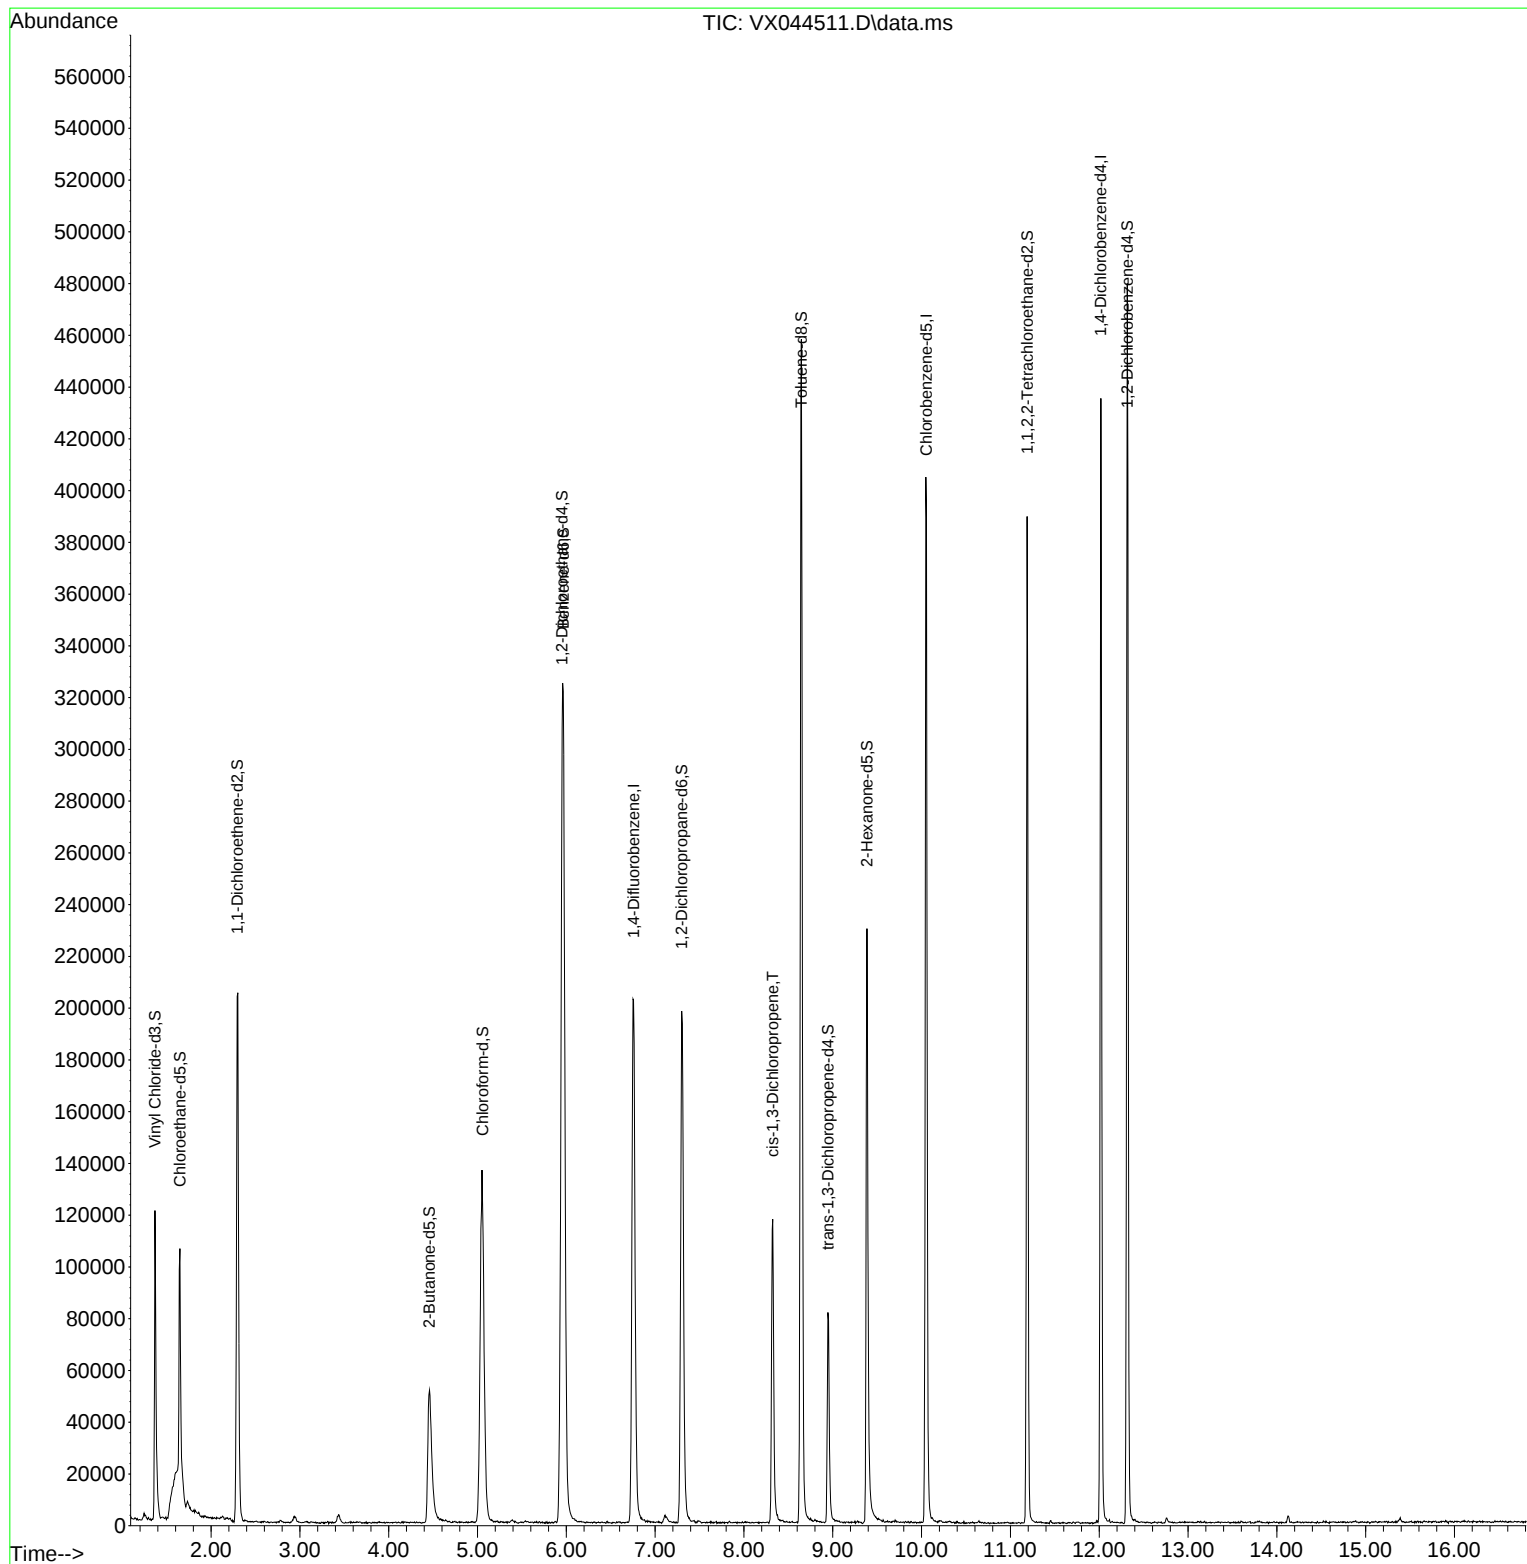

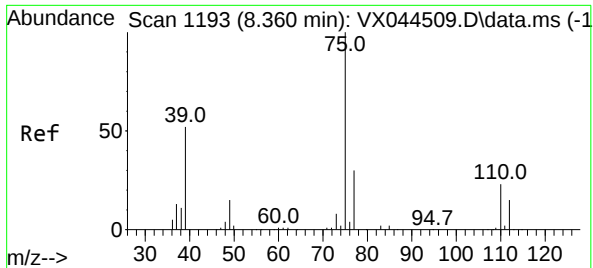

#39
 cis-1,3-Dichloropropene
 Concen: 1.286 ug/L
 RT: 8.324 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VX044511.D
 Acq: 27 Dec 2024 10:58

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 75 Resp: 3022
 Ion Ratio Lower Upper
 75 100
 77 39.3 21.6 40.0

