

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044524.D
 Acq On : 27 Dec 2024 16:31
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 27 22:16:45 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 27 22:07:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	198168	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	169330	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	69786	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	66022	36.406	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	72.820%		
7) Chloroethane-d5	1.642	69	57016	40.587	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	81.180%		
11) 1,1-Dichloroethene-d2	2.294	65	29304	37.784	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	75.560%		
21) 2-Butanone-d5	4.458	46	126288	113.742	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	113.740%		
24) Chloroform-d	5.050	84	171224	49.728	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.460%		
26) 1,2-Dichloroethane-d4	5.952	65	119263	48.979	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.960%		
32) Benzene-d6	5.964	84	297597	50.864	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	101.720%		
36) 1,2-Dichloropropane-d6	7.306	67	102232	56.272	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	112.540%		
41) Toluene-d8	8.647	98	256314	47.379	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.760%		
43) trans-1,3-Dichloroprop...	8.945	79	39598	45.356	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	90.720%		
47) 2-Hexanone-d5	9.384	63	84845	119.776	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	119.780%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	142630	58.550	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	117.100%		
66) 1,2-Dichlorobenzene-d4	12.317	152	91717	56.407	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	112.820%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	8.952	75	2825	1.378	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044524.D
Acq On : 27 Dec 2024 16:31
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Dec 27 22:16:45 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 27 22:07:46 2024
Response via : Initial Calibration

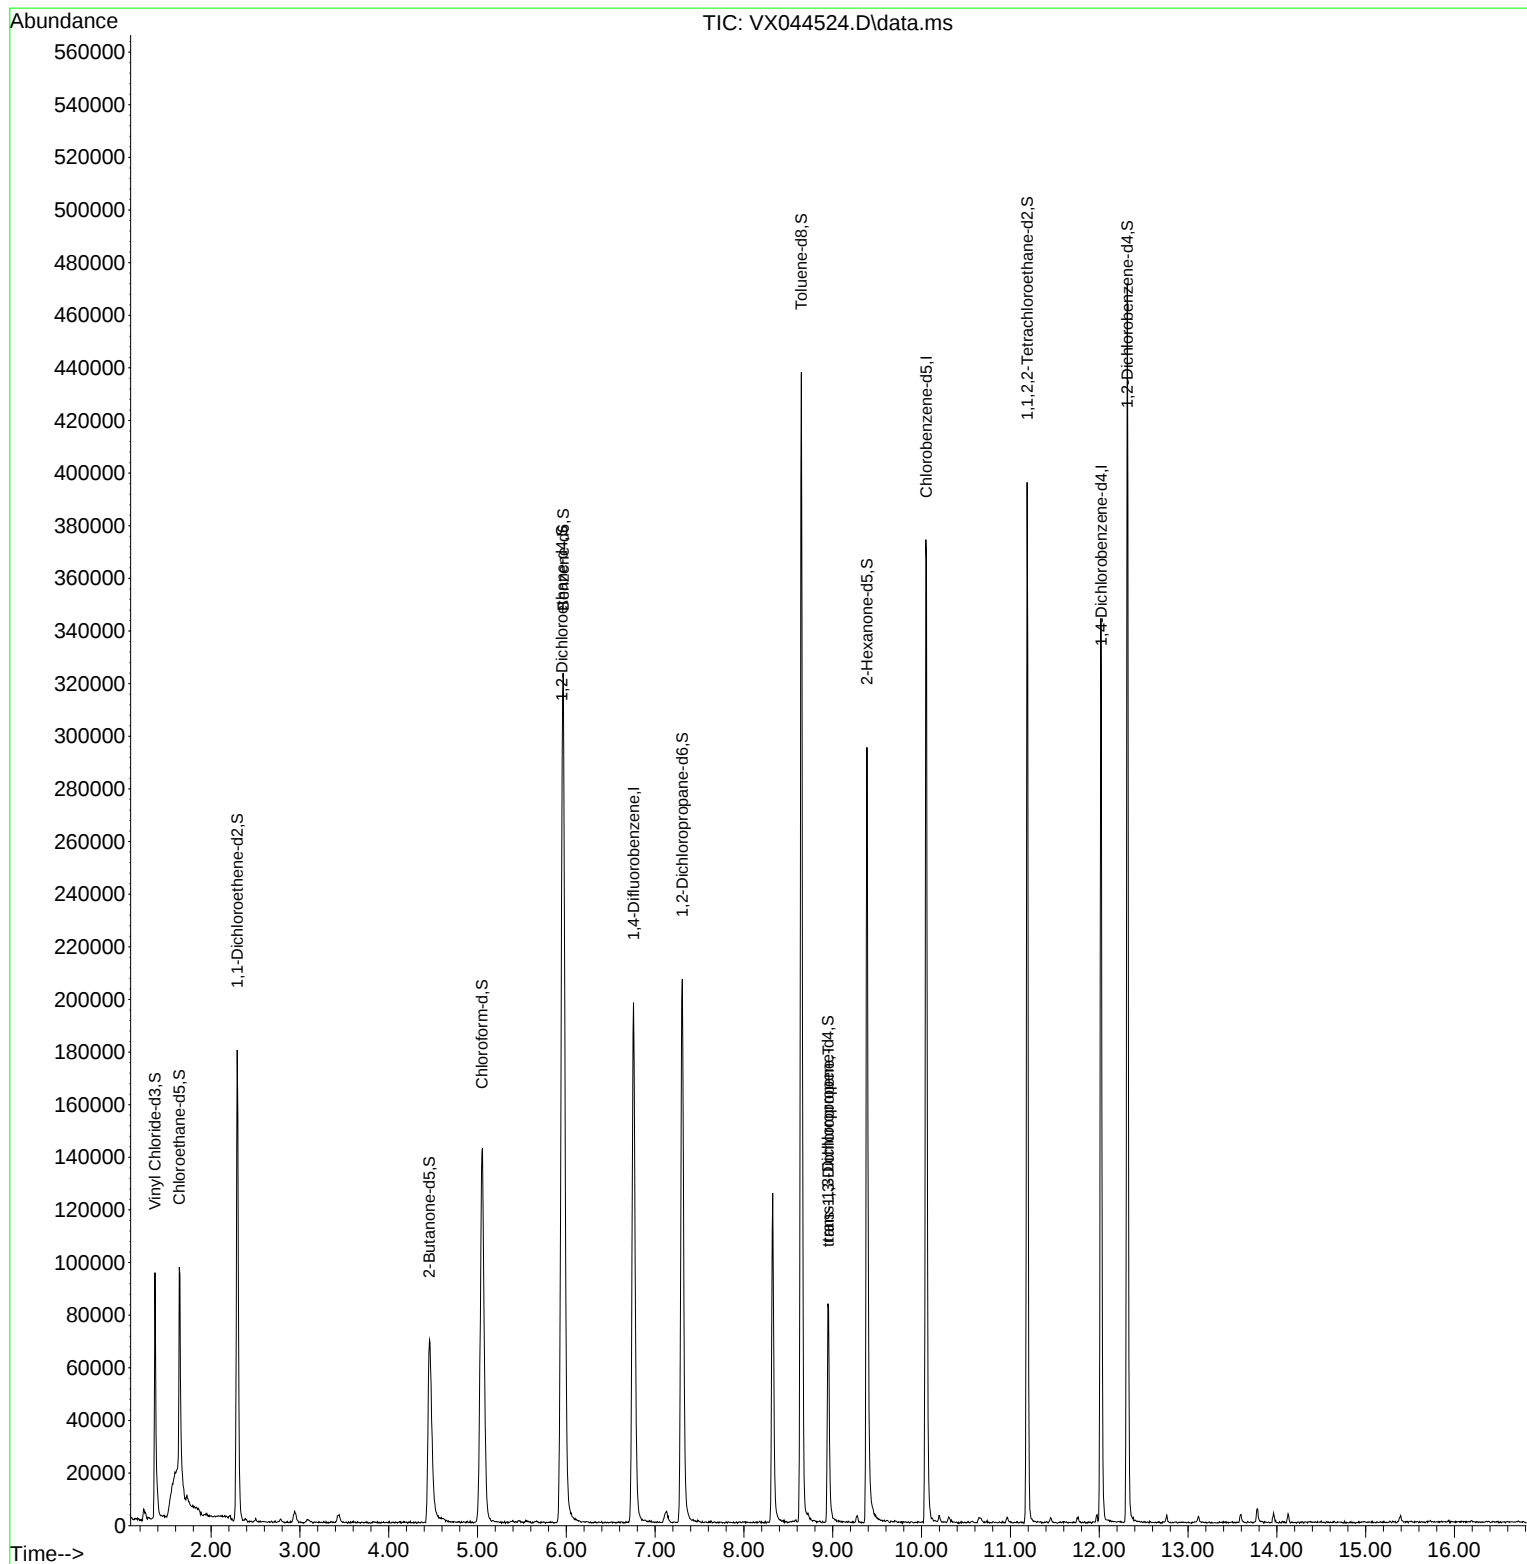

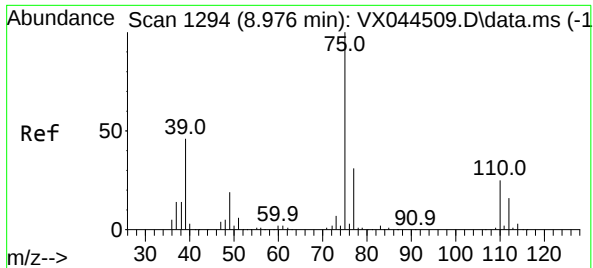

#44
 trans-1,3-Dichloropropene
 Concen: 1.378 ug/L
 RT: 8.952 min Scan# 11
 Delta R.T. -0.024 min
 Lab File: VX044524.D
 Acq: 27 Dec 2024 16:31

Instrument :
 MSVOA_X
 ClientSampleId :

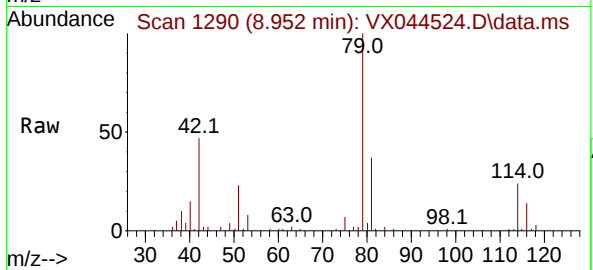

Tgt Ion: 75 Resp: 2825
 Ion Ratio Lower Upper
 75 100
 77 27.6 21.8 40.6

