




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044512.D
Acq On : 27 Dec 2024 11:26
Operator : JC/MD
Sample : P5344-06 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CE8

Manual IntegrationsAPPROVED

Quant Time: Dec 30 03:15:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 27 22:07:46 2024
Response via : Initial Calibration

Reviewed By :John Carlone 12/30/2024
Supervised By :Mahesh Dadoda 12/30/2024

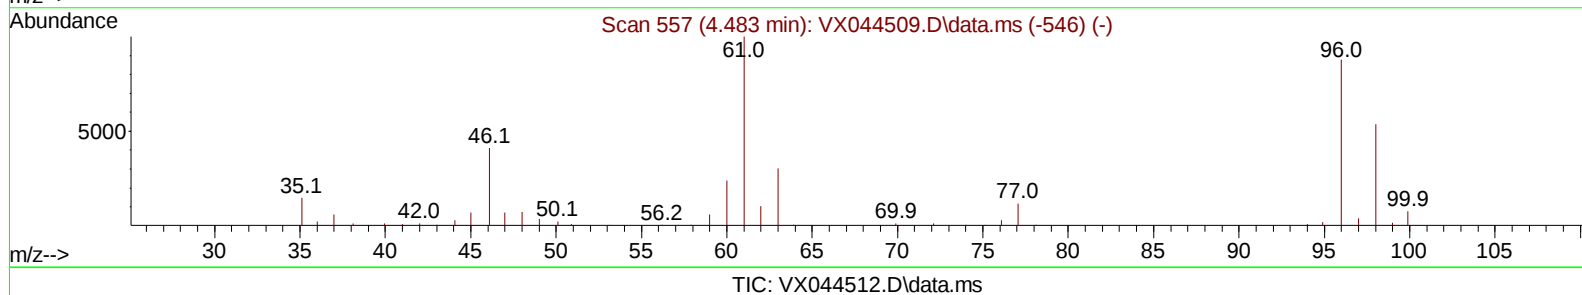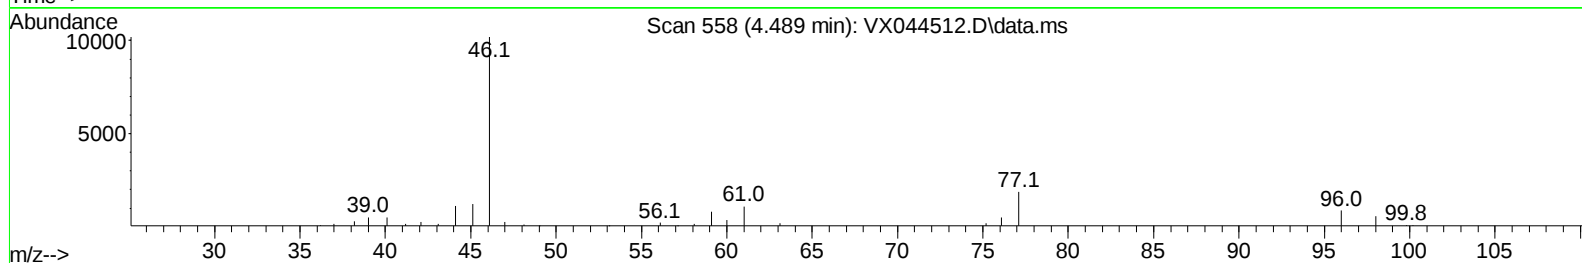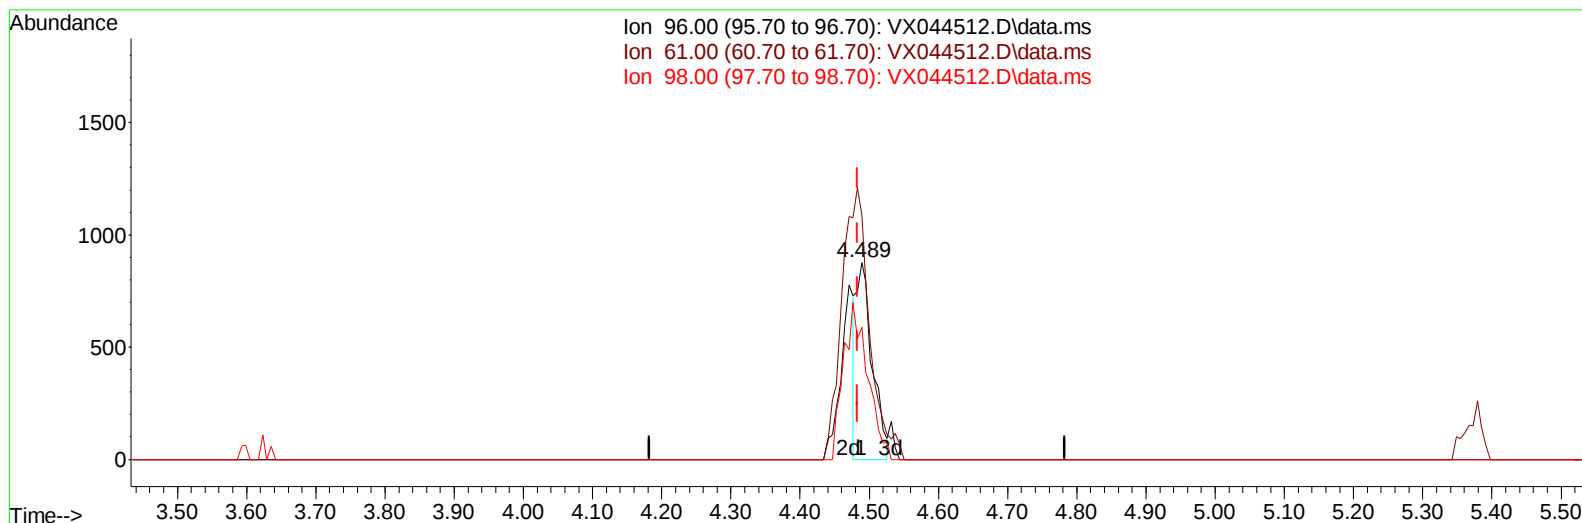

(20) cis-1,2-Dichloroethene (T)

4.489min (+ 0.006) 1.03 ug/L

response 1375

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	121.50	124.06
98.00	63.70	67.05
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044512.D
Acq On : 27 Dec 2024 11:26
Operator : JC/MD
Sample : P5344-06 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CE8

Manual IntegrationsAPPROVED

Quant Time: Dec 27 22:11:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 27 22:07:46 2024
Response via : Initial Calibration

Reviewed By :John Carlone 12/30/2024
Supervised By :Mahesh Dadoda 12/30/2024

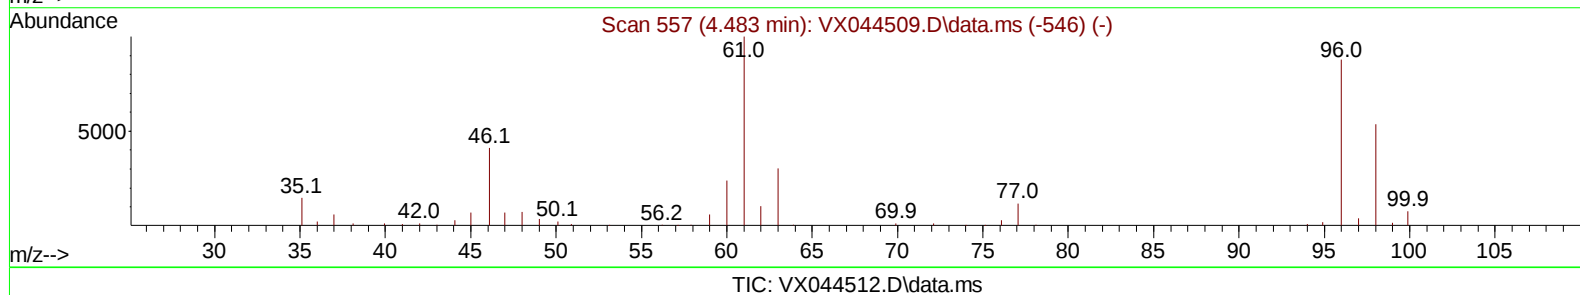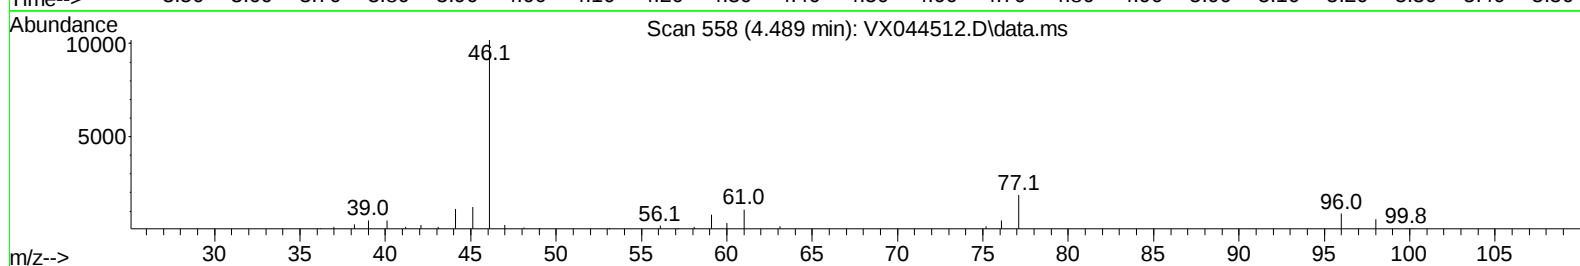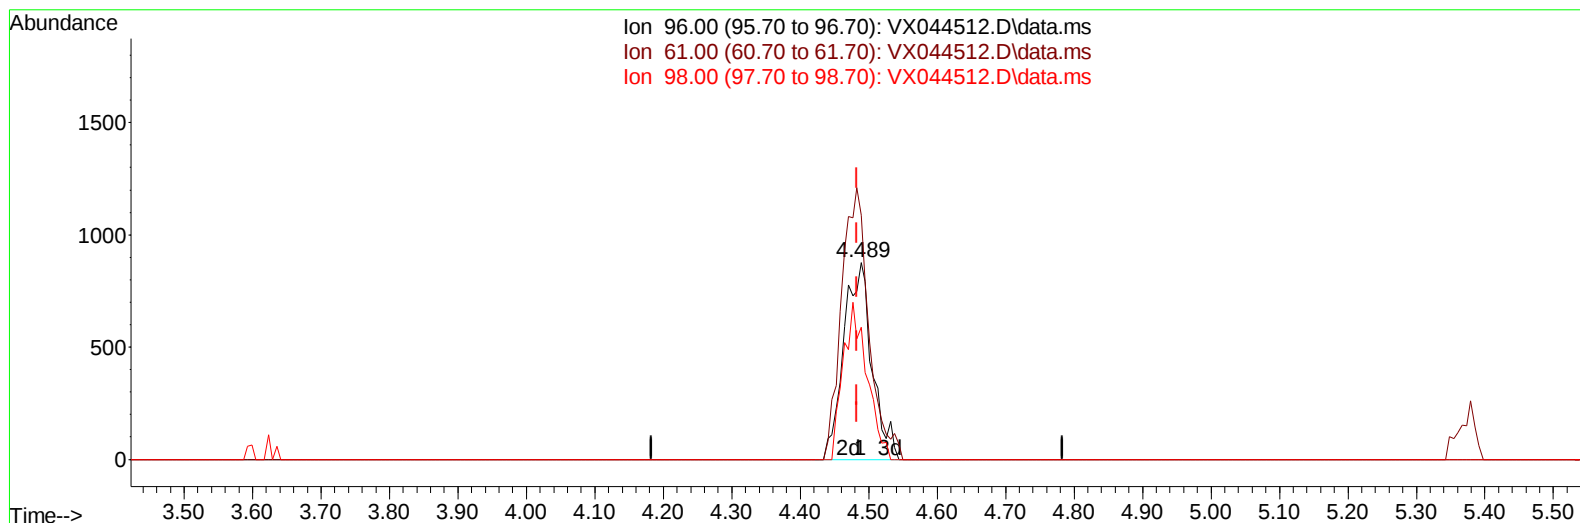

(20) cis-1,2-Dichloroethene (T)

4.489min (+ 0.006) 1.88 ug/L m

response 2508

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	121.50	124.06
98.00	63.70	67.05
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044512.D
 Acq On : 27 Dec 2024 11:26
 Operator : JC/MD
 Sample : P5344-06 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CE8

Manual IntegrationsAPPROVED

Quant Time: Dec 27 22:11:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 27 22:07:46 2024
 Response via : Initial Calibration

Reviewed By :John Carlone 12/30/2024
 Supervised By :Mahesh Dadoda 12/30/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	177954	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.049	117	159236	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	65531	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	72298	44.396	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	88.800%	
7) Chloroethane-d5	1.642	69	53533	42.436	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	84.880%	
11) 1,1-Dichloroethene-d2	2.294	65	30972	44.471	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	88.940%	
21) 2-Butanone-d5	4.452	46	82949	83.195	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	83.200%	
24) Chloroform-d	5.050	84	129603	41.916	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	83.840%	
26) 1,2-Dichloroethane-d4	5.946	65	92348	42.234	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	84.460%	
32) Benzene-d6	5.964	84	258231	46.933	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	93.860%	
36) 1,2-Dichloropropane-d6	7.299	67	77072	45.112	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	90.220%	
41) Toluene-d8	8.647	98	226301	44.483	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	88.960%	
43) trans-1,3-Dichloroprop...	8.945	79	35943	43.779	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	87.560%	
47) 2-Hexanone-d5	9.384	63	59616	89.495	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	89.500%	
56) 1,1,2,2-Tetrachloroeth...	11.189	84	100560	43.897	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	87.800%	
66) 1,2-Dichlorobenzene-d4	12.317	152	74278	48.648	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	97.300%	
Target Compounds						
						Qvalue
9) Trichlorofluoromethane	1.874	101	27332	10.213	ug/L	96
20) cis-1,2-Dichloroethene	4.489	96	2508m	1.878	ug/L	
34) Trichloroethene	7.117	95	1417889	1074.005	ug/L	99
42) Toluene	8.720	91	6676	1.303	ug/L	100
46) Tetrachloroethene	9.269	164	10468	11.886	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044512.D
Acq On : 27 Dec 2024 11:26
Operator : JC/MD
Sample : P5344-06 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CE8

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/30/2024
Supervised By :Mahesh Dadoda 12/30/2024

Quant Time: Dec 27 22:11:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 27 22:07:46 2024
Response via : Initial Calibration

