

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044511.D
 Acq On : 27 Dec 2024 10:58
 Operator : JC/MD
 Sample : VX1227WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK747

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	56	rVB	118892	142894	14.45%	2.077%
2	1.648	88	92	103	rVB	99737	149774	15.15%	2.177%
3	2.300	192	199	209	rBV	204598	333435	33.72%	4.845%
4	2.776	275	277	281	rBV3	909	1248	0.13%	0.018%
5	2.934	298	303	304	rBV2	2159	2574	0.26%	0.037%
6	3.123	332	334	337	rBV3	539	713	0.07%	0.010%
7	3.239	352	353	357	rBV3	479	597	0.06%	0.009%
8	3.288	359	361	362	rBV	492	397	0.04%	0.006%
9	3.312	363	365	367	rVB2	921	808	0.08%	0.012%
10	3.331	367	368	369	rBV	602	376	0.04%	0.005%
11	3.434	378	385	396	rVB3	3282	8046	0.81%	0.117%
12	3.745	434	436	437	rVB	623	359	0.04%	0.005%
13	3.782	439	442	444	rBV3	427	564	0.06%	0.008%
14	3.818	446	448	450	rBV	424	401	0.04%	0.006%
15	3.885	457	459	460	rBV2	459	395	0.04%	0.006%
16	4.312	527	529	532	rBV2	459	418	0.04%	0.006%
17	4.385	539	541	543	rBV2	382	421	0.04%	0.006%
18	4.459	545	553	568	rVV2	51003	163180	16.50%	2.371%
19	5.050	637	650	667	rBV2	136301	417399	42.21%	6.066%
20	5.343	697	698	701	rBV	457	497	0.05%	0.007%
21	5.538	726	730	732	rBV3	802	1093	0.11%	0.016%
22	5.641	745	747	750	rBV3	474	563	0.06%	0.008%
23	5.696	754	756	758	rBV2	567	496	0.05%	0.007%
24	5.781	767	770	771	rVB2	585	454	0.05%	0.007%
25	5.873	782	785	788	rBV3	700	930	0.09%	0.014%
26	5.958	788	799	818	rBV3	324433	988932	100.00%	14.371%
27	6.233	841	844	846	rBV2	538	502	0.05%	0.007%
28	6.361	863	865	868	rVB2	499	416	0.04%	0.006%
29	6.458	879	881	883	rBV	746	584	0.06%	0.008%
30	6.568	897	899	901	rBV3	533	435	0.04%	0.006%
31	6.751	920	929	944	rBV	202304	507650	51.33%	7.377%
32	7.111	982	988	989	rBV4	3111	4435	0.45%	0.064%
33	7.299	1011	1019	1037	rBV	197834	445299	45.03%	6.471%
34	7.482	1047	1049	1050	rBV2	863	744	0.08%	0.011%
35	7.836	1104	1107	1109	rBV2	791	893	0.09%	0.013%
36	7.909	1117	1119	1121	rVB2	536	425	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044511.D
 Acq On : 27 Dec 2024 10:58
 Operator : JC/MD
 Sample : VX1227WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK747

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

37	7.927	1121	1122	1125	rBV2	516	498	0.05%	0.007%
38	8.324	1180	1187	1200	rBV	117542	209822	21.22%	3.049%
39	8.647	1233	1240	1254	rBV	457467	743400	75.17%	10.803%
40	8.946	1284	1289	1299	rBV	80993	128296	12.97%	1.864%
41	9.153	1321	1323	1326	rBV3	478	687	0.07%	0.010%
42	9.281	1340	1344	1345	rBV2	868	922	0.09%	0.013%
43	9.384	1356	1361	1381	rBV	229200	350938	35.49%	5.100%
44	9.567	1389	1391	1394	rVB3	998	725	0.07%	0.011%
45	9.702	1412	1413	1415	rBV2	851	486	0.05%	0.007%
46	9.817	1430	1432	1435	rBV2	602	622	0.06%	0.009%
47	9.848	1435	1437	1439	rVB	651	495	0.05%	0.007%
48	9.884	1441	1443	1445	rVB3	589	474	0.05%	0.007%
49	9.927	1448	1450	1453	rVB2	517	559	0.06%	0.008%
50	9.994	1460	1461	1464	rBV	448	360	0.04%	0.005%
51	10.049	1465	1470	1480	rBV	403632	578072	58.45%	8.400%
52	10.299	1509	1511	1512	rBV	540	437	0.04%	0.006%
53	10.403	1525	1528	1531	rVB3	639	688	0.07%	0.010%
54	10.476	1539	1540	1542	rVB	859	404	0.04%	0.006%
55	10.573	1554	1556	1559	rVB3	640	573	0.06%	0.008%
56	10.646	1566	1568	1570	rVB2	712	441	0.04%	0.006%
57	10.750	1582	1585	1588	rVB3	484	560	0.06%	0.008%
58	10.866	1600	1604	1607	rBV3	335	383	0.04%	0.006%
59	11.189	1652	1657	1672	rVB	388979	482094	48.75%	7.006%
60	11.451	1698	1700	1706	rBV3	1172	1603	0.16%	0.023%
61	11.707	1740	1742	1746	rBV2	607	701	0.07%	0.010%
62	11.750	1746	1749	1751	rBV2	534	902	0.09%	0.013%
63	11.921	1774	1777	1778	rVB2	473	448	0.05%	0.007%
64	11.969	1783	1785	1788	rBV3	807	746	0.08%	0.011%
65	12.018	1788	1793	1802	rBV	434249	543465	54.95%	7.898%
66	12.256	1829	1832	1835	rVB3	589	729	0.07%	0.011%
67	12.317	1835	1842	1854	rBV	479267	623061	63.00%	9.054%
68	12.597	1886	1888	1891	rBV2	347	502	0.05%	0.007%
69	12.622	1891	1892	1894	rVV	561	442	0.04%	0.006%
70	12.664	1898	1899	1902	rBV2	434	513	0.05%	0.007%
71	12.762	1911	1915	1924	rBV4	1903	3567	0.36%	0.052%
72	12.963	1947	1948	1950	rBV	607	428	0.04%	0.006%
73	13.109	1970	1972	1976	rBV3	549	635	0.06%	0.009%
74	13.146	1976	1978	1980	rVV2	650	525	0.05%	0.008%
75	13.189	1983	1985	1987	rVB2	708	459	0.05%	0.007%
76	13.597	2048	2052	2056	rBV4	721	906	0.09%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044511.D
 Acq On : 27 Dec 2024 10:58
 Operator : JC/MD
 Sample : VX1227WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK747

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	14.030	2122	2123	2125	rBV2	437	432	0.04%	0.006%
78	14.128	2133	2139	2143	rBV2	2697	4239	0.43%	0.062%
79	14.292	2163	2166	2168	rVB3	469	436	0.04%	0.006%
80	14.457	2191	2193	2196	rBV2	690	587	0.06%	0.009%
81	14.493	2196	2199	2201	rVV2	309	447	0.05%	0.006%
82	14.524	2203	2204	2208	rVV3	740	671	0.07%	0.010%
83	14.554	2208	2209	2215	rVB4	903	1009	0.10%	0.015%
84	14.597	2215	2216	2217	rBV	654	371	0.04%	0.005%
85	14.829	2251	2254	2256	rBV3	358	488	0.05%	0.007%
86	14.865	2256	2260	2261	rBV4	499	619	0.06%	0.009%
87	14.944	2270	2273	2274	rBV2	436	406	0.04%	0.006%
88	15.024	2284	2286	2290	rVB3	707	857	0.09%	0.012%
89	15.109	2298	2300	2304	rVB2	650	759	0.08%	0.011%
90	15.231	2318	2320	2323	rVB2	655	637	0.06%	0.009%
91	15.255	2323	2324	2327	rBV2	569	432	0.04%	0.006%
92	15.390	2340	2346	2351	rBV4	1897	3366	0.34%	0.049%
93	15.560	2373	2374	2376	rBV	664	534	0.05%	0.008%
94	15.585	2376	2378	2380	rVV2	667	625	0.06%	0.009%
95	15.841	2418	2420	2422	rBV2	511	411	0.04%	0.006%
96	15.902	2428	2430	2435	rVB4	1052	1427	0.14%	0.021%
97	15.956	2435	2439	2440	rBV3	843	1318	0.13%	0.019%
98	16.005	2446	2447	2449	rBV2	469	405	0.04%	0.006%
99	16.091	2458	2461	2462	rBV3	531	604	0.06%	0.009%
100	16.578	2539	2541	2544	rVB3	553	405	0.04%	0.006%

Sum of corrected areas: 6881400




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044511.D
Acq On : 27 Dec 2024 10:58
Operator : JC/MD
Sample : VX1227WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK747

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

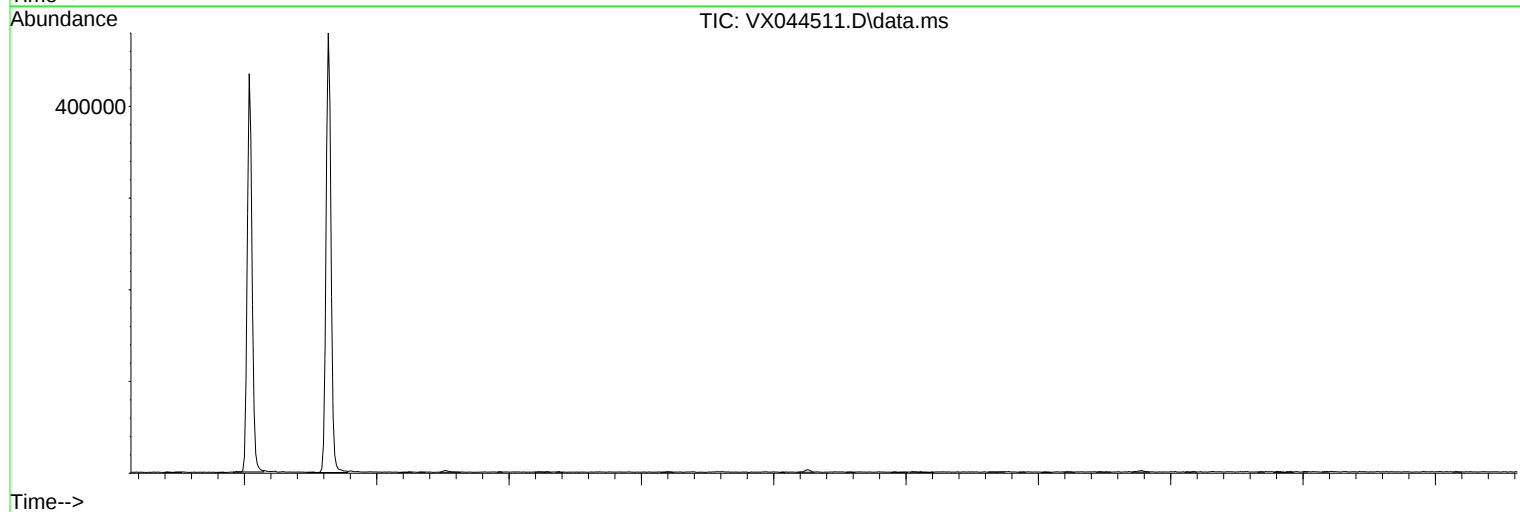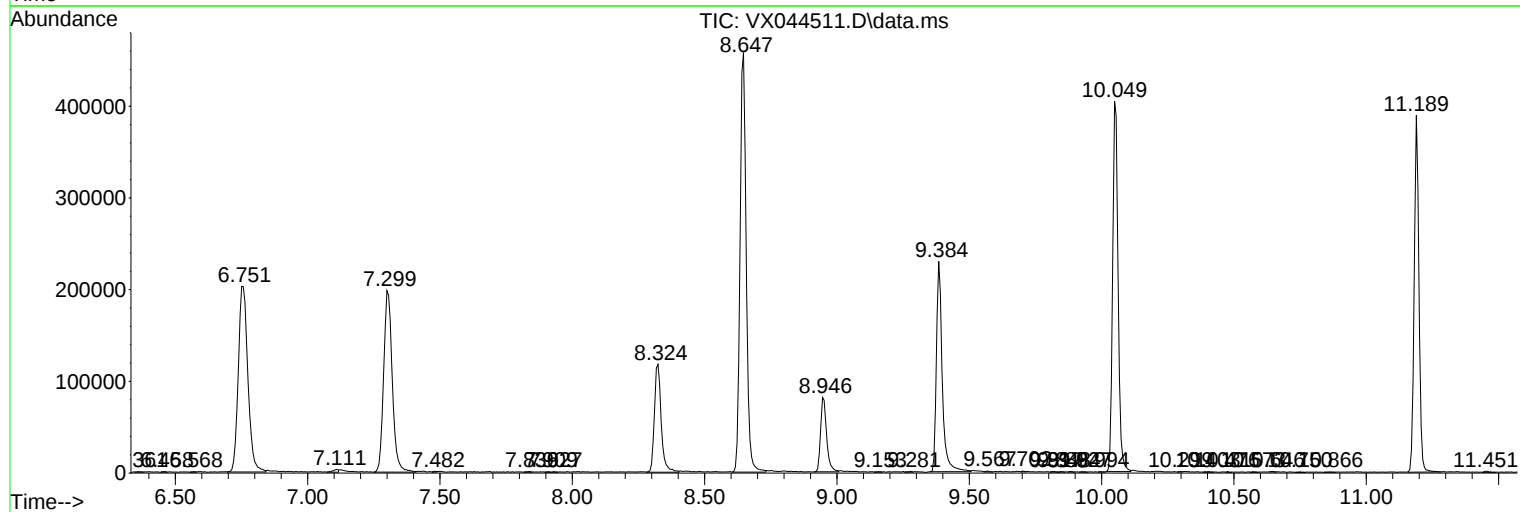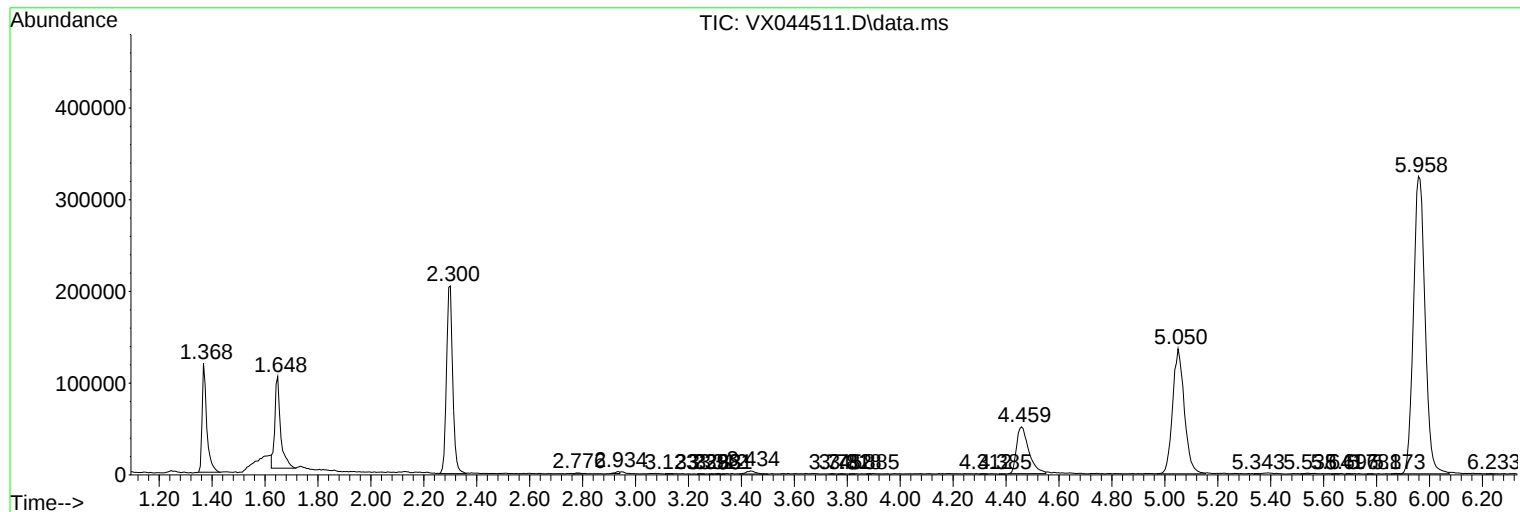

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044511.D
Acq On : 27 Dec 2024 10:58
Operator : JC/MD
Sample : VX1227WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK747

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044511.D
Acq On : 27 Dec 2024 10:58
Operator : JC/MD
Sample : VX1227WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK747

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
