

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044512.D
 Acq On : 27 Dec 2024 11:26
 Operator : JC/MD
 Sample : P5344-06 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044512.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	31	rBV3	3059	5562	0.07%	0.039%
2	1.368	43	46	59	rVB	97788	121839	1.44%	0.847%
3	1.642	88	91	102	rVB	81645	122867	1.45%	0.854%
4	1.874	125	129	136	rVB	45437	66252	0.78%	0.461%
5	2.294	192	198	209	rBV	181809	281126	3.33%	1.955%
6	2.703	261	265	266	rBV2	829	1171	0.01%	0.008%
7	2.782	273	278	285	rVB4	3660	6701	0.08%	0.047%
8	2.934	299	303	310	rVB2	3228	6329	0.07%	0.044%
9	3.093	321	329	331	rBV5	2562	5521	0.07%	0.038%
10	3.184	342	344	347	rBV3	606	768	0.01%	0.005%
11	3.251	353	355	357	rBV	854	879	0.01%	0.006%
12	3.434	378	385	392	rVV4	3595	8500	0.10%	0.059%
13	3.593	409	411	412	rBV	1208	819	0.01%	0.006%
14	3.855	451	454	458	rBV3	534	720	0.01%	0.005%
15	3.898	458	461	462	rBV2	638	441	0.01%	0.003%
16	3.916	462	464	466	rBV3	425	429	0.01%	0.003%
17	3.965	471	472	476	rVB2	465	414	0.00%	0.003%
18	4.007	476	479	480	rBV	659	551	0.01%	0.004%
19	4.111	494	496	499	rVB2	798	508	0.01%	0.004%
20	4.452	545	552	565	rBV	45433	150102	1.78%	1.044%
21	4.879	616	622	623	rBV4	566	889	0.01%	0.006%
22	5.050	638	650	669	rBV	107773	337330	3.99%	2.346%
23	5.361	696	701	702	rBV3	1326	1902	0.02%	0.013%
24	5.848	780	781	785	rVB3	529	417	0.00%	0.003%
25	5.958	788	799	817	rBV3	268923	819344	9.70%	5.698%
26	6.294	852	854	857	rVB3	570	477	0.01%	0.003%
27	6.336	857	861	864	rBV4	681	1128	0.01%	0.008%
28	6.489	882	886	889	rVB3	540	786	0.01%	0.005%
29	6.513	889	890	893	rBV2	451	584	0.01%	0.004%
30	6.586	900	902	904	rBV2	401	455	0.01%	0.003%
31	6.611	904	906	908	rVB	693	499	0.01%	0.003%
32	6.659	910	914	917	rBV3	374	731	0.01%	0.005%
33	6.751	921	929	944	rBV	170420	419559	4.97%	2.918%
34	7.117	977	989	1012	rBV	3956671	8447978	100.00%	58.752%
35	7.299	1012	1019	1037	rVB	159185	364553	4.32%	2.535%
36	7.824	1102	1105	1109	rVV2	686	1037	0.01%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044512.D
 Acq On : 27 Dec 2024 11:26
 Operator : JC/MD
 Sample : P5344-06 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	8.122	1152	1154	1156	rBV2	408	439	0.01%	0.003%
38	8.324	1181	1187	1202	rBV	95856	168269	1.99%	1.170%
39	8.476	1210	1212	1214	rVB2	565	429	0.01%	0.003%
40	8.500	1214	1216	1218	rBV3	688	674	0.01%	0.005%
41	8.586	1225	1230	1233	rBV3	2436	3642	0.04%	0.025%
42	8.647	1233	1240	1248	rBV	371789	604279	7.15%	4.202%
43	8.945	1282	1289	1301	rBV	74120	120143	1.42%	0.836%
44	9.153	1319	1323	1331	rBV6	2819	5060	0.06%	0.035%
45	9.269	1336	1342	1351	rBV	55950	86231	1.02%	0.600%
46	9.336	1351	1353	1355	rVB	625	416	0.00%	0.003%
47	9.384	1356	1361	1375	rBV	210414	331305	3.92%	2.304%
48	9.610	1396	1398	1404	rVB3	2070	2704	0.03%	0.019%
49	10.049	1465	1470	1486	rBV	359507	515200	6.10%	3.583%
50	10.195	1491	1494	1501	rVV3	4715	7154	0.08%	0.050%
51	10.305	1507	1512	1518	rVB2	4565	7413	0.09%	0.052%
52	10.549	1550	1552	1556	rVB2	618	651	0.01%	0.005%
53	10.585	1556	1558	1560	rBV2	670	617	0.01%	0.004%
54	10.646	1561	1568	1576	rBV4	5079	11853	0.14%	0.082%
55	10.787	1589	1591	1592	rBV2	593	479	0.01%	0.003%
56	10.854	1600	1602	1604	rBV2	379	448	0.01%	0.003%
57	10.927	1611	1614	1616	rVB3	641	775	0.01%	0.005%
58	10.963	1616	1620	1627	rBV3	4369	7216	0.09%	0.050%
59	11.067	1635	1637	1640	rBV3	545	748	0.01%	0.005%
60	11.189	1652	1657	1663	rBV	278915	366059	4.33%	2.546%
61	11.451	1696	1700	1704	rBV2	3692	4403	0.05%	0.031%
62	11.567	1717	1719	1720	rBV2	445	414	0.00%	0.003%
63	11.634	1728	1730	1733	rVB3	555	419	0.00%	0.003%
64	11.689	1737	1739	1741	rVB2	504	406	0.00%	0.003%
65	11.713	1741	1743	1745	rBV	553	422	0.00%	0.003%
66	11.756	1746	1750	1753	rBV2	3578	4246	0.05%	0.030%
67	11.841	1762	1764	1767	rVV2	560	741	0.01%	0.005%
68	11.896	1771	1773	1776	rVB	731	553	0.01%	0.004%
69	11.939	1779	1780	1782	rBV2	414	416	0.00%	0.003%
70	11.975	1782	1786	1788	rBV2	3317	4190	0.05%	0.029%
71	12.018	1788	1793	1802	rVV	333112	415785	4.92%	2.892%
72	12.317	1837	1842	1859	rVV	388215	493103	5.84%	3.429%
73	12.725	1907	1909	1910	rVV2	632	463	0.01%	0.003%
74	12.762	1912	1915	1919	rVB3	1902	2449	0.03%	0.017%
75	12.951	1945	1946	1952	rVB2	919	1100	0.01%	0.008%
76	13.122	1969	1974	1979	rVB4	2663	4184	0.05%	0.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044512.D
 Acq On : 27 Dec 2024 11:26
 Operator : JC/MD
 Sample : P5344-06 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	13.164	1979	1981	1984	rBV2	385	462	0.01%	0.003%
78	13.268	1995	1998	1999	rBV2	648	587	0.01%	0.004%
79	13.353	2010	2012	2015	rVB2	451	546	0.01%	0.004%
80	13.554	2042	2045	2048	rBV2	570	933	0.01%	0.006%
81	13.597	2048	2052	2056	rVV6	1763	2707	0.03%	0.019%
82	13.689	2065	2067	2069	rVB2	684	518	0.01%	0.004%
83	13.780	2079	2082	2088	rVB3	2676	3233	0.04%	0.022%
84	13.963	2108	2112	2115	rBV4	2408	3006	0.04%	0.021%
85	14.091	2131	2133	2135	rVV2	529	410	0.00%	0.003%
86	14.127	2135	2139	2144	rVB2	2391	3334	0.04%	0.023%
87	14.195	2149	2150	2154	rBV2	539	591	0.01%	0.004%
88	14.310	2167	2169	2171	rBV2	797	840	0.01%	0.006%
89	14.524	2202	2204	2207	rBV3	613	734	0.01%	0.005%
90	14.713	2233	2235	2237	rVB2	581	419	0.00%	0.003%
91	14.737	2237	2239	2243	rVB2	532	442	0.01%	0.003%
92	14.780	2245	2246	2248	rBV2	698	580	0.01%	0.004%
93	14.938	2268	2272	2273	rBV2	683	673	0.01%	0.005%
94	15.578	2375	2377	2381	rBV4	521	594	0.01%	0.004%
95	15.719	2398	2400	2405	rBV5	660	878	0.01%	0.006%
96	15.902	2428	2430	2432	rVB3	748	550	0.01%	0.004%
97	16.060	2453	2456	2459	rVB3	638	781	0.01%	0.005%
98	16.231	2483	2484	2487	rVB3	600	459	0.01%	0.003%
99	16.487	2524	2526	2529	rVB3	704	694	0.01%	0.005%
100	16.773	2571	2573	2575	rBV2	485	459	0.01%	0.003%




Sum of corrected areas: 14379096

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044512.D
Acq On : 27 Dec 2024 11:26
Operator : JC/MD
Sample : P5344-06 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

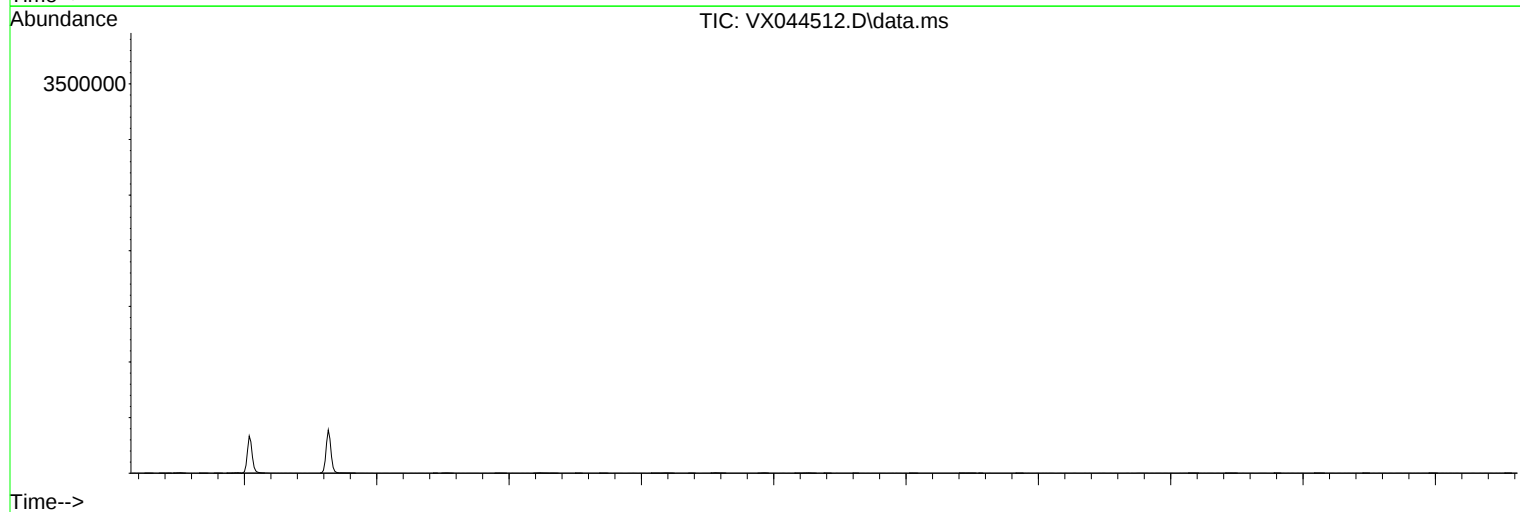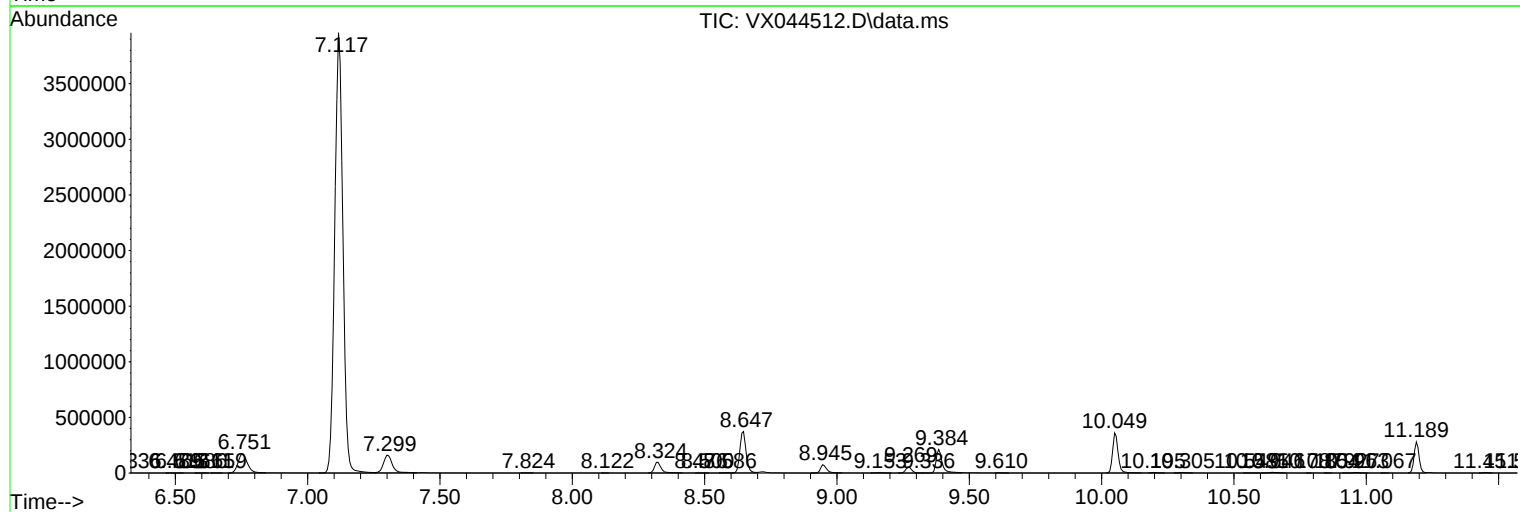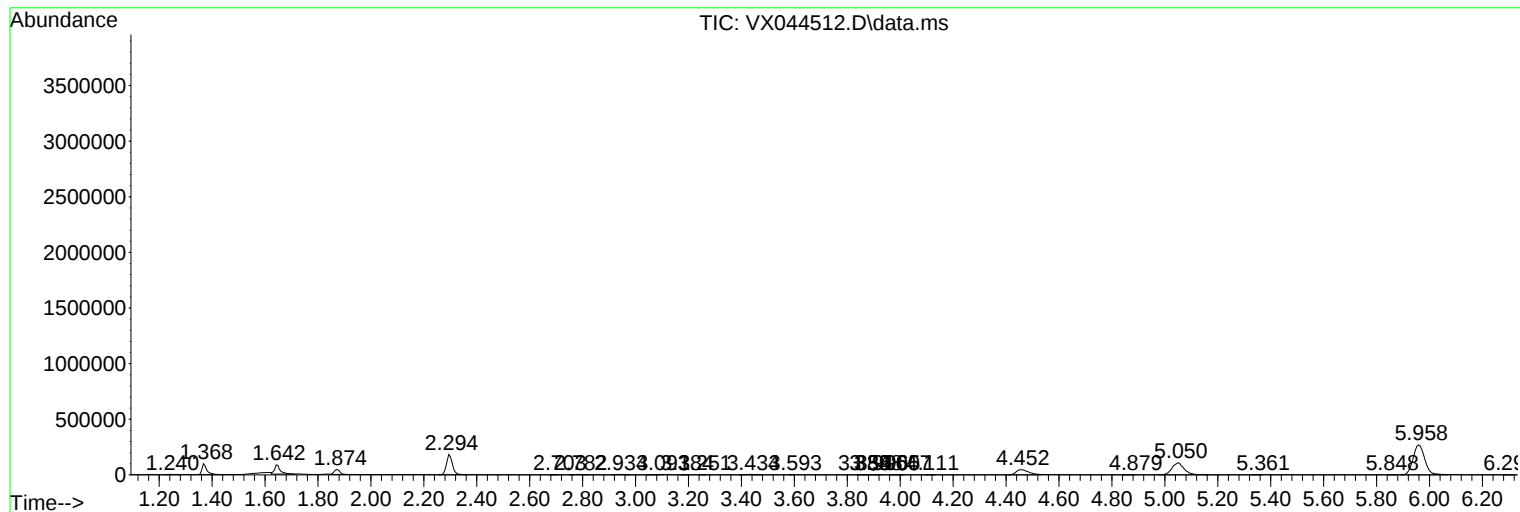

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044512.D
Acq On : 27 Dec 2024 11:26
Operator : JC/MD
Sample : P5344-06 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044512.D
Acq On : 27 Dec 2024 11:26
Operator : JC/MD
Sample : P5344-06 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------