

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044513.D
 Acq On : 27 Dec 2024 11:49
 Operator : JC/MD
 Sample : P5344-09 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044513.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.245	22	26	27	rBV2	3134	3831	0.10%	0.037%
2	1.367	43	46	55	rBV	113693	138799	3.71%	1.348%
3	1.648	89	92	103	rVB	92766	139105	3.72%	1.351%
4	1.867	124	128	133	rVB	17744	24617	0.66%	0.239%
5	2.294	192	198	210	rVB	213160	326037	8.72%	3.166%
6	2.946	299	305	314	rVB3	4389	10777	0.29%	0.105%
7	3.025	314	318	319	rBV2	512	544	0.01%	0.005%
8	3.227	347	351	353	rBV2	461	714	0.02%	0.007%
9	3.440	380	386	393	rVB6	2736	6839	0.18%	0.066%
10	3.531	399	401	404	rBV3	577	747	0.02%	0.007%
11	3.574	406	408	412	rVB3	411	496	0.01%	0.005%
12	3.696	425	428	431	rBV2	531	1012	0.03%	0.010%
13	3.757	435	438	439	rBV2	441	445	0.01%	0.004%
14	3.873	456	457	459	rBV	676	431	0.01%	0.004%
15	3.983	474	475	478	rVB2	692	397	0.01%	0.004%
16	4.044	481	485	487	rBV3	629	813	0.02%	0.008%
17	4.458	545	553	572	rBV	51550	172579	4.62%	1.676%
18	4.867	616	620	623	rVB4	334	523	0.01%	0.005%
19	4.909	625	627	629	rVB2	605	421	0.01%	0.004%
20	4.928	629	630	632	rBV	460	445	0.01%	0.004%
21	4.982	636	639	640	rBV2	581	695	0.02%	0.007%
22	5.049	640	650	666	rBV	124492	396016	10.59%	3.846%
23	5.312	692	693	694	rBV	836	474	0.01%	0.005%
24	5.360	698	701	702	rBV3	730	854	0.02%	0.008%
25	5.476	719	720	723	rBV2	492	415	0.01%	0.004%
26	5.763	764	767	769	rBV3	482	543	0.01%	0.005%
27	5.964	788	800	819	rVV2	330351	973289	26.03%	9.452%
28	6.354	858	864	866	rBV2	700	1192	0.03%	0.012%
29	6.403	870	872	874	rVB2	577	430	0.01%	0.004%
30	6.470	880	883	885	rBV3	470	631	0.02%	0.006%
31	6.756	921	930	949	rBV2	163708	405145	10.83%	3.935%
32	7.006	969	971	974	rBV3	667	807	0.02%	0.008%
33	7.116	980	989	1011	rBV	1703399	3739233	100.00%	36.313%
34	7.305	1012	1020	1039	rVB	194171	434342	11.62%	4.218%
35	7.537	1056	1058	1062	rVB3	675	618	0.02%	0.006%
36	7.592	1065	1067	1071	rVB4	393	486	0.01%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044513.D
 Acq On : 27 Dec 2024 11:49
 Operator : JC/MD
 Sample : P5344-09 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	7.634	1071	1074	1076	rBV2	750	651	0.02%	0.006%
38	7.769	1094	1096	1098	rBV2	457	425	0.01%	0.004%
39	7.860	1109	1111	1114	rVB2	676	541	0.01%	0.005%
40	7.915	1118	1120	1122	rVV2	538	472	0.01%	0.005%
41	7.970	1128	1129	1132	rVV2	840	533	0.01%	0.005%
42	8.323	1179	1187	1200	rBV	130359	222515	5.95%	2.161%
43	8.451	1206	1208	1209	rBV	497	414	0.01%	0.004%
44	8.470	1209	1211	1213	rVV2	428	403	0.01%	0.004%
45	8.537	1221	1222	1227	rBV4	523	772	0.02%	0.007%
46	8.646	1233	1240	1249	rBV	488664	776850	20.78%	7.544%
47	8.945	1284	1289	1307	rBV2	88400	140466	3.76%	1.364%
48	9.171	1324	1326	1330	rBV2	548	619	0.02%	0.006%
49	9.268	1336	1342	1349	rBV	51731	75318	2.01%	0.731%
50	9.384	1356	1361	1377	rBV	249648	389784	10.42%	3.785%
51	9.738	1416	1419	1422	rBV2	545	656	0.02%	0.006%
52	10.006	1460	1463	1465	rBV	395	424	0.01%	0.004%
53	10.049	1465	1470	1487	rVV	327999	484124	12.95%	4.701%
54	10.305	1509	1512	1517	rVB7	884	1562	0.04%	0.015%
55	10.384	1524	1525	1528	rVB2	721	468	0.01%	0.005%
56	10.524	1546	1548	1550	rVB	725	487	0.01%	0.005%
57	10.579	1556	1557	1561	rBV2	424	498	0.01%	0.005%
58	10.744	1579	1584	1585	rBV4	505	753	0.02%	0.007%
59	10.774	1585	1589	1591	rVB2	423	572	0.02%	0.006%
60	10.872	1603	1605	1607	rBV2	408	403	0.01%	0.004%
61	11.061	1634	1636	1638	rVB3	581	572	0.02%	0.006%
62	11.140	1647	1649	1650	rBV	771	531	0.01%	0.005%
63	11.189	1652	1657	1667	rVB	331734	425828	11.39%	4.135%
64	11.298	1672	1675	1676	rBV	798	523	0.01%	0.005%
65	11.384	1686	1689	1694	rBV3	671	915	0.02%	0.009%
66	11.518	1710	1711	1715	rBV2	626	632	0.02%	0.006%
67	11.554	1715	1717	1722	rVB3	596	891	0.02%	0.009%
68	11.646	1729	1732	1734	rBV3	565	548	0.01%	0.005%
69	11.750	1748	1749	1756	rBV4	804	1580	0.04%	0.015%
70	11.914	1772	1776	1778	rBV3	523	512	0.01%	0.005%
71	11.975	1784	1786	1788	rBV2	652	578	0.02%	0.006%
72	12.018	1788	1793	1801	rBV	295256	377959	10.11%	3.670%
73	12.158	1814	1816	1819	rBV3	617	672	0.02%	0.007%
74	12.316	1837	1842	1858	rVB	451565	576135	15.41%	5.595%
75	12.621	1890	1892	1895	rBV2	432	420	0.01%	0.004%
76	12.676	1898	1901	1904	rVB4	760	878	0.02%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044513.D
 Acq On : 27 Dec 2024 11:49
 Operator : JC/MD
 Sample : P5344-09 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	12.707	1904	1906	1907	rBV	584	454	0.01%	0.004%
78	12.755	1911	1914	1920	rVB3	1661	2611	0.07%	0.025%
79	13.005	1953	1955	1960	rBV4	545	710	0.02%	0.007%
80	13.109	1970	1972	1978	rBV2	574	1189	0.03%	0.012%
81	13.316	2002	2006	2007	rBV2	641	629	0.02%	0.006%
82	13.511	2036	2038	2041	rVB3	642	739	0.02%	0.007%
83	13.688	2064	2067	2069	rBV4	643	903	0.02%	0.009%
84	13.725	2071	2073	2076	rVV2	575	486	0.01%	0.005%
85	13.828	2087	2090	2093	rBV4	738	1019	0.03%	0.010%
86	13.853	2093	2094	2096	rVB	753	509	0.01%	0.005%
87	13.877	2096	2098	2100	rBV2	707	622	0.02%	0.006%
88	13.908	2100	2103	2104	rVV3	489	509	0.01%	0.005%
89	14.127	2131	2139	2143	rBV3	2618	4569	0.12%	0.044%
90	14.389	2180	2182	2184	rVB3	541	557	0.01%	0.005%
91	14.414	2184	2186	2188	rBV2	492	410	0.01%	0.004%
92	14.505	2199	2201	2204	rVV2	630	436	0.01%	0.004%
93	15.072	2293	2294	2297	rVB3	652	403	0.01%	0.004%
94	15.115	2297	2301	2302	rBV2	618	707	0.02%	0.007%
95	15.353	2338	2340	2342	rBV2	627	544	0.01%	0.005%
96	15.389	2342	2346	2352	rVB6	1750	2903	0.08%	0.028%
97	15.444	2352	2355	2357	rBV2	621	689	0.02%	0.007%
98	15.505	2361	2365	2368	rBV3	704	1074	0.03%	0.010%
99	16.127	2465	2467	2468	rBV	612	444	0.01%	0.004%
100	16.316	2496	2498	2499	rBV2	656	486	0.01%	0.005%




Sum of corrected areas: 10297228

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044513.D
Acq On : 27 Dec 2024 11:49
Operator : JC/MD
Sample : P5344-09 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

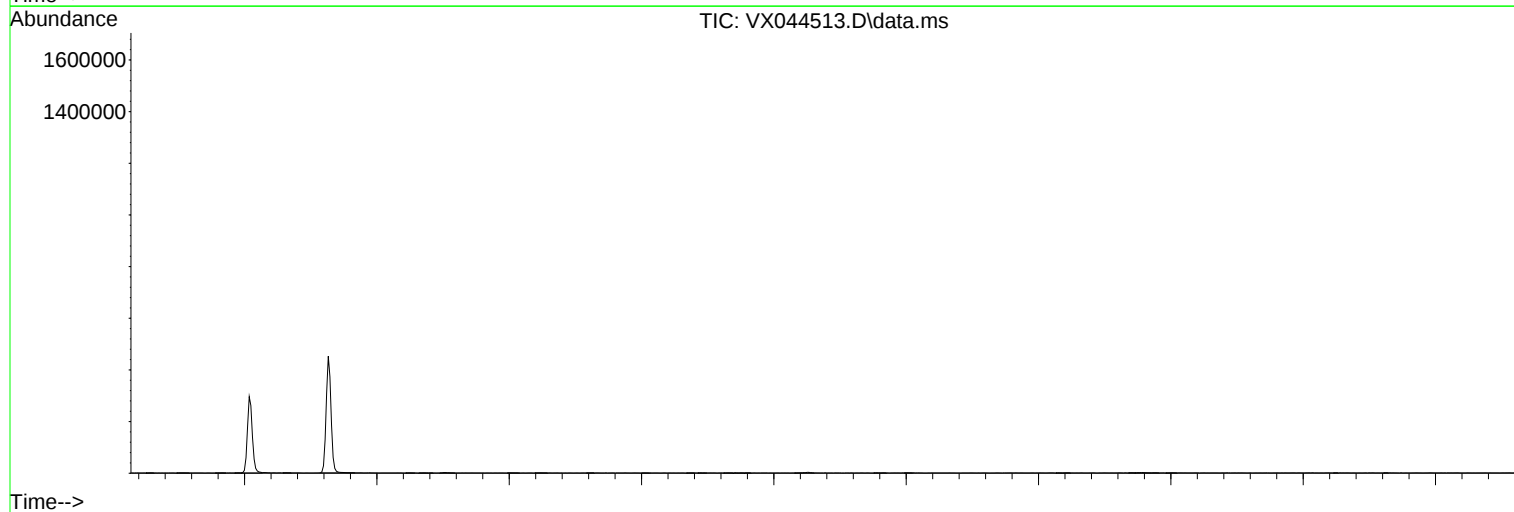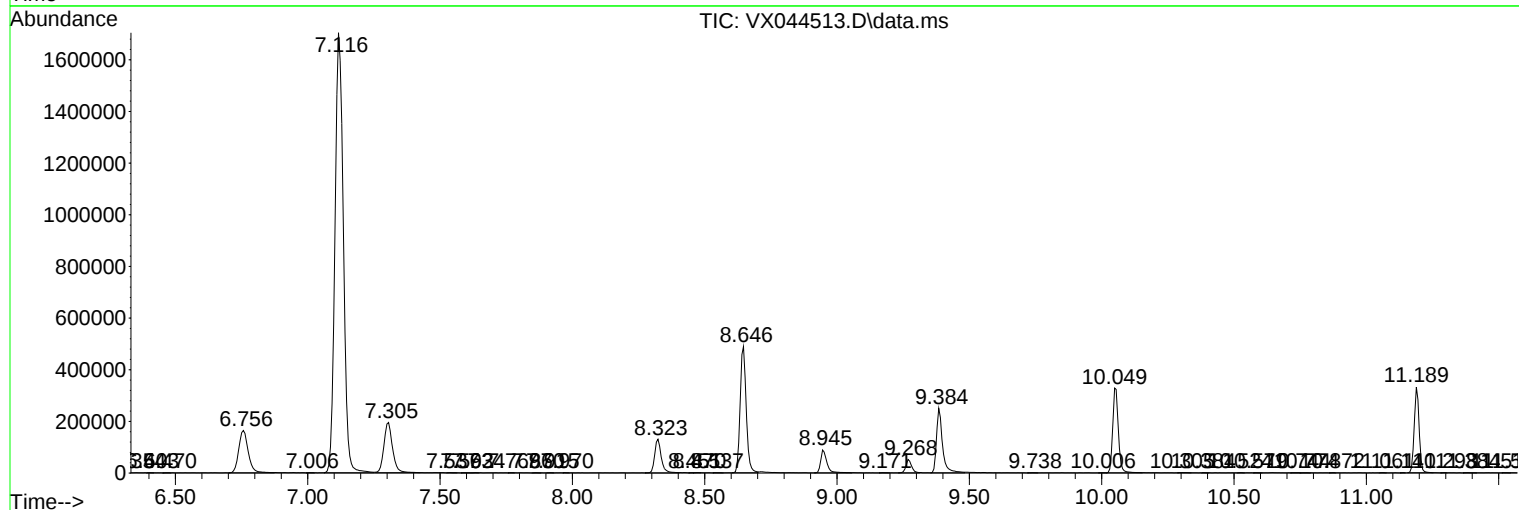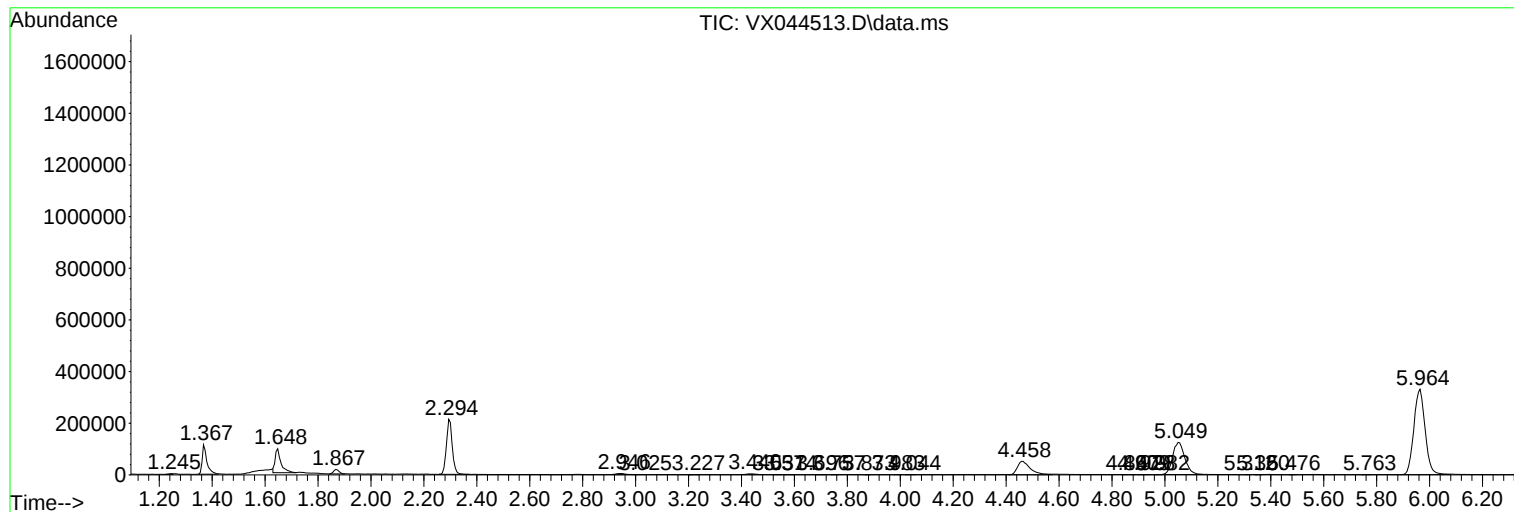

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044513.D
Acq On : 27 Dec 2024 11:49
Operator : JC/MD
Sample : P5344-09 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044513.D
Acq On : 27 Dec 2024 11:49
Operator : JC/MD
Sample : P5344-09 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------