

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044514.D
 Acq On : 27 Dec 2024 12:12
 Operator : JC/MD
 Sample : P5344-12 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COCH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044514.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	27	rBV2	2691	3288	0.01%	0.011%
2	1.368	42	46	56	rBV	116498	139351	0.63%	0.477%
3	1.642	88	91	102	rVB	94995	140954	0.64%	0.483%
4	1.868	124	128	139	rVB	110775	163948	0.75%	0.561%
5	2.294	192	198	209	rBV	208406	325322	1.48%	1.114%
6	2.788	274	279	287	rBV7	3849	6911	0.03%	0.024%
7	2.947	295	305	314	rVV4	3660	9292	0.04%	0.032%
8	3.063	322	324	325	rBV2	681	437	0.00%	0.001%
9	3.087	325	328	331	rVV2	1064	1376	0.01%	0.005%
10	3.142	336	337	339	rVV2	526	353	0.00%	0.001%
11	3.184	342	344	346	rBV2	482	339	0.00%	0.001%
12	3.306	362	364	366	rBV2	523	419	0.00%	0.001%
13	3.434	379	385	399	rBV6	3562	8920	0.04%	0.031%
14	3.593	407	411	412	rBV2	493	628	0.00%	0.002%
15	3.965	469	472	474	rBV3	476	552	0.00%	0.002%
16	4.038	480	484	485	rBV4	592	678	0.00%	0.002%
17	4.123	497	498	502	rVB3	558	344	0.00%	0.001%
18	4.160	502	504	505	rBV	410	389	0.00%	0.001%
19	4.459	542	553	573	rBV	56617	191555	0.87%	0.656%
20	4.879	618	622	624	rVB	595	659	0.00%	0.002%
21	4.904	624	626	628	rBV2	466	422	0.00%	0.001%
22	5.056	639	651	666	rBV	132277	416605	1.90%	1.427%
23	5.385	702	705	706	rBV2	894	893	0.00%	0.003%
24	5.654	747	749	750	rBV2	466	365	0.00%	0.001%
25	5.751	763	765	770	rVB2	607	762	0.00%	0.003%
26	5.843	777	780	783	rVB3	508	564	0.00%	0.002%
27	5.964	787	800	817	rBV2	323696	974458	4.44%	3.337%
28	6.355	861	864	865	rBV3	532	498	0.00%	0.002%
29	6.446	876	879	881	rBV2	566	544	0.00%	0.002%
30	6.757	921	930	948	rBV	195345	477699	2.17%	1.636%
31	6.964	963	964	966	rVB	824	444	0.00%	0.002%
32	7.123	979	990	1012	rBV	10059958	21964736	100.00%	75.220%
33	7.306	1013	1020	1033	rVB	182001	410918	1.87%	1.407%
34	7.629	1071	1073	1076	rVB3	549	356	0.00%	0.001%
35	8.202	1164	1167	1168	rBV2	324	359	0.00%	0.001%
36	8.324	1181	1187	1200	rBV	113411	193979	0.88%	0.664%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044514.D
 Acq On : 27 Dec 2024 12:12
 Operator : JC/MD
 Sample : P5344-12 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COCH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	8.586	1229	1230	1233	rBV3	815	887	0.00%	0.003%
38	8.647	1233	1240	1247	rVV	438504	697782	3.18%	2.390%
39	8.714	1247	1251	1261	rVB	27170	48651	0.22%	0.167%
40	8.946	1284	1289	1300	rBV	76467	124002	0.56%	0.425%
41	9.269	1336	1342	1356	rBV	179009	276184	1.26%	0.946%
42	9.385	1356	1361	1373	rBV	217457	340350	1.55%	1.166%
43	9.842	1432	1436	1437	rBV2	375	363	0.00%	0.001%
44	10.049	1465	1470	1486	rBV	377478	538321	2.45%	1.844%
45	10.202	1491	1495	1499	rVB2	2561	3269	0.01%	0.011%
46	10.305	1508	1512	1519	rBV2	6624	11369	0.05%	0.039%
47	10.397	1525	1527	1530	rBV4	586	655	0.00%	0.002%
48	10.610	1560	1562	1564	rBV2	466	422	0.00%	0.001%
49	10.647	1564	1568	1577	rVB4	4000	6612	0.03%	0.023%
50	10.860	1601	1603	1606	rBV2	458	570	0.00%	0.002%
51	10.903	1606	1610	1611	rVB2	326	374	0.00%	0.001%
52	10.933	1611	1615	1616	rBV3	404	587	0.00%	0.002%
53	10.964	1617	1620	1623	rBV3	777	1029	0.00%	0.004%
54	11.189	1652	1657	1668	rVV	372029	464103	2.11%	1.589%
55	11.299	1673	1675	1680	rBV4	935	1572	0.01%	0.005%
56	11.384	1683	1689	1695	rVV4	1815	3197	0.01%	0.011%
57	11.457	1698	1701	1702	rVB3	1493	1382	0.01%	0.005%
58	11.567	1716	1719	1720	rVB3	622	481	0.00%	0.002%
59	11.610	1720	1726	1727	rBV3	1061	1684	0.01%	0.006%
60	11.677	1735	1737	1739	rVB2	555	443	0.00%	0.002%
61	11.713	1739	1743	1745	rBV2	606	848	0.00%	0.003%
62	11.750	1746	1749	1754	rVB2	4589	6471	0.03%	0.022%
63	11.823	1758	1761	1762	rBV3	313	348	0.00%	0.001%
64	11.939	1778	1780	1784	rBV3	411	601	0.00%	0.002%
65	11.976	1784	1786	1788	rBV2	943	923	0.00%	0.003%
66	12.018	1788	1793	1801	rBV	402265	510051	2.32%	1.747%
67	12.085	1802	1804	1809	rVB3	3935	4899	0.02%	0.017%
68	12.238	1827	1829	1832	rVB3	828	852	0.00%	0.003%
69	12.317	1837	1842	1854	rVV	538184	687862	3.13%	2.356%
70	12.530	1873	1877	1880	rVB4	901	1063	0.00%	0.004%
71	12.597	1885	1888	1890	rBV4	406	476	0.00%	0.002%
72	12.762	1909	1915	1920	rVV2	2130	3419	0.02%	0.012%
73	13.146	1975	1978	1980	rBV2	446	427	0.00%	0.001%
74	13.225	1988	1991	1992	rBV3	394	363	0.00%	0.001%
75	13.359	2012	2013	2016	rBV2	405	475	0.00%	0.002%
76	13.420	2020	2023	2024	rBV2	291	383	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044514.D
 Acq On : 27 Dec 2024 12:12
 Operator : JC/MD
 Sample : P5344-12 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COCH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	13.548	2041	2044	2046	rBV3	283	340	0.00%	0.001%
78	13.609	2051	2054	2055	rBV3	543	496	0.00%	0.002%
79	13.719	2070	2072	2073	rBV2	363	367	0.00%	0.001%
80	14.103	2133	2135	2136	rBV2	472	434	0.00%	0.001%
81	14.128	2136	2139	2145	rVB	3215	4178	0.02%	0.014%
82	14.225	2153	2155	2158	rBV2	358	388	0.00%	0.001%
83	14.292	2164	2166	2168	rBV2	523	528	0.00%	0.002%
84	14.432	2186	2189	2191	rVB4	393	423	0.00%	0.001%
85	14.457	2191	2193	2196	rBV2	715	754	0.00%	0.003%
86	14.487	2196	2198	2199	rBV2	585	527	0.00%	0.002%
87	14.634	2221	2222	2224	rBV	608	365	0.00%	0.001%
88	14.695	2230	2232	2235	rBV2	379	395	0.00%	0.001%
89	14.920	2267	2269	2270	rBV2	577	465	0.00%	0.002%
90	15.097	2297	2298	2300	rBV2	504	427	0.00%	0.001%
91	15.115	2300	2301	2303	rVB	937	465	0.00%	0.002%
92	15.152	2305	2307	2308	rBV	692	476	0.00%	0.002%
93	15.164	2308	2309	2310	rVB	895	327	0.00%	0.001%
94	15.188	2310	2313	2314	rBV2	602	644	0.00%	0.002%
95	15.396	2342	2347	2350	rBV5	1934	2750	0.01%	0.009%
96	15.426	2350	2352	2353	rVB2	935	534	0.00%	0.002%
97	15.524	2366	2368	2371	rBV3	747	749	0.00%	0.003%
98	15.688	2394	2395	2396	rBV	747	329	0.00%	0.001%
99	15.713	2397	2399	2402	rVV2	672	542	0.00%	0.002%
100	16.267	2487	2490	2491	rBV3	630	726	0.00%	0.002%




Sum of corrected areas: 29200696

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044514.D
Acq On : 27 Dec 2024 12:12
Operator : JC/MD
Sample : P5344-12 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

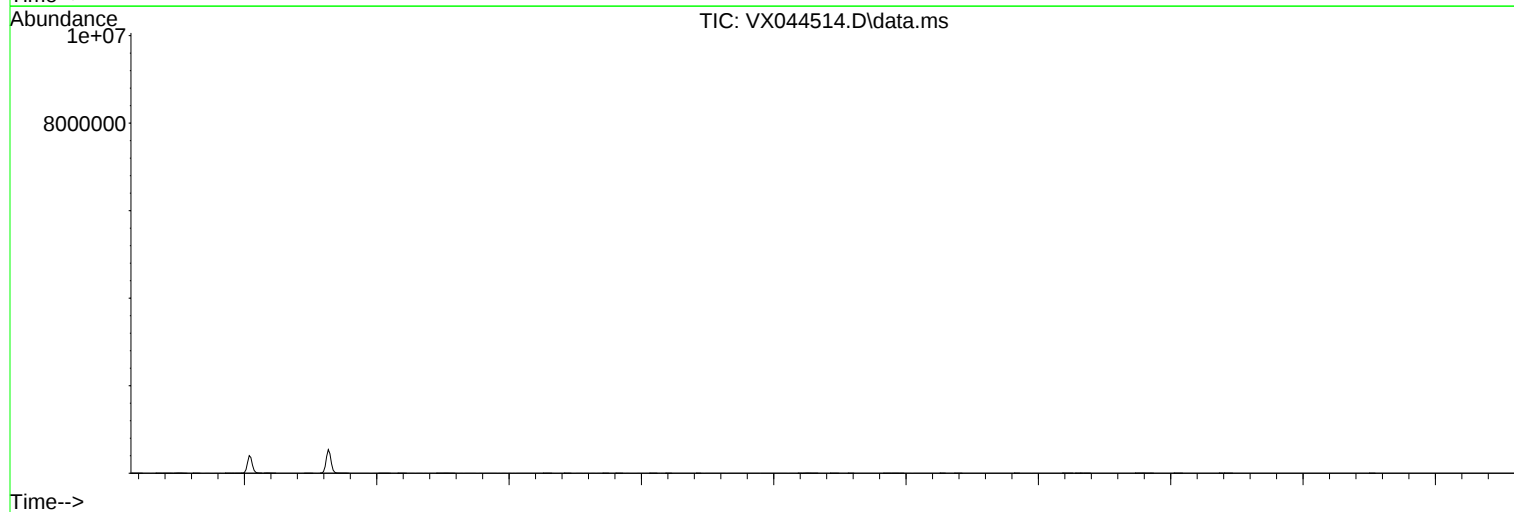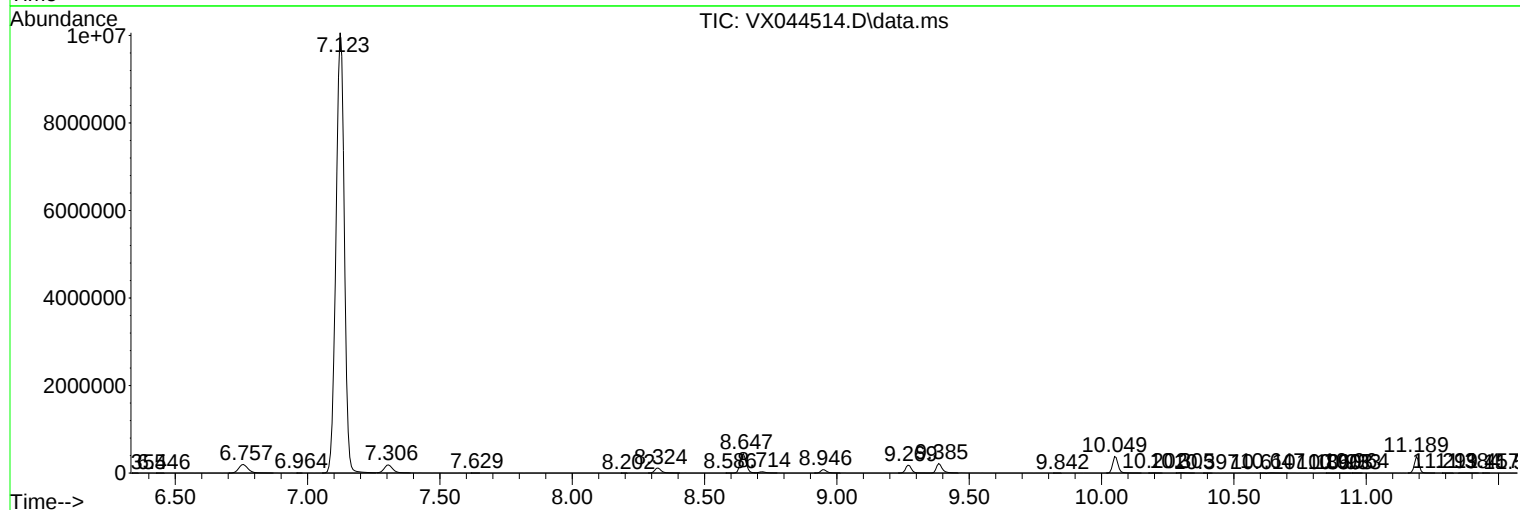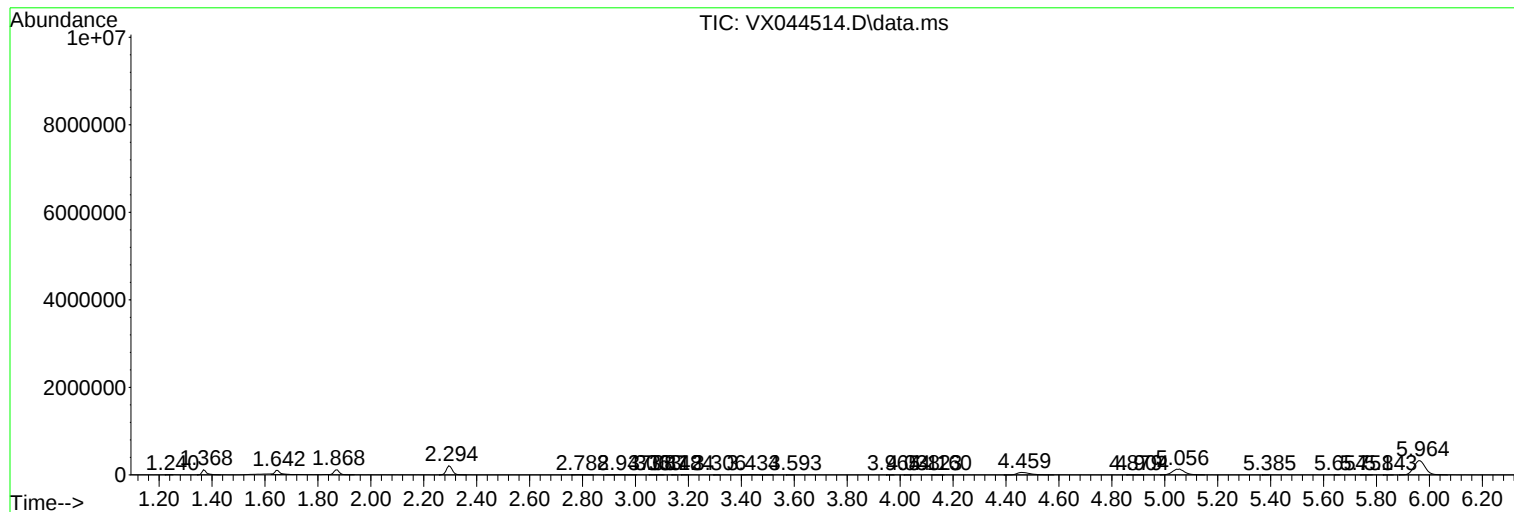

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044514.D
Acq On : 27 Dec 2024 12:12
Operator : JC/MD
Sample : P5344-12 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044514.D
Acq On : 27 Dec 2024 12:12
Operator : JC/MD
Sample : P5344-12 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
