

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044515.D
 Acq On : 27 Dec 2024 12:35
 Operator : JC/MD
 Sample : VIBLK686
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK686

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044515.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.245	23	26	27	rBV	3250	3463	0.37%	0.054%
2	1.367	43	46	56	rVB	105730	126619	13.70%	1.974%
3	1.642	88	91	103	rVB	87098	139271	15.07%	2.172%
4	2.294	192	198	210	rVB	185989	290093	31.39%	4.523%
5	2.788	275	279	281	rBV5	1056	1525	0.16%	0.024%
6	2.812	281	283	285	rVV2	584	494	0.05%	0.008%
7	2.837	285	287	289	rVB	838	621	0.07%	0.010%
8	2.934	295	303	313	rBV2	4873	12291	1.33%	0.192%
9	3.087	325	328	329	rBV4	780	966	0.10%	0.015%
10	3.239	352	353	357	rBV2	543	626	0.07%	0.010%
11	3.282	357	360	362	rVV3	420	556	0.06%	0.009%
12	3.367	373	374	377	rVB2	460	395	0.04%	0.006%
13	3.434	377	385	392	rBV3	3649	8263	0.89%	0.129%
14	3.580	407	409	410	rBV2	541	447	0.05%	0.007%
15	3.690	426	427	431	rBV2	491	453	0.05%	0.007%
16	3.812	445	447	452	rVV3	447	558	0.06%	0.009%
17	3.861	452	455	456	rVB2	678	529	0.06%	0.008%
18	3.885	456	459	460	rBV3	503	377	0.04%	0.006%
19	3.958	470	471	474	rVV	536	422	0.05%	0.007%
20	3.989	474	476	477	rVV2	393	393	0.04%	0.006%
21	4.050	483	486	487	rBV2	608	438	0.05%	0.007%
22	4.129	497	499	504	rBV4	660	810	0.09%	0.013%
23	4.281	520	524	525	rVB	739	501	0.05%	0.008%
24	4.306	525	528	529	rBV2	464	436	0.05%	0.007%
25	4.458	545	553	572	rBV	52714	174482	18.88%	2.721%
26	4.727	594	597	599	rBV3	614	553	0.06%	0.009%
27	4.745	599	600	604	rVV2	588	605	0.07%	0.009%
28	4.794	607	608	611	rVB2	730	483	0.05%	0.008%
29	4.891	622	624	627	rVB2	591	538	0.06%	0.008%
30	4.922	627	629	632	rVB3	467	603	0.07%	0.009%
31	5.056	639	651	667	rBV2	126283	392820	42.50%	6.125%
32	5.214	676	677	682	rBV4	814	849	0.09%	0.013%
33	5.501	722	724	725	rBV	601	493	0.05%	0.008%
34	5.610	740	742	745	rVB2	556	685	0.07%	0.011%
35	5.641	745	747	749	rBV2	475	440	0.05%	0.007%
36	5.708	756	758	762	rBV	456	695	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044515.D
 Acq On : 27 Dec 2024 12:35
 Operator : JC/MD
 Sample : VIBLK686
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK686

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	5.964	787	800	817	rBV2	309021	924274	100.00%	14.412%
38	6.293	852	854	855	rVB2	563	404	0.04%	0.006%
39	6.385	866	869	870	rBV2	569	502	0.05%	0.008%
40	6.513	884	890	891	rBV2	593	793	0.09%	0.012%
41	6.549	895	896	899	rBV3	487	489	0.05%	0.008%
42	6.641	908	911	912	rBV2	428	437	0.05%	0.007%
43	6.659	912	914	916	rBV2	505	411	0.04%	0.006%
44	6.757	921	930	946	rBV2	185657	453664	49.08%	7.074%
45	7.122	982	990	1001	rBV3	46029	109555	11.85%	1.708%
46	7.305	1009	1020	1034	rBV	188199	426510	46.15%	6.650%
47	7.702	1084	1085	1088	rVB2	440	386	0.04%	0.006%
48	7.732	1088	1090	1093	rBV2	601	671	0.07%	0.010%
49	7.994	1130	1133	1136	rBV2	423	663	0.07%	0.010%
50	8.262	1175	1177	1180	rVB2	995	900	0.10%	0.014%
51	8.323	1180	1187	1200	rBV	112649	194278	21.02%	3.029%
52	8.579	1225	1229	1232	rBV4	658	1064	0.12%	0.017%
53	8.647	1234	1240	1251	rVV	434799	679729	73.54%	10.599%
54	8.951	1284	1290	1297	rBV	75128	119276	12.90%	1.860%
55	9.092	1311	1313	1315	rVB2	640	505	0.05%	0.008%
56	9.281	1339	1344	1348	rVV5	1316	2440	0.26%	0.038%
57	9.384	1356	1361	1377	rBV	227218	358115	38.75%	5.584%
58	9.738	1417	1419	1421	rBV2	723	558	0.06%	0.009%
59	10.049	1465	1470	1484	rBV	358877	525927	56.90%	8.201%
60	10.280	1506	1508	1512	rBV3	675	1062	0.11%	0.017%
61	10.317	1512	1514	1516	rVV2	1009	813	0.09%	0.013%
62	10.354	1518	1520	1522	rVV2	442	398	0.04%	0.006%
63	10.555	1549	1553	1556	rVB2	579	940	0.10%	0.015%
64	10.908	1607	1611	1614	rVB3	578	705	0.08%	0.011%
65	11.061	1634	1636	1639	rBV4	537	797	0.09%	0.012%
66	11.189	1652	1657	1669	rVB	340409	436697	47.25%	6.809%
67	11.487	1705	1706	1708	rVV2	574	380	0.04%	0.006%
68	11.524	1710	1712	1718	rBV3	538	1079	0.12%	0.017%
69	11.689	1735	1739	1741	rBV3	498	856	0.09%	0.013%
70	11.811	1757	1759	1760	rBV	397	384	0.04%	0.006%
71	11.865	1766	1768	1770	rBV2	484	476	0.05%	0.007%
72	11.926	1775	1778	1781	rBV3	519	837	0.09%	0.013%
73	12.018	1788	1793	1802	rBV	338935	431440	46.68%	6.727%
74	12.317	1837	1842	1854	rBV	432088	546490	59.13%	8.521%
75	12.506	1871	1873	1874	rBV2	511	492	0.05%	0.008%
76	12.762	1910	1915	1919	rBV4	1900	2786	0.30%	0.043%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044515.D
 Acq On : 27 Dec 2024 12:35
 Operator : JC/MD
 Sample : VIBLK686
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK686

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	12.914	1938	1940	1943	rVB3	416	386	0.04%	0.006%
78	13.054	1960	1963	1965	rBV3	422	580	0.06%	0.009%
79	13.079	1965	1967	1969	rVB3	646	537	0.06%	0.008%
80	13.396	2017	2019	2023	rVB2	615	886	0.10%	0.014%
81	13.707	2067	2070	2073	rBV3	424	534	0.06%	0.008%
82	13.853	2092	2094	2099	rBV3	558	935	0.10%	0.015%
83	14.054	2124	2127	2128	rBV	503	510	0.06%	0.008%
84	14.078	2129	2131	2133	rVV2	643	551	0.06%	0.009%
85	14.127	2135	2139	2145	rVB	3144	4476	0.48%	0.070%
86	14.225	2153	2155	2156	rVB	677	385	0.04%	0.006%
87	14.487	2197	2198	2202	rBV3	401	537	0.06%	0.008%
88	14.597	2213	2216	2220	rVB4	677	998	0.11%	0.016%
89	14.639	2220	2223	2224	rBV2	442	486	0.05%	0.008%
90	14.914	2266	2268	2270	rVV3	468	431	0.05%	0.007%
91	15.072	2292	2294	2299	rBV3	517	878	0.09%	0.014%
92	15.194	2312	2314	2317	rBV2	847	1190	0.13%	0.019%
93	15.225	2317	2319	2322	rVB3	552	534	0.06%	0.008%
94	15.389	2341	2346	2350	rBV5	1663	3182	0.34%	0.050%
95	15.584	2375	2378	2380	rBV3	725	830	0.09%	0.013%
96	15.706	2396	2398	2400	rBV3	504	519	0.06%	0.008%
97	15.761	2405	2407	2410	rVB4	655	567	0.06%	0.009%
98	16.310	2496	2497	2500	rBV3	649	574	0.06%	0.009%
99	16.517	2528	2531	2532	rBV2	587	444	0.05%	0.007%
100	16.566	2538	2539	2540	rBV	779	419	0.05%	0.007%

Sum of corrected areas: 6413345




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044515.D
Acq On : 27 Dec 2024 12:35
Operator : JC/MD
Sample : VIBLK686
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK686

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

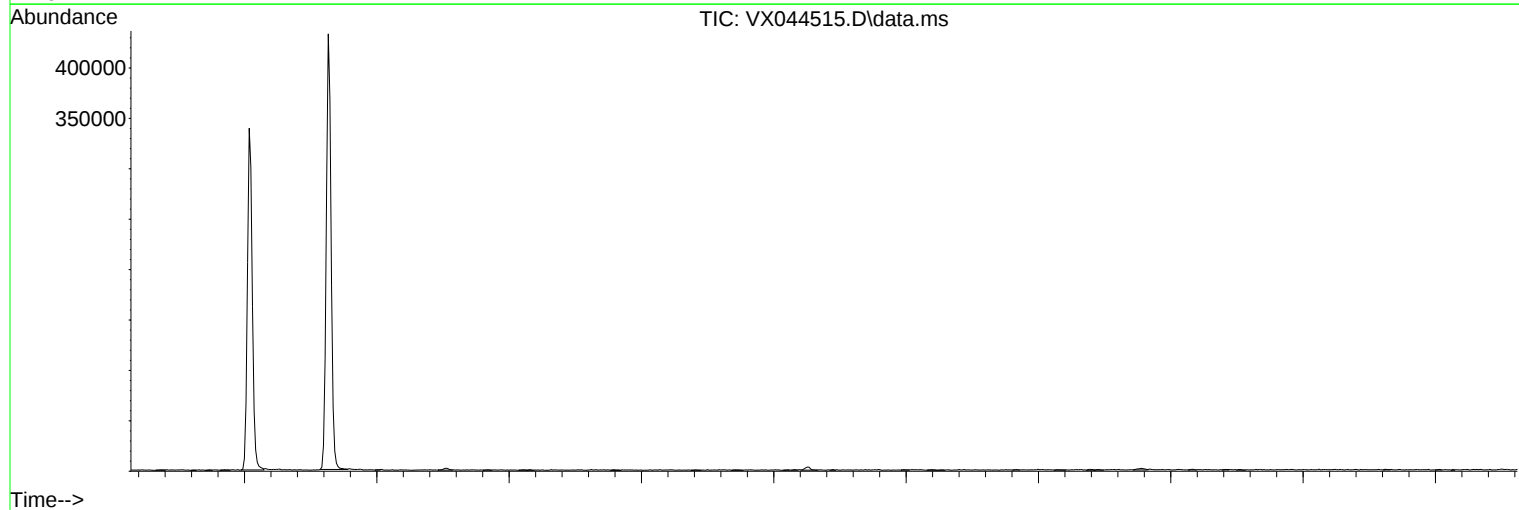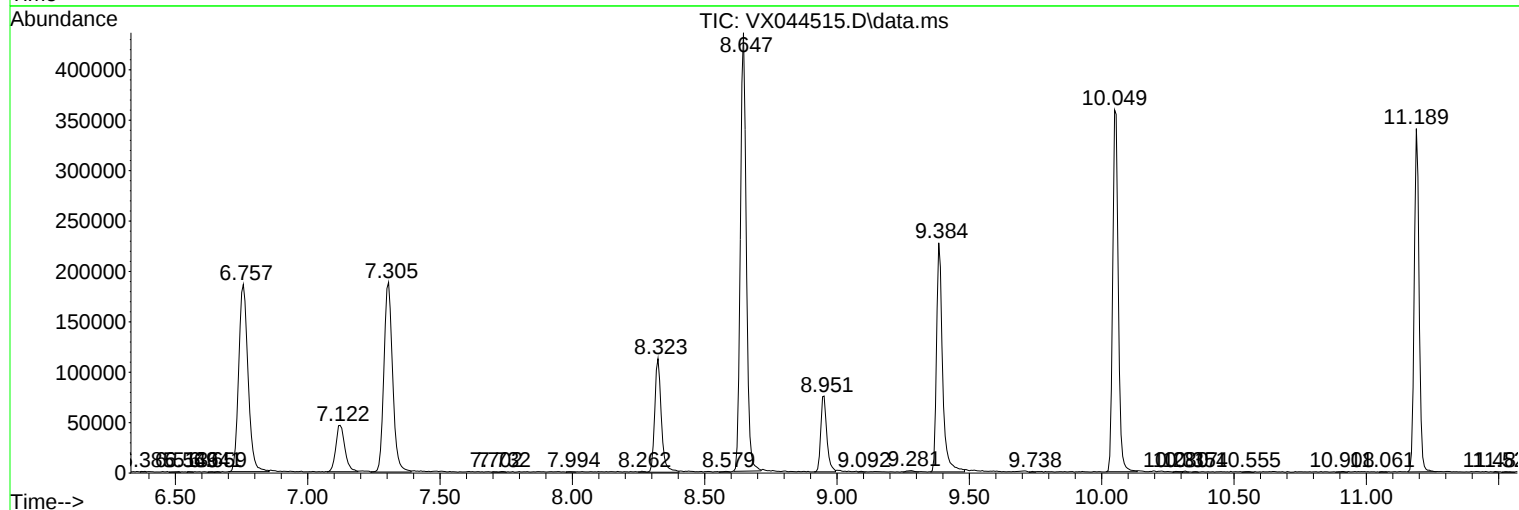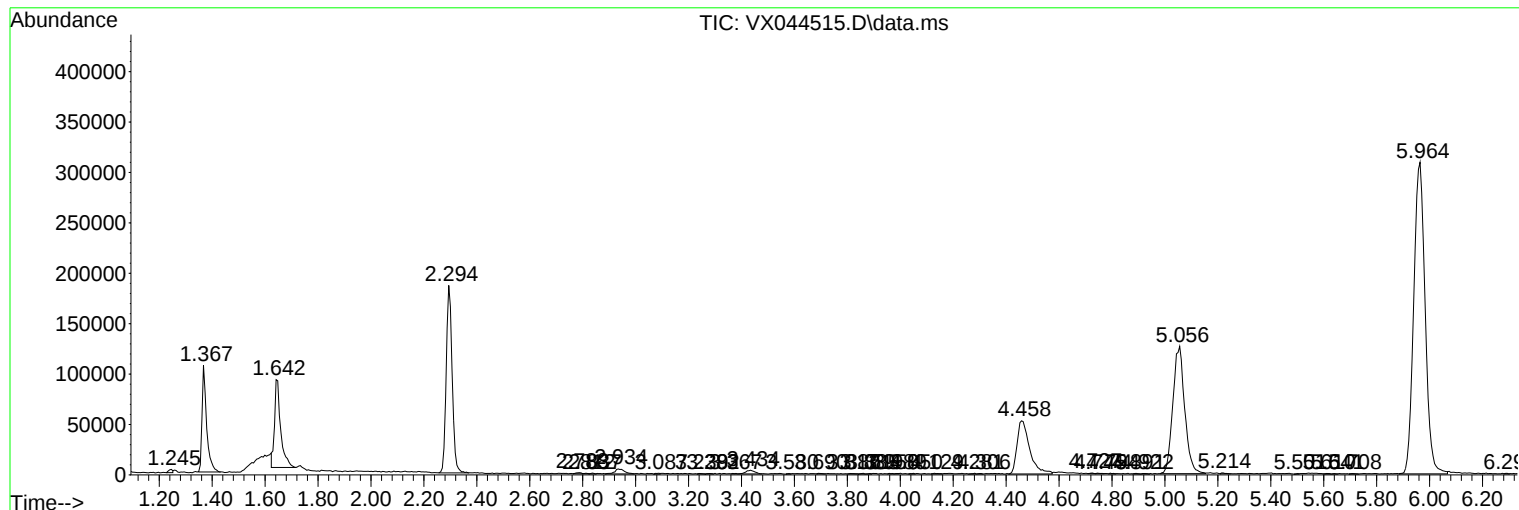

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044515.D
Acq On : 27 Dec 2024 12:35
Operator : JC/MD
Sample : VIBLK686
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK686

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044515.D
Acq On : 27 Dec 2024 12:35
Operator : JC/MD
Sample : VIBLK686
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK686

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
