

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044524.D
 Acq On : 27 Dec 2024 16:31
 Operator : JC/MD
 Sample : VIBLK687
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK687

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044524.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	27	rBV	4620	5594	0.57%	0.082%
2	1.368	42	46	57	rBV	93241	112460	11.52%	1.651%
3	1.642	88	91	103	rVB	88379	129676	13.29%	1.903%
4	2.294	192	198	208	rVB	178767	275763	28.25%	4.048%
5	2.721	266	268	270	rVB3	687	473	0.05%	0.007%
6	2.782	275	278	285	rVB5	1482	2587	0.27%	0.038%
7	2.940	299	304	311	rVB2	4313	9324	0.96%	0.137%
8	3.081	322	327	333	rVV6	1352	3283	0.34%	0.048%
9	3.160	338	340	342	rBV3	600	610	0.06%	0.009%
10	3.270	356	358	361	rVV2	621	472	0.05%	0.007%
11	3.544	402	403	405	rBV	654	505	0.05%	0.007%
12	3.818	447	448	453	rVV2	483	826	0.08%	0.012%
13	4.123	494	498	501	rVB3	646	922	0.09%	0.014%
14	4.227	513	515	517	rBV	643	657	0.07%	0.010%
15	4.330	529	532	534	rBV3	557	541	0.06%	0.008%
16	4.458	546	553	568	rBV	69426	214579	21.99%	3.150%
17	4.843	614	616	620	rVB4	497	555	0.06%	0.008%
18	4.885	620	623	626	rBV4	613	582	0.06%	0.009%
19	4.965	634	636	638	rBV2	370	485	0.05%	0.007%
20	5.056	639	651	668	rVV2	142069	431271	44.19%	6.330%
21	5.306	690	692	693	rVB	876	527	0.05%	0.008%
22	5.324	693	695	697	rBV2	554	574	0.06%	0.008%
23	5.373	699	703	705	rBV3	661	1088	0.11%	0.016%
24	5.458	715	717	719	rBV2	677	840	0.09%	0.012%
25	5.544	729	731	732	rBV2	789	549	0.06%	0.008%
26	5.653	745	749	750	rBV2	490	660	0.07%	0.010%
27	5.873	783	785	788	rBV2	311	479	0.05%	0.007%
28	5.964	788	800	821	rBV2	322946	976019	100.00%	14.327%
29	6.397	869	871	873	rVB2	712	508	0.05%	0.007%
30	6.617	905	907	908	rBV	477	482	0.05%	0.007%
31	6.672	914	916	919	rBV3	618	608	0.06%	0.009%
32	6.757	921	930	945	rBV	197522	474572	48.62%	6.966%
33	6.940	956	960	962	rVV3	571	517	0.05%	0.008%
34	7.129	983	991	999	rVB10	4319	11723	1.20%	0.172%
35	7.306	1011	1020	1037	rBV	206489	465507	47.69%	6.833%
36	7.629	1072	1073	1076	rVB	869	562	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044524.D
 Acq On : 27 Dec 2024 16:31
 Operator : JC/MD
 Sample : VIBLK687
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK687

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	7.671	1076	1080	1082	rBV4	500	650	0.07%	0.010%
38	7.799	1098	1101	1103	rVB2	558	458	0.05%	0.007%
39	7.830	1103	1106	1108	rBV2	539	745	0.08%	0.011%
40	7.915	1117	1120	1122	rVB2	618	612	0.06%	0.009%
41	7.940	1122	1124	1125	rBV2	626	522	0.05%	0.008%
42	8.135	1154	1156	1158	rVB2	511	452	0.05%	0.007%
43	8.238	1171	1173	1175	rBV2	820	565	0.06%	0.008%
44	8.269	1175	1178	1180	rBV3	511	754	0.08%	0.011%
45	8.324	1181	1187	1199	rBV	124921	208599	21.37%	3.062%
46	8.647	1234	1240	1251	rBV	436629	690758	70.77%	10.139%
47	8.945	1284	1289	1299	rBV	83029	133813	13.71%	1.964%
48	9.275	1339	1343	1346	rBV4	2500	3567	0.37%	0.052%
49	9.384	1356	1361	1376	rBV	294459	456202	46.74%	6.696%
50	9.653	1404	1405	1409	rBV3	686	895	0.09%	0.013%
51	9.781	1424	1426	1427	rVB2	761	556	0.06%	0.008%
52	9.799	1427	1429	1430	rBV	753	668	0.07%	0.010%
53	9.848	1435	1437	1440	rVB2	535	549	0.06%	0.008%
54	9.884	1440	1443	1447	rBV3	573	952	0.10%	0.014%
55	10.049	1465	1470	1480	rBV	373598	545084	55.85%	8.001%
56	10.195	1492	1494	1499	rVB4	2525	3162	0.32%	0.046%
57	10.305	1508	1512	1516	rBV5	2201	3608	0.37%	0.053%
58	10.524	1546	1548	1551	rVV2	694	604	0.06%	0.009%
59	10.573	1551	1556	1561	rVV4	683	1266	0.13%	0.019%
60	10.646	1564	1568	1577	rVV6	1984	5394	0.55%	0.079%
61	10.799	1592	1593	1597	rBV3	489	642	0.07%	0.009%
62	10.878	1603	1606	1610	rBV3	481	603	0.06%	0.009%
63	10.963	1616	1620	1624	rBV3	2287	3647	0.37%	0.054%
64	11.122	1641	1646	1648	rVB	486	517	0.05%	0.008%
65	11.189	1651	1657	1665	rBV	395603	507912	52.04%	7.455%
66	11.305	1675	1676	1681	rBV3	401	515	0.05%	0.008%
67	11.451	1696	1700	1704	rBV3	2034	3058	0.31%	0.045%
68	11.762	1746	1751	1754	rVV4	2277	3467	0.36%	0.051%
69	11.835	1761	1763	1765	rVB2	588	498	0.05%	0.007%
70	11.896	1772	1773	1776	rVB2	683	503	0.05%	0.007%
71	11.927	1776	1778	1779	rBV2	695	586	0.06%	0.009%
72	11.975	1782	1786	1788	rVV3	2961	3447	0.35%	0.051%
73	12.018	1788	1793	1806	rVV	343149	447865	45.89%	6.574%
74	12.317	1837	1842	1852	rBV	470598	608063	62.30%	8.926%
75	12.567	1882	1883	1887	rBV4	770	796	0.08%	0.012%
76	12.762	1911	1915	1919	rVB2	2776	3234	0.33%	0.047%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044524.D
 Acq On : 27 Dec 2024 16:31
 Operator : JC/MD
 Sample : VIBLK687
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK687

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	12.866	1927	1932	1935	rVB4	513	821	0.08%	0.012%
78	12.902	1935	1938	1941	rBV3	404	620	0.06%	0.009%
79	13.115	1970	1973	1977	rVB2	2073	2501	0.26%	0.037%
80	13.237	1990	1993	1995	rVV4	440	487	0.05%	0.007%
81	13.597	2048	2052	2058	rVV4	3124	5150	0.53%	0.076%
82	13.670	2062	2064	2067	rBV3	634	591	0.06%	0.009%
83	13.780	2078	2082	2089	rBV2	5005	7596	0.78%	0.111%
84	13.963	2109	2112	2117	rVV2	3866	5363	0.55%	0.079%
85	14.067	2126	2129	2130	rBV3	664	686	0.07%	0.010%
86	14.085	2130	2132	2135	rVB2	637	633	0.06%	0.009%
87	14.127	2135	2139	2143	rBV2	3534	4630	0.47%	0.068%
88	14.243	2154	2158	2160	rBB3	567	777	0.08%	0.011%
89	14.280	2163	2164	2168	rVB3	607	697	0.07%	0.010%
90	14.316	2168	2170	2172	rBV2	536	675	0.07%	0.010%
91	14.365	2175	2178	2180	rBV3	546	716	0.07%	0.011%
92	14.560	2208	2210	2212	rBV3	695	633	0.06%	0.009%
93	14.646	2221	2224	2228	rVB2	620	730	0.07%	0.011%
94	15.127	2301	2303	2306	rBV3	491	522	0.05%	0.008%
95	15.304	2330	2332	2335	rBV3	696	784	0.08%	0.012%
96	15.396	2342	2347	2349	rBV3	2308	3106	0.32%	0.046%
97	15.499	2361	2364	2366	rBV3	553	793	0.08%	0.012%
98	15.713	2397	2399	2401	rBV2	516	695	0.07%	0.010%
99	16.084	2458	2460	2463	rVB2	534	479	0.05%	0.007%
100	16.188	2475	2477	2480	rBV2	630	759	0.08%	0.011%

Sum of corrected areas: 6812612




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044524.D
Acq On : 27 Dec 2024 16:31
Operator : JC/MD
Sample : VIBLK687
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK687

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

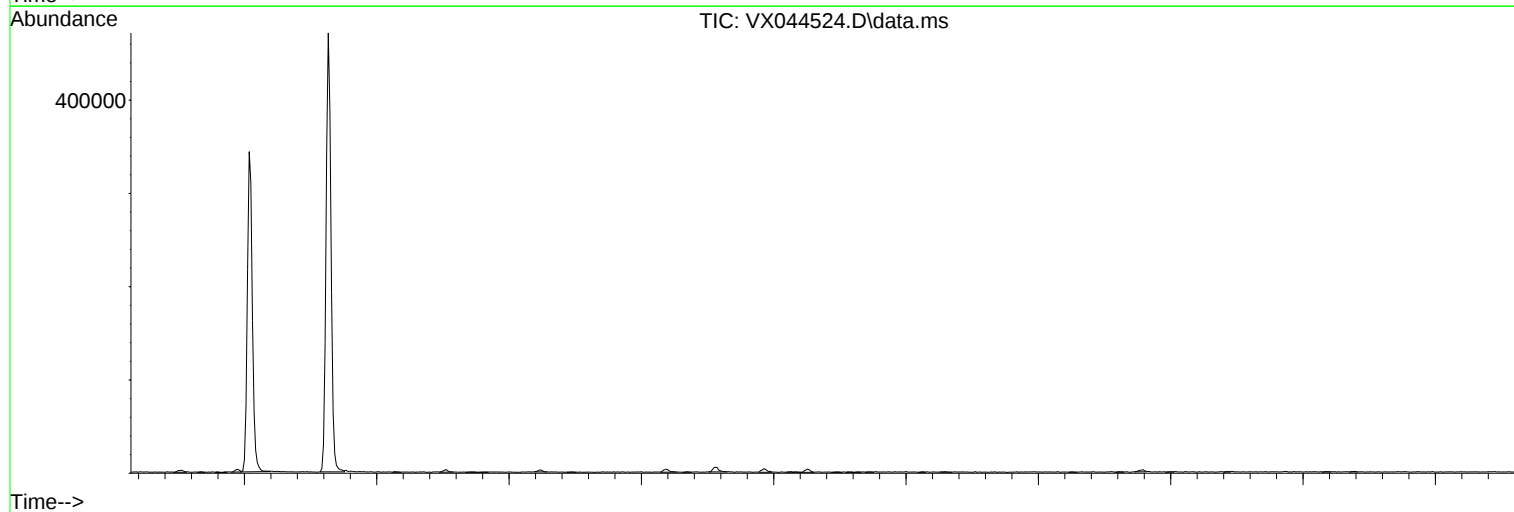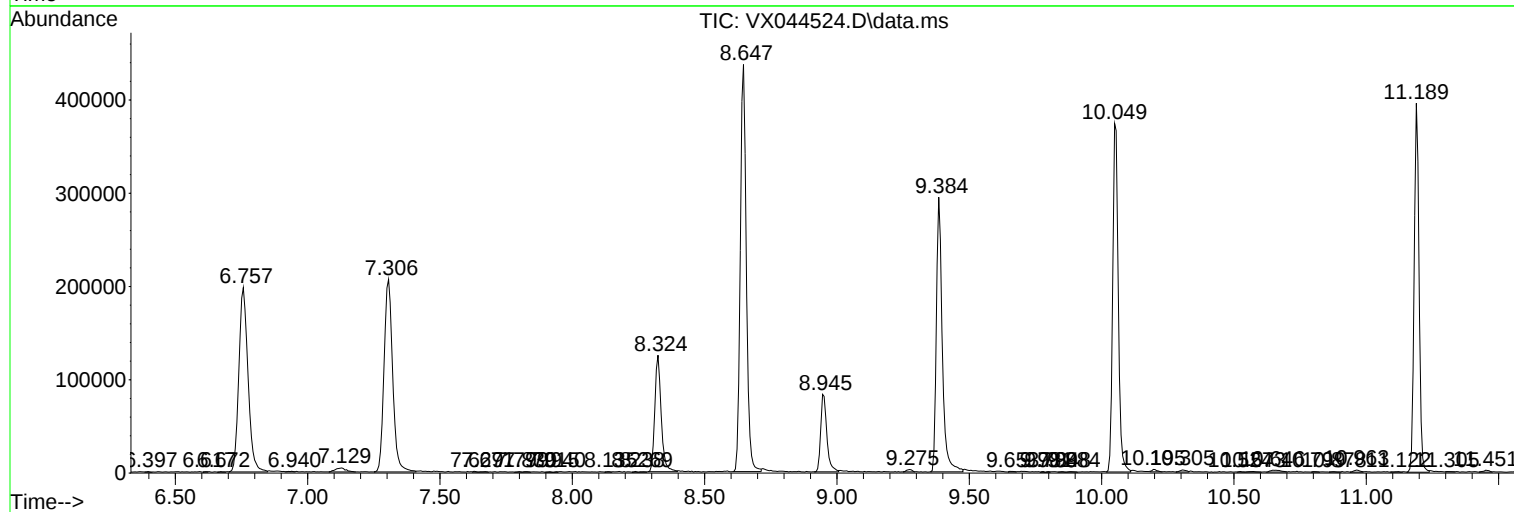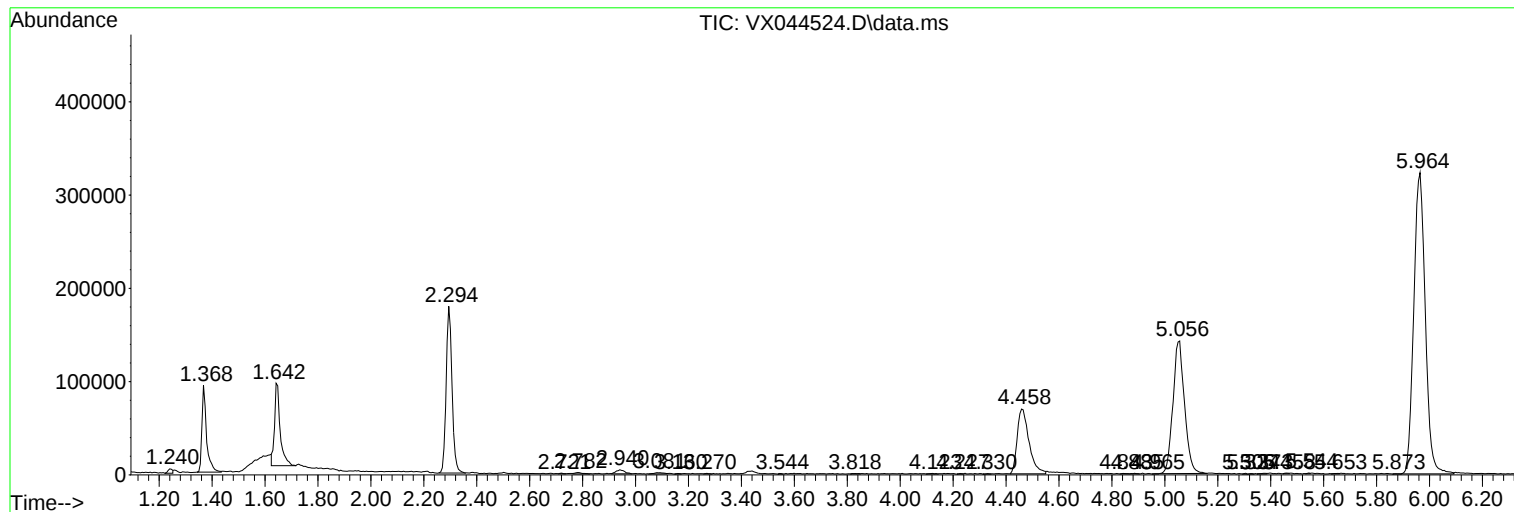

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044524.D
Acq On : 27 Dec 2024 16:31
Operator : JC/MD
Sample : VIBLK687
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK687

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044524.D
Acq On : 27 Dec 2024 16:31
Operator : JC/MD
Sample : VIBLK687
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK687

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
