

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044525.D
 Acq On : 27 Dec 2024 16:54
 Operator : JC/MD
 Sample : P5344-06DL 1000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CE8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M

Title : VOC Analysis

Signal : TIC: VX044525.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	34	rVB3	4250	7084	0.40%	0.083%
2	1.368	42	46	58	rBV	125626	144874	8.18%	1.692%
3	1.618	69	87	88	rBV3	18119	78147	4.41%	0.913%
4	1.642	88	91	102	rVB	93385	146141	8.25%	1.707%
5	2.294	192	198	209	rVB	213756	322668	18.22%	3.769%
6	2.770	274	276	277	rBV	1044	701	0.04%	0.008%
7	2.947	298	305	313	rVV2	6274	14747	0.83%	0.172%
8	3.428	377	384	392	rBV5	3986	9191	0.52%	0.107%
9	3.514	396	398	400	rBV2	494	421	0.02%	0.005%
10	3.550	403	404	407	rBV3	690	639	0.04%	0.007%
11	3.739	433	435	437	rBV2	389	410	0.02%	0.005%
12	3.873	454	457	458	rBV2	823	811	0.05%	0.009%
13	3.916	463	464	467	rBV	582	734	0.04%	0.009%
14	4.056	484	487	490	rBV3	489	916	0.05%	0.011%
15	4.154	501	503	504	rBV2	490	445	0.03%	0.005%
16	4.209	510	512	513	rVB	800	456	0.03%	0.005%
17	4.465	546	554	571	rBV	57720	183217	10.35%	2.140%
18	4.763	602	603	606	rBV2	361	408	0.02%	0.005%
19	5.050	638	650	666	rBV	138473	421608	23.81%	4.924%
20	5.245	680	682	683	rBV	562	426	0.02%	0.005%
21	5.343	696	698	701	rBV2	504	549	0.03%	0.006%
22	5.532	722	729	732	rBV4	617	1627	0.09%	0.019%
23	5.641	745	747	749	rBV2	473	409	0.02%	0.005%
24	5.843	776	780	783	rBV4	342	498	0.03%	0.006%
25	5.964	789	800	817	rBV2	332159	986040	55.69%	11.517%
26	6.214	840	841	844	rBV2	645	736	0.04%	0.009%
27	6.281	850	852	857	rVB4	492	715	0.04%	0.008%
28	6.477	883	884	887	rVV3	512	418	0.02%	0.005%
29	6.757	921	930	942	rBV	192209	467014	26.38%	5.455%
30	6.922	955	957	960	rBV3	612	841	0.05%	0.010%
31	7.117	980	989	1005	rBV	778010	1770473	100.00%	20.678%
32	7.306	1012	1020	1034	rBV2	199036	439780	24.84%	5.136%
33	7.476	1046	1048	1049	rBV2	895	692	0.04%	0.008%
34	7.720	1085	1088	1089	rBV	439	417	0.02%	0.005%
35	7.836	1104	1107	1109	rBV3	444	552	0.03%	0.006%
36	7.915	1118	1120	1123	rBV4	429	468	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044525.D
 Acq On : 27 Dec 2024 16:54
 Operator : JC/MD
 Sample : P5344-06DL 1000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CE8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	7.952	1125	1126	1129	rBV3	559	453	0.03%	0.005%
38	8.208	1167	1168	1171	rBV	661	568	0.03%	0.007%
39	8.281	1178	1180	1181	rBV	837	462	0.03%	0.005%
40	8.324	1181	1187	1198	rBV	117924	201292	11.37%	2.351%
41	8.470	1208	1211	1214	rBV4	625	793	0.04%	0.009%
42	8.519	1217	1219	1221	rBV3	419	404	0.02%	0.005%
43	8.574	1226	1228	1229	rBV2	607	511	0.03%	0.006%
44	8.647	1233	1240	1251	rBV	459274	740608	41.83%	8.650%
45	8.897	1278	1281	1283	rBV3	432	507	0.03%	0.006%
46	8.952	1285	1290	1302	rVV	82484	129983	7.34%	1.518%
47	9.269	1338	1342	1350	rBV2	10528	16731	0.95%	0.195%
48	9.385	1356	1361	1382	rBV	243070	388868	21.96%	4.542%
49	9.702	1411	1413	1415	rBV2	738	545	0.03%	0.006%
50	10.049	1465	1470	1483	rBV	375410	538913	30.44%	6.294%
51	10.201	1492	1495	1502	rVB6	1407	2882	0.16%	0.034%
52	10.250	1502	1503	1505	rBV2	535	467	0.03%	0.005%
53	10.311	1508	1513	1515	rBV5	1189	1916	0.11%	0.022%
54	10.403	1525	1528	1530	rBV3	523	669	0.04%	0.008%
55	10.647	1564	1568	1569	rBV2	1260	1465	0.08%	0.017%
56	10.970	1618	1621	1623	rBV2	968	1241	0.07%	0.014%
57	11.037	1630	1632	1634	rBV2	495	489	0.03%	0.006%
58	11.134	1646	1648	1650	rBV	627	444	0.03%	0.005%
59	11.189	1652	1657	1667	rVV	363201	457384	25.83%	5.342%
60	11.372	1685	1687	1689	rVB2	814	611	0.03%	0.007%
61	11.390	1689	1690	1692	rBV2	743	480	0.03%	0.006%
62	11.445	1696	1699	1700	rBV2	746	815	0.05%	0.010%
63	11.756	1749	1750	1752	rBV	892	507	0.03%	0.006%
64	11.976	1783	1786	1788	rBV4	1516	1950	0.11%	0.023%
65	12.018	1788	1793	1805	rVV	341241	443639	25.06%	5.182%
66	12.183	1819	1820	1824	rVB2	584	440	0.02%	0.005%
67	12.232	1826	1828	1832	rBV3	481	631	0.04%	0.007%
68	12.268	1832	1834	1836	rBV3	452	408	0.02%	0.005%
69	12.317	1837	1842	1851	rBV	464138	592177	33.45%	6.916%
70	12.494	1870	1871	1875	rBV2	523	522	0.03%	0.006%
71	12.732	1906	1910	1911	rBV2	742	971	0.05%	0.011%
72	12.762	1911	1915	1918	rVV2	2407	2956	0.17%	0.035%
73	12.811	1921	1923	1927	rVB2	677	690	0.04%	0.008%
74	12.860	1927	1931	1932	rBV2	604	815	0.05%	0.010%
75	12.939	1942	1944	1949	rVB4	370	625	0.04%	0.007%
76	13.006	1954	1955	1958	rBV2	591	458	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044525.D
 Acq On : 27 Dec 2024 16:54
 Operator : JC/MD
 Sample : P5344-06DL 1000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CE8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	13.116	1971	1973	1977	rVB3	620	901	0.05%	0.011%
78	13.219	1988	1990	1994	rBV2	501	704	0.04%	0.008%
79	13.774	2075	2081	2082	rBV2	1056	1414	0.08%	0.017%
80	13.896	2100	2101	2104	rBV2	439	471	0.03%	0.006%
81	13.969	2109	2113	2116	rVV4	1065	1557	0.09%	0.018%
82	14.128	2135	2139	2143	rVB2	2790	3779	0.21%	0.044%
83	14.207	2146	2152	2154	rBV3	291	633	0.04%	0.007%
84	14.231	2154	2156	2160	rVB2	466	434	0.02%	0.005%
85	14.262	2160	2161	2163	rBV	661	435	0.02%	0.005%
86	14.396	2179	2183	2184	rBV3	462	484	0.03%	0.006%
87	14.573	2211	2212	2216	rBV3	335	436	0.02%	0.005%
88	14.902	2264	2266	2268	rVB2	652	454	0.03%	0.005%
89	15.310	2332	2333	2335	rVB2	735	456	0.03%	0.005%
90	15.335	2335	2337	2339	rBV	469	475	0.03%	0.006%
91	15.359	2339	2341	2343	rVV3	622	695	0.04%	0.008%
92	15.383	2343	2345	2350	rVB2	1412	2145	0.12%	0.025%
93	15.475	2359	2360	2361	rBV	872	447	0.03%	0.005%
94	15.640	2386	2387	2390	rBV	793	476	0.03%	0.006%
95	15.719	2398	2400	2403	rBV3	552	691	0.04%	0.008%
96	15.835	2418	2419	2422	rVV2	908	495	0.03%	0.006%
97	15.926	2432	2434	2437	rBV2	930	1203	0.07%	0.014%
98	16.024	2447	2450	2453	rBV3	582	739	0.04%	0.009%
99	16.359	2504	2505	2508	rBV2	573	414	0.02%	0.005%
100	16.780	2572	2574	2575	rBV2	668	450	0.03%	0.005%

Sum of corrected areas: 8561951




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044525.D
Acq On : 27 Dec 2024 16:54
Operator : JC/MD
Sample : P5344-06DL 1000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CE8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

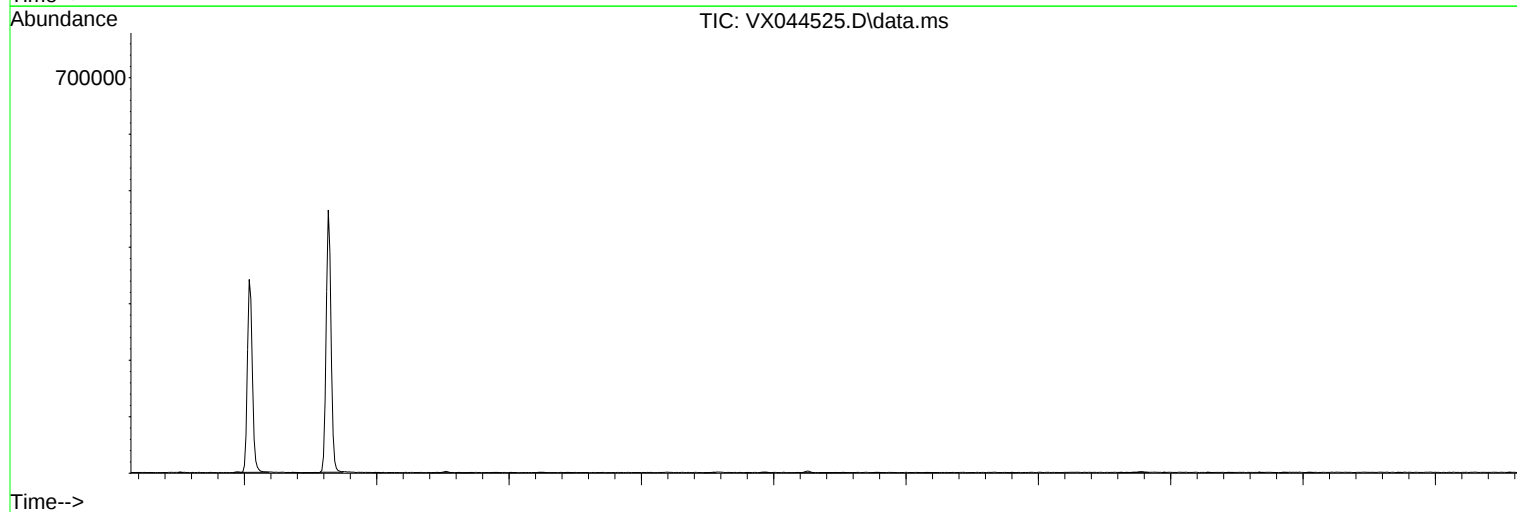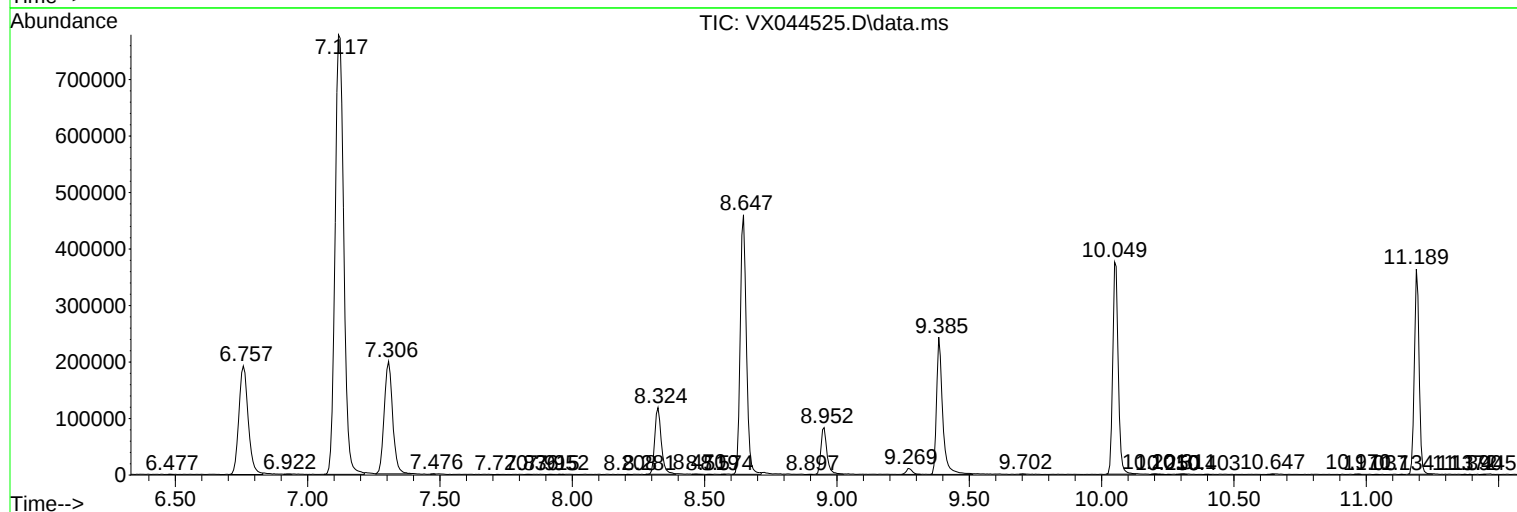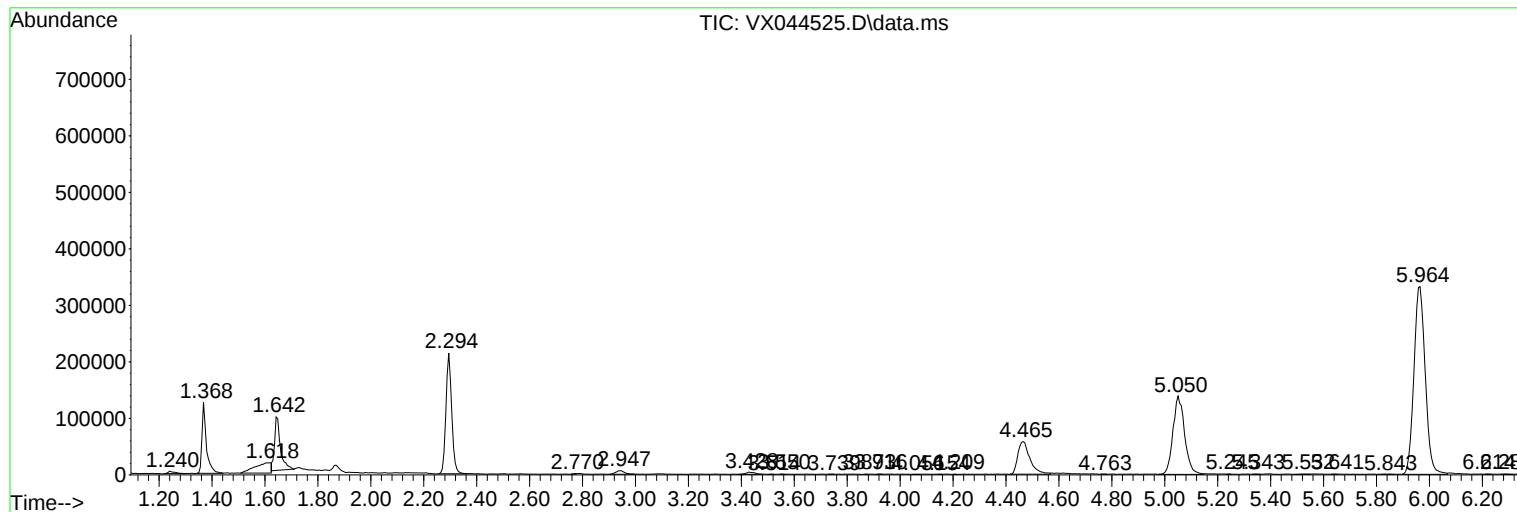

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044525.D
Acq On : 27 Dec 2024 16:54
Operator : JC/MD
Sample : P5344-06DL 1000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CE8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044525.D
Acq On : 27 Dec 2024 16:54
Operator : JC/MD
Sample : P5344-06DL 1000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CE8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
