

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044526.D
 Acq On : 27 Dec 2024 17:17
 Operator : JC/MD
 Sample : P5344-09DL 1000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CG6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	31	rBV2	3475	7346	0.77%	0.101%
2	1.368	43	46	58	rVB	104256	128030	13.47%	1.766%
3	1.599	69	84	85	rBV3	16776	57244	6.02%	0.789%
4	1.642	88	91	105	rVB	92385	166282	17.49%	2.293%
5	2.294	192	198	210	rVB	195267	312683	32.89%	4.312%
6	2.465	225	226	228	rBV2	587	574	0.06%	0.008%
7	2.751	270	273	275	rBV3	687	818	0.09%	0.011%
8	2.837	285	287	290	rBV2	532	496	0.05%	0.007%
9	2.940	298	304	312	rBV2	6576	15368	1.62%	0.212%
10	2.995	312	313	317	rVB2	1088	699	0.07%	0.010%
11	3.056	322	323	327	rVB3	610	567	0.06%	0.008%
12	3.300	362	363	366	rBV3	585	509	0.05%	0.007%
13	3.349	369	371	373	rBV2	715	562	0.06%	0.008%
14	3.434	379	385	390	rVV4	2831	6523	0.69%	0.090%
15	3.776	438	441	444	rVB2	519	511	0.05%	0.007%
16	4.465	546	554	568	rBV	54362	176653	18.58%	2.436%
17	5.050	640	650	667	rVB	131602	399025	41.98%	5.503%
18	5.245	680	682	683	rBV2	533	381	0.04%	0.005%
19	5.306	690	692	695	rBV	652	425	0.04%	0.006%
20	5.775	767	769	772	rBV	434	451	0.05%	0.006%
21	5.836	778	779	784	rVB3	502	571	0.06%	0.008%
22	5.885	784	787	789	rVB3	453	489	0.05%	0.007%
23	5.958	789	799	813	rBV2	322092	950582	100.00%	13.109%
24	6.257	845	848	851	rVB4	530	473	0.05%	0.007%
25	6.354	860	864	867	rBV3	609	913	0.10%	0.013%
26	6.592	901	903	906	rVB2	673	485	0.05%	0.007%
27	6.757	921	930	944	rBV	197155	479101	50.40%	6.607%
28	6.952	961	962	964	rVB2	825	481	0.05%	0.007%
29	6.976	964	966	967	rBV2	806	478	0.05%	0.007%
30	7.123	980	990	1005	rBV	267844	599286	63.04%	8.265%
31	7.305	1012	1020	1037	rBV	194636	434787	45.74%	5.996%
32	7.452	1042	1044	1047	rVB3	759	616	0.06%	0.008%
33	7.568	1058	1063	1064	rBV2	575	799	0.08%	0.011%
34	7.665	1077	1079	1083	rVV2	539	757	0.08%	0.010%
35	7.702	1083	1085	1093	rVB4	506	872	0.09%	0.012%
36	7.897	1115	1117	1118	rBV2	521	463	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044526.D
 Acq On : 27 Dec 2024 17:17
 Operator : JC/MD
 Sample : P5344-09DL 1000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CG6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	7.988	1128	1132	1133	rVB3	709	777	0.08%	0.011%
38	8.324	1181	1187	1200	rBV	112894	193098	20.31%	2.663%
39	8.580	1225	1229	1232	rVB4	784	1207	0.13%	0.017%
40	8.647	1233	1240	1252	rBV	447742	710911	74.79%	9.804%
41	8.952	1284	1290	1302	rBV	76404	123848	13.03%	1.708%
42	9.055	1306	1307	1310	rVB2	919	535	0.06%	0.007%
43	9.183	1327	1328	1331	rVB3	563	508	0.05%	0.007%
44	9.214	1331	1333	1334	rBV2	514	448	0.05%	0.006%
45	9.275	1338	1343	1348	rVV2	8921	12828	1.35%	0.177%
46	9.384	1356	1361	1375	rBV	237112	379712	39.95%	5.236%
47	9.695	1410	1412	1414	rVB3	608	496	0.05%	0.007%
48	9.762	1421	1423	1425	rBV3	667	471	0.05%	0.006%
49	9.866	1438	1440	1443	rVB3	437	421	0.04%	0.006%
50	9.903	1443	1446	1447	rBV3	373	384	0.04%	0.005%
51	10.055	1465	1471	1484	rBV	378021	555387	58.43%	7.659%
52	10.201	1492	1495	1499	rVB3	1465	1967	0.21%	0.027%
53	10.232	1499	1500	1503	rBV3	566	443	0.05%	0.006%
54	10.652	1565	1569	1571	rBV4	688	931	0.10%	0.013%
55	11.189	1652	1657	1670	rBV	345715	445678	46.88%	6.146%
56	11.293	1672	1674	1677	rBV4	519	639	0.07%	0.009%
57	11.457	1698	1701	1702	rBV2	773	706	0.07%	0.010%
58	11.573	1717	1720	1721	rBV2	453	516	0.05%	0.007%
59	11.603	1724	1725	1728	rBV2	529	512	0.05%	0.007%
60	11.738	1744	1747	1748	rBV3	542	533	0.06%	0.007%
61	11.792	1754	1756	1758	rBV2	450	399	0.04%	0.006%
62	11.860	1766	1767	1769	rVB	646	413	0.04%	0.006%
63	11.890	1770	1772	1773	rVB2	552	381	0.04%	0.005%
64	11.975	1781	1786	1788	rBV5	1110	1879	0.20%	0.026%
65	12.018	1788	1793	1805	rVV	346487	463158	48.72%	6.387%
66	12.262	1831	1833	1835	rVB2	794	718	0.08%	0.010%
67	12.280	1835	1836	1837	rBV	745	538	0.06%	0.007%
68	12.317	1837	1842	1852	rBV	451647	575527	60.54%	7.937%
69	12.420	1857	1859	1860	rBV2	631	602	0.06%	0.008%
70	12.689	1901	1903	1904	rBV	546	409	0.04%	0.006%
71	12.719	1906	1908	1911	rVV4	612	663	0.07%	0.009%
72	12.762	1911	1915	1920	rVV	2403	3123	0.33%	0.043%
73	12.829	1924	1926	1928	rBV	595	419	0.04%	0.006%
74	12.890	1934	1936	1939	rVV3	457	413	0.04%	0.006%
75	13.030	1956	1959	1960	rBV2	527	417	0.04%	0.006%
76	13.115	1968	1973	1978	rBV3	966	1469	0.15%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044526.D
 Acq On : 27 Dec 2024 17:17
 Operator : JC/MD
 Sample : P5344-09DL 1000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CG6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	13.207	1986	1988	1990	rBV3	447	431	0.05%	0.006%
78	13.347	2006	2011	2013	rBV2	551	1074	0.11%	0.015%
79	13.542	2041	2043	2045	rBV2	414	505	0.05%	0.007%
80	13.737	2072	2075	2076	rVB2	484	452	0.05%	0.006%
81	13.756	2076	2078	2080	rBV2	427	372	0.04%	0.005%
82	13.798	2082	2085	2088	rVV5	843	1163	0.12%	0.016%
83	13.859	2093	2095	2097	rBV2	490	534	0.06%	0.007%
84	14.127	2136	2139	2145	rVB	3181	4000	0.42%	0.055%
85	14.176	2145	2147	2149	rBV3	528	493	0.05%	0.007%
86	14.249	2157	2159	2161	rBV2	443	390	0.04%	0.005%
87	14.451	2190	2192	2194	rBV	622	503	0.05%	0.007%
88	14.597	2213	2216	2217	rBV	639	492	0.05%	0.007%
89	14.737	2237	2239	2244	rBV4	522	746	0.08%	0.010%
90	14.877	2258	2262	2263	rVB2	533	625	0.07%	0.009%
91	14.896	2263	2265	2267	rBV	573	550	0.06%	0.008%
92	14.932	2270	2271	2273	rVV	775	493	0.05%	0.007%
93	14.969	2275	2277	2278	rBV2	441	396	0.04%	0.005%
94	15.115	2296	2301	2304	rBV4	559	1331	0.14%	0.018%
95	15.164	2308	2309	2311	rBV	595	457	0.05%	0.006%
96	15.286	2327	2329	2337	rVB4	825	1260	0.13%	0.017%
97	15.389	2341	2346	2352	rVV4	2171	3711	0.39%	0.051%
98	16.200	2477	2479	2480	rBV2	577	380	0.04%	0.005%
99	16.286	2489	2493	2494	rBV2	511	450	0.05%	0.006%
100	16.359	2503	2505	2507	rBV2	954	715	0.08%	0.010%

Sum of corrected areas: 7251307




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044526.D
Acq On : 27 Dec 2024 17:17
Operator : JC/MD
Sample : P5344-09DL 1000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CG6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

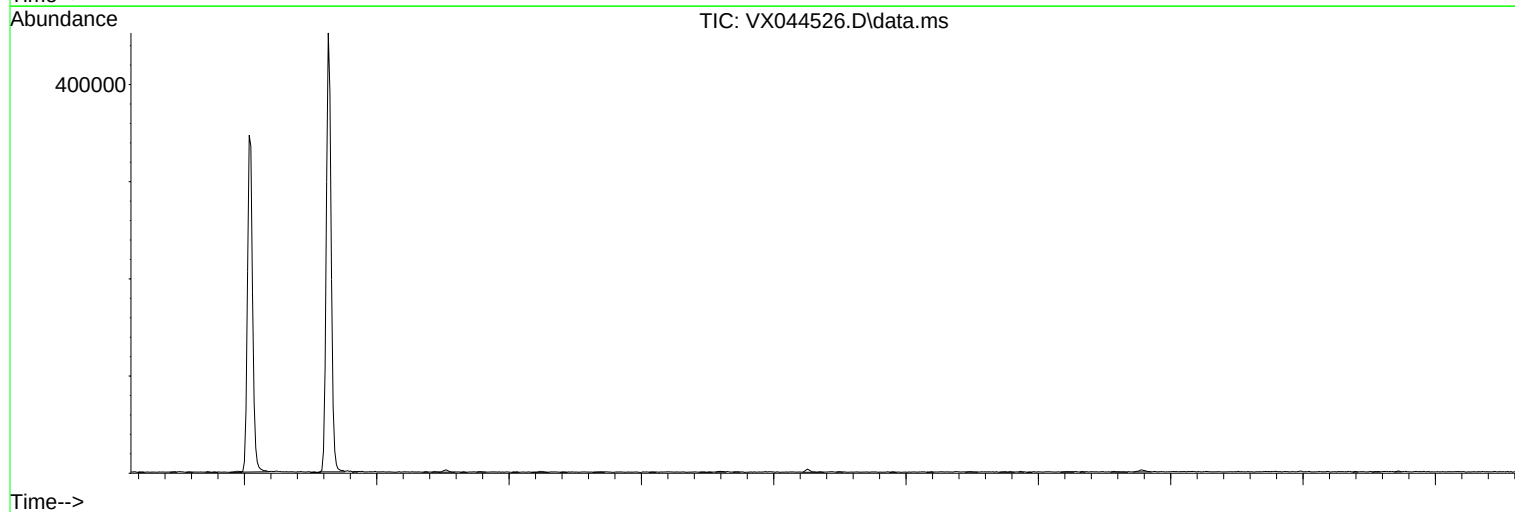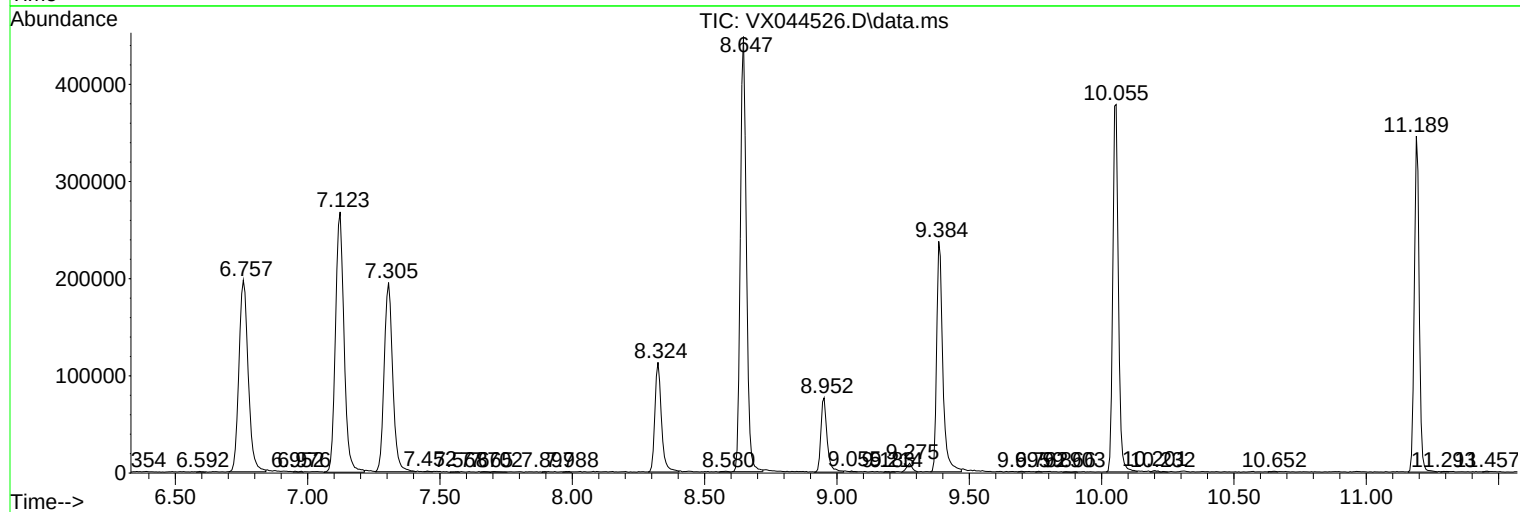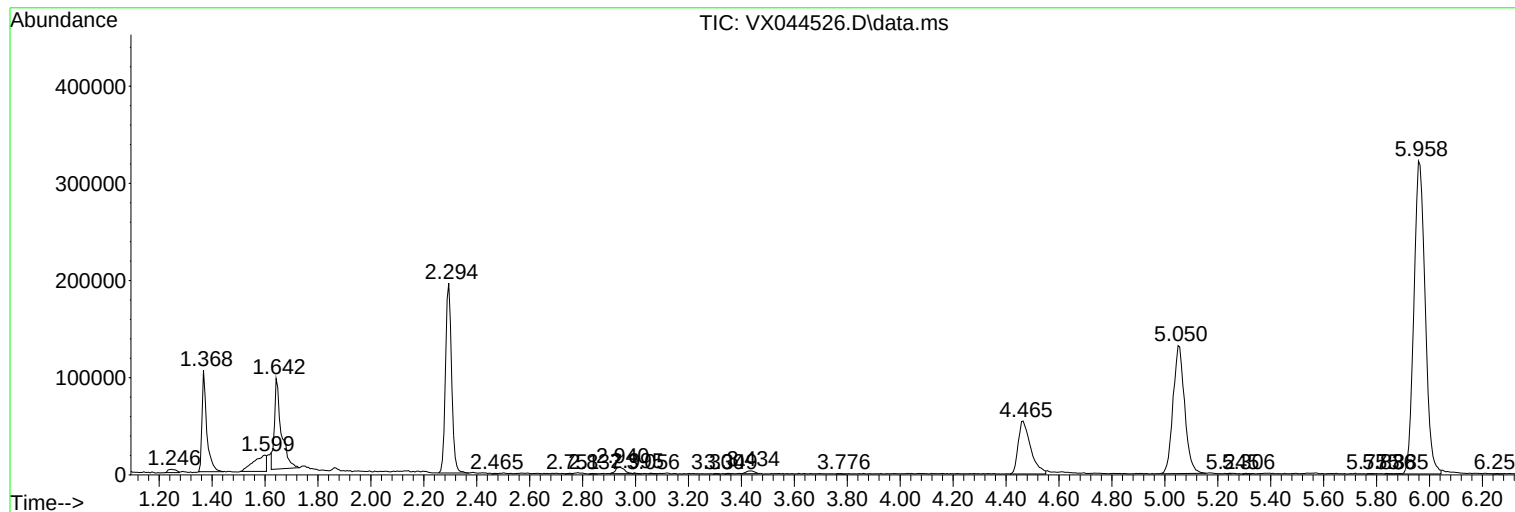

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044526.D
Acq On : 27 Dec 2024 17:17
Operator : JC/MD
Sample : P5344-09DL 1000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CG6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044526.D
Acq On : 27 Dec 2024 17:17
Operator : JC/MD
Sample : P5344-09DL 1000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CG6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------