

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044527.D
 Acq On : 27 Dec 2024 17:40
 Operator : JC/MD
 Sample : P5344-12DL 8000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COCH0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044527.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	23	25	27	rBV	2773	2524	0.26%	0.035%
2	1.368	43	46	58	rVB	117739	140585	14.26%	1.973%
3	1.642	88	91	104	rVB	101114	147755	14.99%	2.073%
4	2.294	192	198	212	rBV	214099	323452	32.81%	4.539%
5	2.782	274	278	283	rVB4	1441	2486	0.25%	0.035%
6	2.831	283	286	290	rBV3	471	674	0.07%	0.009%
7	2.947	298	305	314	rVB2	5906	15347	1.56%	0.215%
8	3.148	336	338	339	rBV2	690	468	0.05%	0.007%
9	3.428	379	384	390	rBV5	2563	5759	0.58%	0.081%
10	3.581	408	409	417	rVB2	700	1130	0.11%	0.016%
11	3.757	436	438	442	rBV2	432	434	0.04%	0.006%
12	3.818	445	448	449	rBV2	427	435	0.04%	0.006%
13	3.873	455	457	458	rBV	629	551	0.06%	0.008%
14	3.977	473	474	477	rBV2	608	640	0.06%	0.009%
15	4.007	477	479	481	rVB	732	496	0.05%	0.007%
16	4.038	481	484	488	rBV4	324	458	0.05%	0.006%
17	4.160	501	504	505	rBV3	482	491	0.05%	0.007%
18	4.465	545	554	571	rBV	59705	186465	18.91%	2.616%
19	5.050	638	650	667	rBV	128775	417640	42.36%	5.860%
20	5.599	738	740	744	rVB4	461	642	0.07%	0.009%
21	5.782	767	770	772	rBV3	594	844	0.09%	0.012%
22	5.958	788	799	823	rBV3	325995	985891	100.00%	13.834%
23	6.172	831	834	835	rBV3	453	479	0.05%	0.007%
24	6.367	864	866	869	rBV3	854	906	0.09%	0.013%
25	6.391	869	870	871	rBV	751	419	0.04%	0.006%
26	6.641	908	911	913	rVB3	515	408	0.04%	0.006%
27	6.757	922	930	946	rBV	191764	469693	47.64%	6.591%
28	7.123	981	990	1005	rBV	195311	440647	44.70%	6.183%
29	7.306	1012	1020	1034	rBV	194812	436525	44.28%	6.125%
30	7.647	1074	1076	1077	rBV	691	494	0.05%	0.007%
31	7.745	1090	1092	1093	rBV	614	420	0.04%	0.006%
32	7.787	1097	1099	1102	rBV3	574	508	0.05%	0.007%
33	7.842	1105	1108	1110	rBV2	314	414	0.04%	0.006%
34	8.123	1152	1154	1155	rBV2	693	478	0.05%	0.007%
35	8.244	1168	1174	1176	rBV2	589	979	0.10%	0.014%
36	8.324	1181	1187	1204	rBV	121848	202202	20.51%	2.837%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044527.D
 Acq On : 27 Dec 2024 17:40
 Operator : JC/MD
 Sample : P5344-12DL 8000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COCH0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	8.501	1215	1216	1219	rBV2	567	457	0.05%	0.006%
38	8.580	1226	1229	1232	rVB3	595	717	0.07%	0.010%
39	8.647	1234	1240	1257	rVV	462380	739141	74.97%	10.372%
40	8.952	1285	1290	1300	rBV	81023	127616	12.94%	1.791%
41	9.098	1312	1314	1315	rBV	587	496	0.05%	0.007%
42	9.165	1322	1325	1328	rVB4	587	636	0.06%	0.009%
43	9.275	1339	1343	1348	rBV3	4097	6724	0.68%	0.094%
44	9.385	1356	1361	1384	rBV	255367	389930	39.55%	5.472%
45	9.702	1411	1413	1417	rVB2	784	653	0.07%	0.009%
46	9.854	1436	1438	1441	rBV3	420	542	0.05%	0.008%
47	9.909	1445	1447	1450	rBV4	633	805	0.08%	0.011%
48	9.951	1452	1454	1457	rVB2	642	645	0.07%	0.009%
49	10.049	1465	1470	1481	rBV	371057	541675	54.94%	7.601%
50	10.439	1531	1534	1535	rVV2	650	595	0.06%	0.008%
51	10.640	1565	1567	1568	rBV2	652	474	0.05%	0.007%
52	10.714	1578	1579	1582	rVB2	713	485	0.05%	0.007%
53	10.854	1599	1602	1604	rBV3	496	622	0.06%	0.009%
54	10.878	1604	1606	1611	rVV3	572	811	0.08%	0.011%
55	11.128	1642	1647	1648	rBV2	638	732	0.07%	0.010%
56	11.189	1652	1657	1668	rBV	367402	458680	46.52%	6.436%
57	11.311	1674	1677	1680	rVB4	748	883	0.09%	0.012%
58	11.354	1682	1684	1689	rVB3	541	599	0.06%	0.008%
59	11.402	1689	1692	1693	rVB	488	419	0.04%	0.006%
60	11.616	1725	1727	1730	rVB3	537	527	0.05%	0.007%
61	11.689	1737	1739	1742	rBV3	455	643	0.07%	0.009%
62	11.756	1747	1750	1751	rBV2	493	571	0.06%	0.008%
63	11.945	1780	1781	1783	rBV2	502	411	0.04%	0.006%
64	12.018	1788	1793	1803	rVV	343116	443583	44.99%	6.224%
65	12.317	1836	1842	1851	rBV	462314	586702	59.51%	8.233%
66	12.640	1892	1895	1897	rBV2	635	712	0.07%	0.010%
67	12.719	1903	1908	1910	rVB3	517	888	0.09%	0.012%
68	12.762	1910	1915	1919	rBV3	2422	3738	0.38%	0.052%
69	12.792	1919	1920	1923	rVB	730	497	0.05%	0.007%
70	12.872	1929	1933	1934	rVB2	494	481	0.05%	0.007%
71	12.951	1944	1946	1950	rVV3	503	515	0.05%	0.007%
72	13.024	1956	1958	1961	rVB2	761	521	0.05%	0.007%
73	13.079	1965	1967	1968	rBV2	455	409	0.04%	0.006%
74	13.103	1969	1971	1972	rVB2	670	414	0.04%	0.006%
75	13.122	1972	1974	1975	rBV2	520	552	0.06%	0.008%
76	13.213	1986	1989	1991	rBV2	402	437	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044527.D
 Acq On : 27 Dec 2024 17:40
 Operator : JC/MD
 Sample : P5344-12DL 8000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CH0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	13.274	1997	1999	2001	rBV2	491	482	0.05%	0.007%
78	13.524	2038	2040	2043	rBV2	519	650	0.07%	0.009%
79	13.548	2043	2044	2047	rVB2	833	526	0.05%	0.007%
80	13.609	2050	2054	2058	rBV3	540	1136	0.12%	0.016%
81	13.701	2067	2069	2073	rVB3	396	515	0.05%	0.007%
82	13.792	2081	2084	2086	rBV2	610	618	0.06%	0.009%
83	13.884	2095	2099	2101	rVB3	473	563	0.06%	0.008%
84	14.128	2135	2139	2143	rVV	3900	4526	0.46%	0.064%
85	14.231	2154	2156	2159	rBV	435	512	0.05%	0.007%
86	14.371	2176	2179	2182	rBV2	623	675	0.07%	0.009%
87	14.548	2205	2208	2212	rVB3	615	694	0.07%	0.010%
88	14.969	2276	2277	2279	rBV2	519	507	0.05%	0.007%
89	15.322	2333	2335	2338	rVB3	650	559	0.06%	0.008%
90	15.390	2343	2346	2350	rVV3	2051	3305	0.34%	0.046%
91	15.450	2354	2356	2358	rBV	454	428	0.04%	0.006%
92	15.487	2361	2362	2364	rBV2	684	428	0.04%	0.006%
93	15.646	2385	2388	2392	rVV3	613	1139	0.12%	0.016%
94	16.280	2490	2492	2494	rBB2	546	411	0.04%	0.006%
95	16.316	2496	2498	2500	rVV3	716	562	0.06%	0.008%
96	16.365	2504	2506	2508	rVB2	646	465	0.05%	0.007%
97	16.438	2517	2518	2521	rBV3	507	411	0.04%	0.006%
98	16.566	2537	2539	2541	rVB	568	421	0.04%	0.006%
99	16.591	2541	2543	2545	rBV3	595	623	0.06%	0.009%
100	16.706	2560	2562	2567	rVB3	710	691	0.07%	0.010%




Sum of corrected areas: 7126524

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044527.D
Acq On : 27 Dec 2024 17:40
Operator : JC/MD
Sample : P5344-12DL 8000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CH0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

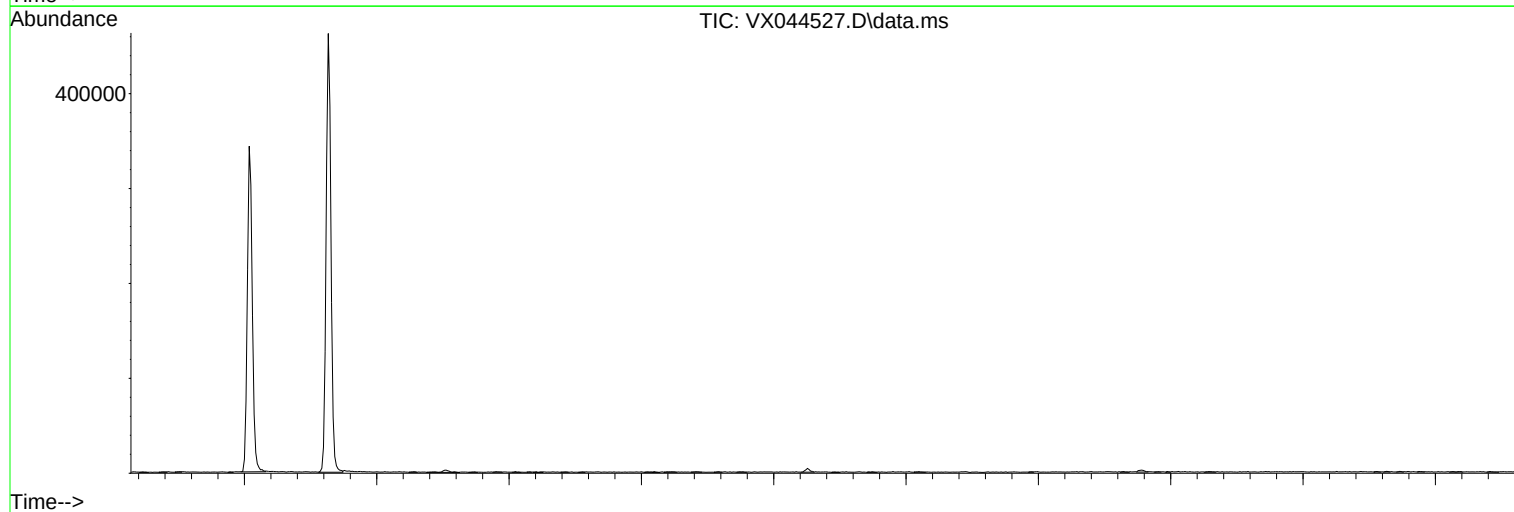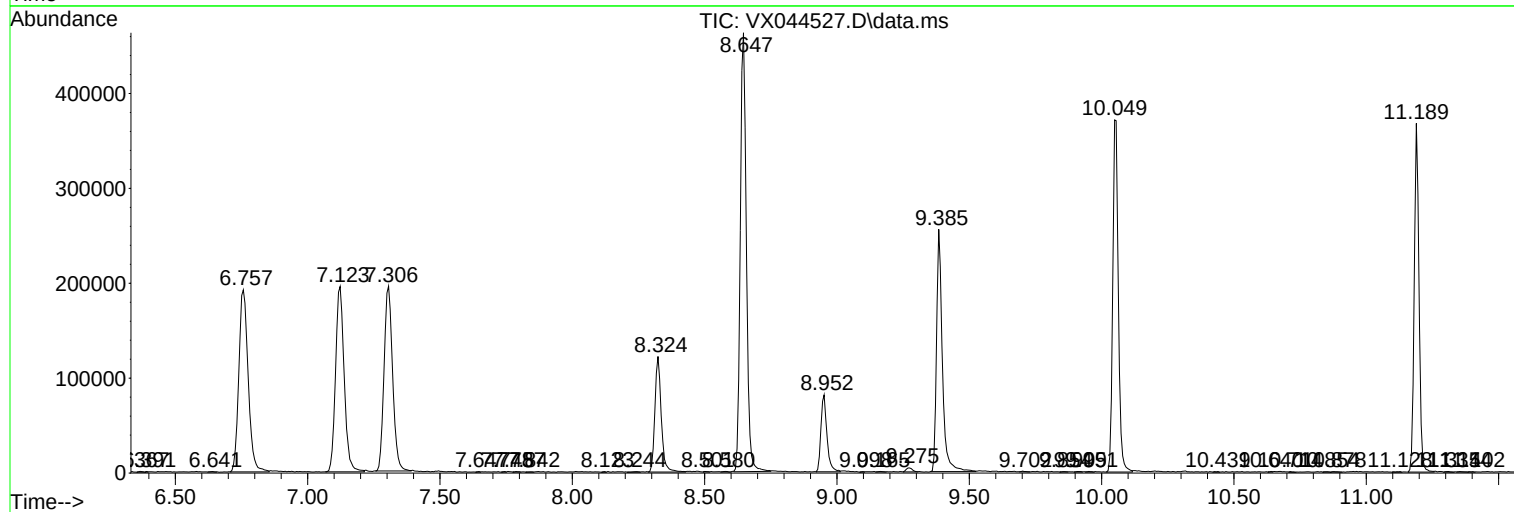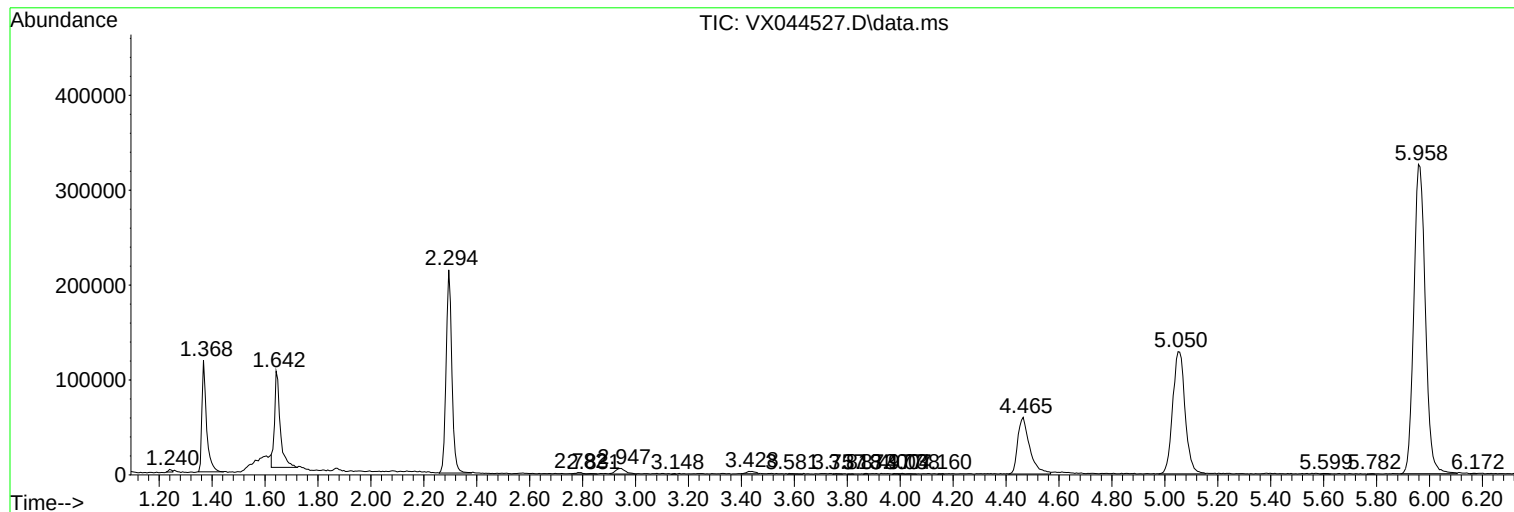

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044527.D
Acq On : 27 Dec 2024 17:40
Operator : JC/MD
Sample : P5344-12DL 8000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CH0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044527.D
Acq On : 27 Dec 2024 17:40
Operator : JC/MD
Sample : P5344-12DL 8000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CH0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
