

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044528.D
 Acq On : 27 Dec 2024 18:03
 Operator : JC/MD
 Sample : VIBLK688
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK688

Integration Parameters: LSCINT.P

Integrator: RTE

Smothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044528.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	27	rBV	3088	3314	0.34%	0.048%
2	1.368	42	46	55	rBV	117567	141953	14.48%	2.058%
3	1.642	88	91	102	rVB	97296	138531	14.13%	2.009%
4	2.294	192	198	211	rVB	208391	318380	32.48%	4.616%
5	2.483	227	229	230	rBV	652	590	0.06%	0.009%
6	2.569	242	243	246	rBV3	741	478	0.05%	0.007%
7	2.715	265	267	268	rBV2	573	438	0.04%	0.006%
8	2.733	268	270	273	rVV2	682	763	0.08%	0.011%
9	2.782	276	278	283	rVB5	1579	2200	0.22%	0.032%
10	2.849	286	289	292	rVB3	498	677	0.07%	0.010%
11	2.934	297	303	309	rBV4	4287	10513	1.07%	0.152%
12	3.093	325	329	331	rBV4	496	537	0.05%	0.008%
13	3.264	354	357	359	rBV3	351	515	0.05%	0.007%
14	3.355	368	372	373	rBV3	520	585	0.06%	0.008%
15	3.440	379	386	392	rBV4	3465	8779	0.90%	0.127%
16	3.636	416	418	421	rVB3	572	535	0.05%	0.008%
17	3.721	429	432	433	rBV3	497	473	0.05%	0.007%
18	3.806	443	446	447	rBV2	467	399	0.04%	0.006%
19	3.818	447	448	451	rBV3	366	409	0.04%	0.006%
20	3.965	470	472	475	rBV2	740	732	0.07%	0.011%
21	4.355	532	536	539	rBV3	550	595	0.06%	0.009%
22	4.385	539	541	543	rBV3	433	415	0.04%	0.006%
23	4.459	546	553	570	rBV	58392	184116	18.78%	2.670%
24	4.855	615	618	620	rBV2	373	375	0.04%	0.005%
25	4.873	620	621	624	rVV2	607	481	0.05%	0.007%
26	4.965	633	636	638	rBV	548	585	0.06%	0.008%
27	5.050	639	650	666	rVV2	135753	416705	42.51%	6.042%
28	5.294	688	690	693	rBV2	404	453	0.05%	0.007%
29	5.385	701	705	708	rBV4	556	916	0.09%	0.013%
30	5.599	739	740	742	rBV	430	416	0.04%	0.006%
31	5.964	788	800	823	rBV2	325663	980265	100.00%	14.214%
32	6.245	844	846	847	rBV2	740	464	0.05%	0.007%
33	6.330	858	860	863	rVB3	494	399	0.04%	0.006%
34	6.422	874	875	880	rBV3	715	1053	0.11%	0.015%
35	6.483	882	885	886	rBV2	511	597	0.06%	0.009%
36	6.659	913	914	917	rBV	347	388	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044528.D
 Acq On : 27 Dec 2024 18:03
 Operator : JC/MD
 Sample : VIBLK688
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK688

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	6.690	917	919	920	rBV	840	438	0.04%	0.006%
38	6.757	921	930	951	rVV	204094	495571	50.55%	7.186%
39	7.129	982	991	998	rBV7	5927	16016	1.63%	0.232%
40	7.306	1011	1020	1033	rBV	201560	447090	45.61%	6.483%
41	7.586	1062	1066	1067	rBV3	630	741	0.08%	0.011%
42	7.641	1073	1075	1076	rVB	843	401	0.04%	0.006%
43	7.757	1092	1094	1097	rBV2	483	534	0.05%	0.008%
44	8.080	1145	1147	1150	rBV2	424	438	0.04%	0.006%
45	8.116	1150	1153	1154	rBV3	561	566	0.06%	0.008%
46	8.324	1181	1187	1201	rBV	118278	204107	20.82%	2.960%
47	8.574	1226	1228	1229	rBV2	529	387	0.04%	0.006%
48	8.647	1232	1240	1251	rBV	455555	734618	74.94%	10.652%
49	8.946	1283	1289	1300	rBV	79861	128194	13.08%	1.859%
50	9.208	1331	1332	1335	rBV2	411	514	0.05%	0.007%
51	9.250	1337	1339	1341	rBV3	464	421	0.04%	0.006%
52	9.317	1348	1350	1353	rBV3	342	358	0.04%	0.005%
53	9.385	1356	1361	1375	rBV	237498	382679	39.04%	5.549%
54	9.628	1398	1401	1402	rBV3	639	480	0.05%	0.007%
55	9.854	1434	1438	1442	rVB4	479	813	0.08%	0.012%
56	9.945	1451	1453	1455	rBV	413	505	0.05%	0.007%
57	9.970	1455	1457	1459	rVB2	500	361	0.04%	0.005%
58	10.049	1465	1470	1480	rBV	402622	568202	57.96%	8.239%
59	10.195	1492	1494	1498	rBV4	957	1286	0.13%	0.019%
60	10.305	1510	1512	1516	rBV3	1124	1335	0.14%	0.019%
61	10.482	1539	1541	1543	rVV2	636	580	0.06%	0.008%
62	10.823	1595	1597	1599	rVB2	389	398	0.04%	0.006%
63	10.927	1612	1614	1616	rBV	423	395	0.04%	0.006%
64	11.073	1636	1638	1642	rVB3	405	447	0.05%	0.006%
65	11.122	1642	1646	1648	rBV3	444	592	0.06%	0.009%
66	11.189	1652	1657	1669	rVV	398567	505416	51.56%	7.328%
67	11.390	1688	1690	1693	rVB4	472	590	0.06%	0.009%
68	11.451	1697	1700	1703	rVV3	588	749	0.08%	0.011%
69	11.555	1715	1717	1720	rBV2	378	392	0.04%	0.006%
70	11.756	1747	1750	1753	rVV2	855	1272	0.13%	0.018%
71	12.018	1788	1793	1804	rVV	412334	516134	52.65%	7.484%
72	12.244	1826	1830	1833	rBV3	502	718	0.07%	0.010%
73	12.317	1837	1842	1855	rBV	515657	641773	65.47%	9.306%
74	12.530	1875	1877	1879	rBV2	511	581	0.06%	0.008%
75	12.646	1895	1896	1900	rVB2	586	571	0.06%	0.008%
76	12.762	1912	1915	1919	rVB2	2416	2856	0.29%	0.041%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
 Data File : VX044528.D
 Acq On : 27 Dec 2024 18:03
 Operator : JC/MD
 Sample : VIBLK688
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK688

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	12.914	1938	1940	1943	rBV	566	579	0.06%	0.008%
78	13.439	2024	2026	2027	rBV	524	423	0.04%	0.006%
79	13.634	2057	2058	2061	rVB2	599	379	0.04%	0.005%
80	13.670	2062	2064	2066	rVB	761	486	0.05%	0.007%
81	13.731	2071	2074	2078	rBV2	881	1049	0.11%	0.015%
82	13.902	2100	2102	2106	rBV4	380	571	0.06%	0.008%
83	13.987	2114	2116	2118	rBV2	610	482	0.05%	0.007%
84	14.091	2131	2133	2134	rBV	562	362	0.04%	0.005%
85	14.128	2134	2139	2145	rVB3	2938	4513	0.46%	0.065%
86	14.420	2186	2187	2190	rBV2	694	632	0.06%	0.009%
87	14.634	2220	2222	2224	rVB2	500	377	0.04%	0.005%
88	14.755	2240	2242	2244	rVB	709	470	0.05%	0.007%
89	14.938	2270	2272	2273	rBV	668	509	0.05%	0.007%
90	15.140	2303	2305	2307	rVB2	792	547	0.06%	0.008%
91	15.298	2329	2331	2334	rVB2	501	627	0.06%	0.009%
92	15.322	2334	2335	2338	rBV2	761	804	0.08%	0.012%
93	15.475	2357	2360	2362	rBV4	609	786	0.08%	0.011%
94	15.542	2370	2371	2374	rVB2	779	508	0.05%	0.007%
95	15.926	2433	2434	2437	rBV2	686	806	0.08%	0.012%
96	16.237	2484	2485	2487	rVB	577	363	0.04%	0.005%
97	16.499	2526	2528	2532	rBV3	871	1383	0.14%	0.020%
98	16.639	2549	2551	2552	rBV2	546	430	0.04%	0.006%
99	16.676	2555	2557	2559	rVV	508	460	0.05%	0.007%
100	16.743	2566	2568	2571	rBV2	521	520	0.05%	0.008%

Sum of corrected areas: 6896609




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044528.D
Acq On : 27 Dec 2024 18:03
Operator : JC/MD
Sample : VIBLK688
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK688

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

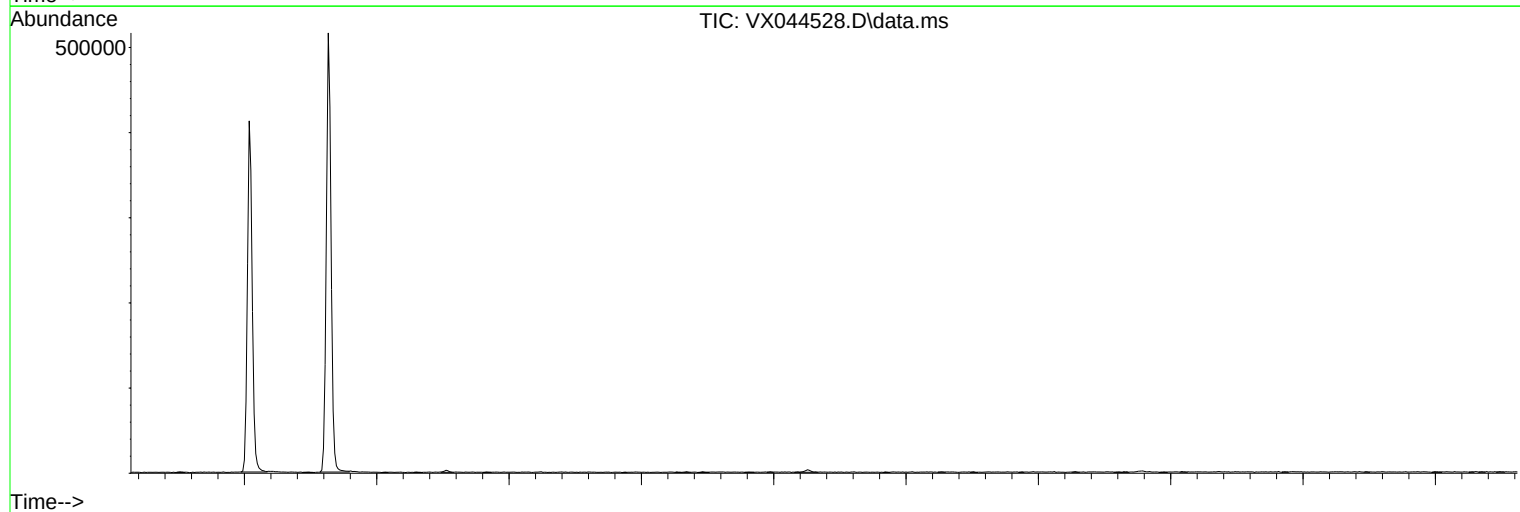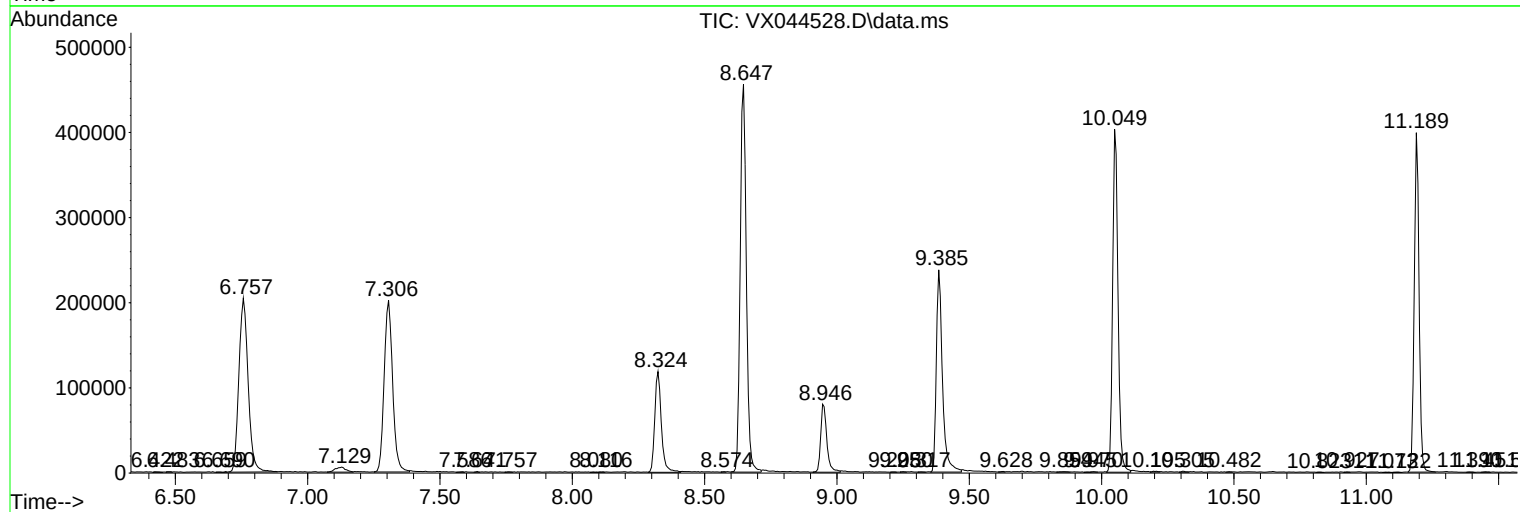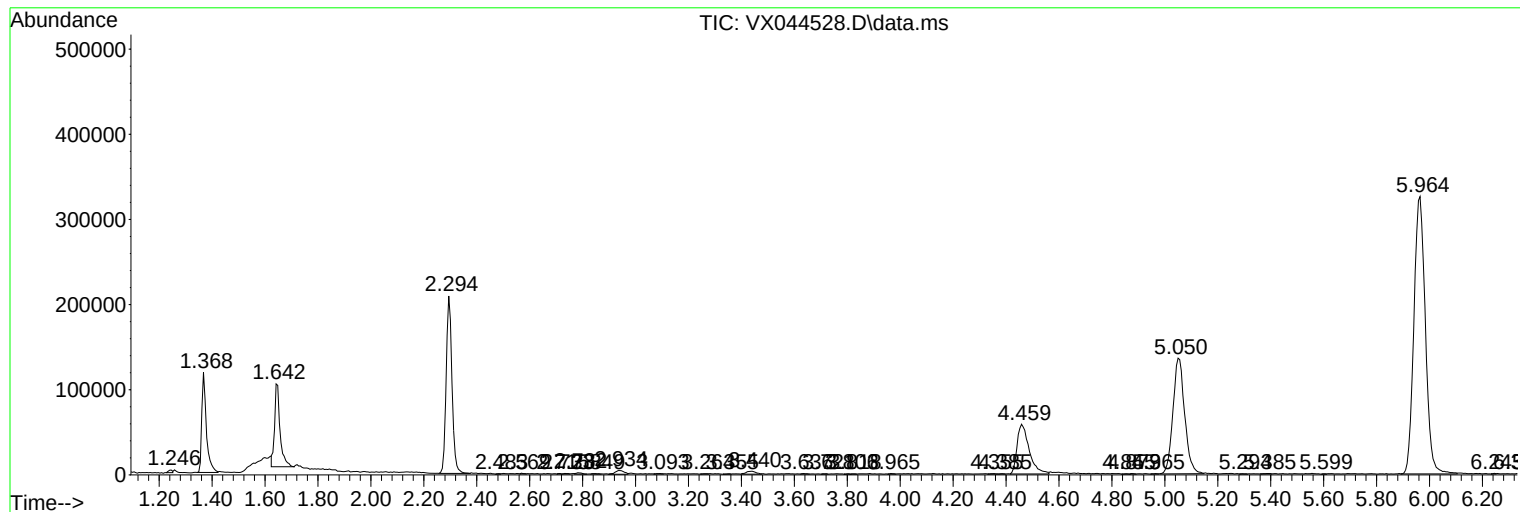

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044528.D
Acq On : 27 Dec 2024 18:03
Operator : JC/MD
Sample : VIBLK688
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK688

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044528.D
Acq On : 27 Dec 2024 18:03
Operator : JC/MD
Sample : VIBLK688
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK688

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
