
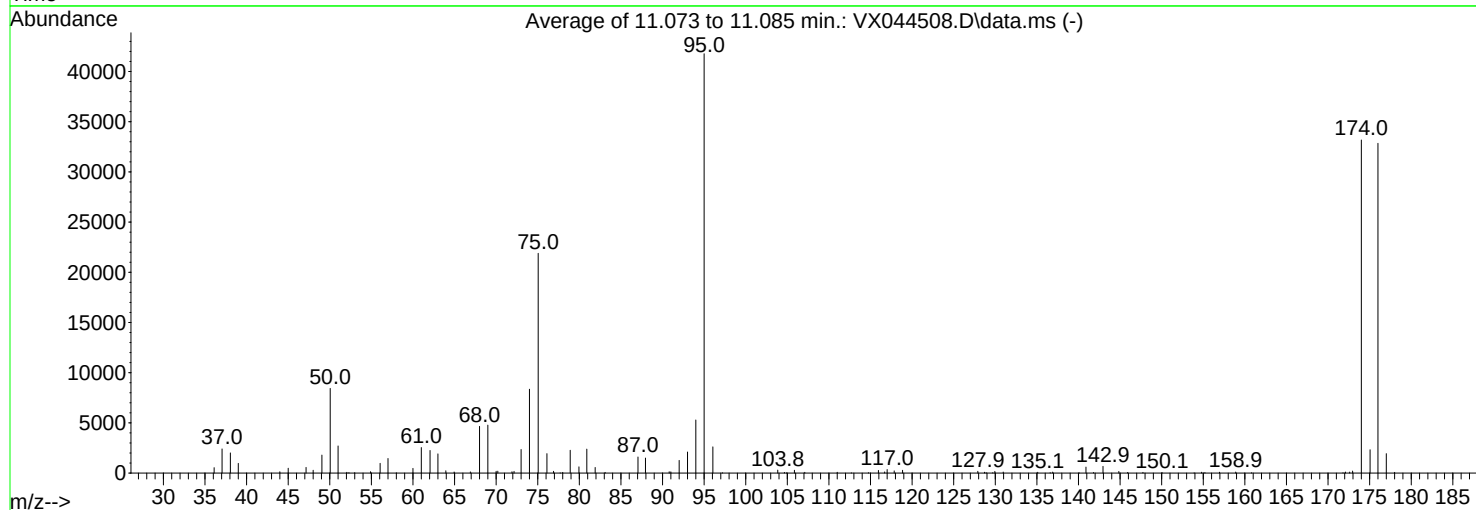


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122724\
Data File : VX044508.D
Acq On : 27 Dec 2024 07:54
Operator : JC/MD
Sample : BFB709
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB709

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Title : VOC Analysis
Last Update : Fri Dec 27 22:07:46 2024

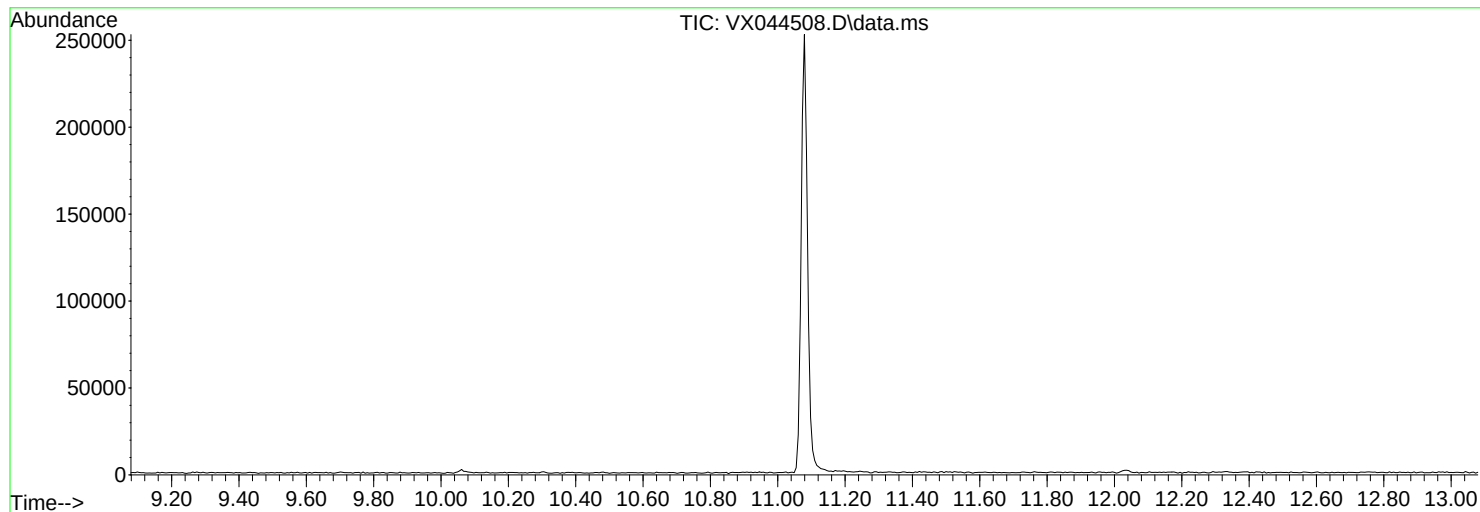

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	8437	PASS
75	95	30	80	52.4	21891	PASS
95	95	100	100	100.0	41771	PASS
96	95	5	9	6.3	2611	PASS
173	174	0.00	2	0.6	202	PASS
174	95	50	120	79.4	33179	PASS
175	174	5	9	7.0	2324	PASS
176	174	95	101	99.0	32848	PASS
177	176	5	9	5.9	1939	PASS

m/z	Abundance
38.10	129.0
38.90	470.0
39.90	542.0
40.90	52.0
44.00	375.0

Instrument :
MSVOA_X
ClientSampleId :
BFB709

m/z	Abundance
36.10	640.0
37.10	2565.0
38.10	2230.0
39.00	1597.0
40.00	702.0
44.00	495.0
44.90	490.0
47.10	533.0
48.10	280.0
49.00	1840.0
50.10	8557.0
51.00	2853.0
52.20	72.0
53.00	95.0
54.90	124.0
56.00	1008.0
57.00	1553.0
58.00	63.0
59.90	440.0
61.00	2762.0
62.10	2329.0
63.00	2096.0
63.90	222.0
65.00	69.0
66.90	53.0
68.00	4827.0
69.00	4997.0
70.00	550.0
71.90	410.0
73.00	2581.0
74.00	8586.0
75.10	22696.0
76.10	2161.0
76.80	178.0
78.00	205.0
78.90	2453.0
79.90	668.0
80.90	2166.0
81.90	481.0
83.10	92.0
87.00	1664.0
87.90	1704.0
90.80	227.0
92.00	1293.0
93.00	1841.0
94.00	5201.0
95.00	40632.0
96.10	2487.0
97.20	107.0
103.80	242.0
104.60	109.0
105.90	273.0
107.10	85.0
111.00	147.0
112.70	68.0
116.00	291.0
116.90	289.0
117.80	218.0
118.90	297.0
127.90	185.0
128.70	112.0
129.70	115.0
130.00	114.0
131.10	63.0
135.10	79.0
136.90	144.0
140.80	489.0
143.00	649.0
144.90	75.0
147.80	64.0
153.90	51.0
154.80	96.0
155.20	82.0
159.00	68.0
172.10	183.0
172.90	316.0
174.00	27864.0
175.10	2117.0
176.00	27488.0
177.00	1939.0
178.10	65.0

Instrument :
MSVOA_X
ClientSampleId :
BFB709

m/z	Abundance
36.10	491.0
37.10	2715.0
38.10	2452.0
39.10	1674.0
40.00	450.0
44.10	622.0
45.00	636.0
47.20	574.0
48.00	351.0
49.10	2079.0
50.00	10410.0
51.00	3178.0
52.00	158.0
54.90	132.0
56.10	1027.0
57.00	1627.0
60.00	605.0
61.00	2838.0
62.10	2716.0
63.00	2318.0
64.00	339.0
64.90	198.0
66.90	178.0
68.00	5534.0
69.00	5470.0
70.20	387.0
72.20	218.0
73.00	2593.0
74.00	9017.0
75.00	25816.0
76.10	2162.0
76.90	245.0
77.70	55.0
78.90	2428.0
80.00	685.0
80.90	2983.0
81.90	786.0
83.10	111.0
87.00	1842.0
88.00	1864.0
91.00	381.0
91.90	1462.0
93.00	2873.0
94.00	6358.0
95.00	49888.0
96.00	3261.0
103.80	372.0
104.70	93.0
105.80	369.0
107.10	89.0
111.00	99.0
114.80	64.0
116.00	226.0
117.00	462.0
117.90	288.0
118.80	326.0
128.00	254.0
128.70	152.0
129.90	203.0
130.90	128.0
135.10	67.0
136.90	159.0
140.90	849.0
141.80	104.0
143.00	697.0
144.90	268.0
145.90	90.0
147.70	66.0
150.00	84.0
154.80	71.0
155.20	63.0
156.90	111.0
158.90	117.0
160.80	111.0
171.80	106.0
172.60	303.0
174.00	39032.0
175.00	2809.0
176.00	38480.0
177.00	2280.0
178.10	57.0

Instrument :
MSVOA_X
ClientSampleId :
BFB709

m/z	Abundance
35.90	255.0
36.20	240.0
37.00	1934.0
38.00	1723.0
39.00	1036.0
40.00	437.0
44.10	417.0
45.10	322.0
47.20	585.0
47.90	220.0
49.10	1456.0
50.10	6344.0
51.00	2072.0
52.30	128.0
54.90	164.0
56.10	884.0
57.00	1175.0
60.10	358.0
61.00	2030.0
62.00	1713.0
63.00	1326.0
64.00	138.0
64.90	69.0
66.90	131.0
68.00	3600.0
69.00	3862.0
70.20	193.0
72.10	296.0
73.00	1866.0
74.00	7453.0
75.00	17160.0
76.10	1485.0
77.00	112.0
78.90	1938.0
80.00	506.0
80.90	2017.0
81.90	409.0
87.10	1295.0
87.90	922.0
90.80	176.0
92.10	1039.0
93.00	1587.0
94.00	4307.0
95.00	34792.0
96.00	2085.0
103.90	279.0
104.90	76.0
105.80	211.0
107.10	62.0
114.70	60.0
115.90	274.0
116.70	343.0
117.10	312.0
117.90	156.0
118.80	214.0
127.80	92.0
128.90	133.0
130.00	195.0
130.90	127.0
135.10	102.0
136.60	125.0
140.10	54.0
141.00	458.0
141.80	67.0
142.90	657.0
144.80	149.0
145.90	96.0
147.80	84.0
150.10	64.0
154.80	97.0
157.00	151.0
158.80	132.0
172.10	139.0
173.00	289.0
174.00	32640.0
175.00	2047.0
176.00	32576.0
177.00	1599.0
177.90	88.0

Instrument :
MSVOA_X
ClientSampleId :
BFB709