

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122820\
 Data File : VX020409.D
 Acq On : 28 Dec 2020 13:35
 Operator : JC/MD
 Sample : L5219-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SS013-13-TB-122320

Quant Time: Dec 29 00:39:12 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 18 13:09:49 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.629	168	252172	50.00	ug/l	0.01
34) 1,4-Difluorobenzene	6.830	114	411558	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.098	117	379342	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.061	152	159082	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.032	65	156948	46.43	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	92.86%
35) Dibromofluoromethane	5.465	113	128396	48.77	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	97.54%
50) Toluene-d8	8.696	98	501286	49.47	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	98.94%
62) 4-Bromofluorobenzene	11.122	95	174207	44.91	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	89.82%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\WX122820\
Data File : VX020409.D
Acq On : 28 Dec 2020 13:35
Operator : JC/MD
Sample : L5219-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SS013-13-TB-122320

Quant Time: Dec 29 00:39:12 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 18 13:09:49 2020
Response via : Initial Calibration




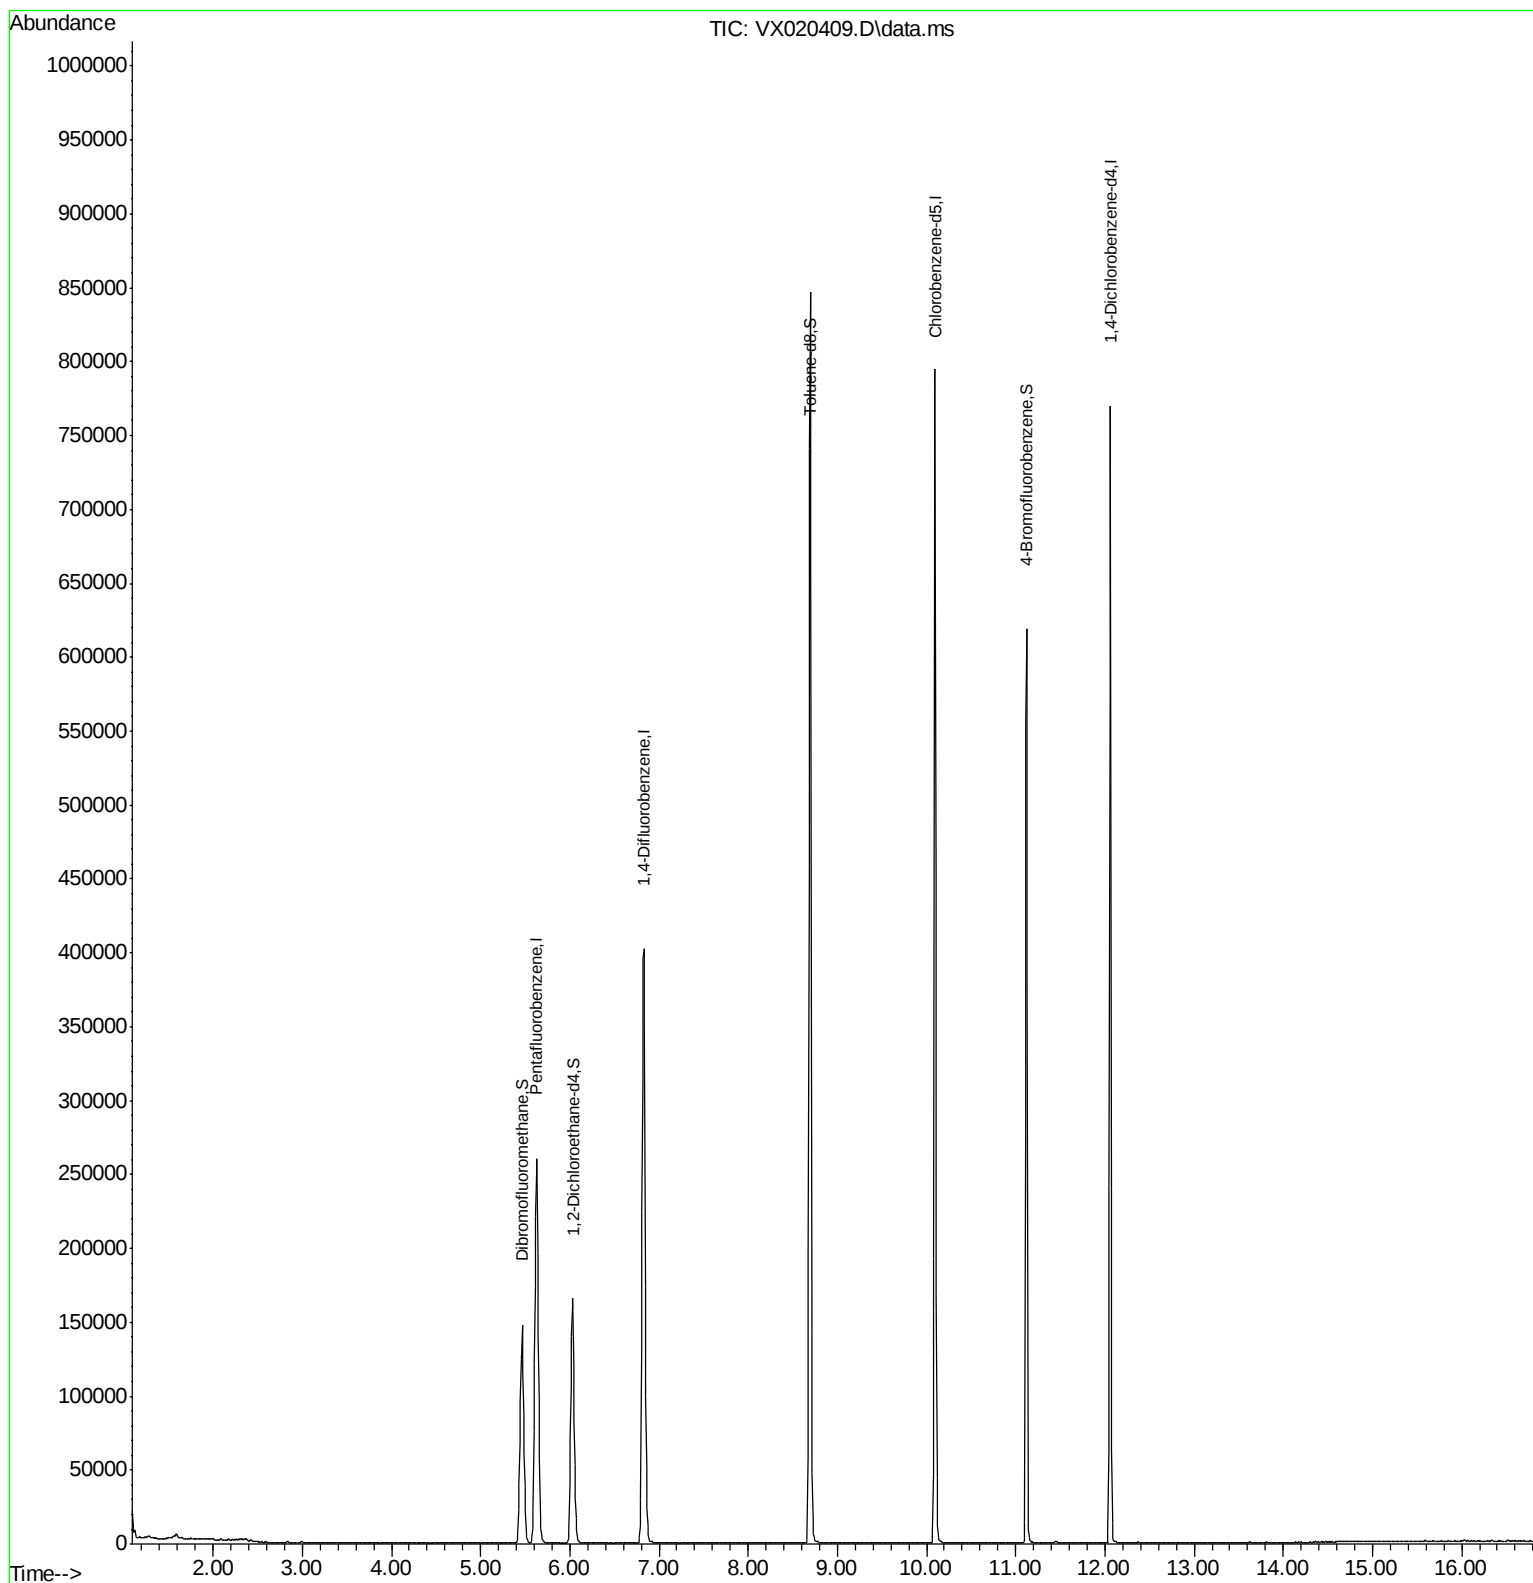


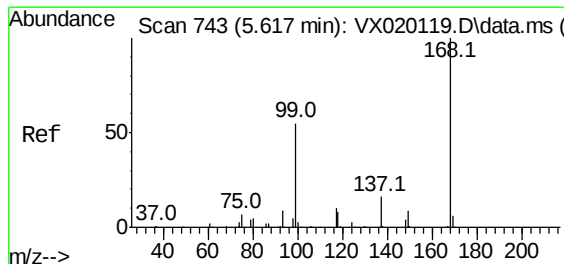

Pentafluorobenzene
 Concen: 50.00 ug/l
 RT: 5.629 min Scan# 745
 Delta R.T. 0.012 min
 Lab File: VX020409.D
 Acq: 28 Dec 2020 13:35




Instrument :
 MSVOA_X
 ClientSampleId :
 SS013-13-TB-122320


Tgt Ion:168 Resp: 252172
 Ion Ratio Lower Upper
 168 100
 99 55.3 45.8 68.6

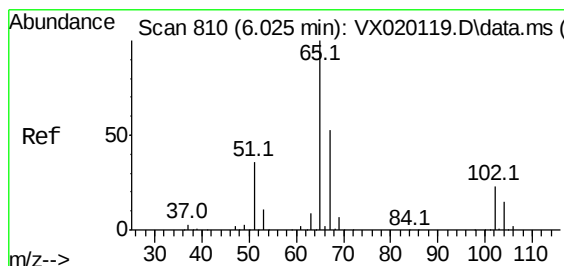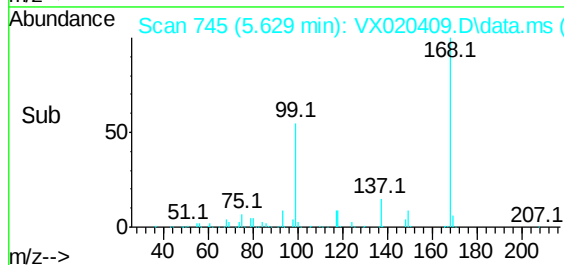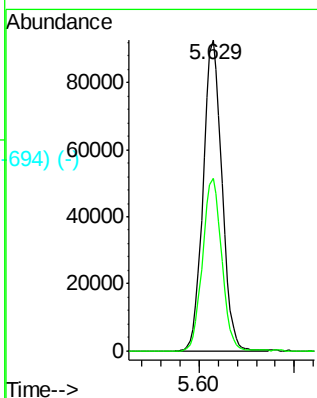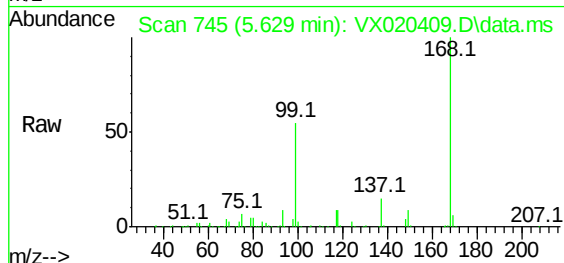

1,2-Dichloroethane-d4
 Concen: 46.43 ug/l
 RT: 6.032 min Scan# 811
 Delta R.T. 0.006 min
 Lab File: VX020409.D
 Acq: 28 Dec 2020 13:35

Tgt Ion: 65 Resp: 156948
 Ion Ratio Lower Upper
 65 100
 67 54.5 0.0 105.4


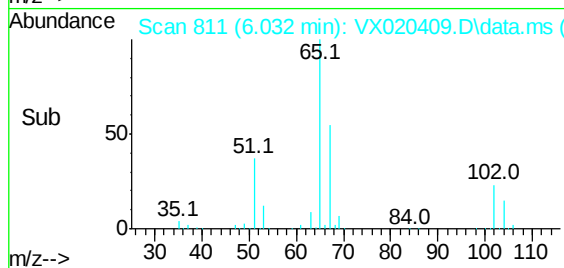
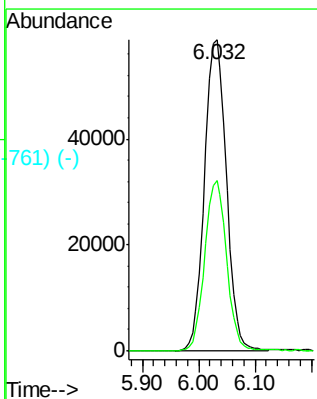
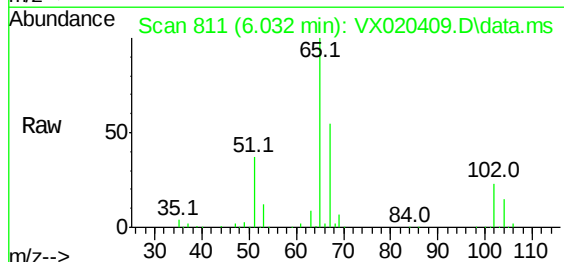


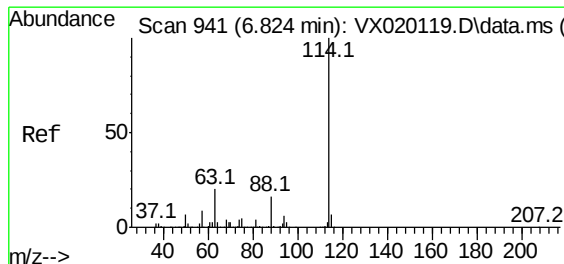

1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 6.830 min Scan# 942
 Delta R.T. 0.006 min
 Lab File: VX020409.D
 Acq: 28 Dec 2020 13:35




Instrument :
 MSVOA_X
 ClientSampleId :
 SS013-13-TB-122320


Tgt Ion:	114	Resp:	411558
Ion Ratio	Lower	Upper	
114	100		
63	20.5	0.0	40.8
88	16.6	0.0	32.8

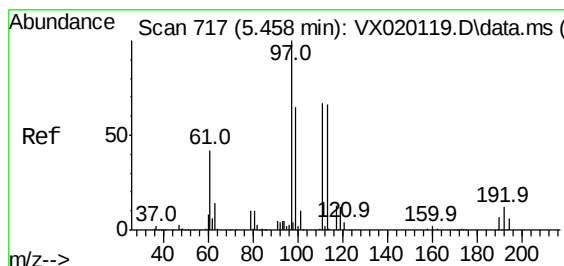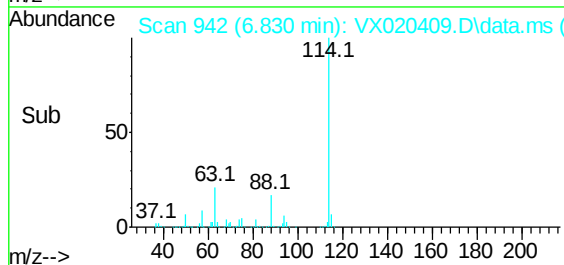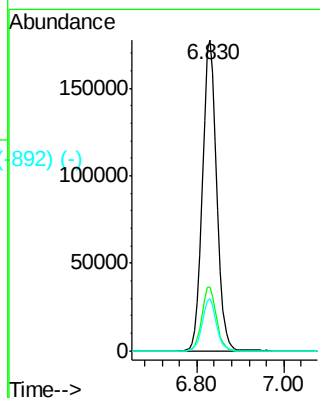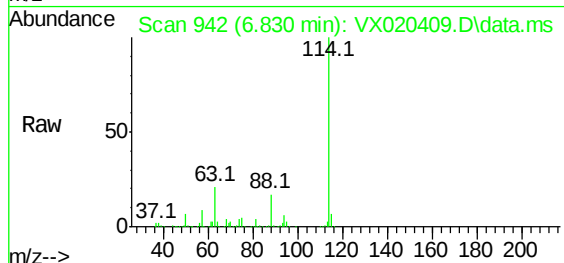

Dibromofluoromethane
 Concen: 48.77 ug/l
 RT: 5.465 min Scan# 718
 Delta R.T. 0.007 min
 Lab File: VX020409.D
 Acq: 28 Dec 2020 13:35

Tgt Ion:	113	Resp:	128396
Ion Ratio	Lower	Upper	
113	100		
111	104.3	81.9	122.9
192	21.4	16.7	25.1


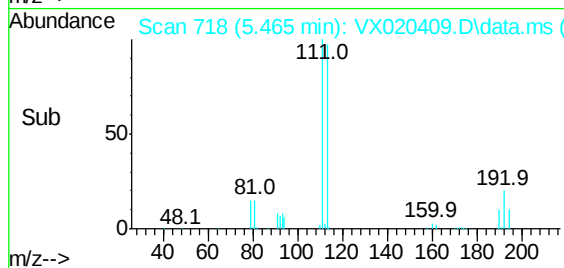
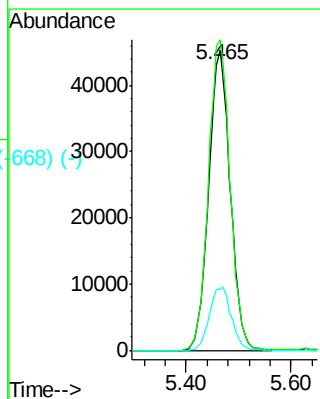
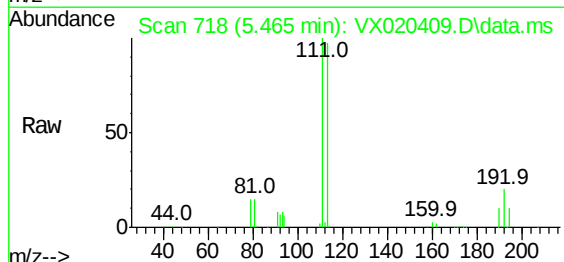


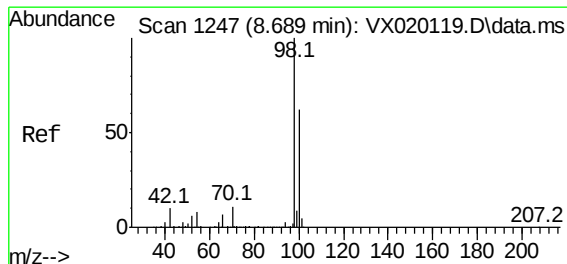

#599 (-)
Toluene-d8
Concen: 49.47 ug/l
RT: 8.696 min Scan# 1248
Delta R.T. 0.007 min
Lab File: VX020409.D
Acq: 28 Dec 2020 13:35




Instrument :
MSVOA_X
ClientSampleId :
SS013-13-TB-122320


Tgt Ion: 98 Resp: 501286
Ion Ratio Lower Upper
98 100
100 66.4 51.9 77.9

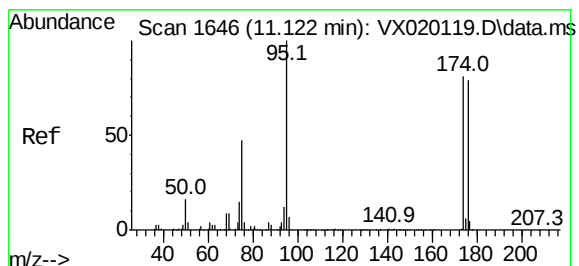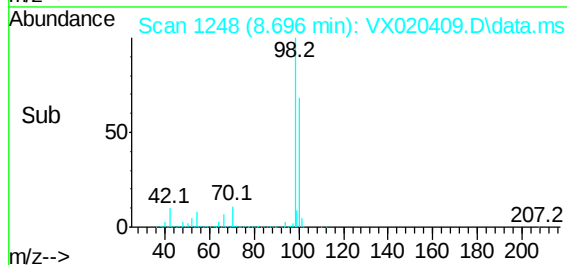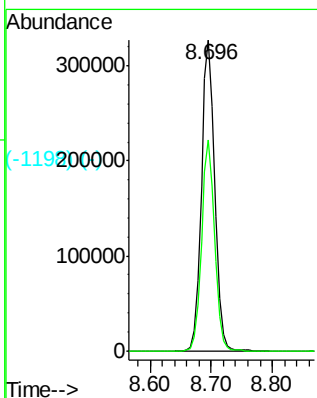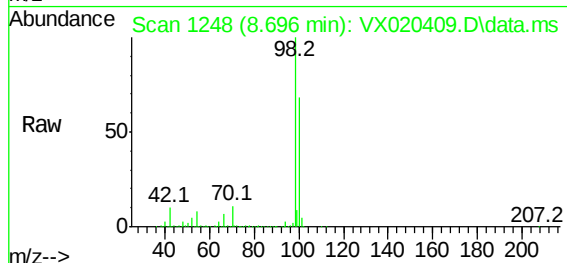

#639 (-)
4-Bromofluorobenzene
Concen: 44.91 ug/l
RT: 11.122 min Scan# 1646
Delta R.T. 0.000 min
Lab File: VX020409.D
Acq: 28 Dec 2020 13:35

Tgt Ion: 95 Resp: 174207
Ion Ratio Lower Upper
95 100
174 77.0 0.0 154.6
176 73.8 0.0 155.8


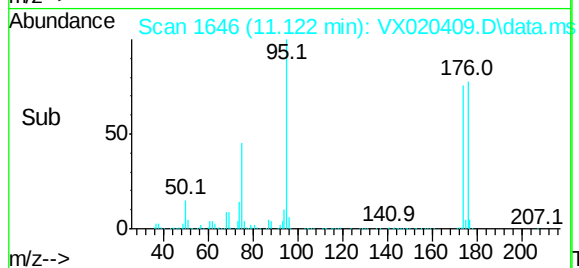
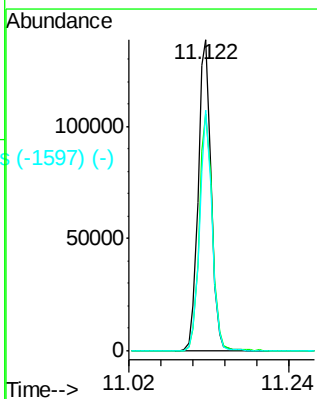
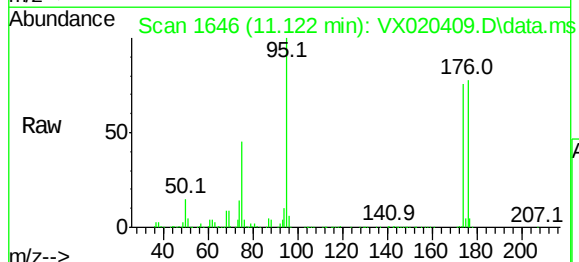


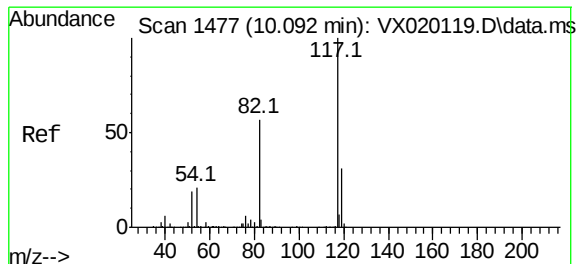

#6270 (-)
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.098 min Scan# 1478
Delta R.T. 0.006 min
Lab File: VX020409.D
Acq: 28 Dec 2020 13:35

Instrument :
MSVOA_X
ClientSampleId :
SS013-13-TB-122320

Tgt Ion:117 Resp: 379342
Ion Ratio Lower Upper
117 100
82 55.6 47.4 71.2
119 32.5 26.6 39.8

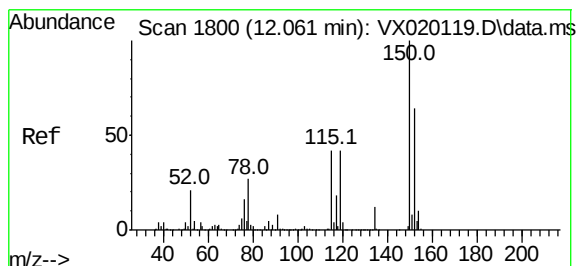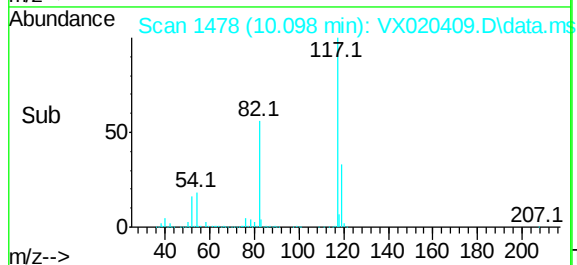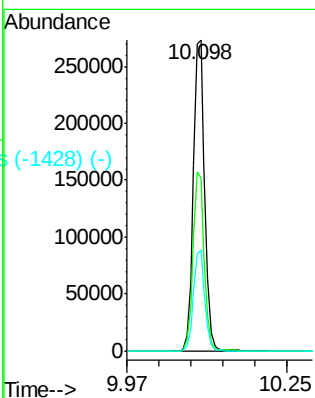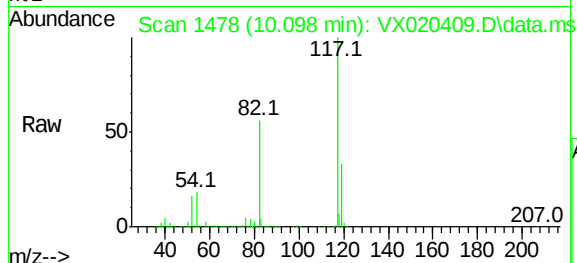

#1794 (-)
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.061 min Scan# 1800
Delta R.T. -0.000 min
Lab File: VX020409.D
Acq: 28 Dec 2020 13:35

Tgt Ion:152 Resp: 159082
Ion Ratio Lower Upper
152 100
115 59.4 41.1 123.3
150 156.1 0.0 349.0

