

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122820\
 Data File : VX020412.D
 Acq On : 28 Dec 2020 14:46
 Operator : JC/MD
 Sample : L5219-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SS013-13-6512-122320

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
 Title : SW846 8260

Signal : TIC: VX020412.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.776	107	113	123	rVB	429853	596242	23.03%	1.650%
2	2.374	203	211	224	rVB	343107	661341	25.55%	1.830%
3	2.575	237	244	256	rBV	24892	46975	1.81%	0.130%
4	2.825	276	285	293	rBV	458243	985751	38.08%	2.727%
5	2.910	293	299	308	rVB	121730	249781	9.65%	0.691%
6	3.148	327	338	356	rBV	1085350	2447938	94.57%	6.773%
7	4.117	485	497	511	rBV	53547	163519	6.32%	0.452%
8	4.282	511	524	530	rVV	129191	384802	14.87%	1.065%
9	4.373	530	539	552	rVV	594682	1727684	66.74%	4.780%
10	4.526	552	564	577	rVB3	26130	100912	3.90%	0.279%
11	5.202	659	675	698	rBV2	66441	241799	9.34%	0.669%
12	5.464	706	718	724	rBV	147268	426512	16.48%	1.180%
13	5.550	724	732	739	rVV	391748	1201204	46.40%	3.323%
14	5.629	739	745	750	rVV	272199	760161	29.37%	2.103%
15	5.696	750	756	776	rVV	369620	1122144	43.35%	3.105%
16	5.916	779	792	802	rVV	101798	324060	12.52%	0.897%
17	6.031	802	811	826	rVV	160850	431382	16.66%	1.193%
18	6.233	828	844	851	rVV2	171512	591256	22.84%	1.636%
19	6.324	852	859	868	rVV3	322801	964294	37.25%	2.668%
20	6.428	868	876	893	rVB	194229	542211	20.95%	1.500%
21	6.830	930	942	962	rBV	398404	940450	36.33%	2.602%
22	7.440	1028	1042	1053	rVV	1126575	2588613	100.00%	7.162%
23	7.556	1053	1061	1065	rVV	34496	70739	2.73%	0.196%
24	7.617	1065	1071	1075	rVV2	48745	104762	4.05%	0.290%
25	7.653	1075	1077	1082	rVV	20957	40619	1.57%	0.112%
26	7.708	1082	1086	1097	rVV	44942	87348	3.37%	0.242%
27	7.824	1097	1105	1114	rVB2	74006	158600	6.13%	0.439%
28	8.031	1128	1139	1151	rVB3	172914	459052	17.73%	1.270%
29	8.159	1151	1160	1168	rBV	255322	512594	19.80%	1.418%
30	8.232	1168	1172	1176	rVV	38421	65409	2.53%	0.181%
31	8.373	1187	1195	1200	rBV	46743	91324	3.53%	0.253%
32	8.513	1214	1218	1222	rVV	23782	40001	1.55%	0.111%
33	8.561	1222	1226	1232	rVB2	19714	36231	1.40%	0.100%
34	8.647	1232	1240	1243	rBV2	243421	444442	17.17%	1.230%
35	8.696	1243	1248	1261	rVB	886160	1512912	58.44%	4.186%
36	8.818	1261	1268	1273	rBV	112572	193128	7.46%	0.534%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122820\
 Data File : VX020412.D
 Acq On : 28 Dec 2020 14:46
 Operator : JC/MD
 Sample : L5219-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SS013-13-6512-122320

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
 Title : SW846 8260

37	8.891	1273	1280	1286	rVB	67638	132578	5.12%	0.367%
38	9.019	1296	1301	1308	rVB	220516	353130	13.64%	0.977%
39	9.147	1313	1322	1328	rBV	109895	178009	6.88%	0.492%
40	9.549	1383	1388	1392	rBV2	59604	97607	3.77%	0.270%
41	9.604	1392	1397	1402	rVV	223209	316518	12.23%	0.876%
42	9.659	1402	1406	1411	rVV	125408	188042	7.26%	0.520%
43	9.872	1434	1441	1454	rVB4	33797	75448	2.91%	0.209%
44	10.092	1472	1477	1483	rBV	818426	1112068	42.96%	3.077%
45	10.171	1483	1490	1494	rVB	93618	138316	5.34%	0.383%
46	10.317	1509	1514	1519	rBV2	57653	119306	4.61%	0.330%
47	10.494	1538	1543	1549	rBV	28540	40453	1.56%	0.112%
48	10.628	1555	1565	1573	rBV2	46000	126151	4.87%	0.349%
49	10.817	1584	1596	1604	rBV2	77547	140614	5.43%	0.389%
50	10.896	1604	1609	1616	rBV3	46844	81580	3.15%	0.226%
51	11.000	1621	1626	1631	rBV	136552	171386	6.62%	0.474%
52	11.122	1640	1646	1650	rBV	667308	845110	32.65%	2.338%
53	11.165	1650	1653	1658	rVV2	36335	49563	1.91%	0.137%
54	11.262	1665	1669	1673	rVB2	35081	46097	1.78%	0.128%
55	11.341	1678	1682	1693	rVV	105895	134277	5.19%	0.371%
56	11.652	1723	1733	1742	rBV6	40117	85165	3.29%	0.236%
57	11.750	1742	1749	1753	rBV	41841	60440	2.33%	0.167%
58	11.902	1766	1774	1776	rBV	75062	120241	4.64%	0.333%
59	11.927	1776	1778	1785	rVB	179260	206630	7.98%	0.572%
60	12.061	1795	1800	1805	rBV	867277	1054577	40.74%	2.918%
61	12.213	1821	1825	1830	rBV	90967	110745	4.28%	0.306%
62	12.286	1830	1837	1841	rVV	349737	442065	17.08%	1.223%
63	12.354	1841	1848	1857	rVB2	154312	262178	10.13%	0.725%
64	12.445	1857	1863	1868	rBV	145541	187839	7.26%	0.520%
65	12.652	1888	1897	1900	rBV	551443	685432	26.48%	1.896%
66	12.683	1900	1902	1907	rVV	213635	268084	10.36%	0.742%
67	12.744	1907	1912	1918	rVV3	396830	710732	27.46%	1.966%
68	12.799	1918	1921	1927	rVV2	40077	58135	2.25%	0.161%
69	12.878	1927	1934	1939	rVB3	126253	200998	7.76%	0.556%
70	12.963	1939	1948	1954	rBV	414198	588393	22.73%	1.628%
71	13.067	1960	1965	1971	rVB3	69138	113947	4.40%	0.315%
72	13.134	1971	1976	1980	rBV2	68777	109977	4.25%	0.304%
73	13.177	1980	1983	1986	rVV2	99195	108427	4.19%	0.300%
74	13.207	1986	1988	1991	rVB	84015	79266	3.06%	0.219%
75	13.329	2003	2008	2014	rVB2	1007663	1390250	53.71%	3.846%
76	13.408	2018	2021	2024	rVV	58001	69571	2.69%	0.192%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122820\
 Data File : VX020412.D
 Acq On : 28 Dec 2020 14:46
 Operator : JC/MD
 Sample : L5219-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SS013-13-6512-122320

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
 Title : SW846 8260

77	13.463	2027	2030	2035	rVB	44500	58640	2.27%	0.162%
78	13.548	2039	2044	2046	rBV2	57293	78483	3.03%	0.217%
79	13.579	2046	2049	2052	rVV	80252	108604	4.20%	0.300%
80	13.622	2052	2056	2060	rVV2	200482	291217	11.25%	0.806%
81	13.683	2060	2066	2067	rVV2	142872	266561	10.30%	0.737%
82	13.701	2067	2069	2078	rVB2	234851	367194	14.18%	1.016%
83	13.792	2078	2084	2087	rBV	78701	106810	4.13%	0.296%
84	13.835	2087	2091	2096	rVB	78072	102695	3.97%	0.284%
85	13.890	2096	2100	2105	rVB	113340	139757	5.40%	0.387%
86	13.969	2105	2113	2116	rBV2	166813	252095	9.74%	0.697%
87	14.012	2116	2120	2123	rVV2	70513	96081	3.71%	0.266%
88	14.109	2132	2136	2139	rBV2	55533	78525	3.03%	0.217%
89	14.146	2139	2142	2146	rVB2	42380	50041	1.93%	0.138%
90	14.268	2155	2162	2169	rVB3	149602	306100	11.82%	0.847%
91	14.359	2173	2177	2181	rVB	51466	60695	2.34%	0.168%
92	14.414	2181	2186	2190	rVB2	70626	93893	3.63%	0.260%
93	14.457	2190	2193	2198	rVB	28965	36719	1.42%	0.102%
94	14.518	2198	2203	2213	rBV2	199537	293914	11.35%	0.813%
95	14.676	2222	2229	2232	rBV	139127	198475	7.67%	0.549%
96	14.713	2232	2235	2239	rVB2	52530	64049	2.47%	0.177%
97	14.823	2247	2253	2257	rBV2	235827	323915	12.51%	0.896%
98	15.225	2313	2319	2327	rVB3	26814	49350	1.91%	0.137%
99	15.524	2361	2368	2373	rBV	36590	60155	2.32%	0.166%
100	15.664	2384	2391	2394	rBV	51069	85707	3.31%	0.237%


Sum of corrected areas: 36145212

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122820\
Data File : VX020412.D
Acq On : 28 Dec 2020 14:46
Operator : JC/MD
Sample : L5219-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SS013-13-6512-122320

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

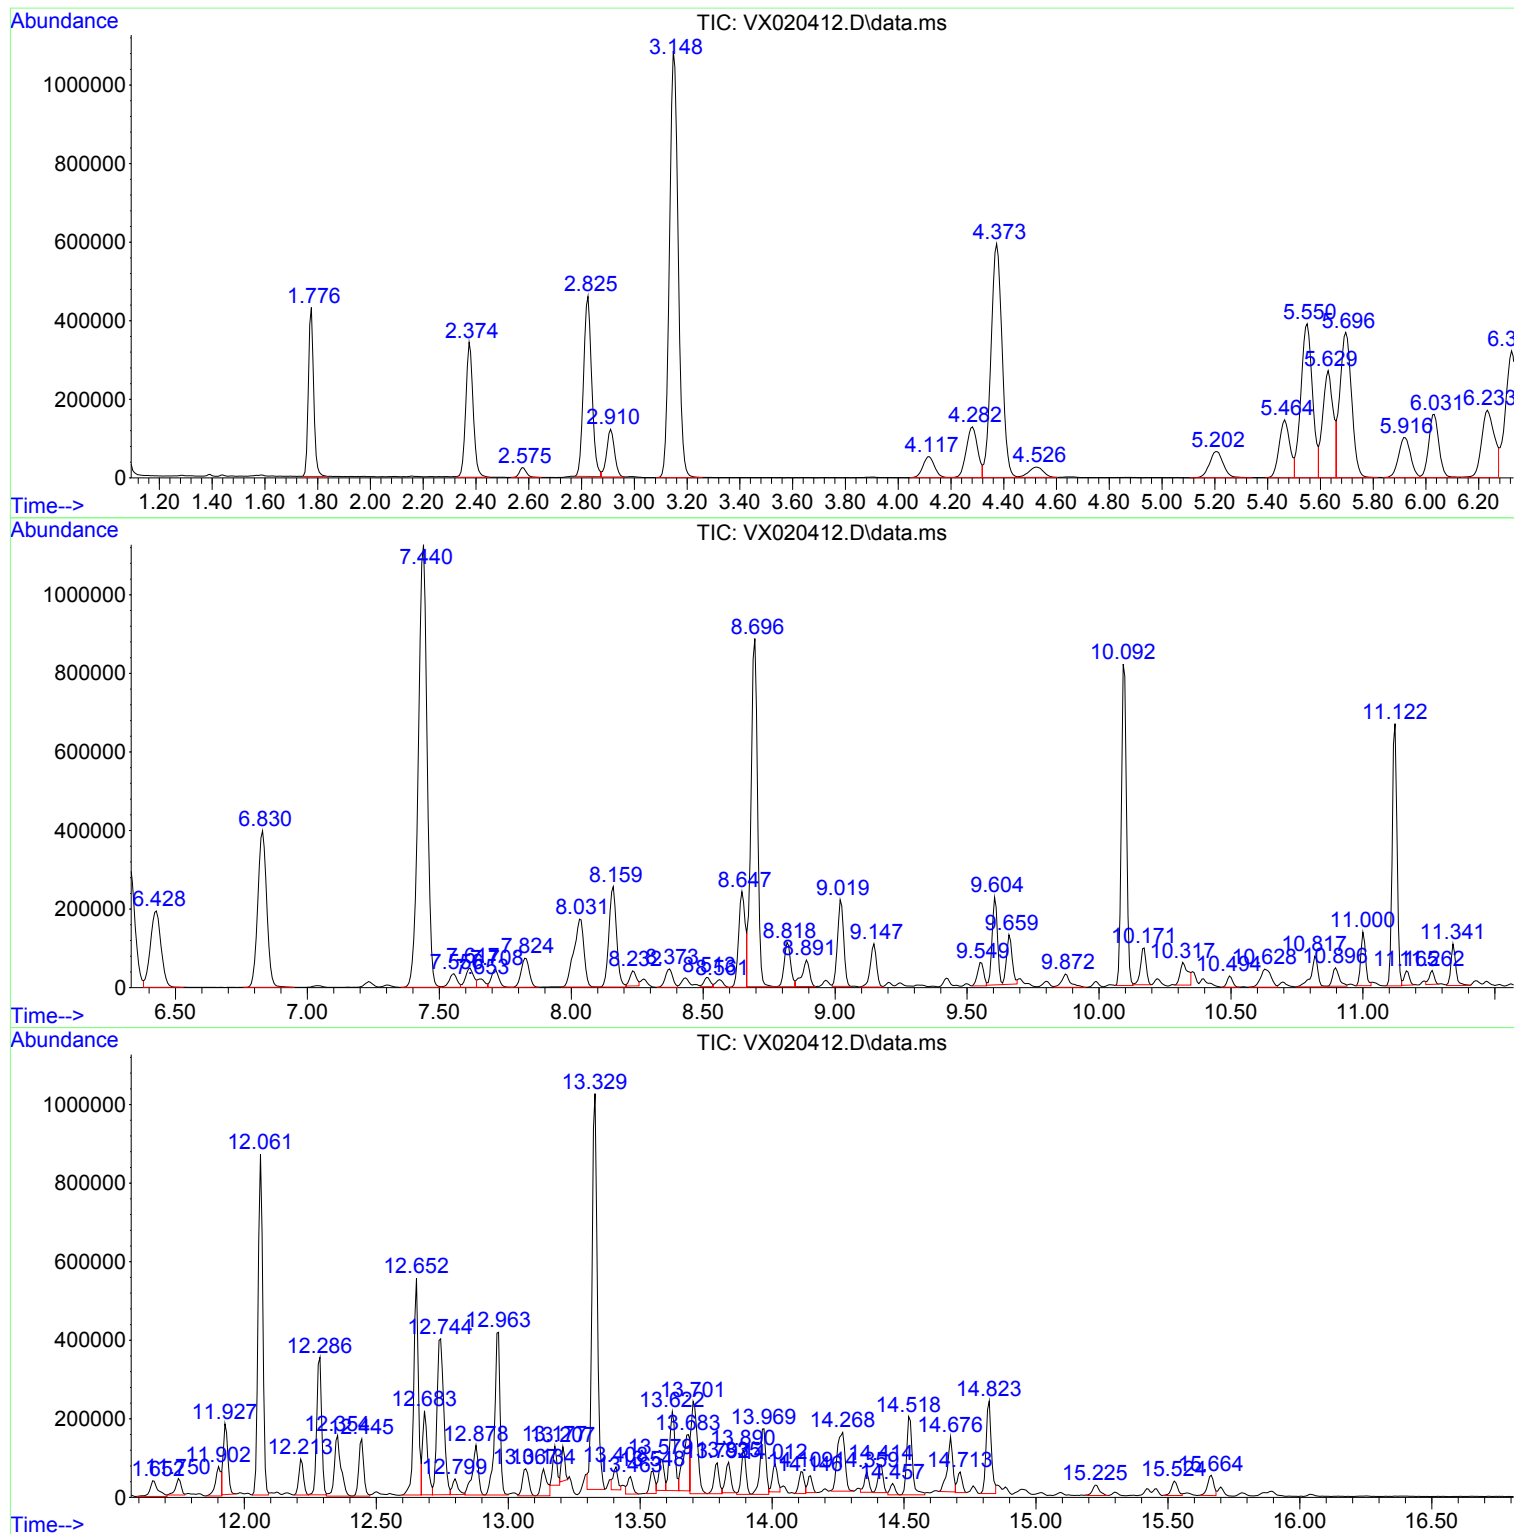

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122820\
Data File : VX020412.D
Acq On : 28 Dec 2020 14:46
Operator : JC/MD
Sample : L5219-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SS013-13-6512-122320

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122820\
Data File : VX020412.D
Acq On : 28 Dec 2020 14:46
Operator : JC/MD
Sample : L5219-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SS013-13-6512-122320

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------