


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122820\
Data File : VX020400.D
Acq On : 28 Dec 2020 08:47
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
Title : SW846 8260
Last Update : Fri Dec 18 13:09:49 2020

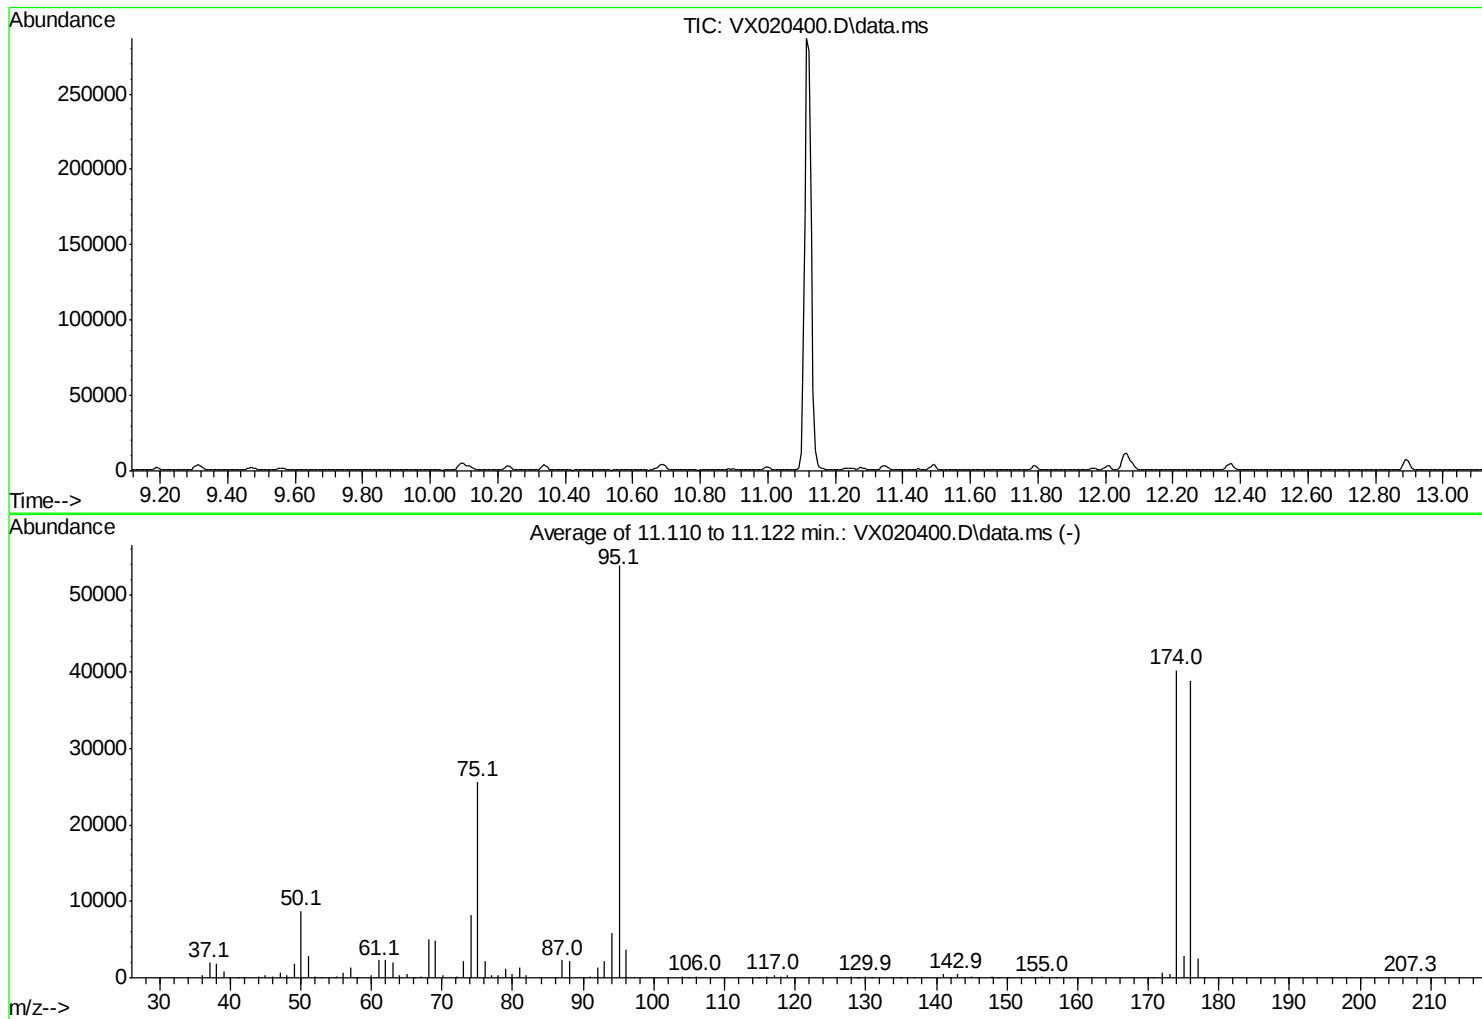

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1638

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.2	8702	PASS
75	95	30	60	47.6	25653	PASS
95	95	100	100	100.0	53864	PASS
96	95	5	9	6.8	3684	PASS
173	174	0.00	2	1.1	431	PASS
174	95	50	100	74.6	40165	PASS
175	174	5	9	7.3	2917	PASS
176	174	95	101	96.8	38869	PASS
177	176	5	9	6.4	2488	PASS