

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
 Data File : VX026106.D
 Acq On : 28 Dec 2021 18:50
 Operator : JC/MD
 Sample : M5153-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
 Title : VOC Analysis

Signal : TIC: VX026106.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	55	rVB	136306	148815	16.38%	2.159%
2	1.672	92	96	102	rBV	112731	130233	14.34%	1.890%
3	2.313	195	201	212	rVB	217573	357393	39.34%	5.185%
4	2.477	227	228	230	rBV2	608	568	0.06%	0.008%
5	2.514	232	234	238	rVB2	1010	1317	0.14%	0.019%
6	2.593	244	247	252	rVB	884	1452	0.16%	0.021%
7	2.721	266	268	271	rVB	911	906	0.10%	0.013%
8	2.940	298	304	313	rBV3	2959	7718	0.85%	0.112%
9	3.038	319	320	324	rBV2	395	527	0.06%	0.008%
10	3.099	328	330	333	rVB	604	540	0.06%	0.008%
11	3.136	333	336	339	rBV	503	707	0.08%	0.010%
12	3.306	361	364	367	rVB	358	496	0.05%	0.007%
13	3.550	403	404	407	rVB	662	600	0.07%	0.009%
14	4.111	491	496	497	rBV	585	860	0.09%	0.012%
15	4.373	537	539	542	rBV2	493	550	0.06%	0.008%
16	4.458	544	553	568	rBV	71023	205194	22.59%	2.977%
17	4.678	587	589	591	rBV	808	820	0.09%	0.012%
18	4.708	593	594	597	rVB	900	509	0.06%	0.007%
19	4.958	630	635	638	rVV	492	909	0.10%	0.013%
20	5.062	640	652	667	rBV	118181	369049	40.62%	5.355%
21	5.970	788	801	815	rBV3	310178	908441	100.00%	13.181%
22	6.422	874	875	878	rBV2	500	593	0.07%	0.009%
23	6.519	888	891	893	rVB	666	686	0.08%	0.010%
24	6.763	920	931	947	rVV	225487	534316	58.82%	7.752%
25	6.958	961	963	966	rVB	634	630	0.07%	0.009%
26	6.995	966	969	972	rVB	561	647	0.07%	0.009%
27	7.117	982	989	995	rBV4	3364	8393	0.92%	0.122%
28	7.312	1012	1021	1033	rBV	183548	411296	45.27%	5.967%
29	7.476	1045	1048	1050	rBV3	554	799	0.09%	0.012%
30	7.726	1087	1089	1094	rVB2	610	807	0.09%	0.012%
31	8.001	1132	1134	1136	rBV2	564	583	0.06%	0.008%
32	8.061	1143	1144	1147	rBV	677	550	0.06%	0.008%
33	8.104	1149	1151	1154	rVB	529	571	0.06%	0.008%
34	8.250	1170	1175	1181	rVB4	2522	4397	0.48%	0.064%
35	8.324	1181	1187	1201	rBV	134734	222827	24.53%	3.233%
36	8.519	1215	1219	1222	rVB	454	576	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
 Data File : VX026106.D
 Acq On : 28 Dec 2021 18:50
 Operator : JC/MD
 Sample : M5153-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
 Title : VOC Analysis

37	8.647	1234	1240	1248	rBV	454110	725136	79.82%	10.521%
38	8.720	1248	1252	1258	rVB3	7244	12076	1.33%	0.175%
39	8.878	1276	1278	1282	rVB	681	720	0.08%	0.010%
40	8.952	1284	1290	1299	rBV	98865	141396	15.56%	2.052%
41	9.134	1318	1320	1323	rVV	780	578	0.06%	0.008%
42	9.275	1340	1343	1347	rVB3	868	1354	0.15%	0.020%
43	9.384	1356	1361	1374	rVB	318221	446983	49.20%	6.485%
44	9.659	1403	1406	1407	rBV	677	544	0.06%	0.008%
45	9.890	1443	1444	1448	rVB	571	500	0.06%	0.007%
46	10.055	1465	1471	1480	rBV	454269	614588	67.65%	8.917%
47	10.189	1491	1493	1498	rBV2	761	1300	0.14%	0.019%
48	10.305	1509	1512	1516	rVB3	1240	1624	0.18%	0.024%
49	10.403	1526	1528	1530	rBV2	604	588	0.06%	0.009%
50	10.433	1530	1533	1538	rVV2	633	989	0.11%	0.014%
51	10.634	1564	1566	1568	rBV	597	629	0.07%	0.009%
52	10.762	1584	1587	1589	rVB	646	607	0.07%	0.009%
53	10.799	1589	1593	1596	rVB2	739	1113	0.12%	0.016%
54	10.835	1596	1599	1600	rBV2	569	620	0.07%	0.009%
55	10.866	1602	1604	1607	rVB	511	496	0.05%	0.007%
56	11.024	1625	1630	1632	rBV2	562	773	0.09%	0.011%
57	11.122	1640	1646	1651	rBV	4288	5866	0.65%	0.085%
58	11.195	1652	1658	1666	rVV	315377	403736	44.44%	5.858%
59	11.463	1699	1702	1703	rBV2	741	677	0.07%	0.010%
60	11.604	1722	1725	1726	rBV2	579	650	0.07%	0.009%
61	11.683	1735	1738	1742	rVB3	605	696	0.08%	0.010%
62	11.750	1744	1749	1756	rVB3	3500	5990	0.66%	0.087%
63	11.841	1761	1764	1769	rVB3	609	981	0.11%	0.014%
64	11.933	1776	1779	1783	rBV4	1861	2393	0.26%	0.035%
65	11.969	1783	1785	1786	rVV	668	495	0.05%	0.007%
66	12.024	1789	1794	1803	rVV	460963	564630	62.15%	8.192%
67	12.128	1807	1811	1813	rVV3	1862	3187	0.35%	0.046%
68	12.152	1813	1815	1819	rVV2	3146	3595	0.40%	0.052%
69	12.323	1834	1843	1851	rBV	465404	595946	65.60%	8.647%
70	12.427	1857	1860	1865	rBV3	1765	2866	0.32%	0.042%
71	12.603	1886	1889	1892	rBV3	670	847	0.09%	0.012%
72	12.768	1912	1916	1920	rBV3	1275	2223	0.24%	0.032%
73	13.115	1972	1973	1976	rBV	643	693	0.08%	0.010%
74	13.176	1981	1983	1986	rVV	596	505	0.06%	0.007%
75	13.237	1989	1993	1995	rBV2	474	524	0.06%	0.008%
76	13.286	1998	2001	2002	rVB	679	518	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
 Data File : VX026106.D
 Acq On : 28 Dec 2021 18:50
 Operator : JC/MD
 Sample : M5153-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
 Title : VOC Analysis

77	13.335	2008	2009	2013	rBV	586	800	0.09%	0.012%
78	13.597	2049	2052	2055	rBV2	1010	1499	0.17%	0.022%
79	13.652	2059	2061	2064	rBV2	524	659	0.07%	0.010%
80	13.932	2106	2107	2109	rBV	666	565	0.06%	0.008%
81	14.103	2133	2135	2136	rVB2	1090	637	0.07%	0.009%
82	14.127	2136	2139	2143	rBV2	671	1255	0.14%	0.018%
83	14.384	2178	2181	2183	rVB2	667	786	0.09%	0.011%
84	14.640	2219	2223	2224	rBV	697	1093	0.12%	0.016%
85	14.658	2224	2226	2228	rVV2	672	580	0.06%	0.008%
86	14.719	2233	2236	2237	rBV	533	515	0.06%	0.007%
87	14.737	2237	2239	2241	rBV	693	591	0.07%	0.009%
88	15.024	2284	2286	2289	rVB2	685	662	0.07%	0.010%
89	15.115	2299	2301	2303	rVB	658	541	0.06%	0.008%
90	15.225	2316	2319	2321	rVB2	698	786	0.09%	0.011%
91	15.341	2337	2338	2341	rBV2	634	609	0.07%	0.009%
92	15.377	2343	2344	2346	rBV	705	527	0.06%	0.008%
93	15.493	2362	2363	2368	rBV2	591	723	0.08%	0.010%
94	15.908	2429	2431	2434	rBV	597	856	0.09%	0.012%
95	16.170	2472	2474	2475	rBV2	744	524	0.06%	0.008%
96	16.206	2478	2480	2483	rVB	744	642	0.07%	0.009%
97	16.371	2505	2507	2510	rBV	549	608	0.07%	0.009%
98	16.395	2510	2511	2514	rVV	711	586	0.06%	0.009%
99	16.487	2522	2526	2527	rBV2	610	751	0.08%	0.011%
100	16.615	2544	2547	2548	rBV2	604	588	0.06%	0.009%


Sum of corrected areas: 6892290

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
Data File : VX026106.D
Acq On : 28 Dec 2021 18:50
Operator : JC/MD
Sample : M5153-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

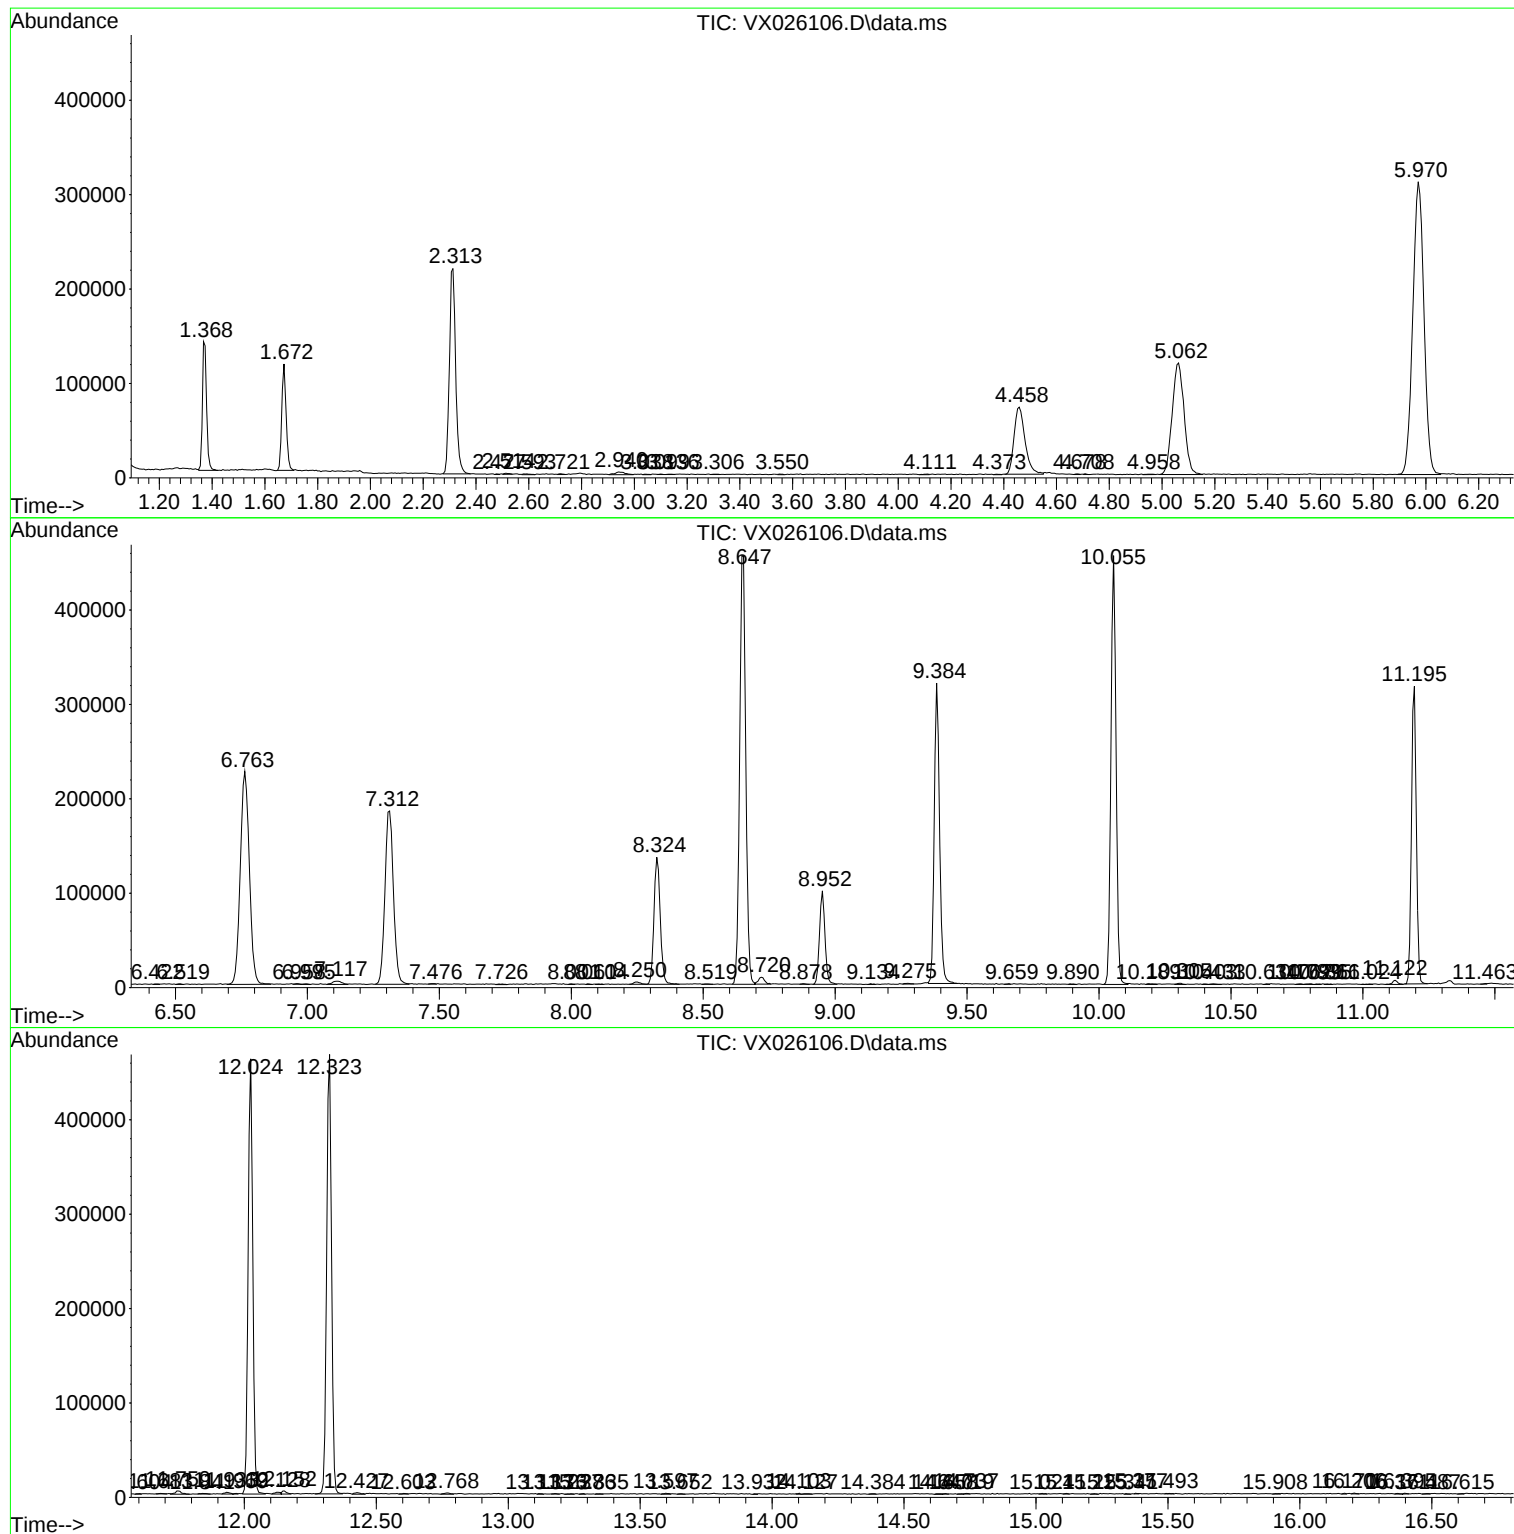

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
Data File : VX026106.D
Acq On : 28 Dec 2021 18:50
Operator : JC/MD
Sample : M5153-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
Data File : VX026106.D
Acq On : 28 Dec 2021 18:50
Operator : JC/MD
Sample : M5153-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc