

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
 Data File : VX026108.D
 Acq On : 28 Dec 2021 19:37
 Operator : JC/MD
 Sample : M5232-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
 Title : VOC Analysis

Signal : TIC: VX026108.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	55	rVB	130407	138113	16.10%	2.202%
2	1.672	92	96	106	rVB	106794	121973	14.22%	1.945%
3	2.312	195	201	211	rBV	209299	332784	38.80%	5.306%
4	2.447	221	223	226	rVB	947	962	0.11%	0.015%
5	2.489	226	230	232	rBV	848	1270	0.15%	0.020%
6	2.623	250	252	255	rBV2	542	837	0.10%	0.013%
7	2.794	276	280	285	rVB4	1549	2727	0.32%	0.043%
8	2.879	293	294	297	rBV	616	559	0.07%	0.009%
9	2.946	297	305	314	rVB3	2831	7855	0.92%	0.125%
10	3.373	372	375	376	rBV	805	589	0.07%	0.009%
11	3.574	405	408	409	rBV2	611	659	0.08%	0.011%
12	3.629	414	417	420	rVB2	412	452	0.05%	0.007%
13	3.934	466	467	470	rVB2	539	457	0.05%	0.007%
14	4.196	508	510	512	rVB	853	458	0.05%	0.007%
15	4.227	512	515	517	rBV	600	611	0.07%	0.010%
16	4.343	532	534	540	rVB	406	623	0.07%	0.010%
17	4.458	545	553	567	rBV2	66073	191920	22.38%	3.060%
18	4.702	592	593	596	rBV2	571	553	0.06%	0.009%
19	4.818	611	612	615	rBV2	589	486	0.06%	0.008%
20	4.867	615	620	622	rBV2	469	925	0.11%	0.015%
21	4.946	632	633	637	rVV2	466	513	0.06%	0.008%
22	5.062	641	652	670	rVV	110303	345514	40.29%	5.509%
23	5.184	670	672	677	rVV3	465	549	0.06%	0.009%
24	5.355	697	700	702	rBV	699	746	0.09%	0.012%
25	5.385	704	705	708	rVB2	991	784	0.09%	0.013%
26	5.416	708	710	712	rBV2	607	518	0.06%	0.008%
27	5.513	724	726	729	rBV2	585	712	0.08%	0.011%
28	5.580	735	737	742	rVB2	805	1025	0.12%	0.016%
29	5.726	759	761	764	rVV	429	501	0.06%	0.008%
30	5.781	767	770	773	rBV2	391	541	0.06%	0.009%
31	5.873	783	785	788	rBV	741	609	0.07%	0.010%
32	5.976	788	802	818	rVV2	290496	857585	100.00%	13.674%
33	6.092	818	821	823	rBV	802	839	0.10%	0.013%
34	6.300	853	855	857	rBV2	747	772	0.09%	0.012%
35	6.391	869	870	874	rVB	651	519	0.06%	0.008%
36	6.556	895	897	900	rVV2	586	594	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
 Data File : VX026108.D
 Acq On : 28 Dec 2021 19:37
 Operator : JC/MD
 Sample : M5232-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
 Title : VOC Analysis

37	6.769	923	932	944	rVV	187513	450211	52.50%	7.178%
38	6.921	956	957	961	rVB2	475	449	0.05%	0.007%
39	7.110	983	988	995	rVB4	3569	7679	0.90%	0.122%
40	7.312	1012	1021	1035	rBV	181674	391007	45.59%	6.234%
41	7.458	1044	1045	1046	rBV	895	567	0.07%	0.009%
42	7.885	1112	1115	1118	rBV2	416	545	0.06%	0.009%
43	7.933	1118	1123	1127	rBV3	847	1475	0.17%	0.024%
44	8.074	1144	1146	1147	rBV2	786	541	0.06%	0.009%
45	8.171	1160	1162	1165	rBV2	484	473	0.06%	0.008%
46	8.330	1181	1188	1195	rBV	122702	205686	23.98%	3.280%
47	8.470	1209	1211	1213	rVB	690	620	0.07%	0.010%
48	8.574	1227	1228	1231	rVV	851	709	0.08%	0.011%
49	8.653	1234	1241	1248	rVV	429927	679286	79.21%	10.831%
50	8.720	1249	1252	1261	rVV	6690	11726	1.37%	0.187%
51	8.823	1267	1269	1271	rVB2	641	494	0.06%	0.008%
52	8.952	1285	1290	1299	rVV	92932	130675	15.24%	2.084%
53	9.110	1315	1316	1320	rVB2	537	557	0.06%	0.009%
54	9.165	1322	1325	1327	rBV2	506	666	0.08%	0.011%
55	9.238	1335	1337	1339	rBV2	476	569	0.07%	0.009%
56	9.384	1356	1361	1374	rVB	286014	411895	48.03%	6.567%
57	9.909	1444	1447	1448	rBV	473	559	0.07%	0.009%
58	9.964	1454	1456	1460	rVB	702	699	0.08%	0.011%
59	10.018	1464	1465	1466	rBV	748	507	0.06%	0.008%
60	10.055	1466	1471	1480	rVB	388370	516681	60.25%	8.238%
61	10.195	1491	1494	1500	rVB3	878	1790	0.21%	0.029%
62	10.299	1510	1511	1517	rVB3	1374	1878	0.22%	0.030%
63	10.719	1577	1580	1581	rBV	741	671	0.08%	0.011%
64	10.774	1587	1589	1594	rBV	716	862	0.10%	0.014%
65	10.817	1594	1596	1598	rBV	667	634	0.07%	0.010%
66	11.122	1643	1646	1650	rVB	3270	3855	0.45%	0.061%
67	11.195	1652	1658	1664	rBV	295459	382682	44.62%	6.102%
68	11.329	1676	1680	1687	rVB4	3413	5480	0.64%	0.087%
69	11.451	1698	1700	1702	rBV	700	512	0.06%	0.008%
70	11.549	1712	1716	1717	rBV3	571	608	0.07%	0.010%
71	11.756	1744	1750	1753	rBV4	3200	4570	0.53%	0.073%
72	11.933	1775	1779	1784	rVB3	1400	2285	0.27%	0.036%
73	12.024	1789	1794	1800	rBV	392523	459909	53.63%	7.333%
74	12.323	1836	1843	1850	rBV	451952	556773	64.92%	8.878%
75	12.414	1856	1858	1859	rBV	647	484	0.06%	0.008%
76	12.481	1865	1869	1872	rVB3	873	1300	0.15%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
 Data File : VX026108.D
 Acq On : 28 Dec 2021 19:37
 Operator : JC/MD
 Sample : M5232-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
 Title : VOC Analysis

77	12.731	1907	1910	1911	rBV2	474	552	0.06%	0.009%
78	13.048	1959	1962	1965	rBV4	521	702	0.08%	0.011%
79	13.109	1970	1972	1975	rBV2	523	624	0.07%	0.010%
80	13.195	1985	1986	1987	rBV	958	509	0.06%	0.008%
81	13.335	2006	2009	2010	rBV	589	468	0.05%	0.007%
82	13.432	2023	2025	2028	rVB	524	618	0.07%	0.010%
83	13.664	2060	2063	2065	rBV	708	789	0.09%	0.013%
84	13.774	2079	2081	2085	rBV2	646	857	0.10%	0.014%
85	13.877	2096	2098	2101	rVV2	544	718	0.08%	0.011%
86	13.975	2112	2114	2116	rVB	735	585	0.07%	0.009%
87	14.054	2124	2127	2128	rBV	701	540	0.06%	0.009%
88	14.097	2131	2134	2136	rBV	557	721	0.08%	0.011%
89	14.243	2156	2158	2163	rVB2	573	869	0.10%	0.014%
90	14.280	2163	2164	2168	rVB3	579	562	0.07%	0.009%
91	14.316	2168	2170	2175	rVB2	620	1121	0.13%	0.018%
92	14.353	2175	2176	2178	rBV	693	671	0.08%	0.011%
93	14.499	2196	2200	2201	rBV	778	583	0.07%	0.009%
94	14.798	2247	2249	2252	rVB	812	728	0.08%	0.012%
95	14.883	2261	2263	2266	rBV	829	585	0.07%	0.009%
96	15.048	2288	2290	2292	rBV	484	530	0.06%	0.008%
97	15.633	2384	2386	2387	rBV2	797	513	0.06%	0.008%
98	15.773	2406	2409	2410	rBV2	625	728	0.08%	0.012%
99	15.969	2439	2441	2442	rBV2	612	553	0.06%	0.009%
100	16.700	2559	2561	2564	rBV	649	891	0.10%	0.014%




Sum of corrected areas: 6271720

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
Data File : VX026108.D
Acq On : 28 Dec 2021 19:37
Operator : JC/MD
Sample : M5232-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

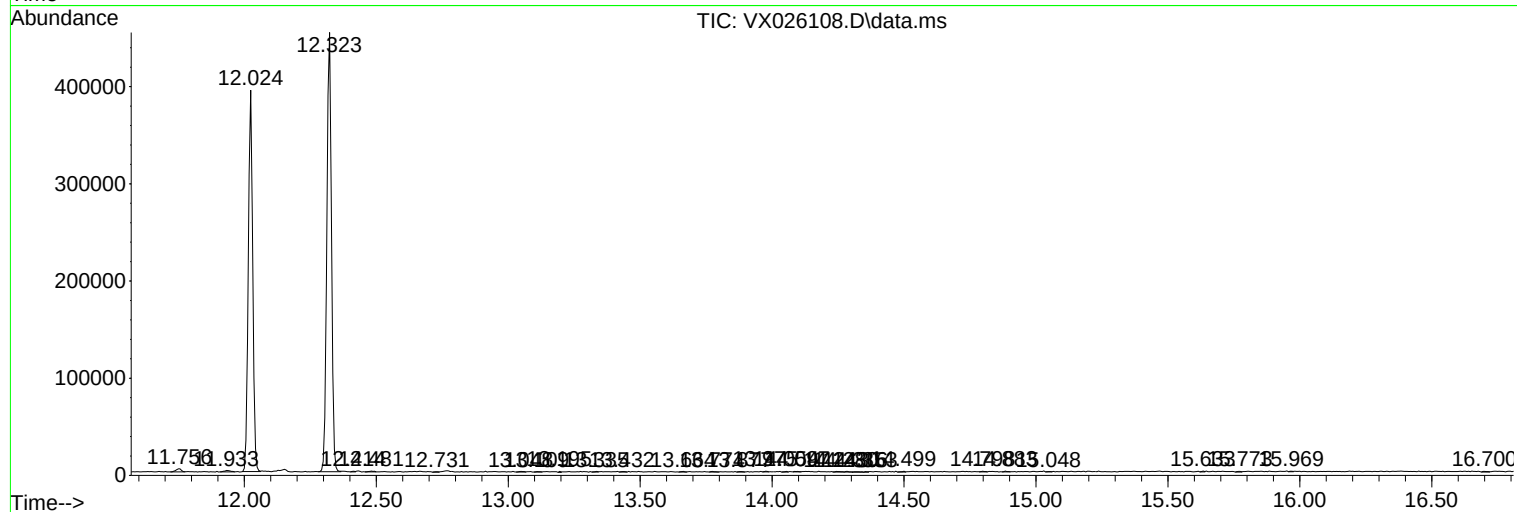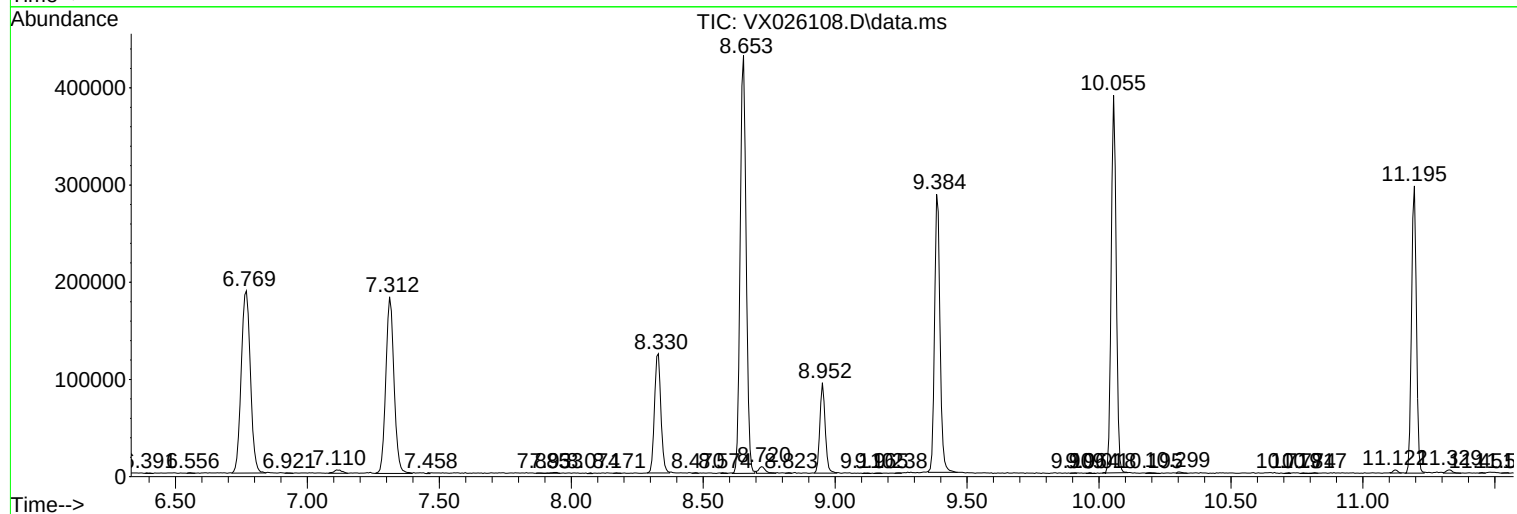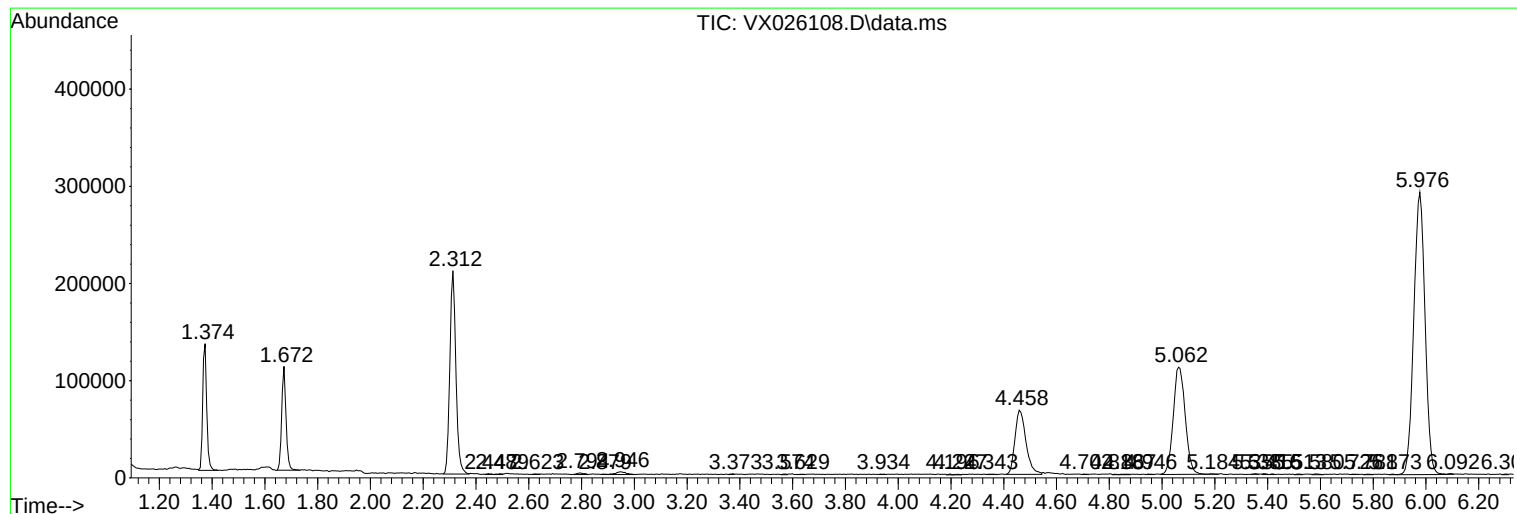

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
Data File : VX026108.D
Acq On : 28 Dec 2021 19:37
Operator : JC/MD
Sample : M5232-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
Data File : VX026108.D
Acq On : 28 Dec 2021 19:37
Operator : JC/MD
Sample : M5232-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc