

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
 Data File : VX026109.D
 Acq On : 28 Dec 2021 20:00
 Operator : JC/MD
 Sample : M5123-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGL60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
 Title : VOC Analysis

Signal : TIC: VX026109.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	53	rVB	139389	148900	16.46%	2.148%
2	1.672	92	96	102	rBV	112940	129723	14.34%	1.871%
3	2.312	195	201	208	rBV	230155	354532	39.19%	5.114%
4	2.386	209	213	222	rVB	22043	36792	4.07%	0.531%
5	2.520	231	235	240	rVB2	3368	5429	0.60%	0.078%
6	2.562	240	242	247	rBV	469	543	0.06%	0.008%
7	2.648	254	256	261	rBV2	574	952	0.11%	0.014%
8	2.794	274	280	290	rBV3	8962	17294	1.91%	0.249%
9	2.953	302	306	311	rVB2	2201	3513	0.39%	0.051%
10	3.081	326	327	330	rBV2	647	760	0.08%	0.011%
11	3.446	385	387	390	rBV2	497	705	0.08%	0.010%
12	3.501	395	396	399	rVV	662	644	0.07%	0.009%
13	3.843	449	452	456	rVB	715	899	0.10%	0.013%
14	4.245	517	518	521	rBV	602	573	0.06%	0.008%
15	4.361	536	537	540	rBV2	811	704	0.08%	0.010%
16	4.458	543	553	565	rBV	73748	210755	23.30%	3.040%
17	4.836	613	615	617	rBV	946	771	0.09%	0.011%
18	5.062	641	652	667	rVV	126385	383408	42.38%	5.530%
19	5.403	706	708	712	rVB3	530	608	0.07%	0.009%
20	5.538	729	730	733	rBV2	845	906	0.10%	0.013%
21	5.787	768	771	773	rBV	723	924	0.10%	0.013%
22	5.976	790	802	818	rVV2	304746	904614	100.00%	13.048%
23	6.214	838	841	843	rBV	532	513	0.06%	0.007%
24	6.769	923	932	945	rBV	215926	515414	56.98%	7.434%
25	7.110	983	988	995	rVB4	4029	8760	0.97%	0.126%
26	7.312	1010	1021	1037	rBV	190340	415197	45.90%	5.989%
27	7.482	1046	1049	1053	rBV3	907	1572	0.17%	0.023%
28	7.549	1056	1060	1063	rBV2	572	1022	0.11%	0.015%
29	7.629	1071	1073	1079	rBV2	663	1123	0.12%	0.016%
30	7.677	1079	1081	1085	rVB	690	639	0.07%	0.009%
31	7.842	1106	1108	1113	rVB	800	911	0.10%	0.013%
32	7.897	1113	1117	1119	rBV2	436	701	0.08%	0.010%
33	7.933	1119	1123	1126	rBV4	796	1455	0.16%	0.021%
34	8.330	1181	1188	1197	rBV	133985	221957	24.54%	3.201%
35	8.433	1203	1205	1208	rVB	793	805	0.09%	0.012%
36	8.476	1210	1212	1216	rVB4	1155	1534	0.17%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
 Data File : VX026109.D
 Acq On : 28 Dec 2021 20:00
 Operator : JC/MD
 Sample : M5123-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGL60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
 Title : VOC Analysis

37	8.653	1234	1241	1249	rBV	468849	722135	79.83%	10.416%
38	8.720	1249	1252	1259	rVB	7660	11798	1.30%	0.170%
39	8.787	1261	1263	1265	rVB2	857	755	0.08%	0.011%
40	8.817	1265	1268	1271	rBV2	791	1277	0.14%	0.018%
41	8.860	1273	1275	1278	rBV2	608	661	0.07%	0.010%
42	8.903	1281	1282	1285	rBV2	575	789	0.09%	0.011%
43	8.952	1285	1290	1298	rBV	96829	137945	15.25%	1.990%
44	9.336	1349	1353	1354	rBV3	890	1281	0.14%	0.018%
45	9.384	1356	1361	1374	rVB	317601	453857	50.17%	6.546%
46	10.055	1465	1471	1482	rBV	442223	602120	66.56%	8.685%
47	10.311	1509	1513	1517	rVB3	1793	2730	0.30%	0.039%
48	10.354	1517	1520	1522	rBV	533	615	0.07%	0.009%
49	10.482	1539	1541	1544	rVB2	728	739	0.08%	0.011%
50	10.591	1556	1559	1563	rBV2	487	747	0.08%	0.011%
51	10.652	1566	1569	1572	rBV3	1049	1624	0.18%	0.023%
52	10.774	1587	1589	1592	rVB2	699	538	0.06%	0.008%
53	10.817	1595	1596	1599	rBV	609	505	0.06%	0.007%
54	10.890	1604	1608	1609	rBV2	494	585	0.06%	0.008%
55	10.921	1611	1613	1615	rVB	731	587	0.06%	0.008%
56	10.945	1615	1617	1619	rBV2	1025	963	0.11%	0.014%
57	10.963	1619	1620	1625	rVB2	875	908	0.10%	0.013%
58	11.024	1626	1630	1635	rVB2	5531	7983	0.88%	0.115%
59	11.073	1635	1638	1639	rBV	589	706	0.08%	0.010%
60	11.122	1642	1646	1650	rVB	5486	6758	0.75%	0.097%
61	11.195	1652	1658	1666	rBV	307903	404748	44.74%	5.838%
62	11.372	1685	1687	1688	rBV	903	687	0.08%	0.010%
63	11.445	1697	1699	1701	rBV	842	627	0.07%	0.009%
64	11.475	1701	1704	1709	rBV3	2097	3302	0.37%	0.048%
65	11.549	1714	1716	1719	rVB3	1080	934	0.10%	0.013%
66	11.677	1733	1737	1740	rBV4	878	1392	0.15%	0.020%
67	11.750	1746	1749	1755	rVB4	4663	6538	0.72%	0.094%
68	11.841	1761	1764	1770	rBV3	1828	2239	0.25%	0.032%
69	11.933	1776	1779	1782	rBV3	2556	3008	0.33%	0.043%
70	11.975	1782	1786	1789	rBV3	1857	2163	0.24%	0.031%
71	12.024	1789	1794	1802	rBV	447378	538948	59.58%	7.774%
72	12.128	1805	1811	1812	rBV3	2001	2907	0.32%	0.042%
73	12.238	1827	1829	1830	rBV2	717	566	0.06%	0.008%
74	12.323	1835	1843	1851	rVV	465774	593194	65.57%	8.556%
75	12.427	1857	1860	1864	rVB4	1595	1866	0.21%	0.027%
76	12.585	1883	1886	1888	rVB2	1397	1407	0.16%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
 Data File : VX026109.D
 Acq On : 28 Dec 2021 20:00
 Operator : JC/MD
 Sample : M5123-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGL60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
 Title : VOC Analysis

77	12.664	1896	1899	1903	rVB3	1314	1929	0.21%	0.028%
78	12.701	1903	1905	1909	rVB2	1027	968	0.11%	0.014%
79	12.768	1912	1916	1921	rBV3	1719	2947	0.33%	0.043%
80	13.061	1959	1964	1967	rBV3	1280	2020	0.22%	0.029%
81	13.103	1967	1971	1972	rBV3	631	797	0.09%	0.011%
82	13.164	1978	1981	1985	rBV3	815	792	0.09%	0.011%
83	13.475	2027	2032	2035	rBV	948	1821	0.20%	0.026%
84	13.524	2037	2040	2042	rBV2	748	841	0.09%	0.012%
85	13.560	2044	2046	2048	rVV	659	557	0.06%	0.008%
86	13.780	2078	2082	2090	rVB	6148	7609	0.84%	0.110%
87	13.908	2101	2103	2105	rBV2	754	659	0.07%	0.010%
88	13.963	2110	2112	2114	rVB	889	686	0.08%	0.010%
89	13.987	2114	2116	2118	rVB	732	565	0.06%	0.008%
90	14.323	2169	2171	2175	rBV	1016	791	0.09%	0.011%
91	14.786	2244	2247	2251	rVB4	1388	1815	0.20%	0.026%
92	15.188	2311	2313	2316	rVB2	731	676	0.07%	0.010%
93	15.328	2331	2336	2340	rBV4	2267	3549	0.39%	0.051%
94	15.530	2367	2369	2370	rBV	627	523	0.06%	0.008%
95	15.591	2378	2379	2382	rBV	790	878	0.10%	0.013%
96	15.645	2387	2388	2391	rBV2	669	678	0.07%	0.010%
97	16.084	2457	2460	2461	rBV3	1423	1528	0.17%	0.022%
98	16.438	2516	2518	2521	rVB	826	564	0.06%	0.008%
99	16.566	2537	2539	2541	rBV2	656	588	0.07%	0.008%
100	16.743	2566	2568	2569	rBV	623	515	0.06%	0.007%




Sum of corrected areas: 6932980

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
Data File : VX026109.D
Acq On : 28 Dec 2021 20:00
Operator : JC/MD
Sample : M5123-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGL60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

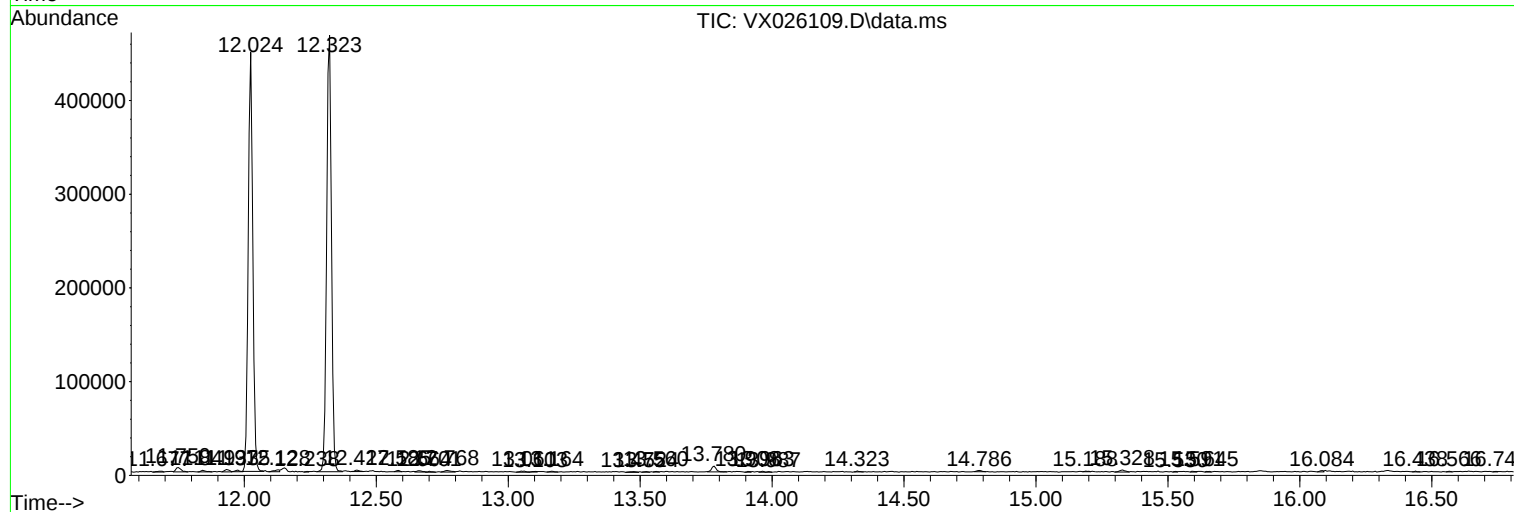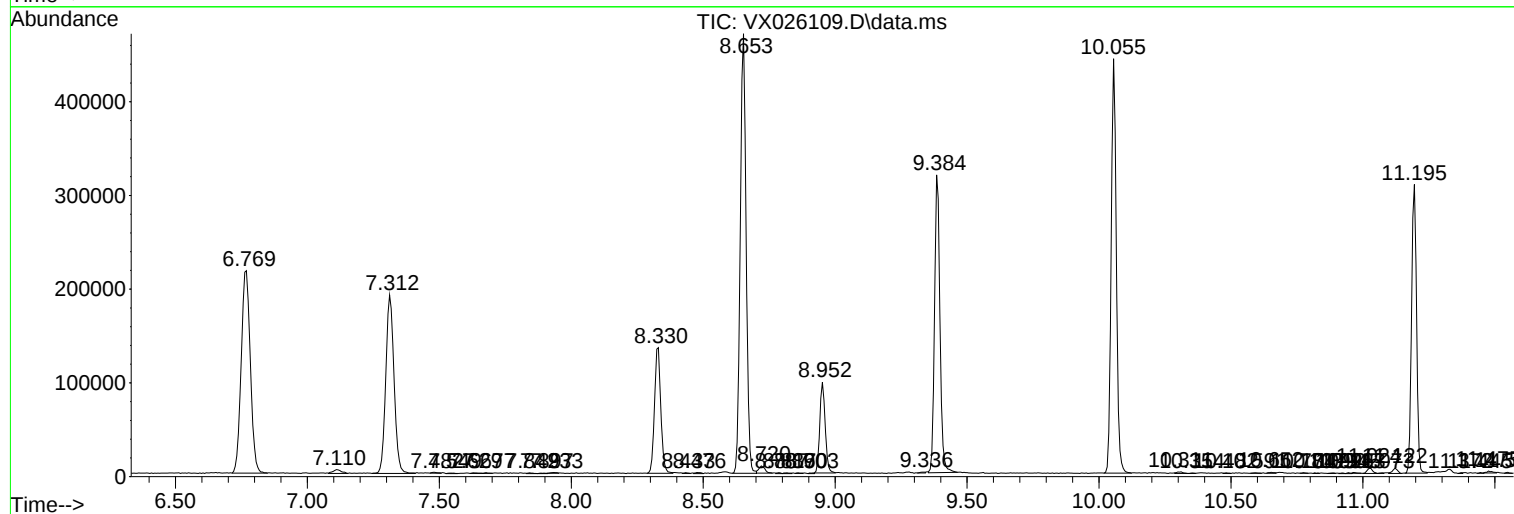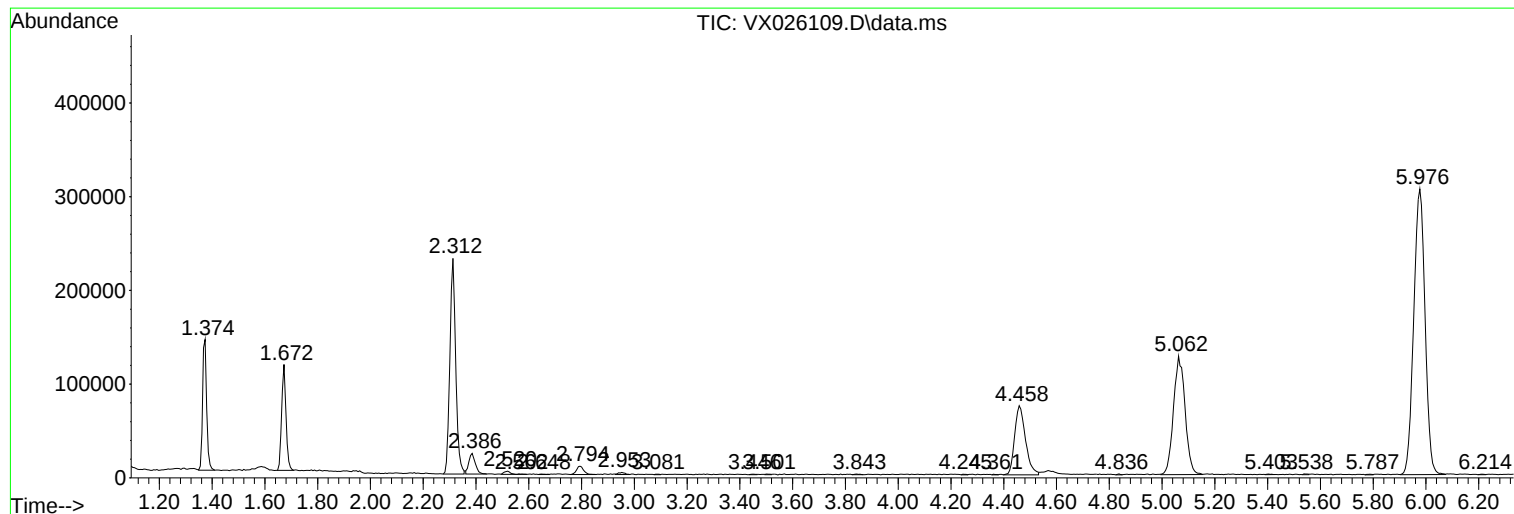

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
Data File : VX026109.D
Acq On : 28 Dec 2021 20:00
Operator : JC/MD
Sample : M5123-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGL60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
Data File : VX026109.D
Acq On : 28 Dec 2021 20:00
Operator : JC/MD
Sample : M5123-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGL60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------