

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
 Data File : VX026110.D
 Acq On : 28 Dec 2021 20:23
 Operator : JC/MD
 Sample : M5123-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
 Title : VOC Analysis

Signal : TIC: VX026110.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	54	rVB	135277	143921	16.08%	2.177%
2	1.673	92	96	101	rBV	111872	127153	14.21%	1.923%
3	2.313	195	201	219	rVB	218869	358778	40.08%	5.426%
4	2.508	232	233	236	rBV2	769	640	0.07%	0.010%
5	2.800	276	281	286	rVB3	1720	3048	0.34%	0.046%
6	3.172	339	342	343	rBV2	660	780	0.09%	0.012%
7	3.319	364	366	368	rBV	961	928	0.10%	0.014%
8	3.471	389	391	397	rVB	422	459	0.05%	0.007%
9	3.599	409	412	415	rBV	649	717	0.08%	0.011%
10	3.764	438	439	442	rVV2	445	442	0.05%	0.007%
11	3.825	445	449	450	rBV2	585	576	0.06%	0.009%
12	3.995	473	477	479	rBV	436	543	0.06%	0.008%
13	4.075	488	490	491	rBV	569	439	0.05%	0.007%
14	4.203	507	511	514	rBV2	569	874	0.10%	0.013%
15	4.355	532	536	537	rBV2	482	595	0.07%	0.009%
16	4.459	541	553	568	rBV2	65563	194769	21.76%	2.945%
17	5.062	641	652	667	rBV	122203	361098	40.34%	5.461%
18	5.550	730	732	733	rVV2	621	468	0.05%	0.007%
19	5.769	767	768	770	rBV	531	429	0.05%	0.006%
20	5.806	773	774	776	rVV	638	430	0.05%	0.007%
21	5.830	776	778	783	rVV2	652	1047	0.12%	0.016%
22	5.873	783	785	787	rVV	824	548	0.06%	0.008%
23	5.977	787	802	820	rVV2	301156	895076	100.00%	13.536%
24	6.092	820	821	823	rVV	871	582	0.07%	0.009%
25	6.111	823	824	827	rVB2	858	639	0.07%	0.010%
26	6.190	834	837	838	rBV	916	841	0.09%	0.013%
27	6.208	838	840	841	rVV	745	495	0.06%	0.007%
28	6.330	859	860	863	rBV	412	535	0.06%	0.008%
29	6.495	885	887	890	rVB2	810	743	0.08%	0.011%
30	6.519	890	891	893	rBV	571	491	0.05%	0.007%
31	6.574	898	900	904	rVV2	571	644	0.07%	0.010%
32	6.769	922	932	945	rBV	202489	491156	54.87%	7.428%
33	6.989	966	968	971	rBV	690	585	0.07%	0.009%
34	7.117	982	989	995	rVB4	3398	7795	0.87%	0.118%
35	7.312	1012	1021	1033	rBV	188250	410135	45.82%	6.202%
36	7.489	1048	1050	1054	rVV2	934	1120	0.13%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
 Data File : VX026110.D
 Acq On : 28 Dec 2021 20:23
 Operator : JC/MD
 Sample : M5123-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
 Title : VOC Analysis

37	7.556	1060	1061	1063	rVB	733	435	0.05%	0.007%
38	7.580	1063	1065	1068	rBV	499	619	0.07%	0.009%
39	7.775	1093	1097	1098	rBV	457	492	0.05%	0.007%
40	7.812	1101	1103	1109	rVB3	655	977	0.11%	0.015%
41	7.909	1117	1119	1120	rBV	555	498	0.06%	0.008%
42	8.037	1137	1140	1141	rBV	668	552	0.06%	0.008%
43	8.104	1149	1151	1152	rBV	627	433	0.05%	0.007%
44	8.281	1178	1180	1181	rBV	552	429	0.05%	0.006%
45	8.330	1181	1188	1195	rBV	129377	215030	24.02%	3.252%
46	8.562	1223	1226	1229	rVB2	892	940	0.11%	0.014%
47	8.604	1229	1233	1234	rBV	633	1026	0.11%	0.016%
48	8.653	1234	1241	1248	rVV	456361	711491	79.49%	10.760%
49	8.726	1248	1253	1262	rVB2	6883	13277	1.48%	0.201%
50	8.787	1262	1263	1266	rBV	772	715	0.08%	0.011%
51	8.854	1271	1274	1277	rVB	406	517	0.06%	0.008%
52	8.952	1285	1290	1304	rBV	95382	138337	15.46%	2.092%
53	9.043	1304	1305	1309	rVB	681	435	0.05%	0.007%
54	9.153	1320	1323	1324	rBV2	559	499	0.06%	0.008%
55	9.281	1340	1344	1348	rBV2	951	1466	0.16%	0.022%
56	9.336	1348	1353	1355	rVV4	1186	2335	0.26%	0.035%
57	9.385	1356	1361	1382	rVB	294161	415211	46.39%	6.279%
58	9.561	1388	1390	1395	rBV	803	1096	0.12%	0.017%
59	9.769	1421	1424	1426	rBV2	765	1029	0.11%	0.016%
60	10.055	1466	1471	1484	rVB	428086	567118	63.36%	8.576%
61	10.305	1509	1512	1514	rBV2	1196	1720	0.19%	0.026%
62	10.372	1520	1523	1525	rBV	568	527	0.06%	0.008%
63	10.671	1569	1572	1573	rBV2	489	438	0.05%	0.007%
64	10.707	1576	1578	1579	rVV2	903	616	0.07%	0.009%
65	10.756	1582	1586	1589	rBV2	604	897	0.10%	0.014%
66	11.037	1629	1632	1633	rBV	640	537	0.06%	0.008%
67	11.067	1636	1637	1640	rVB	609	442	0.05%	0.007%
68	11.122	1642	1646	1651	rBV3	3639	5273	0.59%	0.080%
69	11.195	1652	1658	1665	rVV	316578	394553	44.08%	5.967%
70	11.329	1676	1680	1683	rVB2	3705	5106	0.57%	0.077%
71	11.445	1697	1699	1701	rBV2	676	553	0.06%	0.008%
72	11.488	1701	1706	1708	rBV3	1325	1959	0.22%	0.030%
73	11.750	1746	1749	1753	rVV4	3063	3904	0.44%	0.059%
74	11.841	1762	1764	1768	rVB	1055	980	0.11%	0.015%
75	11.933	1775	1779	1782	rBV2	2036	2661	0.30%	0.040%
76	12.024	1789	1794	1804	rVB	417764	509692	56.94%	7.708%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
 Data File : VX026110.D
 Acq On : 28 Dec 2021 20:23
 Operator : JC/MD
 Sample : M5123-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
 Title : VOC Analysis

77	12.091	1804	1805	1807	rBV	598	514	0.06%	0.008%
78	12.128	1807	1811	1812	rVV3	1243	1766	0.20%	0.027%
79	12.152	1812	1815	1820	rVB4	2452	3514	0.39%	0.053%
80	12.323	1835	1843	1851	rBV	444978	577528	64.52%	8.734%
81	12.616	1889	1891	1893	rBV2	482	547	0.06%	0.008%
82	12.658	1895	1898	1901	rBV2	933	1274	0.14%	0.019%
83	12.817	1923	1924	1929	rVB	619	529	0.06%	0.008%
84	12.866	1929	1932	1933	rBV	599	543	0.06%	0.008%
85	13.055	1960	1963	1966	rVB	893	1022	0.11%	0.015%
86	13.116	1972	1973	1979	rVB2	770	817	0.09%	0.012%
87	13.335	2006	2009	2011	rBV	575	551	0.06%	0.008%
88	13.353	2011	2012	2016	rVB	558	614	0.07%	0.009%
89	13.469	2028	2031	2032	rBV2	684	614	0.07%	0.009%
90	13.603	2052	2053	2058	rBV2	712	1012	0.11%	0.015%
91	13.933	2103	2107	2110	rVB2	618	1003	0.11%	0.015%
92	13.957	2110	2111	2114	rBV2	610	658	0.07%	0.010%
93	14.036	2122	2124	2127	rBV2	654	811	0.09%	0.012%
94	14.140	2140	2141	2144	rVB	1110	1002	0.11%	0.015%
95	14.170	2144	2146	2150	rBV2	381	687	0.08%	0.010%
96	14.304	2164	2168	2170	rVB	561	832	0.09%	0.013%
97	14.902	2264	2266	2267	rBV	748	527	0.06%	0.008%
98	15.060	2290	2292	2294	rBV	630	439	0.05%	0.007%
99	16.408	2511	2513	2517	rVB	783	743	0.08%	0.011%
100	16.719	2562	2564	2566	rBV	658	612	0.07%	0.009%


Sum of corrected areas: 6612493

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
Data File : VX026110.D
Acq On : 28 Dec 2021 20:23
Operator : JC/MD
Sample : M5123-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

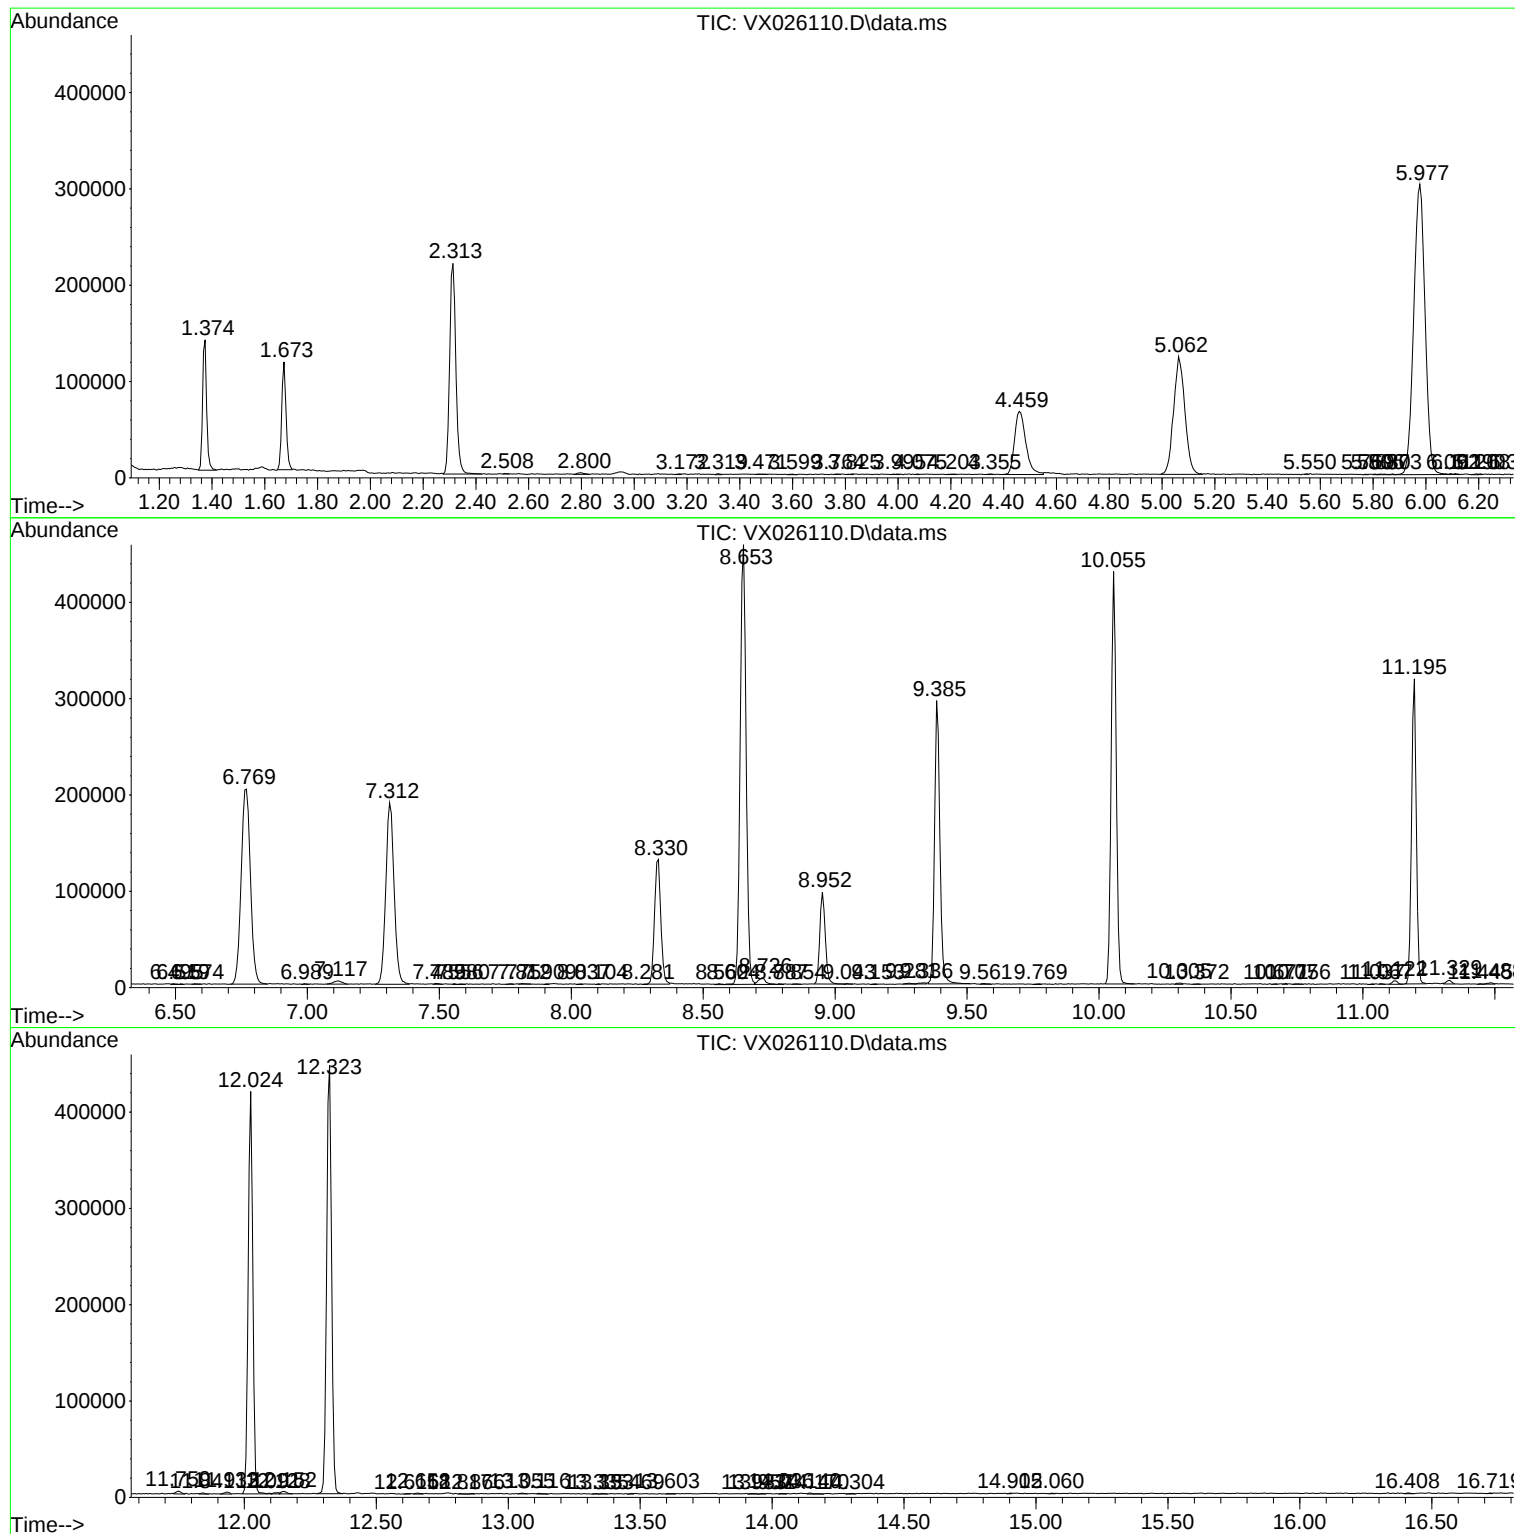

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
Data File : VX026110.D
Acq On : 28 Dec 2021 20:23
Operator : JC/MD
Sample : M5123-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
Data File : VX026110.D
Acq On : 28 Dec 2021 20:23
Operator : JC/MD
Sample : M5123-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc