

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
 Data File : VX026113.D
 Acq On : 28 Dec 2021 21:32
 Operator : JC/MD
 Sample : M5216-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COHB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
 Title : VOC Analysis

Signal : TIC: VX026113.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	55	rVB	131868	138207	15.36%	1.853%
2	1.672	92	96	105	rVB	107941	128748	14.31%	1.726%
3	2.313	195	201	211	rVB	215629	344378	38.27%	4.617%
4	2.947	298	305	315	rVV	25199	58458	6.50%	0.784%
5	3.038	318	320	322	rVB	924	579	0.06%	0.008%
6	3.093	327	329	331	rBV2	929	692	0.08%	0.009%
7	3.294	359	362	363	rBV	673	701	0.08%	0.009%
8	3.385	375	377	381	rBV	793	830	0.09%	0.011%
9	3.763	435	439	442	rBV2	682	785	0.09%	0.011%
10	3.837	449	451	455	rBV	903	1406	0.16%	0.019%
11	3.910	461	463	465	rBV	668	748	0.08%	0.010%
12	4.013	478	480	482	rBV	1007	928	0.10%	0.012%
13	4.123	497	498	499	rBV	839	596	0.07%	0.008%
14	4.221	512	514	515	rBV	896	793	0.09%	0.011%
15	4.245	517	518	521	rVB	1329	712	0.08%	0.010%
16	4.300	521	527	529	rBV2	900	1745	0.19%	0.023%
17	4.465	545	554	566	rBV	67317	195540	21.73%	2.621%
18	4.824	611	613	615	rBV	1034	873	0.10%	0.012%
19	4.843	615	616	619	rVB	785	657	0.07%	0.009%
20	4.989	638	640	641	rBV	1157	838	0.09%	0.011%
21	5.068	642	653	668	rVB	124505	360968	40.11%	4.839%
22	5.233	678	680	685	rVB	609	926	0.10%	0.012%
23	5.556	731	733	734	rBV	835	675	0.08%	0.009%
24	5.653	744	749	752	rBV	1091	2037	0.23%	0.027%
25	5.684	752	754	758	rBV	1250	1557	0.17%	0.021%
26	5.714	758	759	763	rVV	795	765	0.09%	0.010%
27	5.976	790	802	824	rVB2	296346	899848	100.00%	12.064%
28	6.165	832	833	836	rBV	829	629	0.07%	0.008%
29	6.415	870	874	877	rBV2	798	1182	0.13%	0.016%
30	6.531	887	893	896	rBV	1007	2038	0.23%	0.027%
31	6.617	905	907	910	rBV	782	801	0.09%	0.011%
32	6.769	923	932	942	rBV	204083	483103	53.69%	6.477%
33	6.940	957	960	964	rBV	1083	1319	0.15%	0.018%
34	7.123	984	990	994	rVB6	3334	7217	0.80%	0.097%
35	7.177	997	999	1002	rVB	710	583	0.06%	0.008%
36	7.214	1002	1005	1006	rBV	1036	941	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
 Data File : VX026113.D
 Acq On : 28 Dec 2021 21:32
 Operator : JC/MD
 Sample : M5216-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COHB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
 Title : VOC Analysis

37	7.312	1013	1021	1033	rBV	183642	396584	44.07%	5.317%
38	7.726	1085	1089	1090	rVV	822	789	0.09%	0.011%
39	7.744	1090	1092	1094	rVB	923	683	0.08%	0.009%
40	7.763	1094	1095	1098	rBV	584	702	0.08%	0.009%
41	7.854	1108	1110	1111	rBV	916	595	0.07%	0.008%
42	7.879	1113	1114	1118	rVV	630	646	0.07%	0.009%
43	7.946	1119	1125	1127	rVV4	927	1739	0.19%	0.023%
44	8.220	1168	1170	1173	rBV	699	698	0.08%	0.009%
45	8.330	1182	1188	1196	rBV	130982	213420	23.72%	2.861%
46	8.470	1210	1211	1214	rBV3	778	756	0.08%	0.010%
47	8.653	1233	1241	1249	rBV	449957	695518	77.29%	9.324%
48	8.726	1249	1253	1258	rVB2	7567	11774	1.31%	0.158%
49	8.781	1258	1262	1264	rBV3	528	826	0.09%	0.011%
50	8.866	1274	1276	1278	rBV	827	1005	0.11%	0.013%
51	8.952	1285	1290	1299	rBV	98557	138565	15.40%	1.858%
52	9.384	1356	1361	1375	rVB	292529	424927	47.22%	5.697%
53	9.762	1421	1423	1426	rVB	998	695	0.08%	0.009%
54	9.793	1426	1428	1430	rBV	578	636	0.07%	0.009%
55	9.957	1453	1455	1456	rBV	881	667	0.07%	0.009%
56	10.055	1465	1471	1484	rVV2	422668	797320	88.61%	10.689%
57	10.238	1499	1501	1502	rBV	1247	874	0.10%	0.012%
58	10.305	1509	1512	1516	rVB3	1365	2004	0.22%	0.027%
59	10.463	1537	1538	1541	rBV	937	913	0.10%	0.012%
60	11.122	1642	1646	1652	rVB3	3414	5382	0.60%	0.072%
61	11.195	1652	1658	1666	rBV	305863	391899	43.55%	5.254%
62	11.329	1676	1680	1686	rVB2	5245	7435	0.83%	0.100%
63	11.476	1700	1704	1708	rBV3	1639	3036	0.34%	0.041%
64	11.543	1714	1715	1718	rVB	1047	936	0.10%	0.013%
65	11.622	1722	1728	1729	rBV	764	1133	0.13%	0.015%
66	11.725	1741	1745	1746	rVV2	724	976	0.11%	0.013%
67	11.750	1746	1749	1752	rVB3	2923	3485	0.39%	0.047%
68	11.835	1761	1763	1765	rBV3	631	673	0.07%	0.009%
69	11.896	1771	1773	1777	rVB	877	593	0.07%	0.008%
70	11.933	1777	1779	1781	rBV3	1975	2295	0.26%	0.031%
71	11.969	1781	1785	1789	rVV	19223	26074	2.90%	0.350%
72	12.024	1789	1794	1805	rVB2	424014	708092	78.69%	9.493%
73	12.219	1823	1826	1830	rBV2	2865	3084	0.34%	0.041%
74	12.323	1838	1843	1852	rVB3	474075	740207	82.26%	9.924%
75	12.524	1874	1876	1878	rBV	878	724	0.08%	0.010%
76	12.658	1895	1898	1900	rBV2	1058	1276	0.14%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
 Data File : VX026113.D
 Acq On : 28 Dec 2021 21:32
 Operator : JC/MD
 Sample : M5216-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COHB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
 Title : VOC Analysis

77	12.762	1913	1915	1920	rVB2	1723	1870	0.21%	0.025%
78	12.805	1920	1922	1923	rVB2	998	581	0.06%	0.008%
79	12.926	1940	1942	1944	rBV	755	609	0.07%	0.008%
80	13.054	1961	1963	1966	rVV2	895	985	0.11%	0.013%
81	13.219	1988	1990	1993	rBV	757	860	0.10%	0.012%
82	13.439	2025	2026	2029	rBV	749	687	0.08%	0.009%
83	13.591	2045	2051	2059	rVV	105206	137253	15.25%	1.840%
84	13.646	2059	2060	2062	rVB	1215	602	0.07%	0.008%
85	13.737	2073	2075	2076	rVV	1032	625	0.07%	0.008%
86	13.768	2079	2080	2085	rVB3	800	971	0.11%	0.013%
87	13.963	2103	2112	2117	rBV3	26611	37265	4.14%	0.500%
88	14.127	2136	2139	2140	rBV2	846	801	0.09%	0.011%
89	14.347	2173	2175	2177	rBV	816	745	0.08%	0.010%
90	14.365	2177	2178	2181	rBV	788	592	0.07%	0.008%
91	14.786	2243	2247	2252	rVB2	5320	6635	0.74%	0.089%
92	15.152	2305	2307	2309	rBV	752	855	0.10%	0.011%
93	15.255	2319	2324	2328	rVB2	19685	27738	3.08%	0.372%
94	15.530	2366	2369	2370	rBV	1109	782	0.09%	0.010%
95	15.895	2427	2429	2430	rBV2	869	764	0.08%	0.010%
96	16.054	2453	2455	2459	rVV	1259	1482	0.16%	0.020%
97	16.164	2470	2473	2475	rBV	1136	1315	0.15%	0.018%
98	16.334	2500	2501	2505	rBV	862	853	0.09%	0.011%
99	16.548	2534	2536	2538	rBV	1212	1187	0.13%	0.016%
100	16.725	2563	2565	2567	rVB	889	629	0.07%	0.008%


Sum of corrected areas: 7459125

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
Data File : VX026113.D
Acq On : 28 Dec 2021 21:32
Operator : JC/MD
Sample : M5216-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COHB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

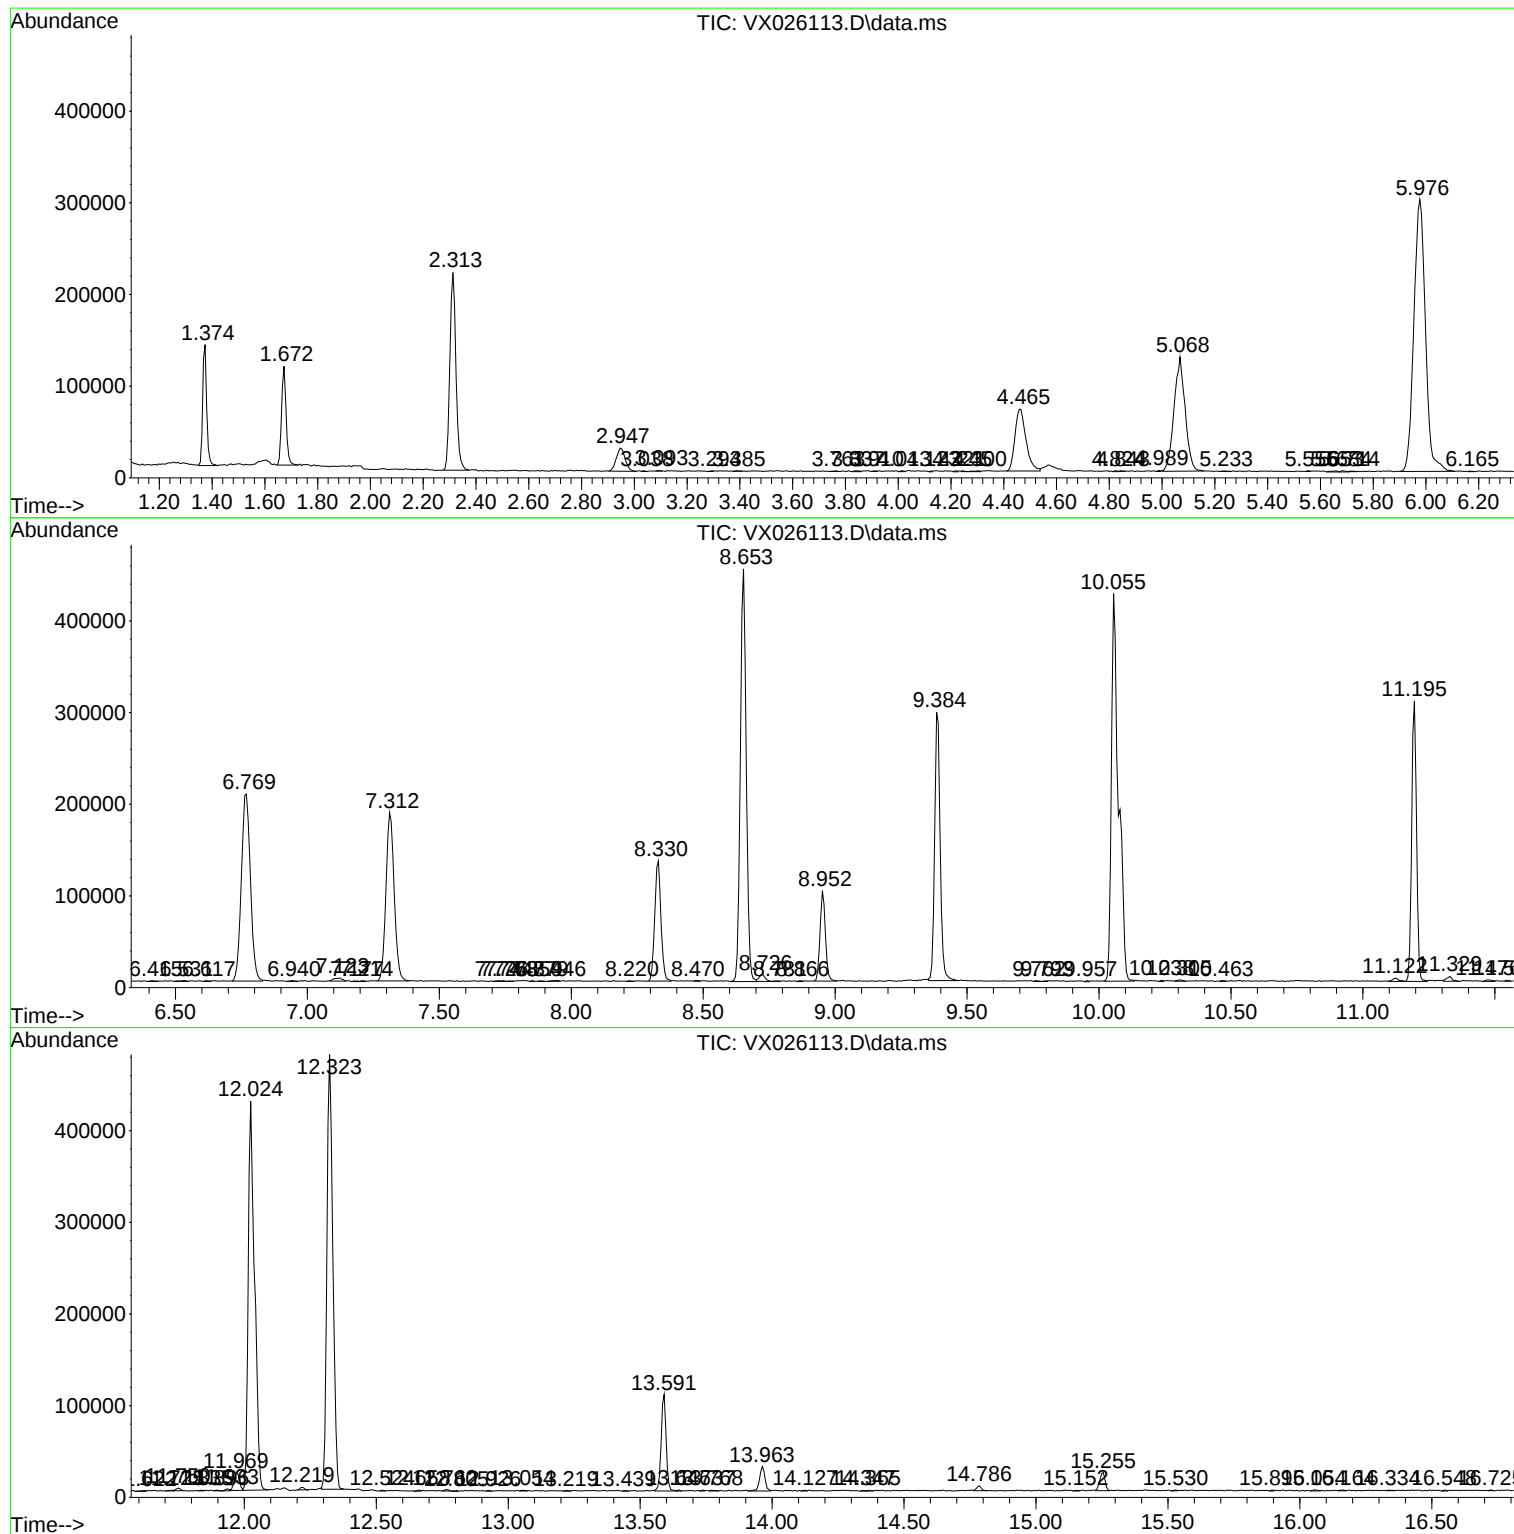

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
Data File : VX026113.D
Acq On : 28 Dec 2021 21:32
Operator : JC/MD
Sample : M5216-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COHB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
Data File : VX026113.D
Acq On : 28 Dec 2021 21:32
Operator : JC/MD
Sample : M5216-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COHB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc